

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061319\
Data File : P0057127.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jun 2019 16:27
Operator : SM/SJ
Sample : K2944-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FESB-6(4.5-5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 03:43:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.244	3.563	637073	629494	16.641	19.088
2)	SA Decachlor...	9.811	8.493	778482	505524	15.860	14.177

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061319\
Data File : PO057127.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jun 2019 16:27
Operator : SM/SJ
Sample : K2944-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FESB-6(4.5-5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 03:43:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

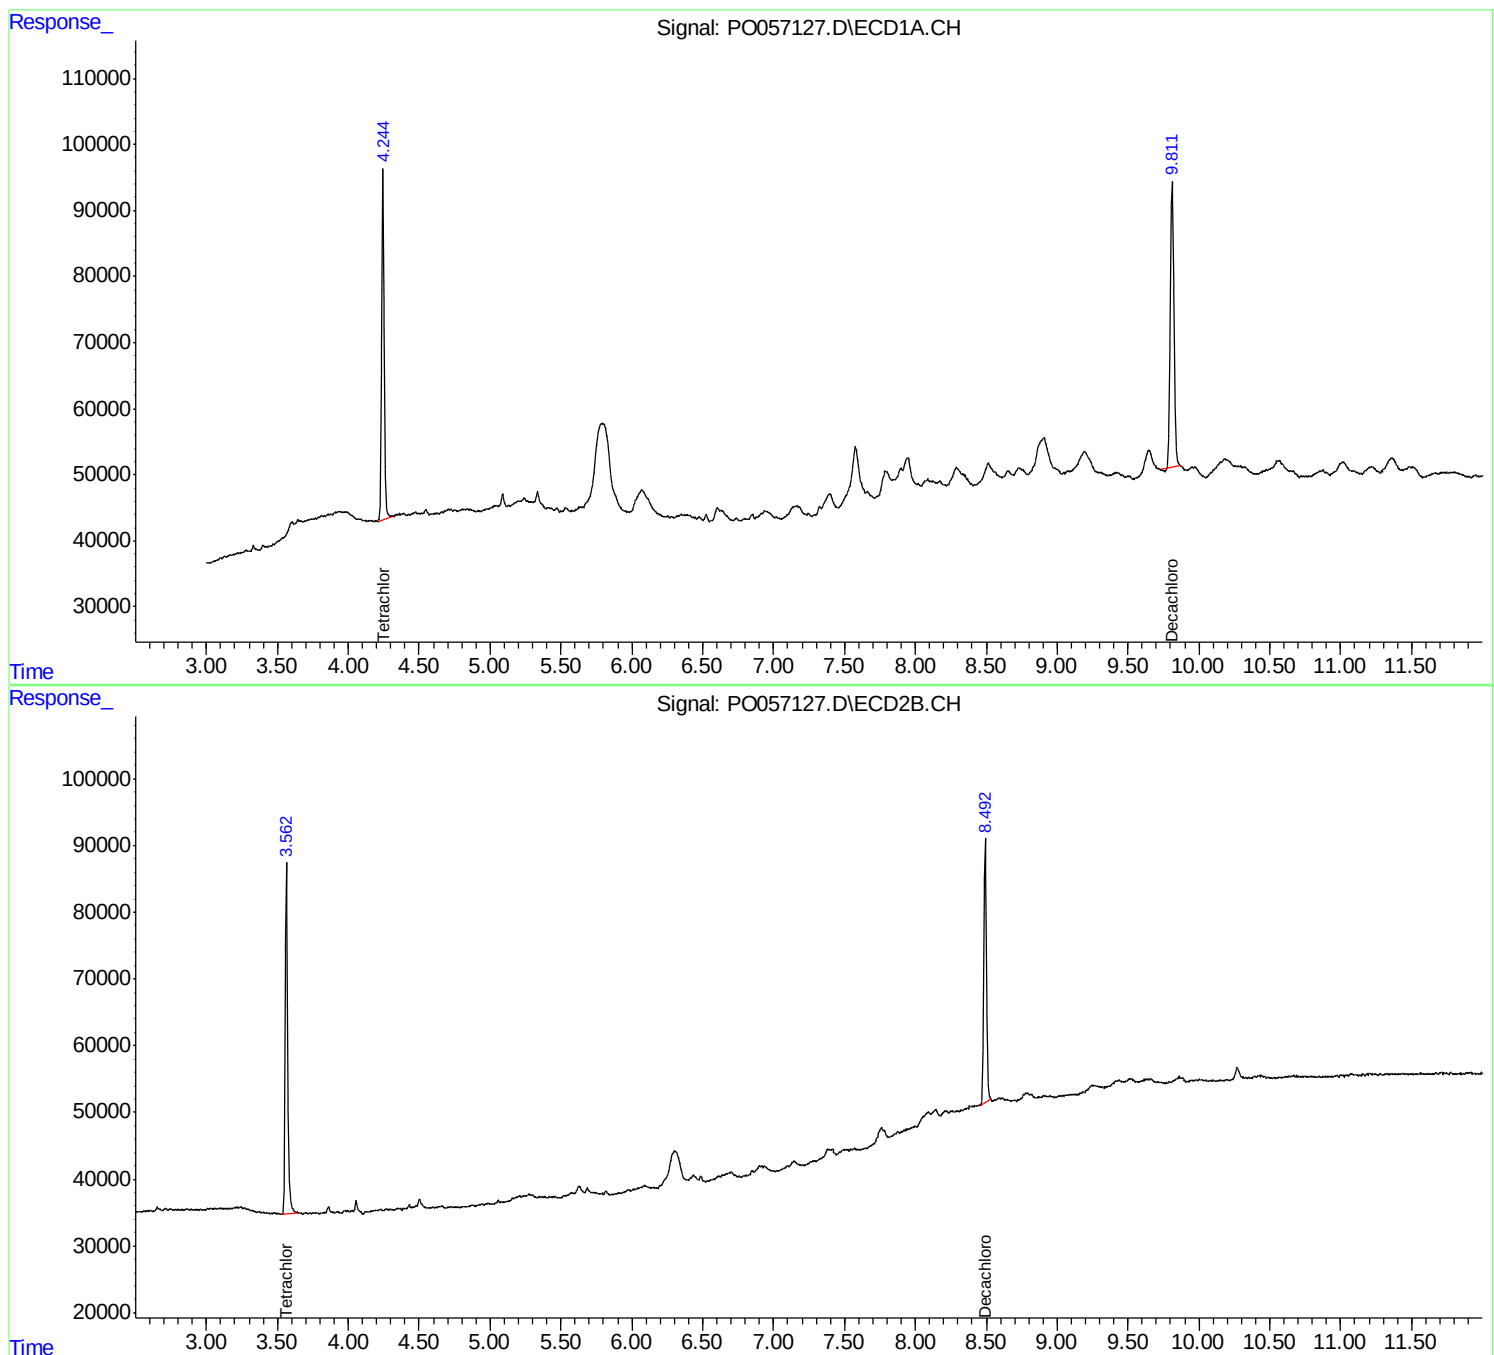


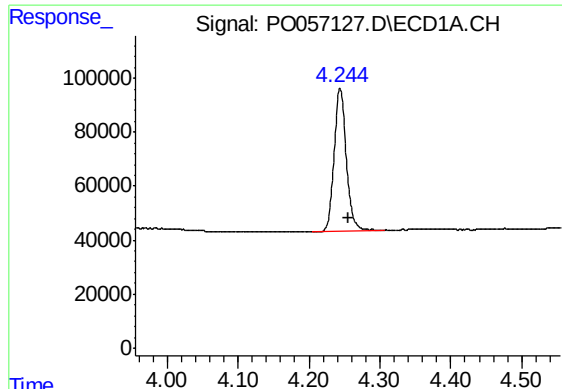

#1 Tetrachloro-m-xylene


R.T.: 4.244 min
Delta R.T.: -0.012 min
Response: 637073
Conc: 16.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
FESB-6(4.5-5)

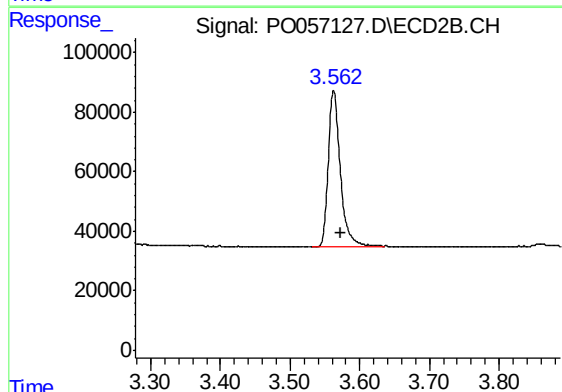


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.011 min
Response: 629494
Conc: 19.09 ng/ml

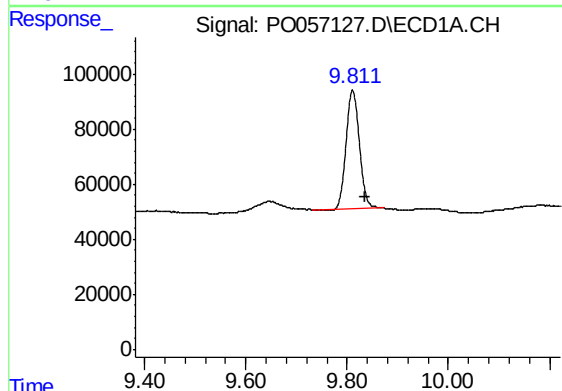

#2 Decachlorobiphenyl

R.T.: 9.811 min
Delta R.T.: -0.025 min
Response: 778482
Conc: 15.86 ng/ml

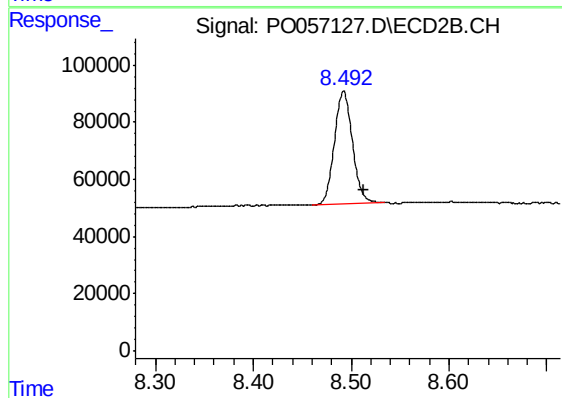

#2 Decachlorobiphenyl

R.T.: 8.493 min
Delta R.T.: -0.020 min
Response: 505524
Conc: 14.18 ng/ml