

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061319\
 Data File : P0057142.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jun 2019 20:42
 Operator : SM/SJ
 Sample : K3333-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONCRETE-5

Manual Integrations
 APPROVED

Ankita
 6/14/2019 11:08:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 03:47:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.242	3.563	688478	671423	17.984	20.359
2)	SA Decachlor...	9.805	8.491	1220309	809423	24.862	22.700m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061319\
Data File : PO057142.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jun 2019 20:42
Operator : SM/SJ
Sample : K3333-05
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CONCRETE-5


Manual Integrations
APPROVED

Ankita
6/14/2019 11:08:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 03:47:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

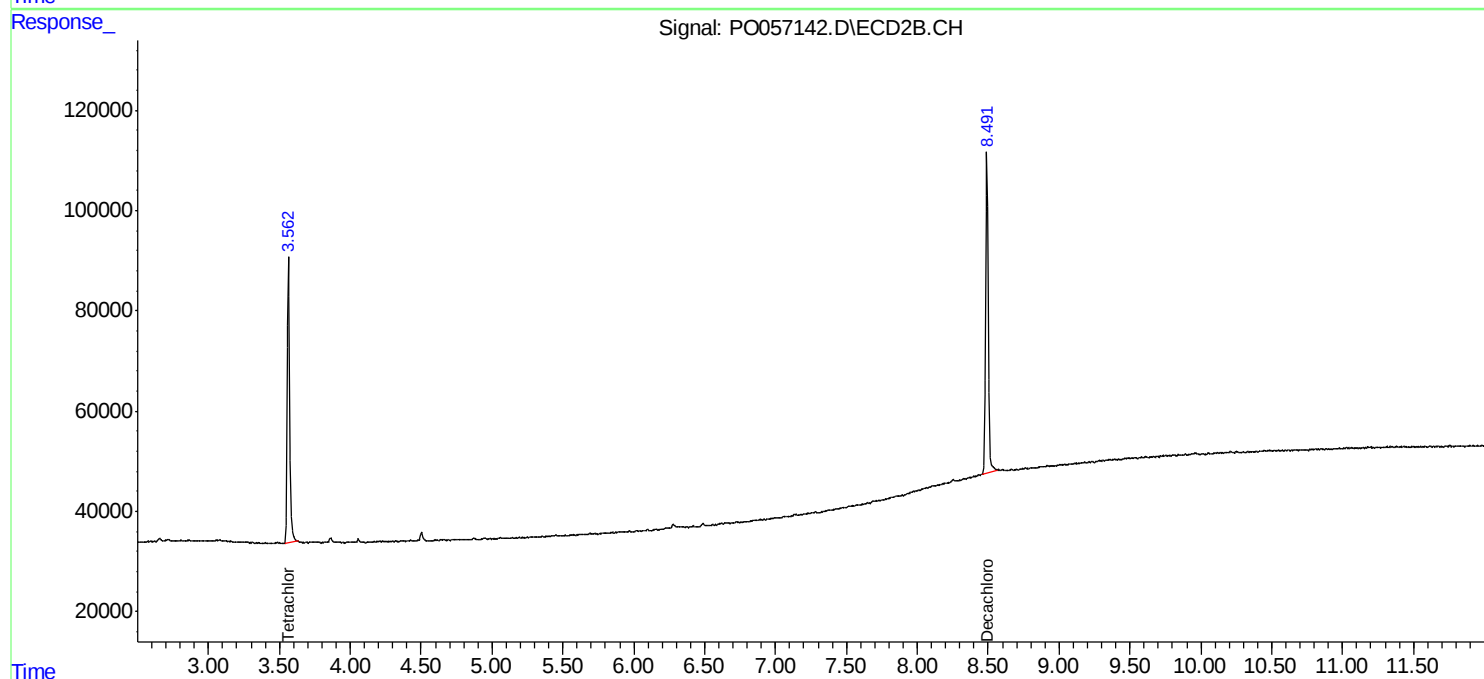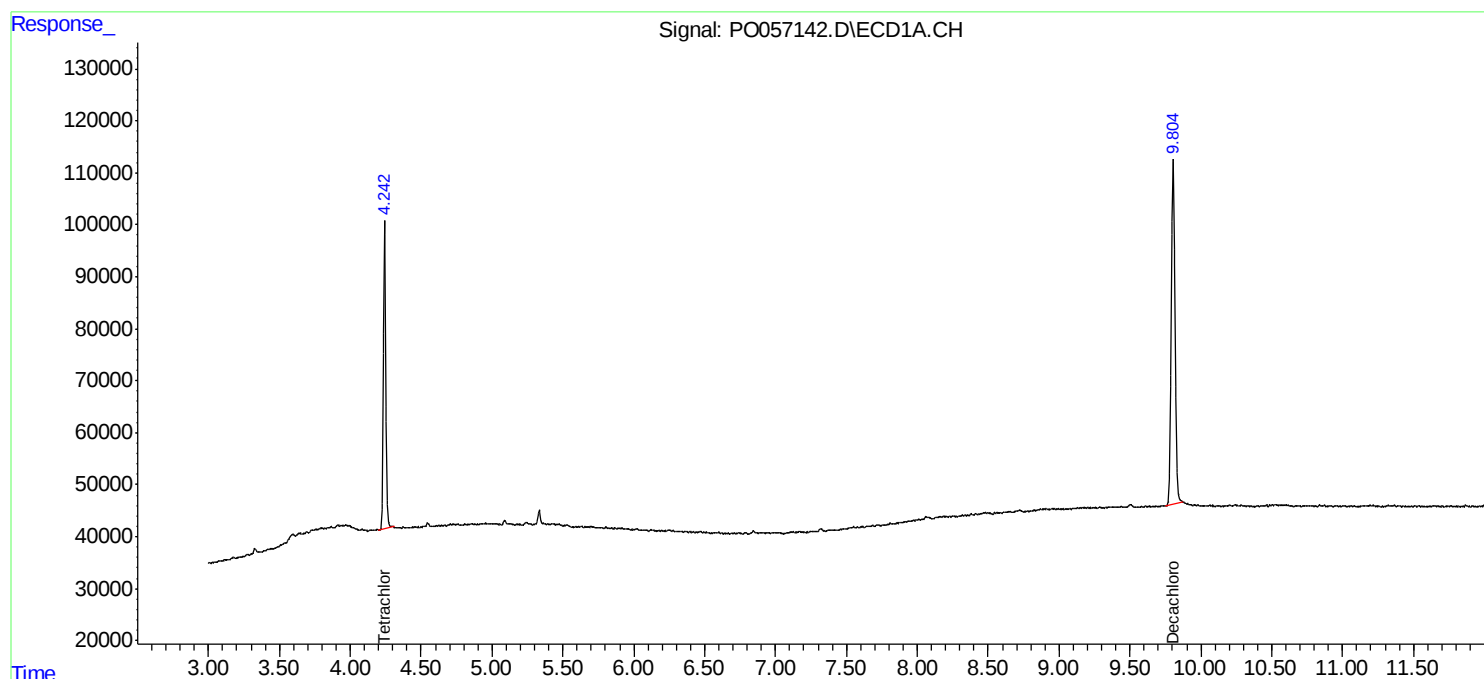

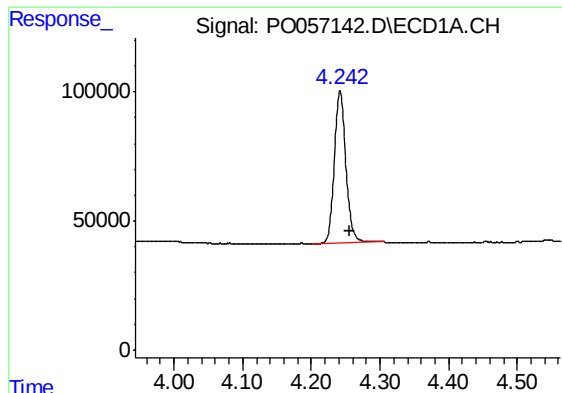


#1 Tetrachloro-m-xylene

R.T.: 4.242 min
Delta R.T.: -0.014 min
Response: 688478
Conc: 17.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-5


Manual Integrations
APPROVED

Ankita
6/14/2019 11:08:57 AM

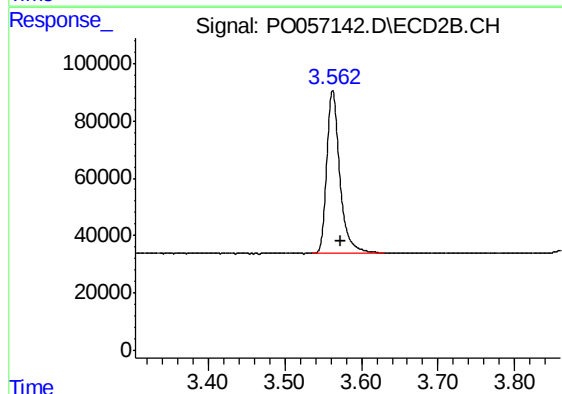


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.010 min
Response: 671423
Conc: 20.36 ng/ml

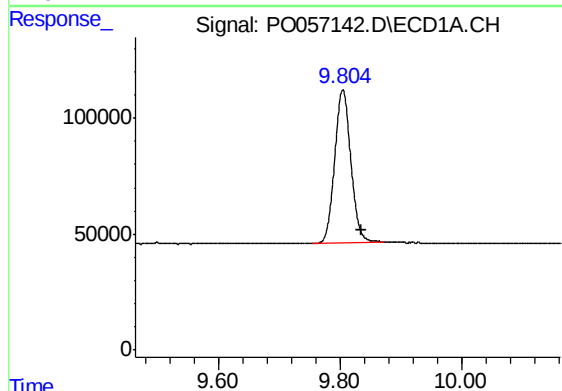

#2 Decachlorobiphenyl

R.T.: 9.805 min
Delta R.T.: -0.031 min
Response: 1220309
Conc: 24.86 ng/ml

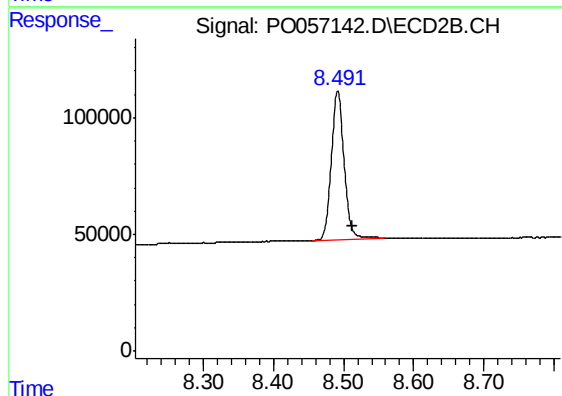

#2 Decachlorobiphenyl

R.T.: 8.491 min
Delta R.T.: -0.022 min
Response: 809423
Conc: 22.70 ng/ml m