

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061319\
 Data File : P0057148.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jun 2019 22:25
 Operator : SM/SJ
 Sample : K3340-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B-730(2)

Manual Integrations
 APPROVED

Ankita
 6/14/2019 11:09:06 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 03:49:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.241	3.562	623697	687065	16.292	20.834 #
2)	SA Decachlor...	9.803	8.489	1063780	689847	21.673m	19.347m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061319\
Data File : P0057148.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jun 2019 22:25
Operator : SM/SJ
Sample : K3340-03
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
B-730(2)


Manual Integrations
APPROVED

Ankita
6/14/2019 11:09:06 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 03:49:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

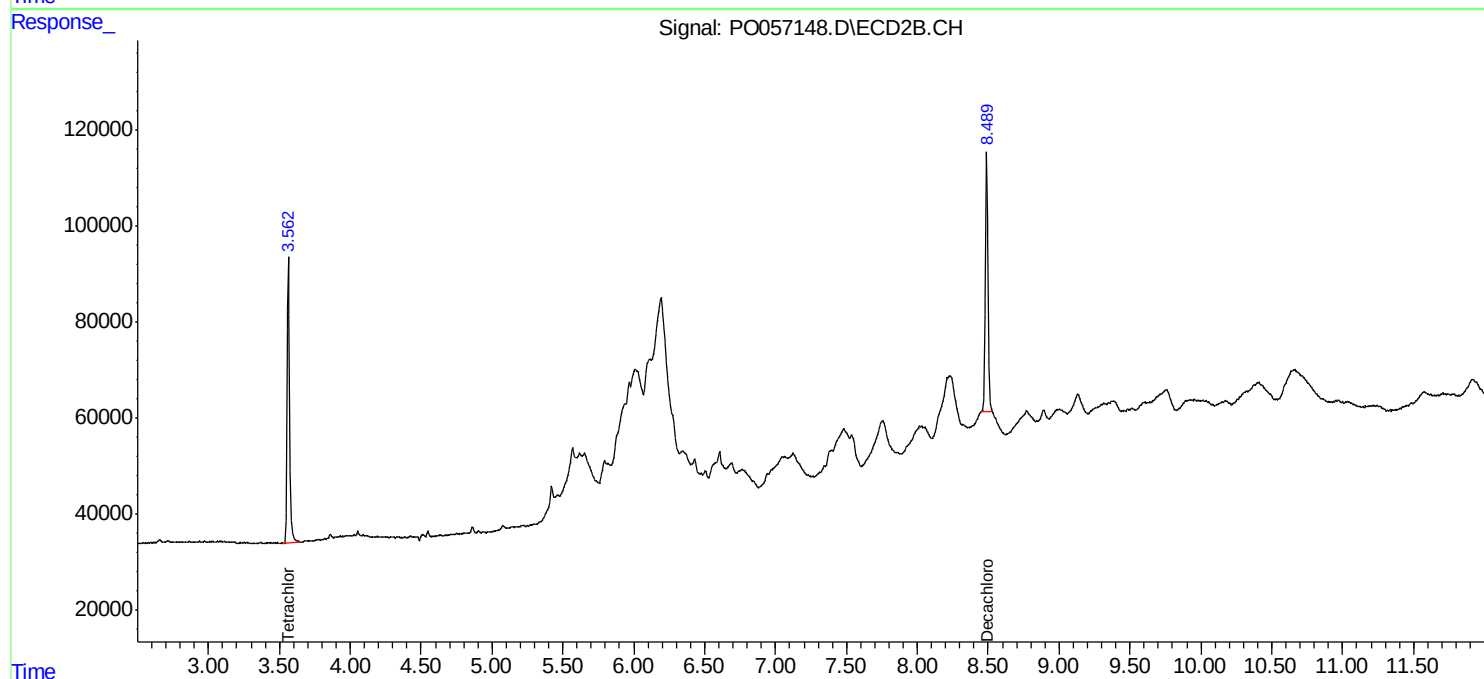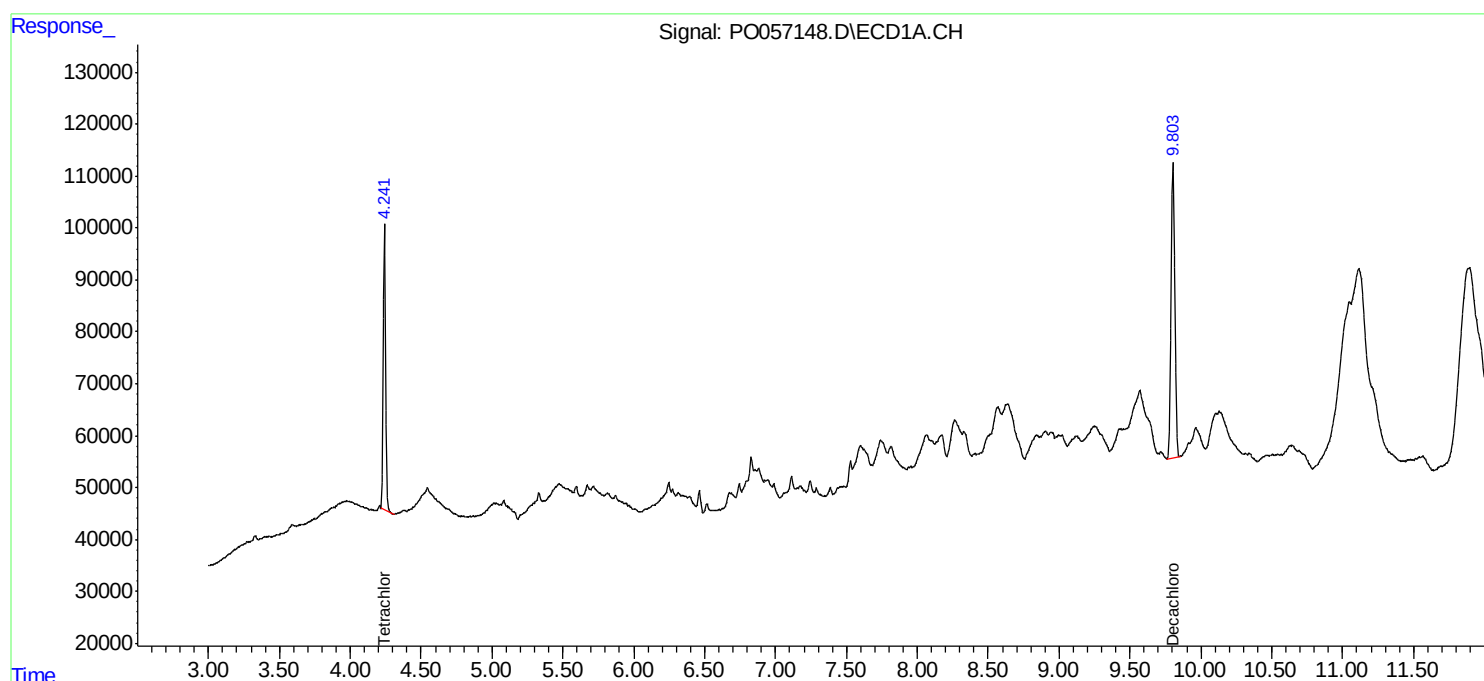

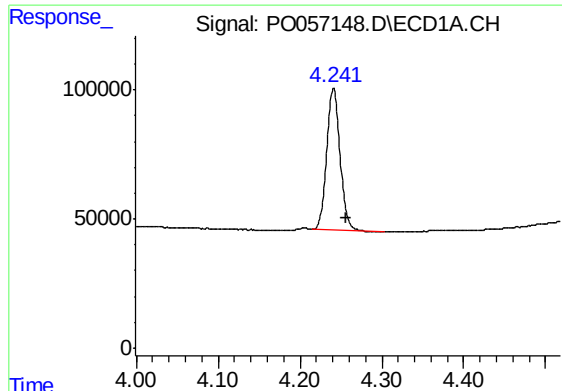


#1 Tetrachloro-m-xylene

R.T.: 4.241 min
Delta R.T.: -0.015 min
Response: 623697
Conc: 16.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
B-730(2)


Manual Integrations
APPROVED

Ankita
6/14/2019 11:09:06 AM

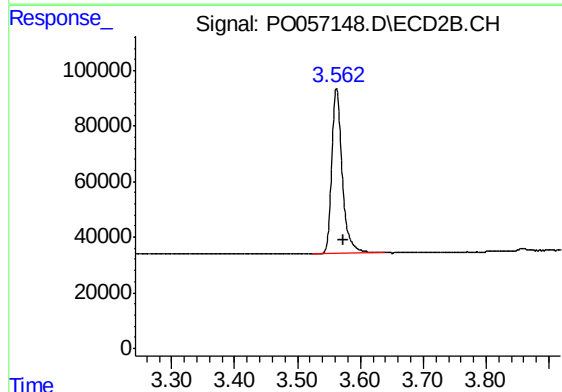


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: -0.011 min
Response: 687065
Conc: 20.83 ng/ml

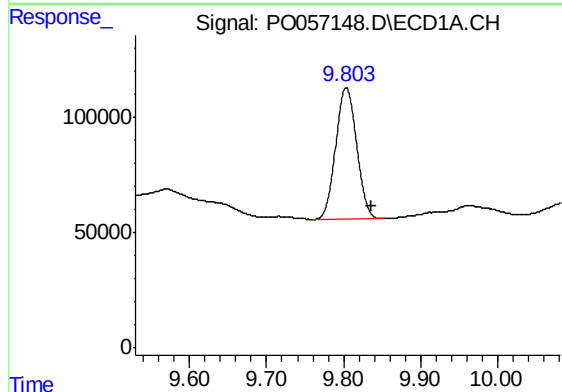

#2 Decachlorobiphenyl

R.T.: 9.803 min
Delta R.T.: -0.034 min
Response: 1063780
Conc: 21.67 ng/ml m

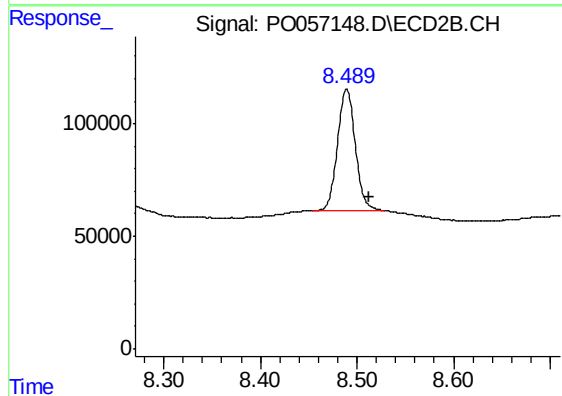

#2 Decachlorobiphenyl

R.T.: 8.489 min
Delta R.T.: -0.024 min
Response: 689847
Conc: 19.35 ng/ml m