

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061419\
 Data File : P0057159.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jun 2019 10:00
 Operator : SM/SJ
 Sample : K3343-01DL 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-0D015-03-008DL

Manual Integrations
 APPROVED

Ankita
 6/18/2019 9:33:33 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 11:23:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.254	3.564	365334	342505	9.543	10.386
2)	SA Decachlor...	9.823	8.494	563050	381946	11.471	10.712
Target Compounds							
26)	L6 AR-1254-1	6.259	5.423	1385416	1371100	503.287m	518.428
27)	L6 AR-1254-2	6.476	5.569	2434775	1400065	626.858	649.441m
28)	L6 AR-1254-3	6.841	5.969	2739361	2447795	664.347	668.602
29)	L6 AR-1254-4	7.125	6.196	2515526	1730144	835.769	787.527
30)	L6 AR-1254-5	7.541	6.608	3305584	2574054	877.828	811.943m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061419\
Data File : PO057159.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jun 2019 10:00
Operator : SM/SJ
Sample : K3343-01DL 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-0D015-03-008DL


Manual Integrations
APPROVED

Ankita
6/18/2019 9:33:33 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 11:23:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

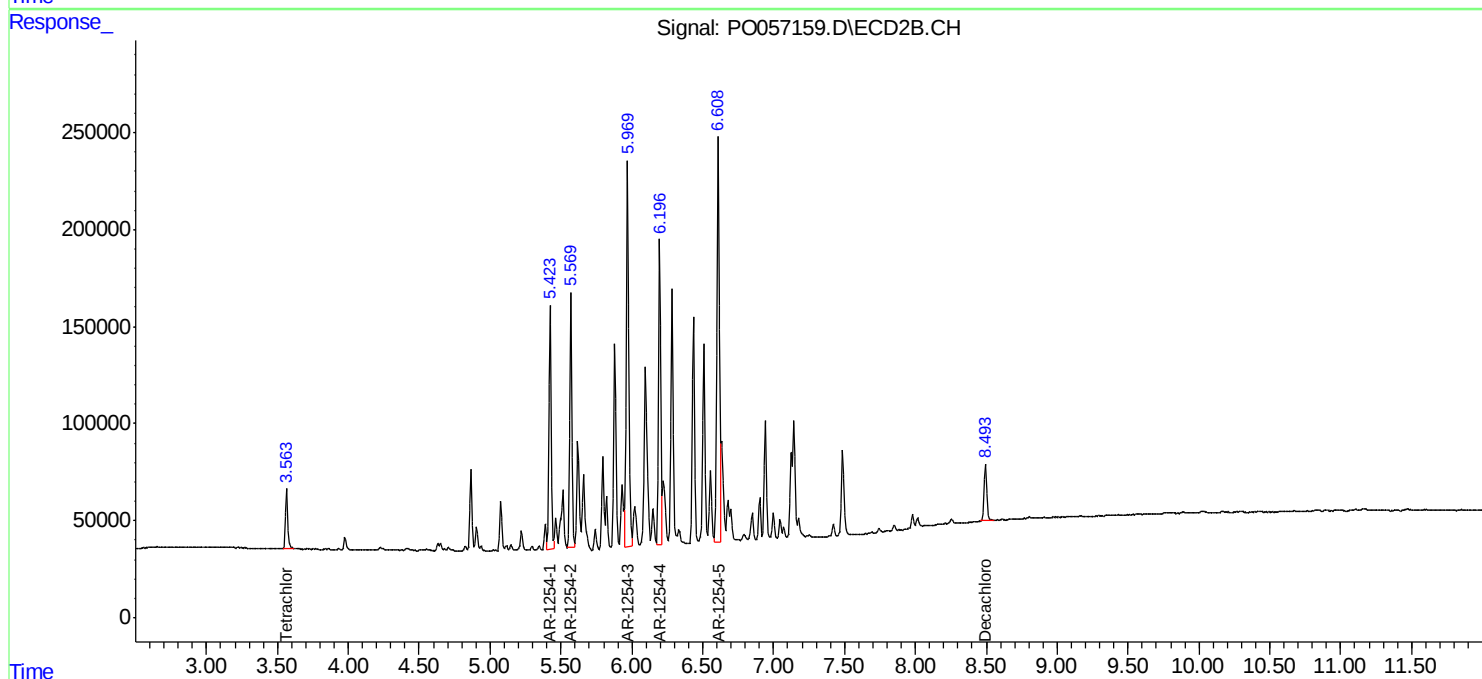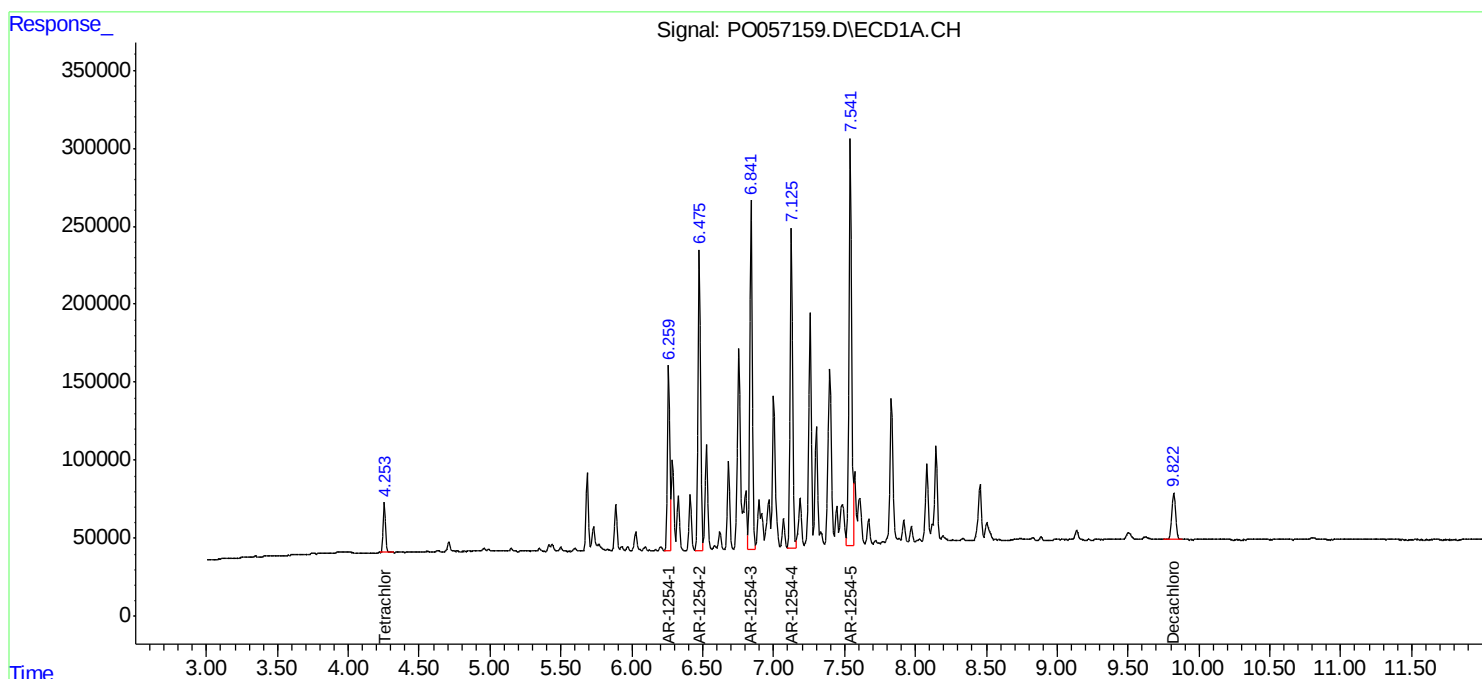

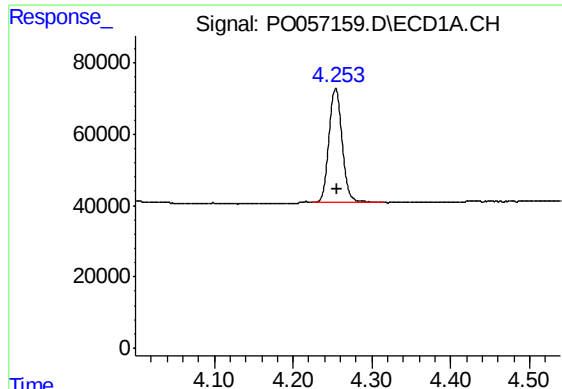


#1 Tetrachloro-m-xylene

R.T.: 4.254 min
Delta R.T.: -0.002 min
Response: 365334
Conc: 9.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-0D015-03-008DL


Manual Integrations
APPROVED

Ankita
6/18/2019 9:33:33 AM

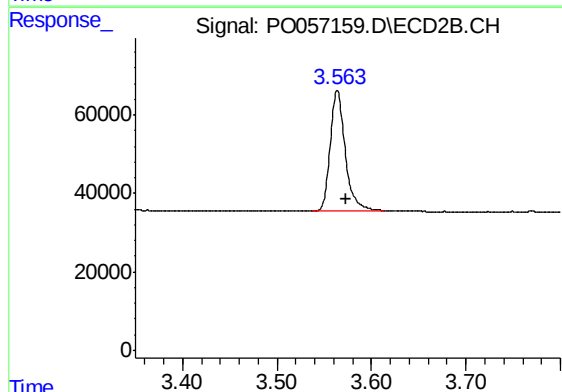


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: -0.009 min
Response: 342505
Conc: 10.39 ng/ml

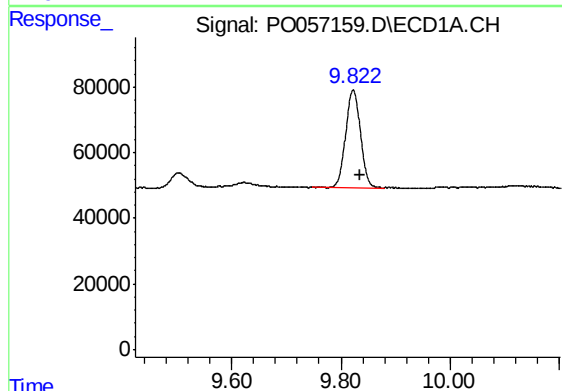


#2 Decachlorobiphenyl

R.T.: 9.823 min
Delta R.T.: -0.014 min
Response: 563050
Conc: 11.47 ng/ml

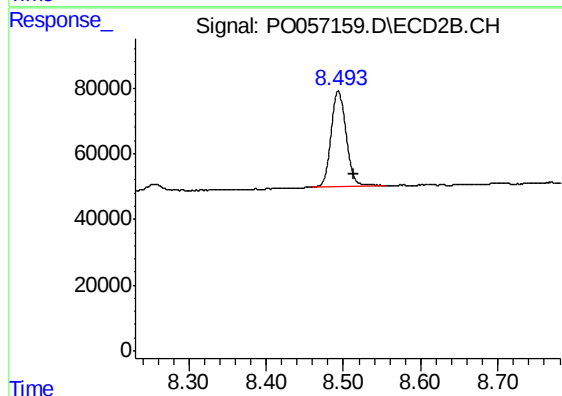

#2 Decachlorobiphenyl

R.T.: 8.494 min
Delta R.T.: -0.019 min
Response: 381946
Conc: 10.71 ng/ml

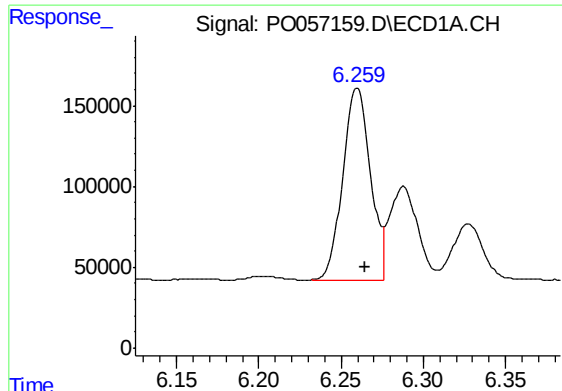


#26 AR-1254-1

R.T.: 6.259 min
Delta R.T.: -0.005 min
Response: 1385416
Conc: 503.29 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-0D015-03-008DL


Manual Integrations
APPROVED

Ankita
6/18/2019 9:33:33 AM

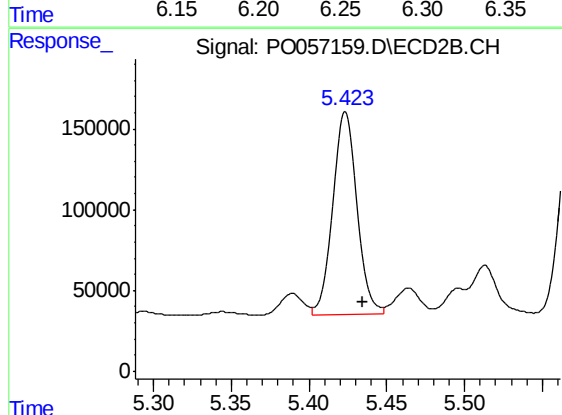


#26 AR-1254-1

R.T.: 5.423 min
Delta R.T.: -0.011 min
Response: 1371100
Conc: 518.43 ng/ml

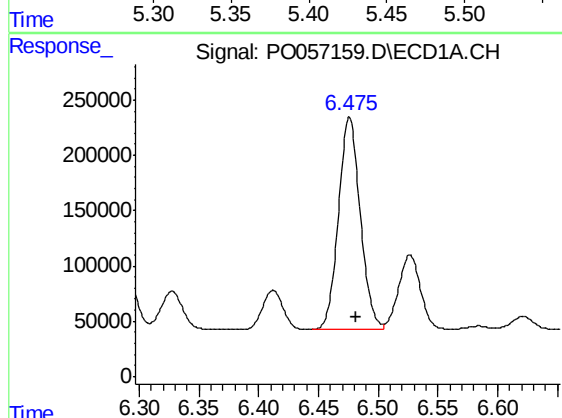


#27 AR-1254-2

R.T.: 6.476 min
Delta R.T.: -0.005 min
Response: 2434775
Conc: 626.86 ng/ml

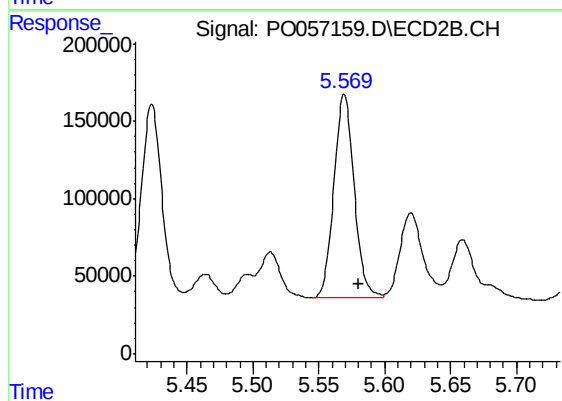

#27 AR-1254-2

R.T.: 5.569 min
Delta R.T.: -0.011 min
Response: 1400065
Conc: 649.44 ng/ml m

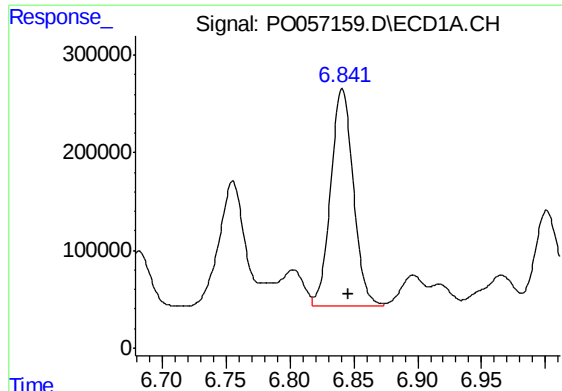


#28 AR-1254-3

R.T.: 6.841 min
Delta R.T.: -0.005 min
Response: 2739361
Conc: 664.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-0D015-03-008DL


Manual Integrations
APPROVED

Ankita
6/18/2019 9:33:33 AM

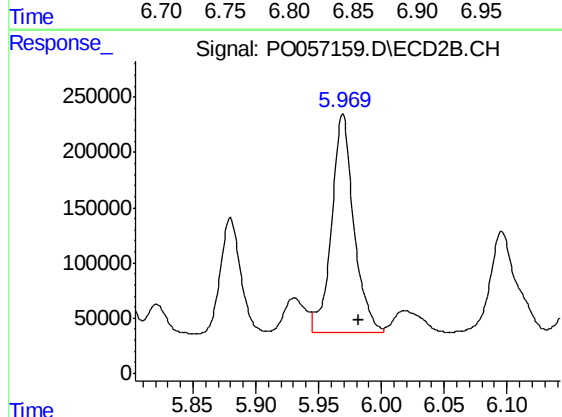


#28 AR-1254-3

R.T.: 5.969 min
Delta R.T.: -0.012 min
Response: 2447795
Conc: 668.60 ng/ml

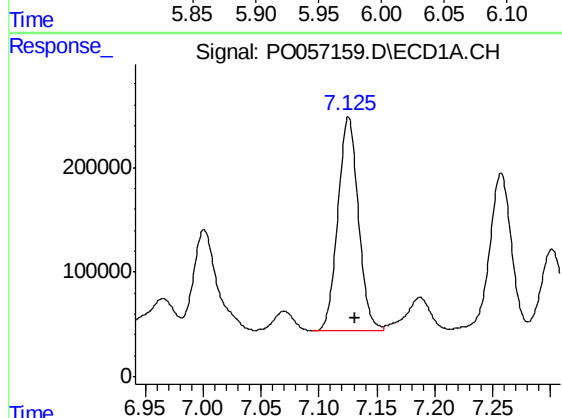


#29 AR-1254-4

R.T.: 7.125 min
Delta R.T.: -0.006 min
Response: 2515526
Conc: 835.77 ng/ml

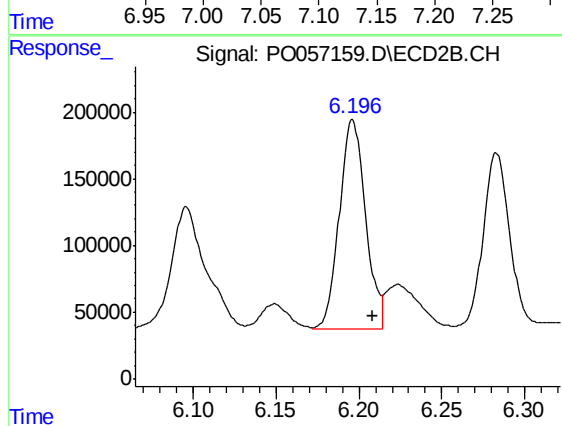

#29 AR-1254-4

R.T.: 6.196 min
Delta R.T.: -0.012 min
Response: 1730144
Conc: 787.53 ng/ml

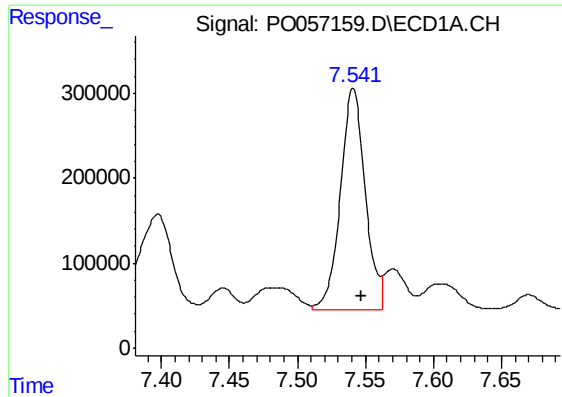


#30 AR-1254-5

R.T.: 7.541 min
Delta R.T.: -0.006 min
Response: 3305584
Conc: 877.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-0D015-03-008DL

Manual Integrations
APPROVED

Ankita
6/18/2019 9:33:33 AM

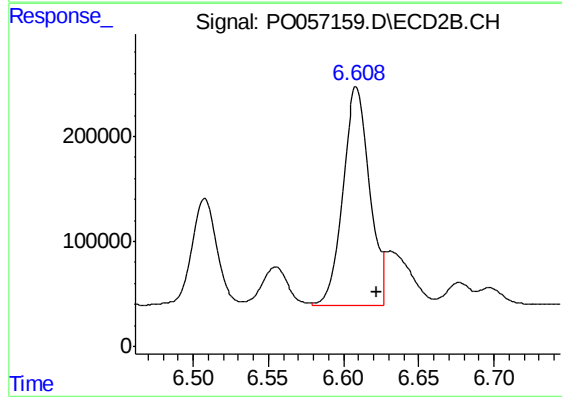

#30 AR-1254-5

R.T.: 6.608 min
Delta R.T.: -0.014 min
Response: 2574054
Conc: 811.94 ng/ml m