

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061419\
 Data File : P0057186.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jun 2019 20:47
 Operator : SM/SJ
 Sample : K3361-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BAT-B15

Manual Integrations
 APPROVED

Ankita
 6/18/2019 9:49:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 23:37:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.238	3.561	554114	549667	14.474m	16.667
2)	SA Decachlor...	9.799	8.486	687176	433298	14.000	12.152

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061419\
Data File : PO057186.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jun 2019 20:47
Operator : SM/SJ
Sample : K3361-04
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BAT-B15


Manual Integrations
APPROVED

Ankita
6/18/2019 9:49:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 23:37:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

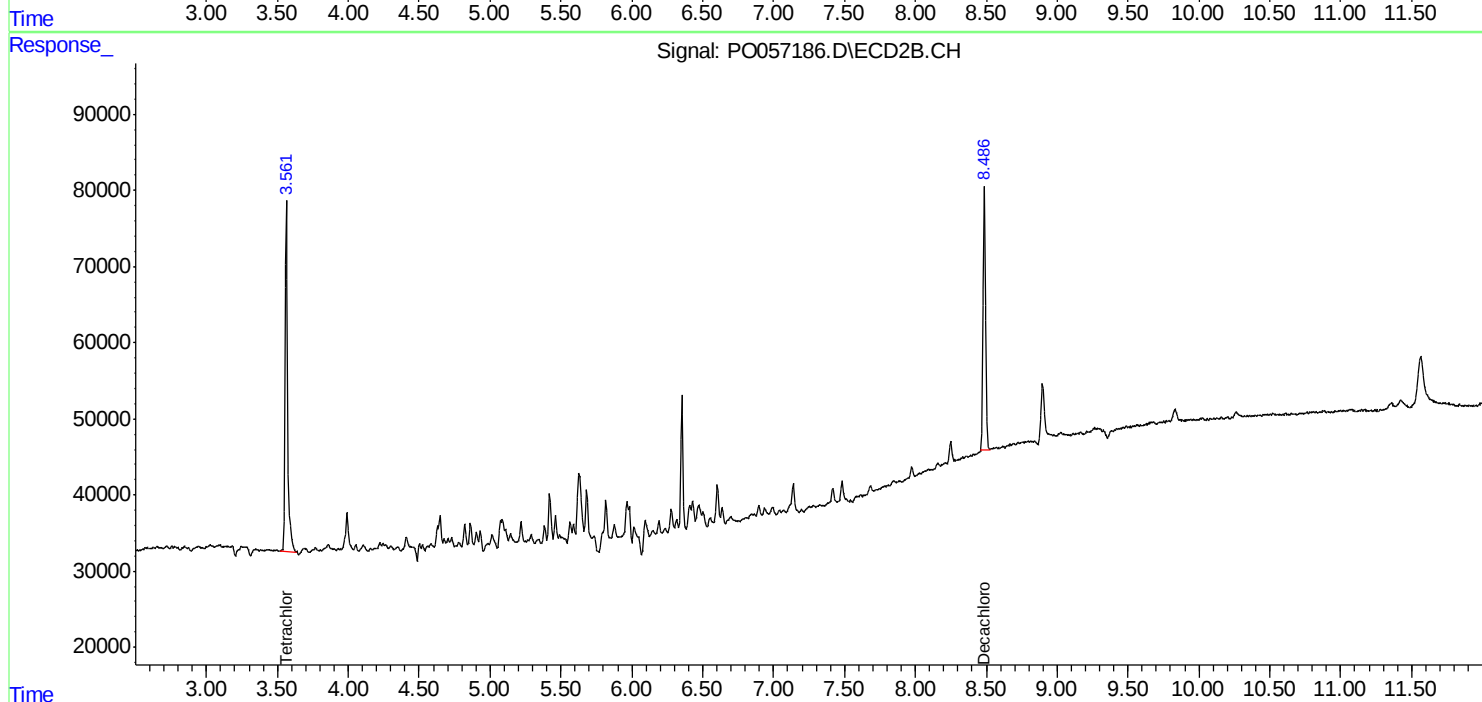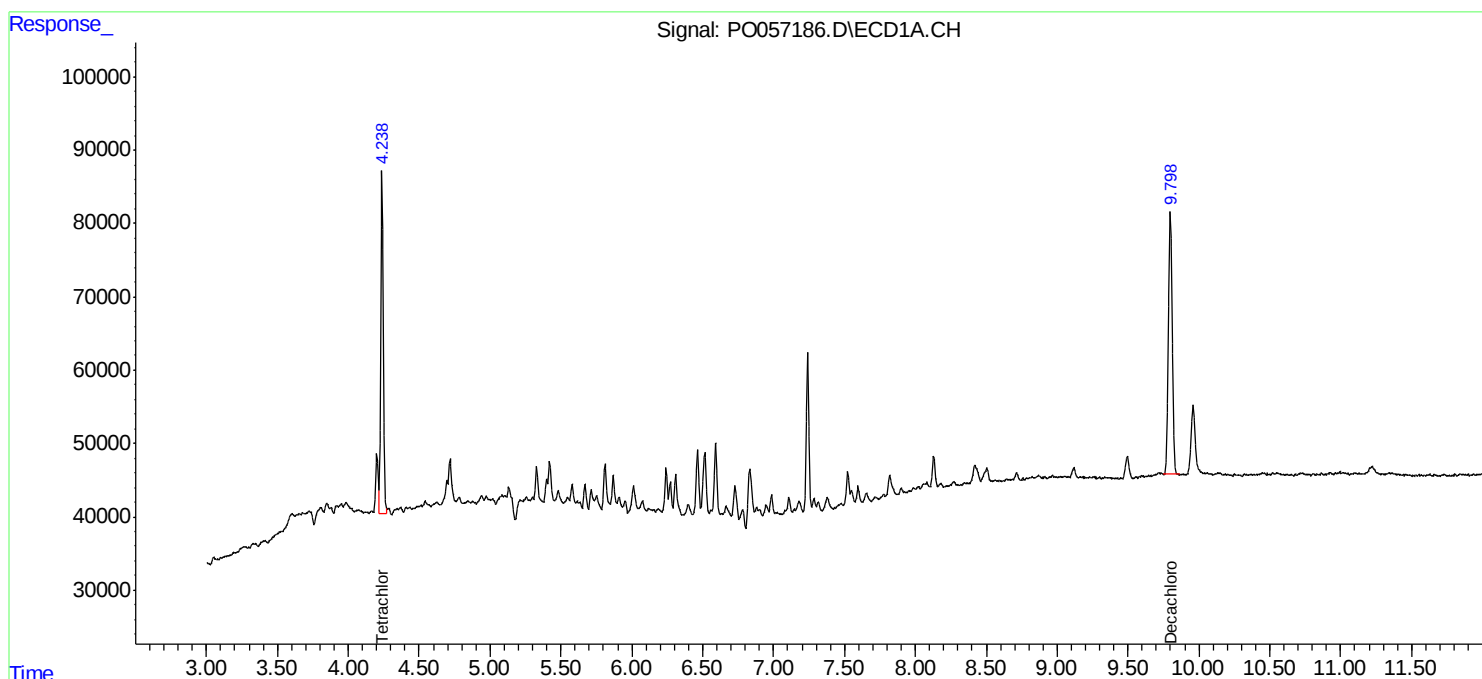

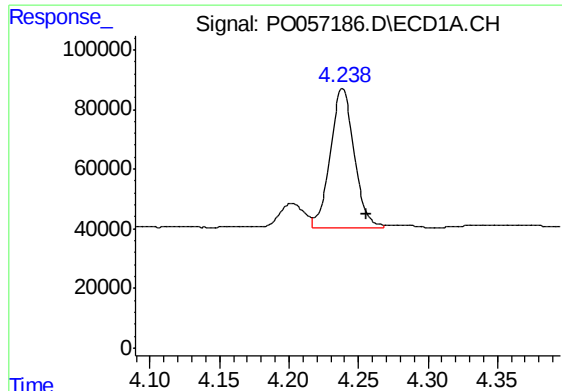


#1 Tetrachloro-m-xylene

R.T.: 4.238 min
Delta R.T.: -0.018 min
Response: 554114
Conc: 14.47 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BAT-B15


Manual Integrations
APPROVED

Ankita
6/18/2019 9:49:21 AM

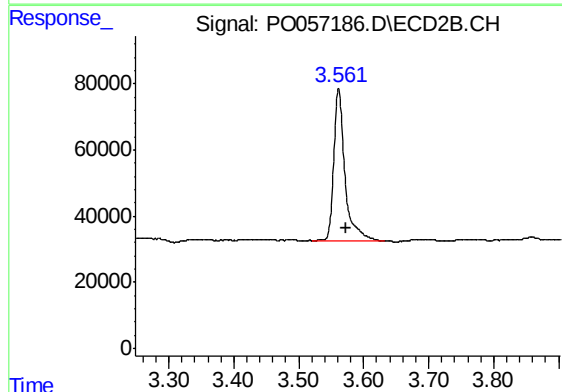


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: -0.012 min
Response: 549667
Conc: 16.67 ng/ml

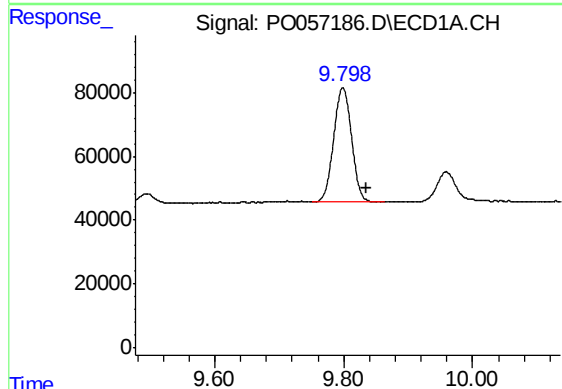

#2 Decachlorobiphenyl

R.T.: 9.799 min
Delta R.T.: -0.037 min
Response: 687176
Conc: 14.00 ng/ml

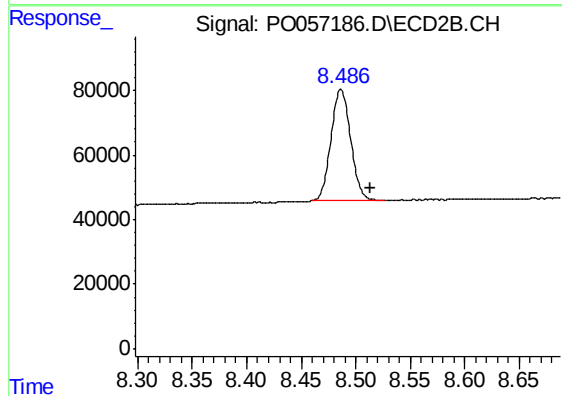

#2 Decachlorobiphenyl

R.T.: 8.486 min
Delta R.T.: -0.027 min
Response: 433298
Conc: 12.15 ng/ml