

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061520\
 Data File : P0068943.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jun 2020 9:58
 Operator : DD\AJ
 Sample : L2932-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-042720-SR-19

Manual Integrations
 APPROVED

Sohil
 6/16/2020 8:37:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 06:14:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 13 01:32:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.411	3.570	629367	756874	23.067	21.304
2) SA Decachlor...	10.081	8.781	816421	817684	18.181	15.979

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061520\
Data File : P0068943.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jun 2020 9:58
Operator : DD\AJ
Sample : L2932-19
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-042720-SR-19


Manual Integrations
APPROVED

Sohil
6/16/2020 8:37:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 06:14:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061220.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 13 01:32:21 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

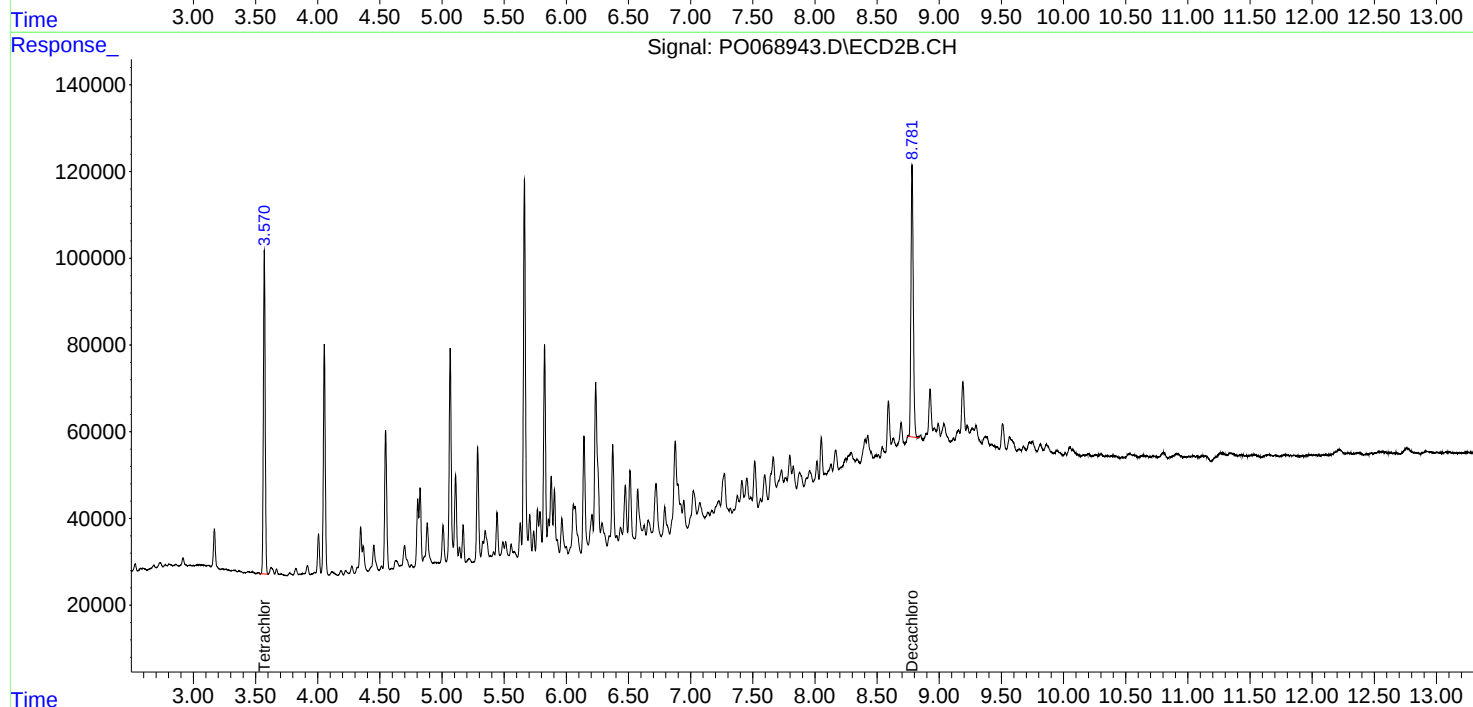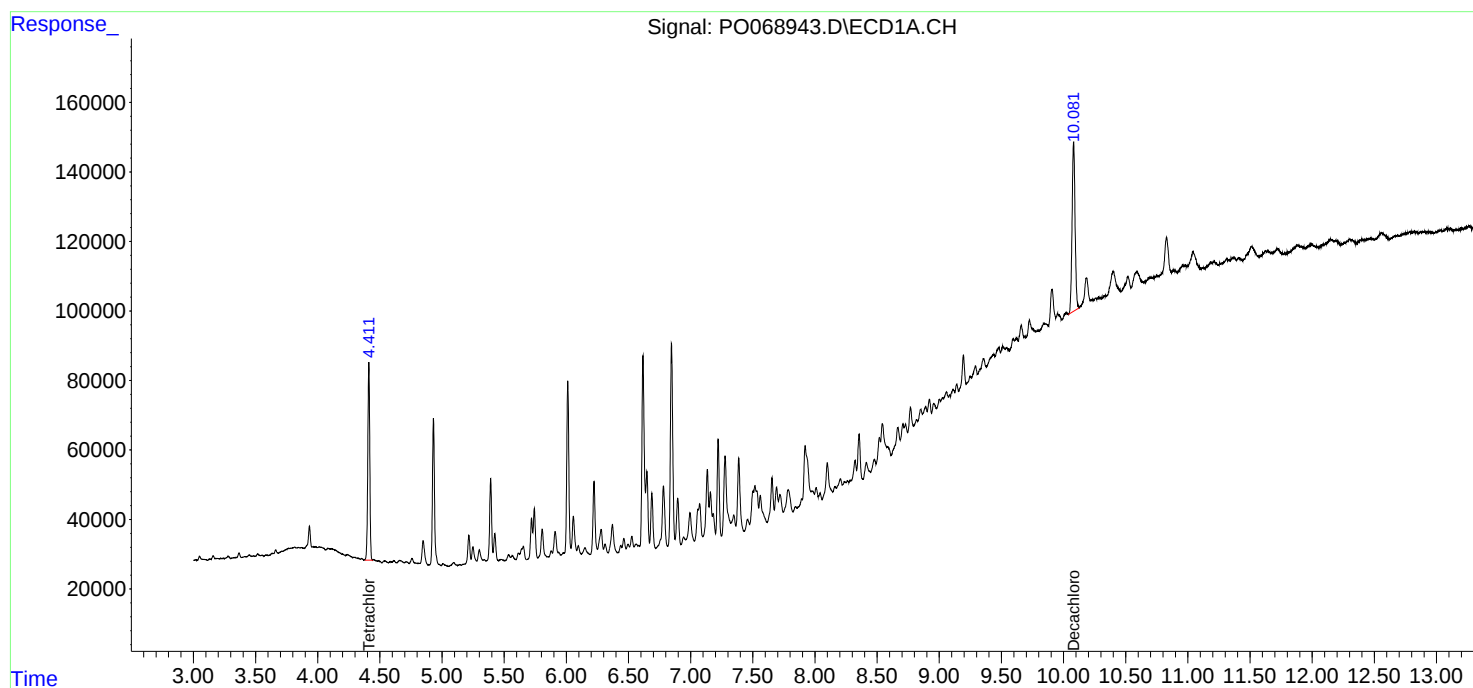

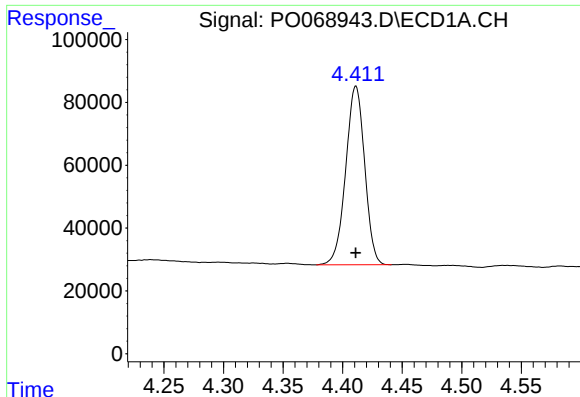


#1 Tetrachloro-m-xylene

R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 629367
Conc: 23.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-042720-SR-19


Manual Integrations
APPROVED

Sohil
6/16/2020 8:37:03 AM

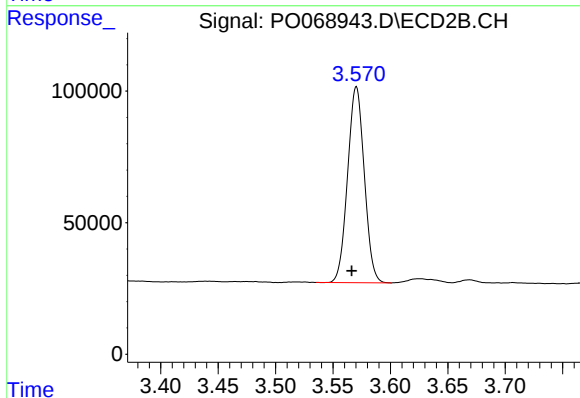


#1 Tetrachloro-m-xylene

R.T.: 3.570 min
Delta R.T.: 0.004 min
Response: 756874
Conc: 21.30 ng/ml

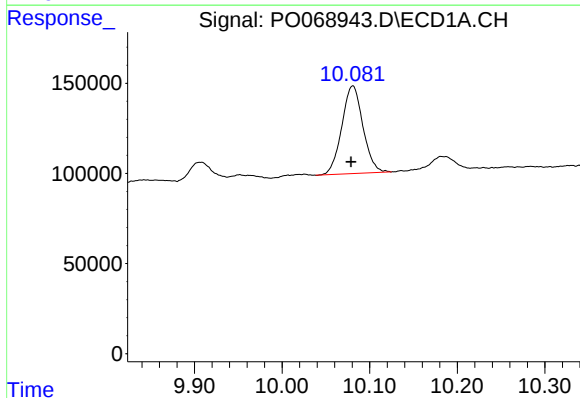

#2 Decachlorobiphenyl

R.T.: 10.081 min
Delta R.T.: 0.002 min
Response: 816421
Conc: 18.18 ng/ml

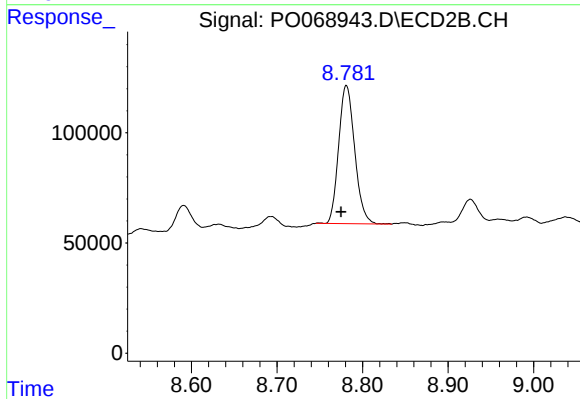

#2 Decachlorobiphenyl

R.T.: 8.781 min
Delta R.T.: 0.006 min
Response: 817684
Conc: 15.98 ng/ml