

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061720\
 Data File : P0069008.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jun 2020 10:08
 Operator : DD\AJ
 Sample : L2965-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OFFICE-SLAB-2

Manual Integrations
 APPROVED

Sohil
 6/18/2020 3:07:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 14:24:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 13 01:32:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.416	3.567	435975	518672	15.979	14.599
2) SA Decachlor...	10.079	8.777	540832	653093	12.044	12.763m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061720\
Data File : P0069008.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jun 2020 10:08
Operator : DD\AJ
Sample : L2965-10
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OFFICE-SLAB-2


Manual Integrations
APPROVED

Sohil
6/18/2020 3:07:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 14:24:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061220.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 13 01:32:21 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

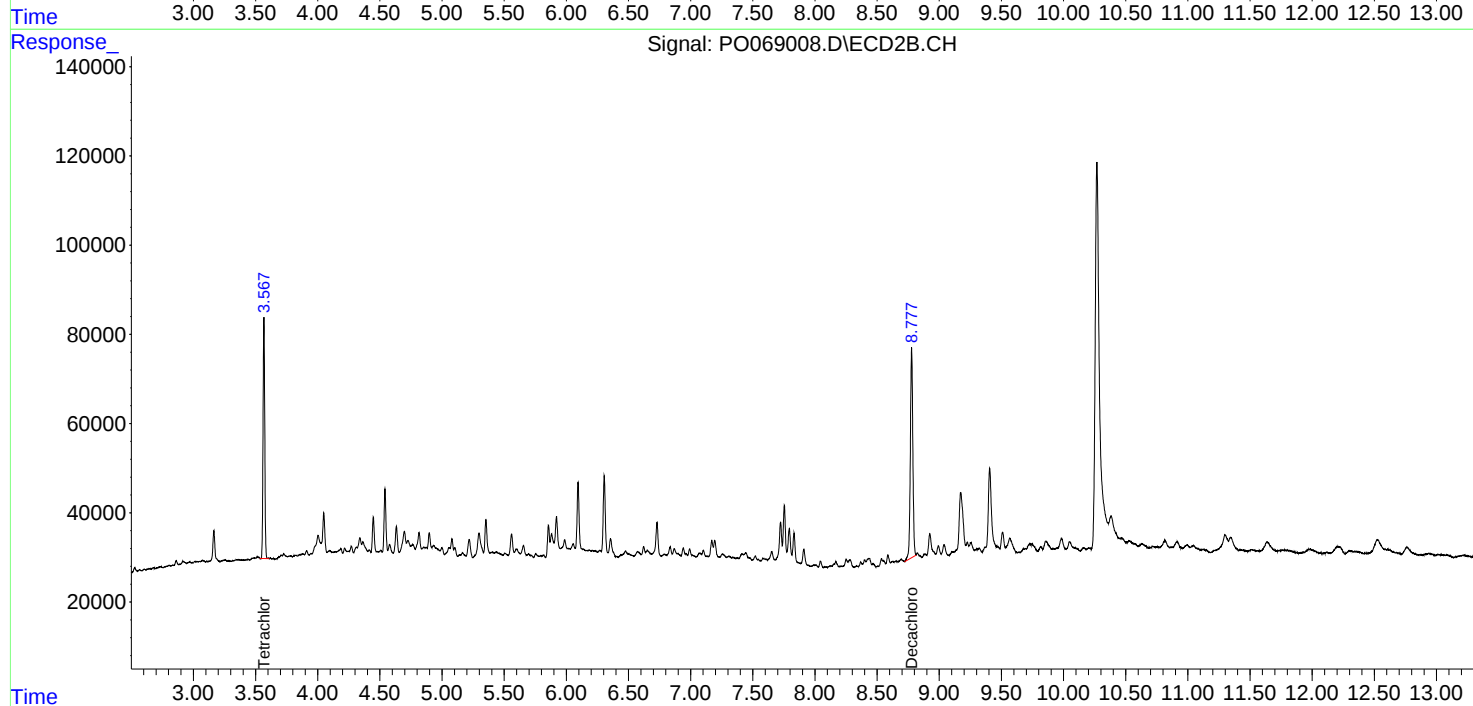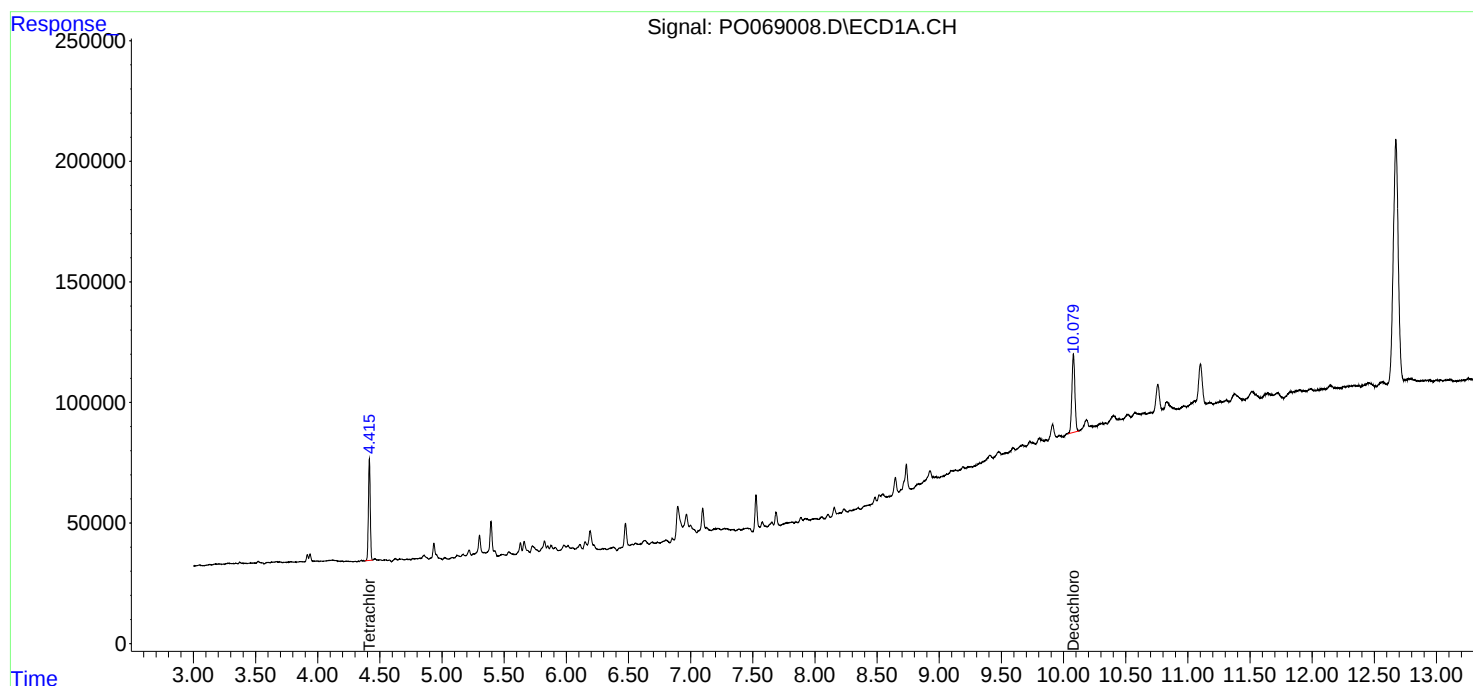

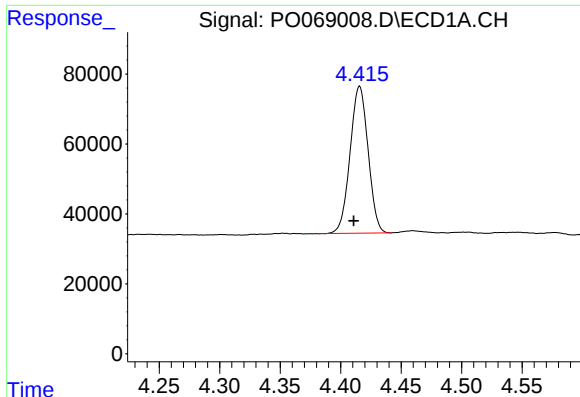


#1 Tetrachloro-m-xylene

R.T.: 4.416 min
Delta R.T.: 0.005 min
Response: 435975
Conc: 15.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
OFFICE-SLAB-2


Manual Integrations
APPROVED

Sohil
6/18/2020 3:07:22 PM

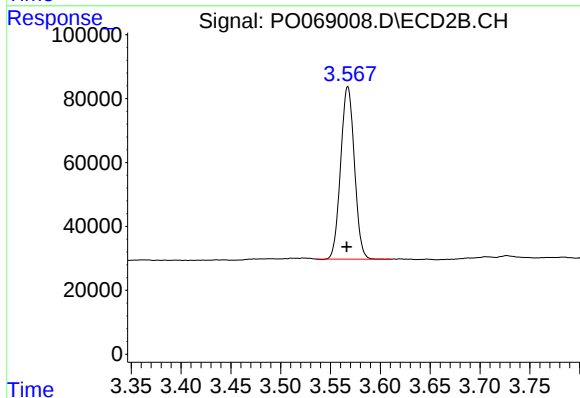


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: 0.001 min
Response: 518672
Conc: 14.60 ng/ml

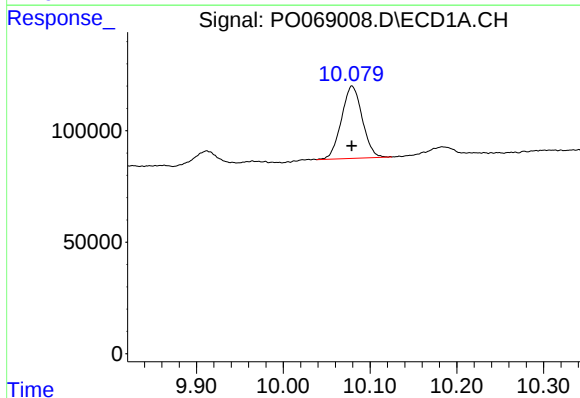

#2 Decachlorobiphenyl

R.T.: 10.079 min
Delta R.T.: 0.000 min
Response: 540832
Conc: 12.04 ng/ml

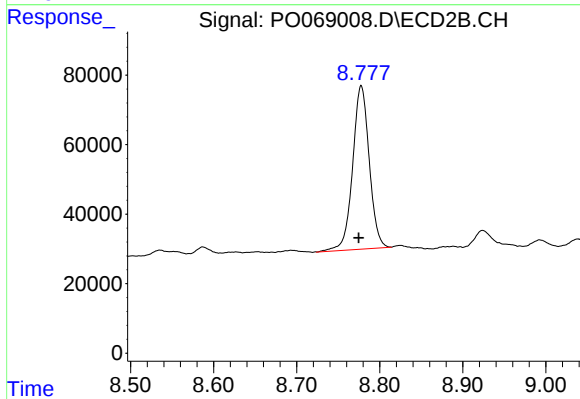

#2 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: 0.003 min
Response: 653093
Conc: 12.76 ng/ml m