

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061720\
 Data File : P0069011.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jun 2020 13:43
 Operator : DD\AJ
 Sample : L2811-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NB-08-061620

Manual Integrations
 APPROVED

Sohil
 6/18/2020 3:07:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 14:25:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jun 13 01:32:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.405	3.564	698362	841498	25.595	23.686
2) SA Decachlor...	10.070	8.770	907581	929030	20.211m	18.155m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061720\
Data File : P0069011.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jun 2020 13:43
Operator : DD\AJ
Sample : L2811-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
NB-08-061620


Manual Integrations
APPROVED

Sohil
6/18/2020 3:07:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 14:25:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061220.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jun 13 01:32:21 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

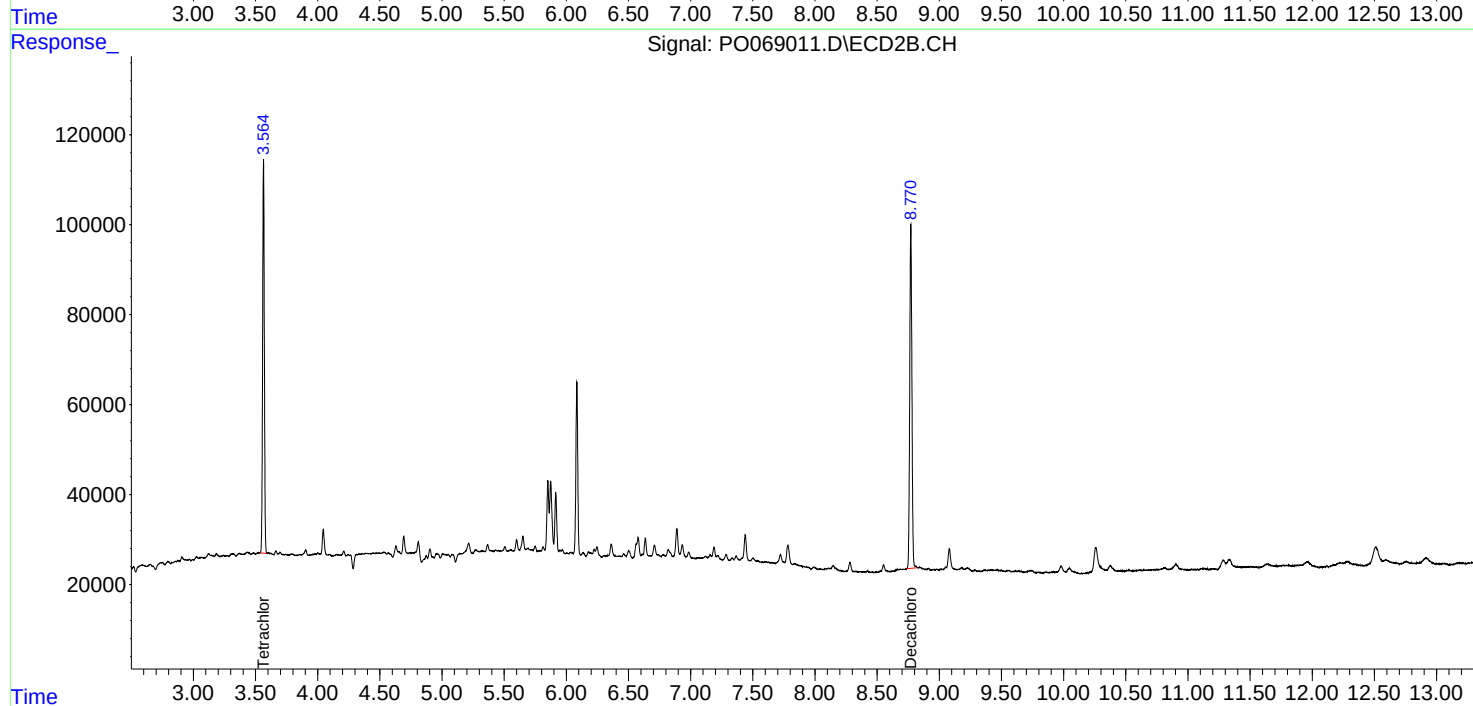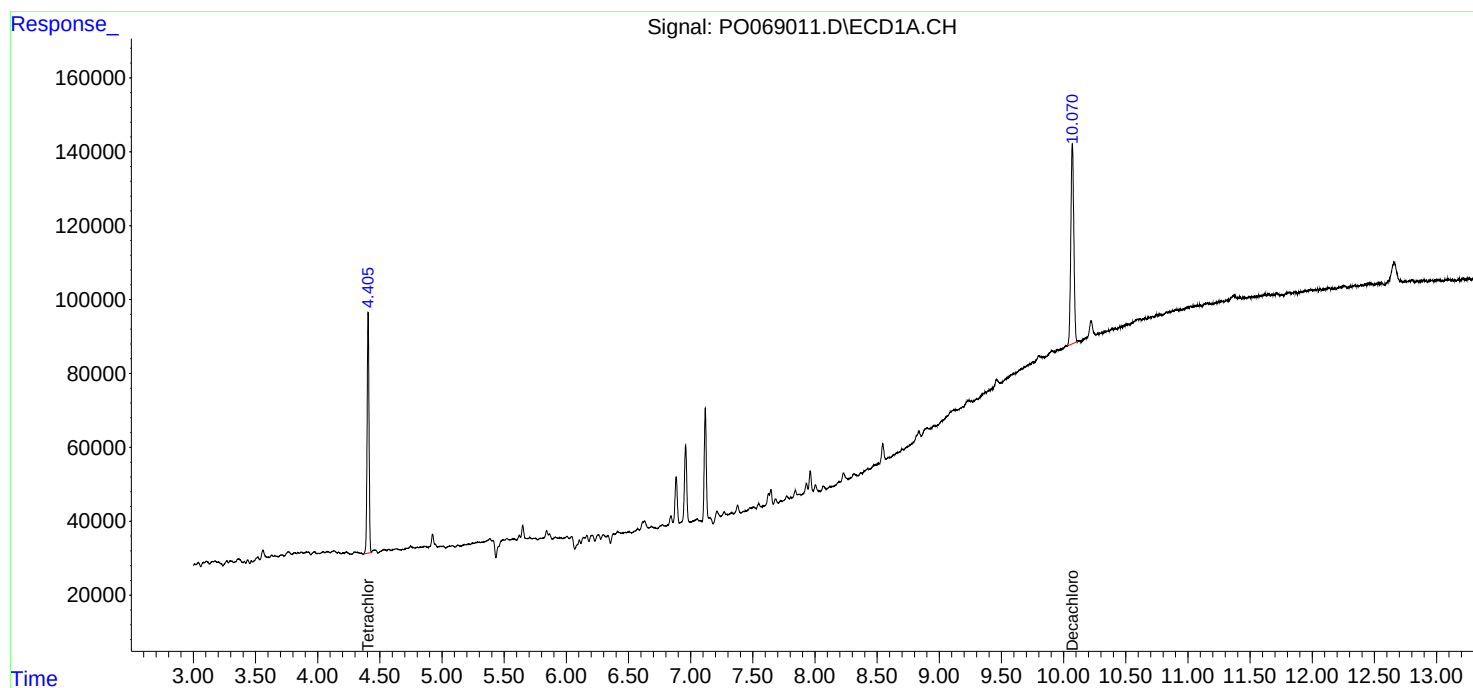

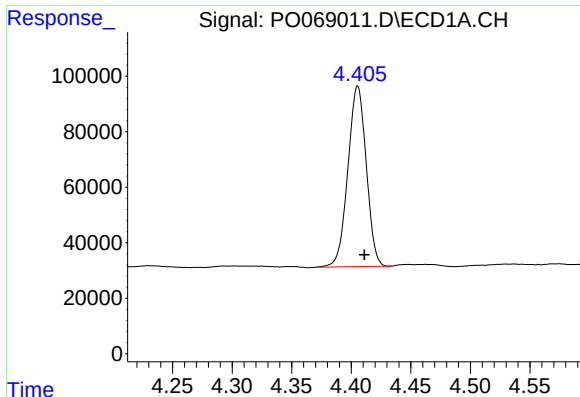


#1 Tetrachloro-m-xylene

R.T.: 4.405 min
Delta R.T.: -0.006 min
Response: 698362
Conc: 25.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
NB-08-061620


Manual Integrations
APPROVED

Sohil
6/18/2020 3:07:23 PM

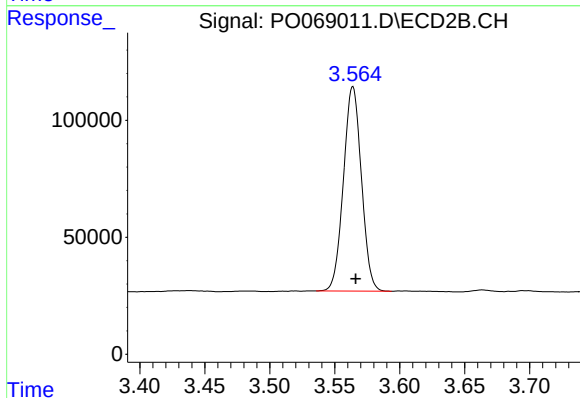


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: -0.002 min
Response: 841498
Conc: 23.69 ng/ml

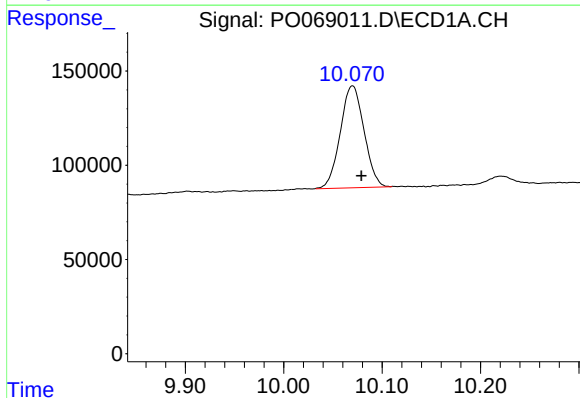

#2 Decachlorobiphenyl

R.T.: 10.070 min
Delta R.T.: -0.009 min
Response: 907581
Conc: 20.21 ng/ml m

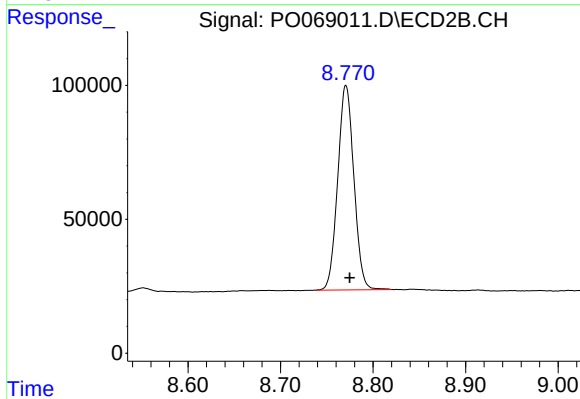

#2 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.005 min
Response: 929030
Conc: 18.16 ng/ml m