

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0061818\
Data File : P0045887.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2018 11:42
Operator : SM/UA
Sample : J3488-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FS-RO-3091RE

Manual Integrations
APPROVED

UGO
6/21/2018 3:15:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 11:57:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.392	3.625	5062686	2696291	25.804	28.770
2) SA Decachlor...	10.054	8.599	1843548	907173	9.147	11.484m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0061818\
Data File : P0045887.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2018 11:42
Operator : SM/UA
Sample : J3488-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FS-RO-3091RE


Manual Integrations
APPROVED

UGO
6/21/2018 3:15:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 11:57:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

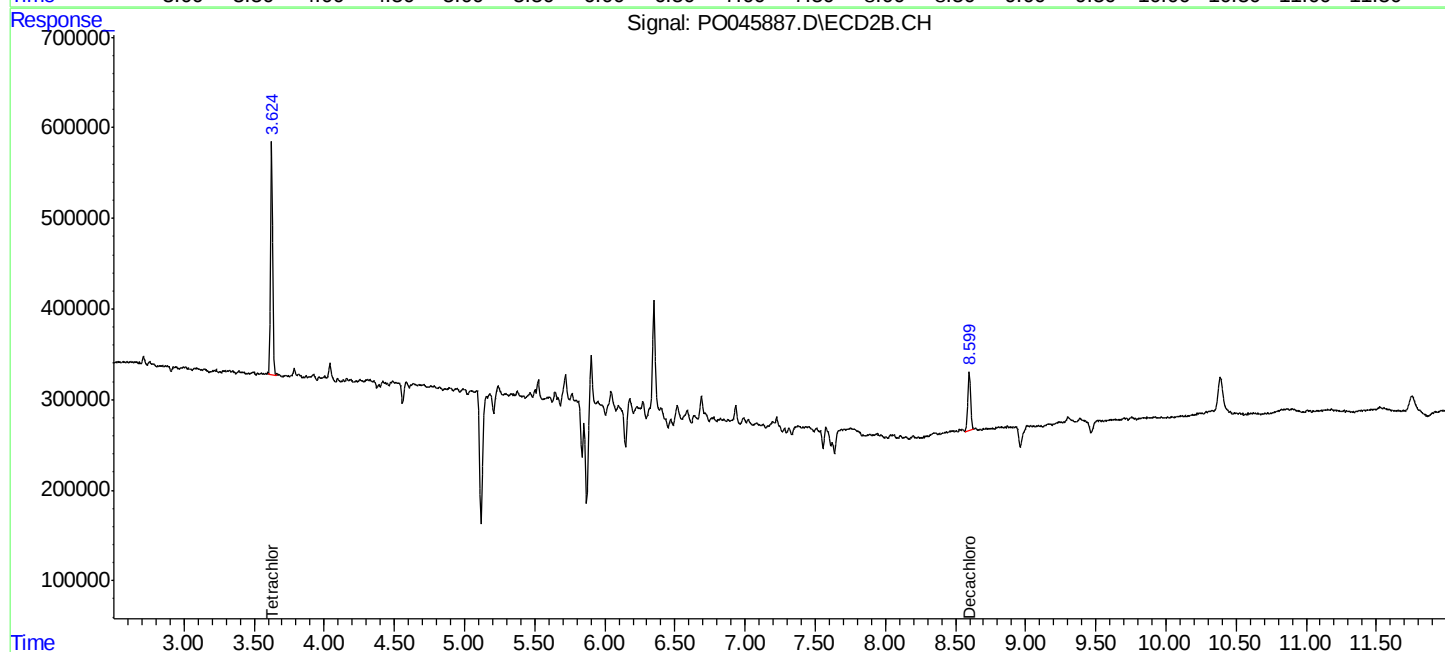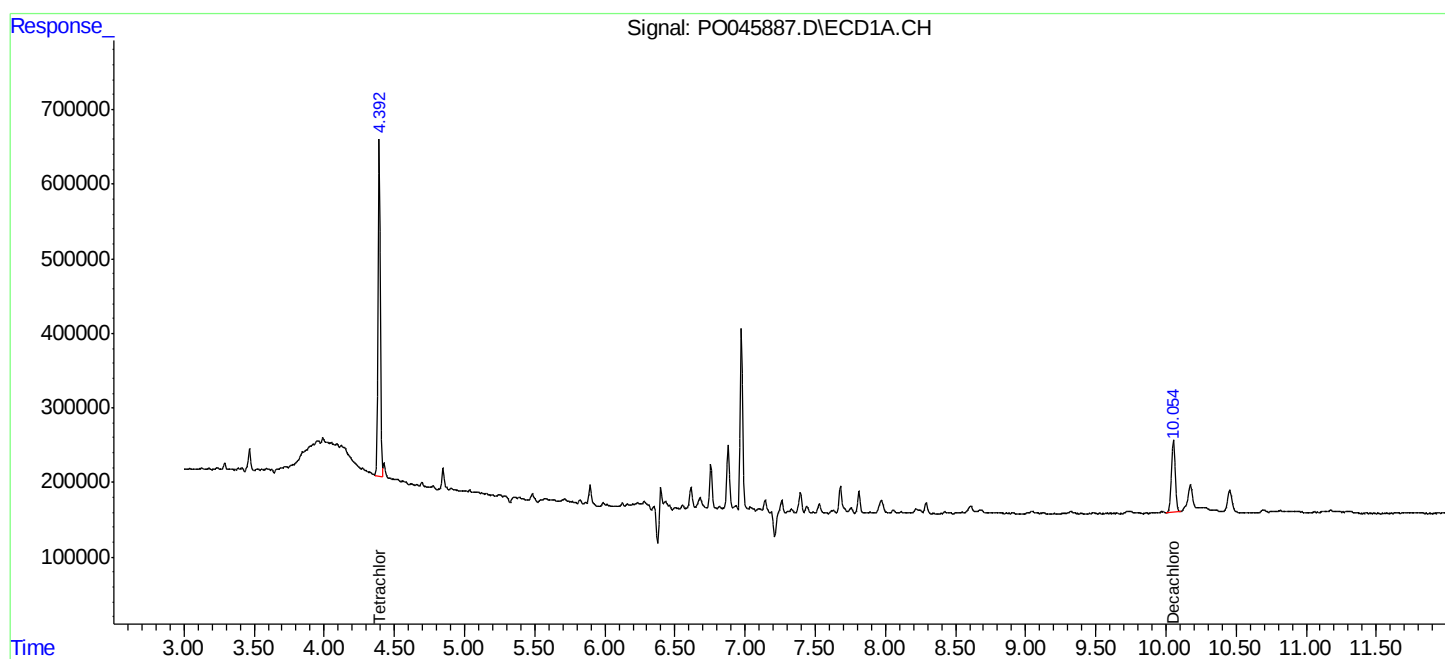

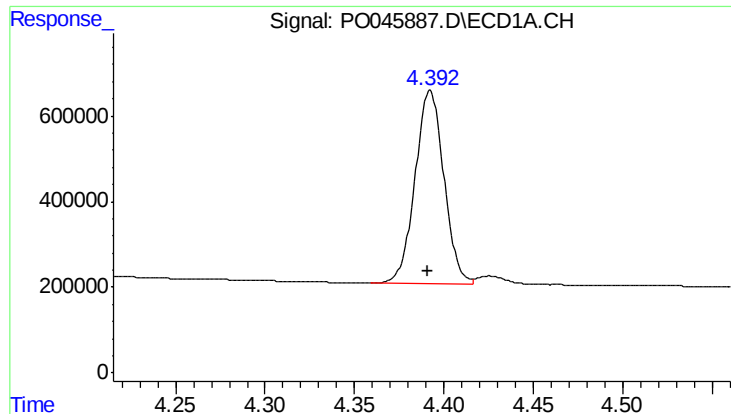


#1 Tetrachloro-m-xylene

R.T.: 4.392 min
Delta R.T.: 0.001 min
Response: 5062686
Conc: 25.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
FS-RO-3091RE


Manual Integrations
APPROVED

UGO
6/21/2018 3:15:07 PM

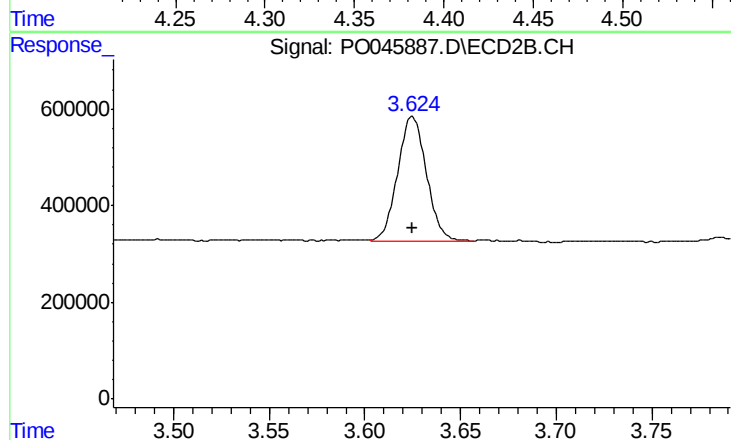


#1 Tetrachloro-m-xylene

R.T.: 3.625 min
Delta R.T.: 0.000 min
Response: 2696291
Conc: 28.77 ng/ml

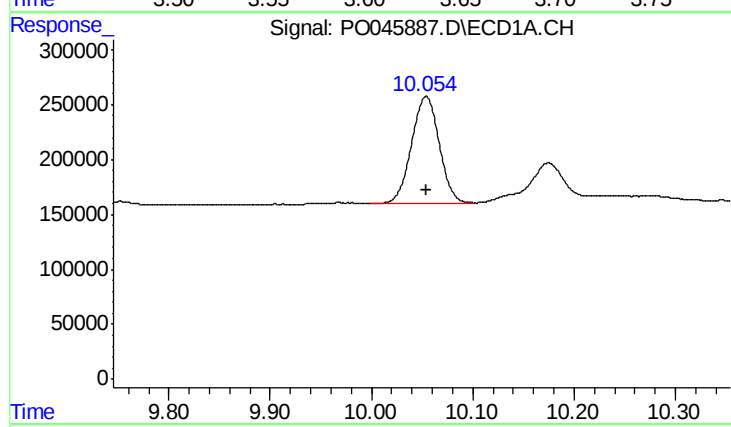

#2 Decachlorobiphenyl

R.T.: 10.054 min
Delta R.T.: 0.000 min
Response: 1843548
Conc: 9.15 ng/ml

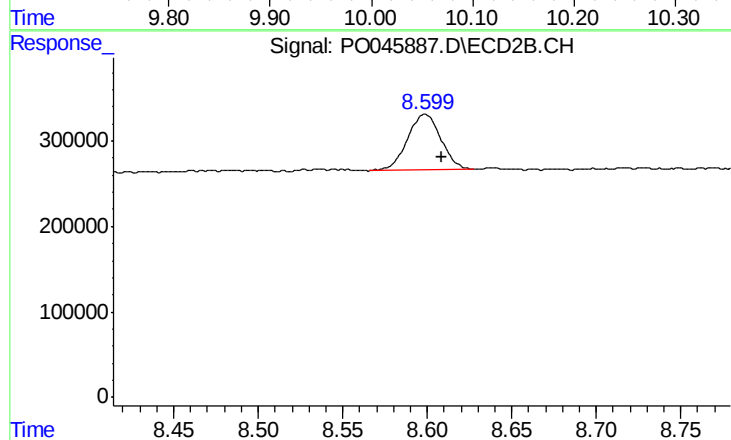

#2 Decachlorobiphenyl

R.T.: 8.599 min
Delta R.T.: -0.009 min
Response: 907173
Conc: 11.48 ng/ml m