

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0061818\
Data File : P0045899.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2018 20:03
Operator : SM/UA
Sample : J3579-01 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
A456050

Manual Integrations
APPROVED

UGO
6/21/2018 3:16:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:19:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.386	3.621	388237	145937	1.979	1.557
2)	SA Decachlor...	10.056	8.601	313833	317195	1.557m	4.016 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0061818\
Data File : P0045899.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2018 20:03
Operator : SM/UA
Sample : J3579-01 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
A456050


Manual Integrations
APPROVED

UGO
6/21/2018 3:16:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:19:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

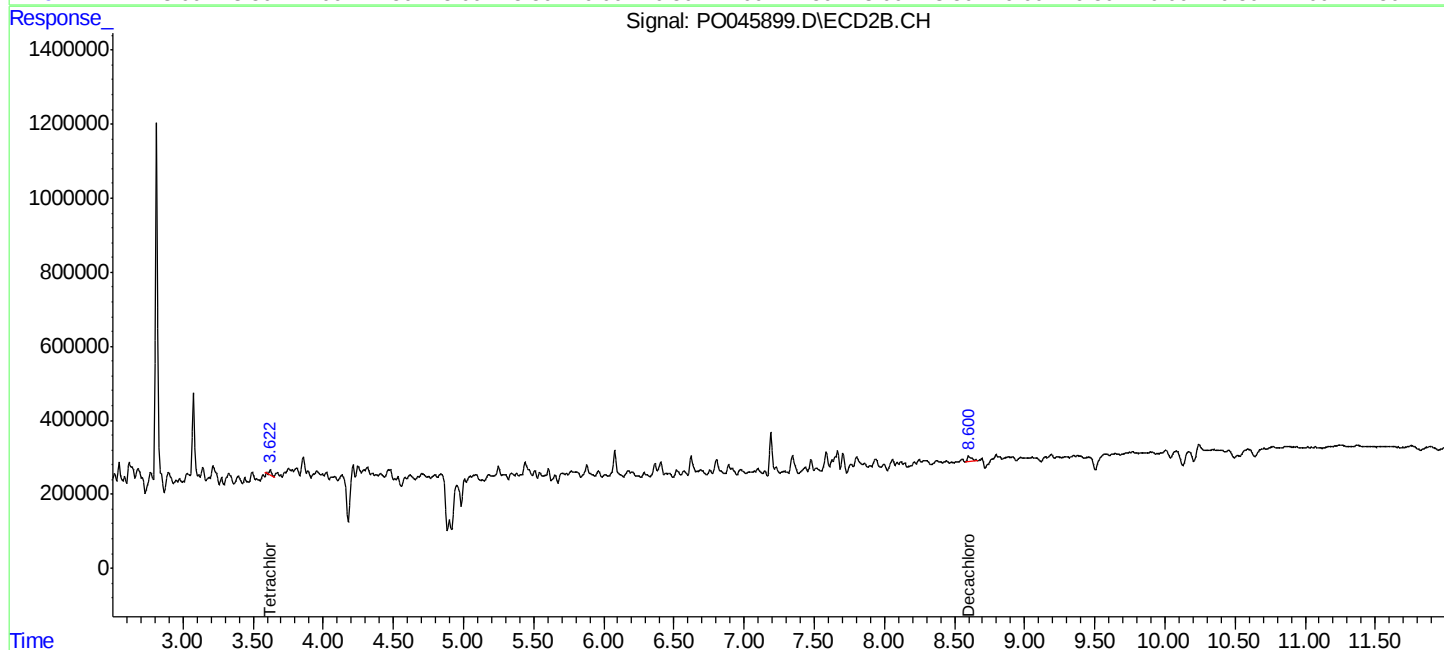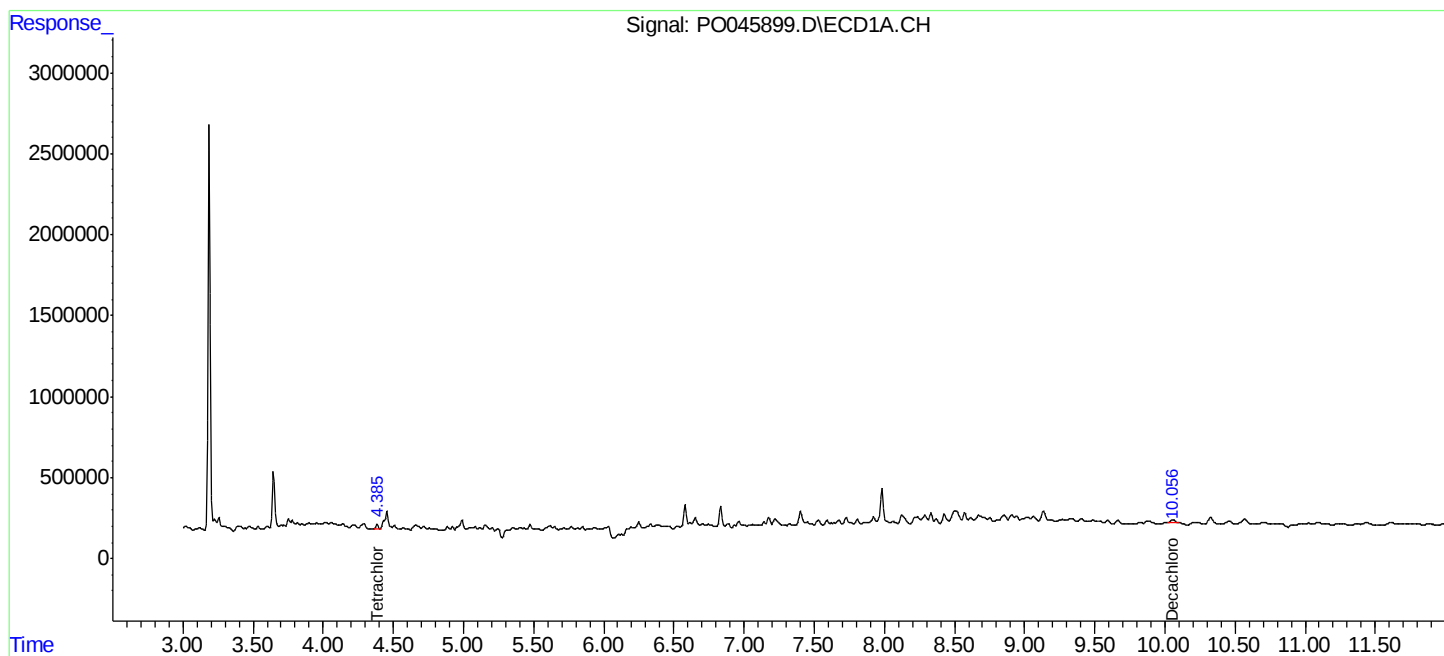

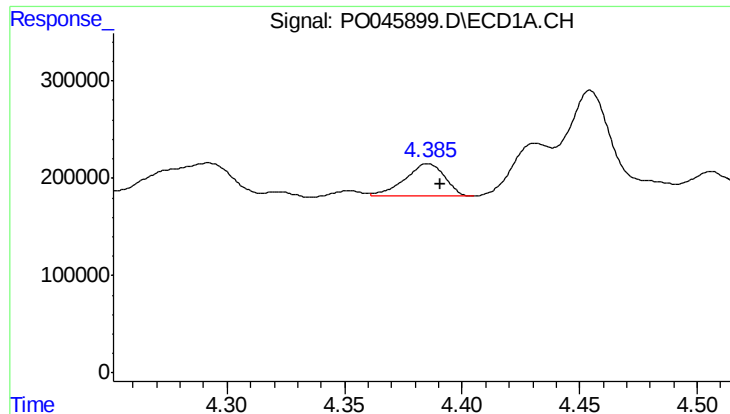


#1 Tetrachloro-m-xylene

R.T.: 4.386 min
Delta R.T.: -0.005 min
Response: 388237
Conc: 1.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
A456050


Manual Integrations
APPROVED

UGO
6/21/2018 3:16:23 PM

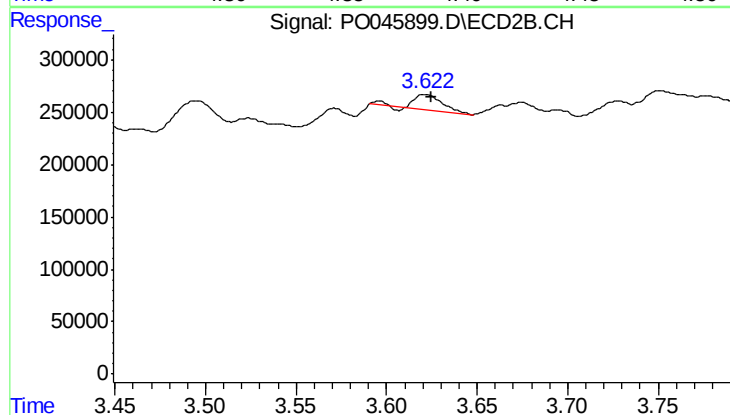


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.004 min
Response: 145937
Conc: 1.56 ng/ml

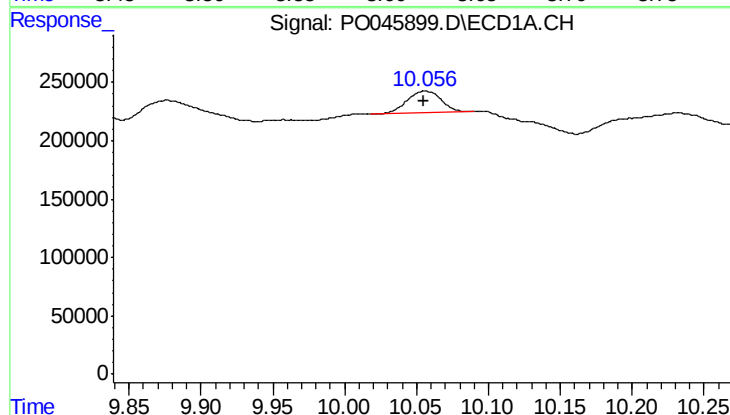

#2 Decachlorobiphenyl

R.T.: 10.056 min
Delta R.T.: 0.001 min
Response: 313833
Conc: 1.56 ng/ml m

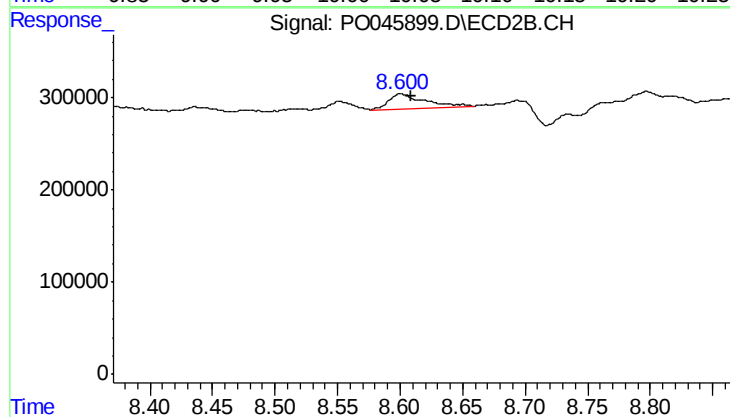

#2 Decachlorobiphenyl

R.T.: 8.601 min
Delta R.T.: -0.007 min
Response: 317195
Conc: 4.02 ng/ml