

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0061818\
 Data File : P0045913.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jun 2018 23:47
 Operator : SM/UA
 Sample : J3464-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-38-COMP

Manual Integrations
 APPROVED

UGO
 6/21/2018 3:15:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 01:58:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 15 08:20:04 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.386	3.617	5710046	4091692	29.103	43.659 #
2) SA Decachlor...	10.055	8.597	3821119	1855322	18.958	23.488
Target Compounds						
31) L7 AR-1260-1	7.141	6.174	333846	252836	31.402	45.572 #
32) L7 AR-1260-2	7.396	6.360	337792	311615	26.826	44.887 #
33) L7 AR-1260-3	7.677	6.687	431030	288520	28.610	39.854 #
34) L7 AR-1260-4	8.291	7.223	495582	306830	23.708	27.499m
35) L7 AR-1260-5	8.609	7.569	356133	243815	25.981	30.548

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0061818\
Data File : P0045913.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jun 2018 23:47
Operator : SM/UA
Sample : J3464-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-38-COMP


Manual Integrations
APPROVED

UGO
6/21/2018 3:15:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:58:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

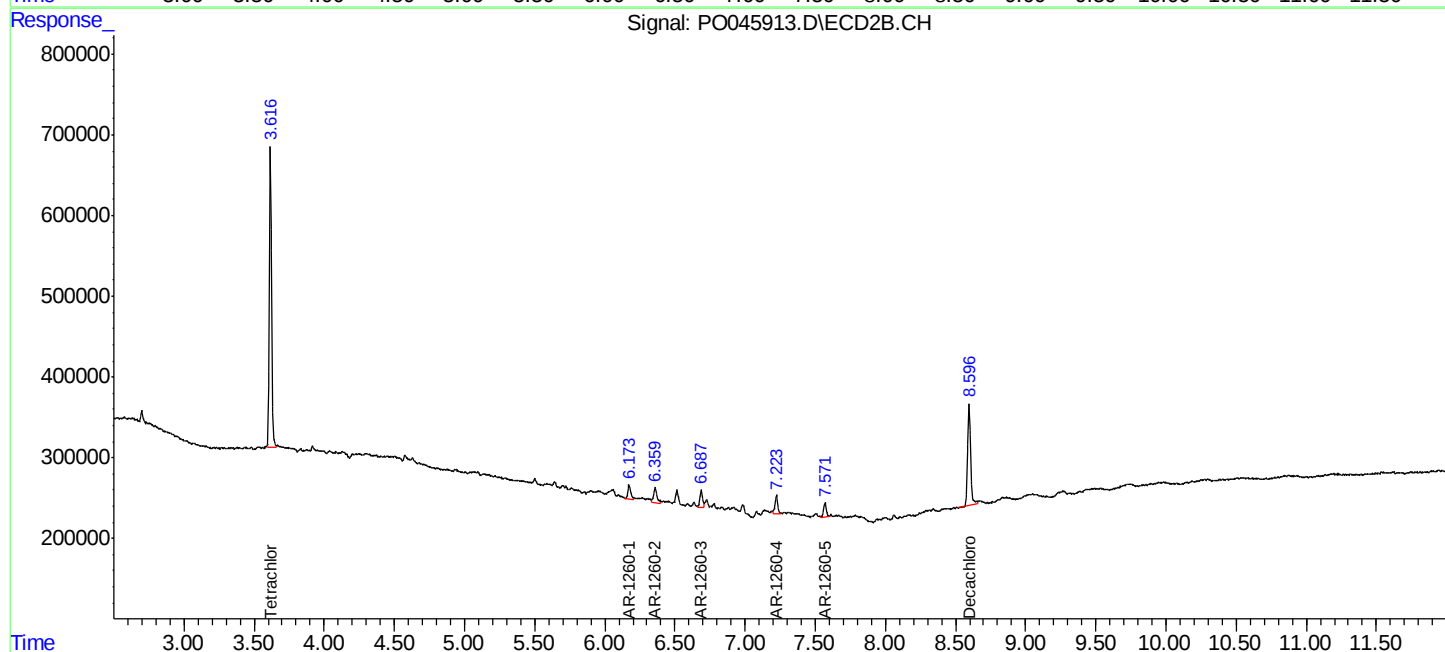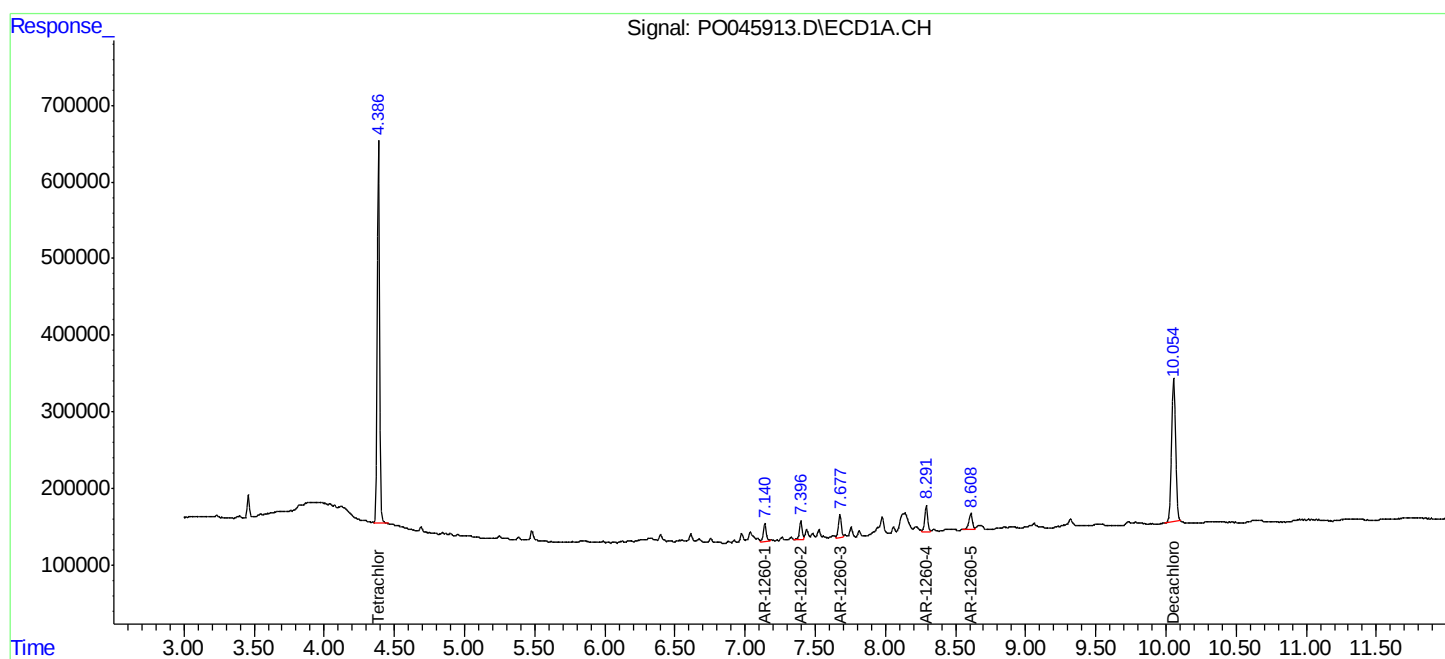

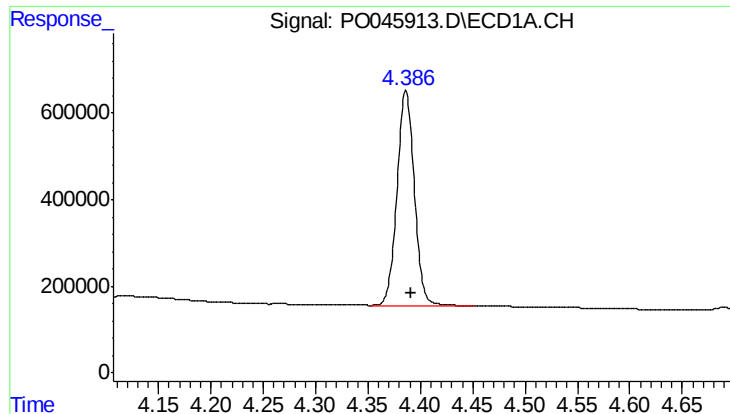


#1 Tetrachloro-m-xylene

R.T.: 4.386 min
Delta R.T.: -0.005 min
Response: 5710046
Conc: 29.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-38-COMP


Manual Integrations
APPROVED

UGO
6/21/2018 3:15:51 PM

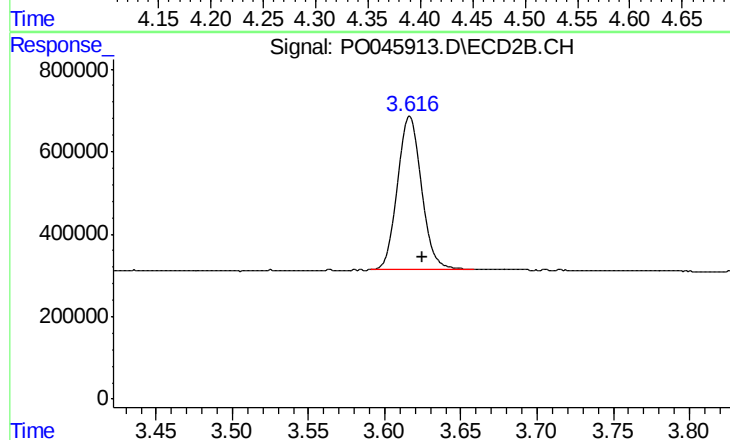


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: -0.008 min
Response: 4091692
Conc: 43.66 ng/ml

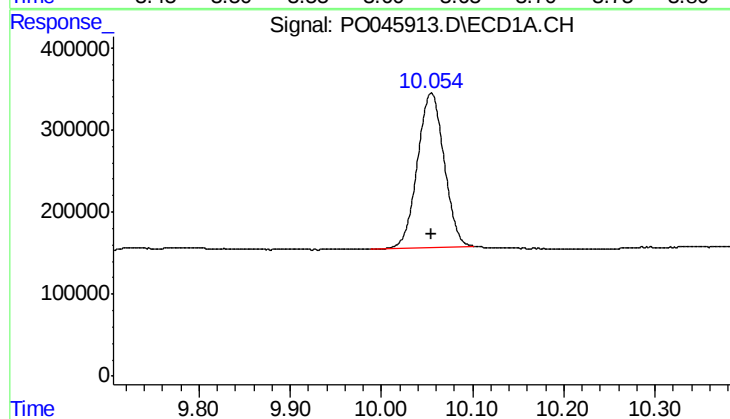


#2 Decachlorobiphenyl

R.T.: 10.055 min
Delta R.T.: 0.000 min
Response: 3821119
Conc: 18.96 ng/ml

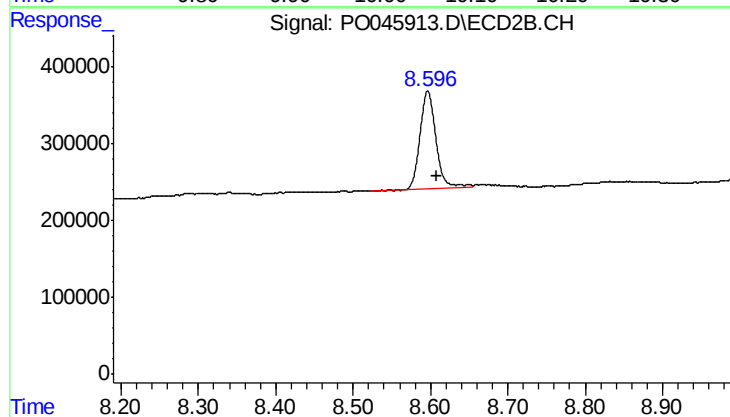

#2 Decachlorobiphenyl

R.T.: 8.597 min
Delta R.T.: -0.012 min
Response: 1855322
Conc: 23.49 ng/ml

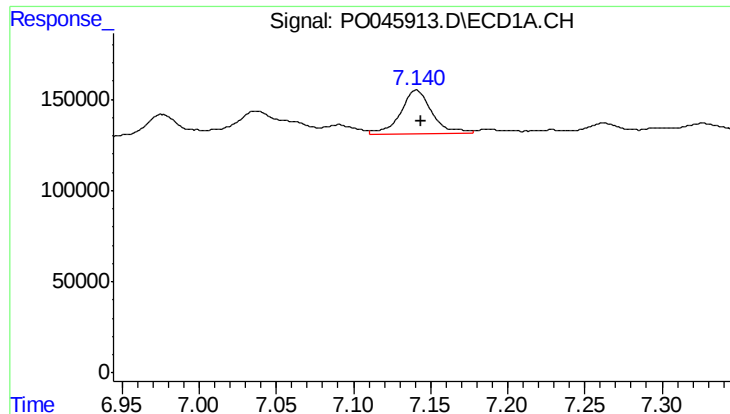


#31 AR-1260-1

R.T.: 7.141 min
Delta R.T.: -0.003 min
Response: 333846
Conc: 31.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-38-COMP


Manual Integrations
APPROVED

UGO
6/21/2018 3:15:51 PM

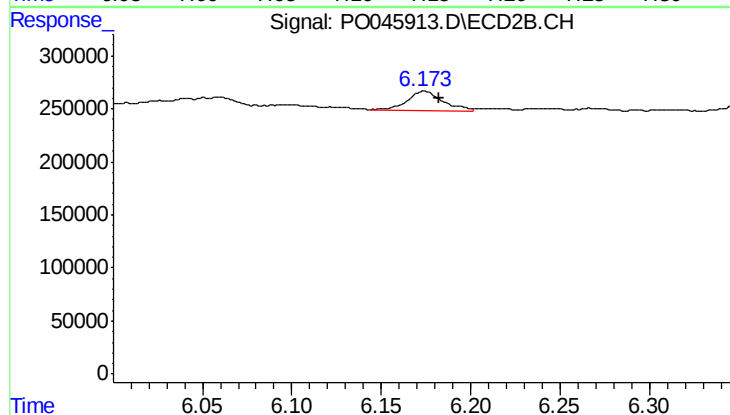


#31 AR-1260-1

R.T.: 6.174 min
Delta R.T.: -0.008 min
Response: 252836
Conc: 45.57 ng/ml

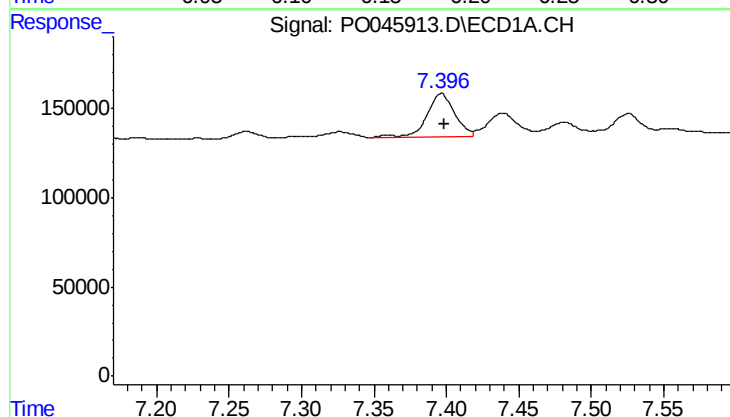


#32 AR-1260-2

R.T.: 7.396 min
Delta R.T.: -0.002 min
Response: 337792
Conc: 26.83 ng/ml

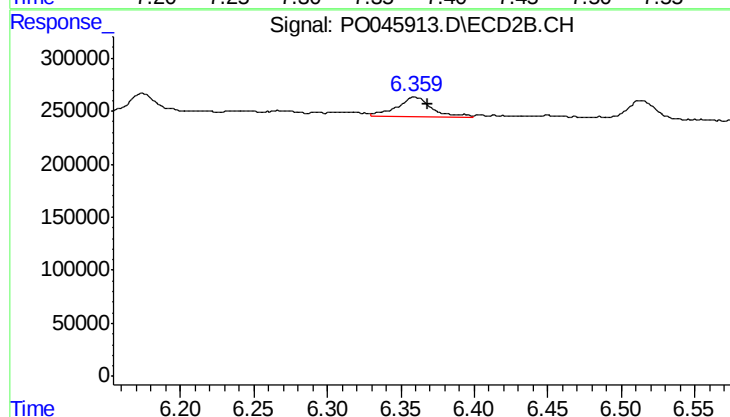

#32 AR-1260-2

R.T.: 6.360 min
Delta R.T.: -0.009 min
Response: 311615
Conc: 44.89 ng/ml

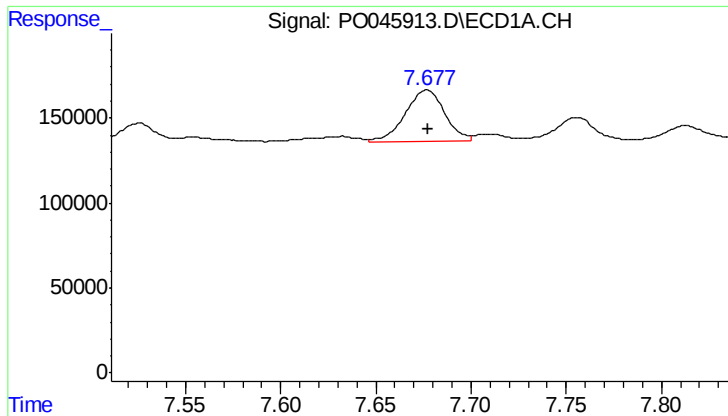


#33 AR-1260-3

R.T.: 7.677 min
Delta R.T.: 0.000 min
Response: 431030
Conc: 28.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-38-COMP


Manual Integrations
APPROVED

UGO
6/21/2018 3:15:51 PM

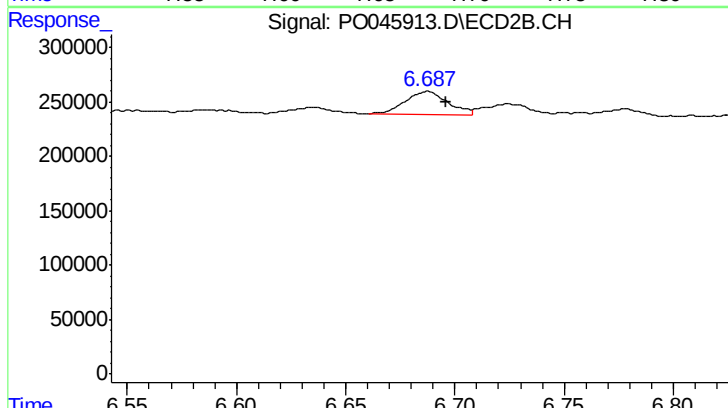


#33 AR-1260-3

R.T.: 6.687 min
Delta R.T.: -0.009 min
Response: 288520
Conc: 39.85 ng/ml

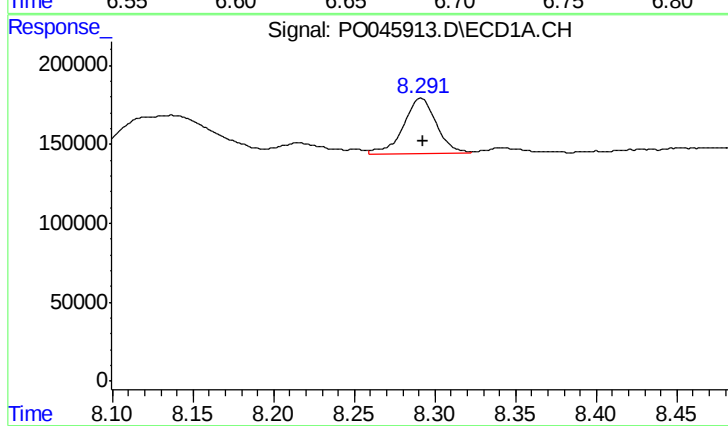


#34 AR-1260-4

R.T.: 8.291 min
Delta R.T.: -0.001 min
Response: 495582
Conc: 23.71 ng/ml

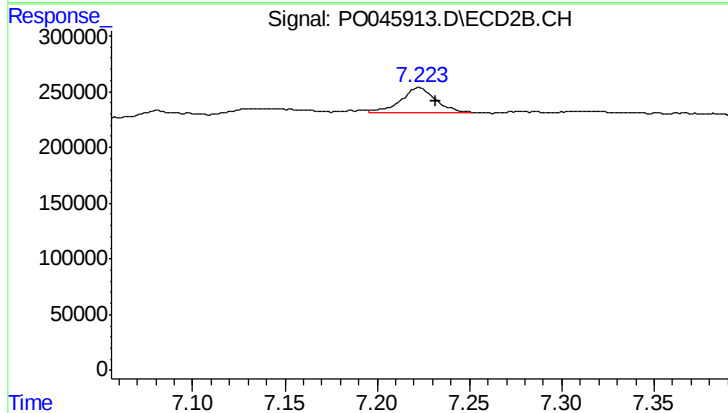

#34 AR-1260-4

R.T.: 7.223 min
Delta R.T.: -0.009 min
Response: 306830
Conc: 27.50 ng/ml m

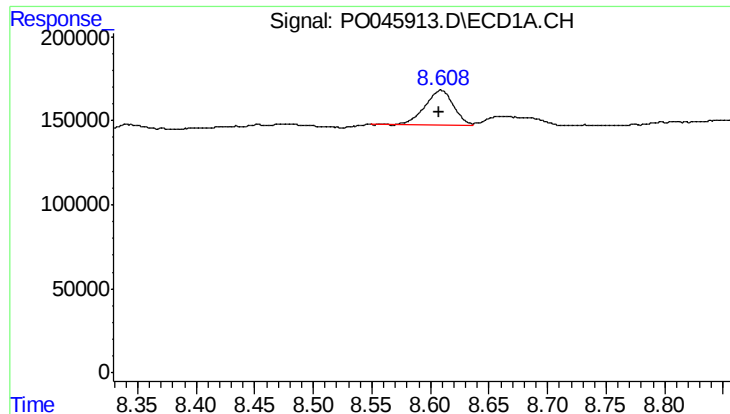


#35 AR-1260-5

R.T.: 8.609 min
Delta R.T.: 0.001 min
Response: 356133
Conc: 25.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-38-COMP

Manual Integrations
APPROVED

UGO
6/21/2018 3:15:51 PM

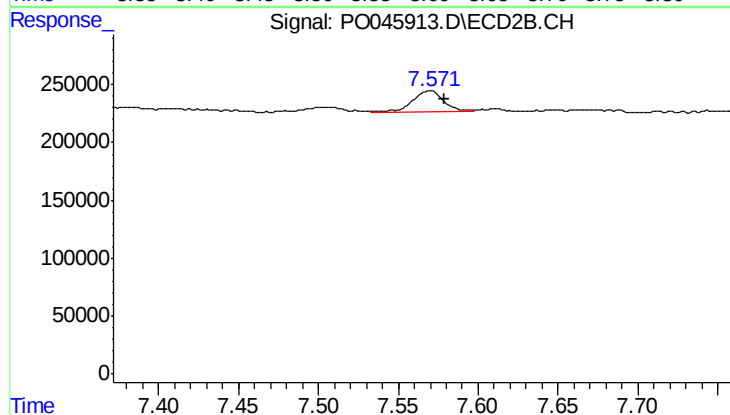

#35 AR-1260-5

R.T.: 7.569 min
Delta R.T.: -0.010 min
Response: 243815
Conc: 30.55 ng/ml