

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0061818\
 Data File : P0045930.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jun 2018 4:18
 Operator : SM/UA
 Sample : J3504-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-44COMP

Manual Integrations
 APPROVED

UGO
 6/21/2018 3:15:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 07:04:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 15 08:20:04 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.386	3.616	9421467	5103550	48.020	54.456
2) SA Decachlor...	10.053	8.596	5347651	2418389	26.532	30.616
Target Compounds						
31) L7 AR-1260-1	7.141	6.173	3203488	1235629	301.322	222.716m#
32) L7 AR-1260-2	7.396	6.359	2328822	993196	184.946	143.065m
33) L7 AR-1260-3	7.677	6.686	3381188	1632369	224.425	225.481m
34) L7 AR-1260-4	8.290	7.222	2228766	1613630	106.619	144.616 #
35) L7 AR-1260-5	8.608	7.569	1983686	1435860	144.714	179.903

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0061818\
Data File : P0045930.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jun 2018 4:18
Operator : SM/UA
Sample : J3504-01
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-44COMP


Manual Integrations
APPROVED

UGO
6/21/2018 3:15:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 07:04:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061418.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 15 08:20:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

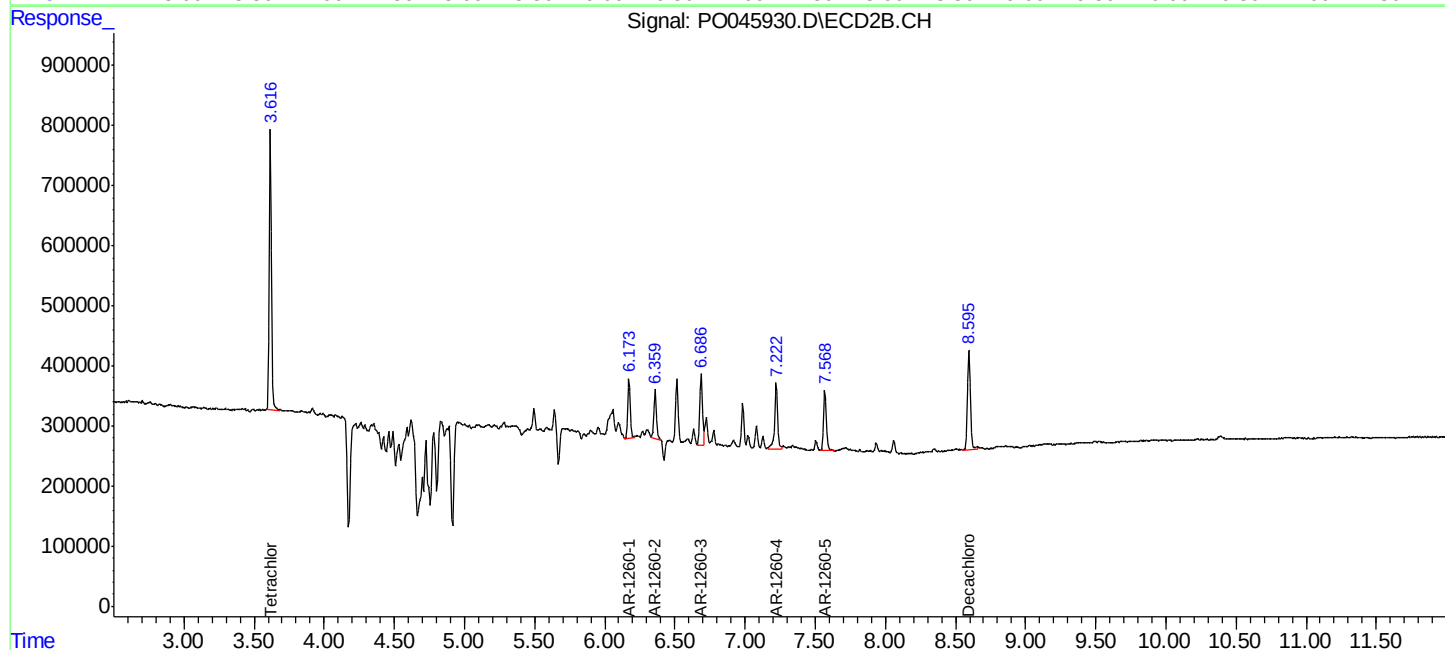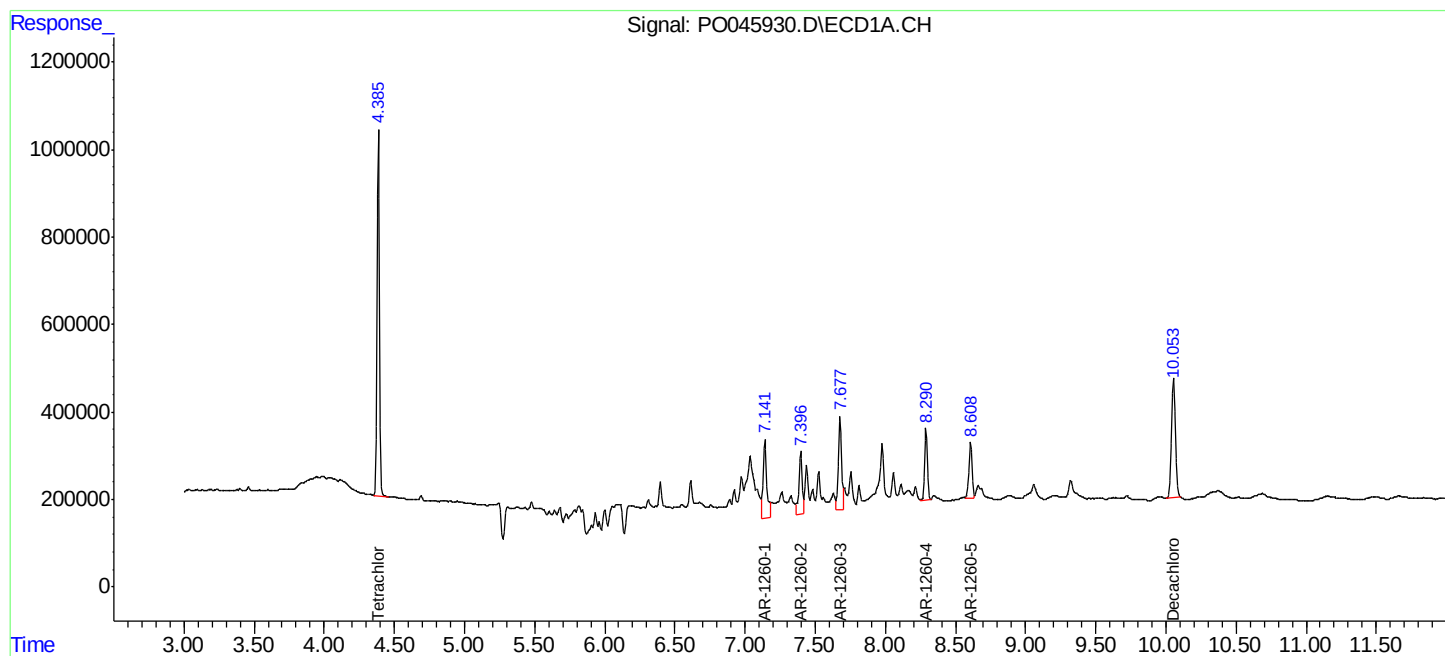

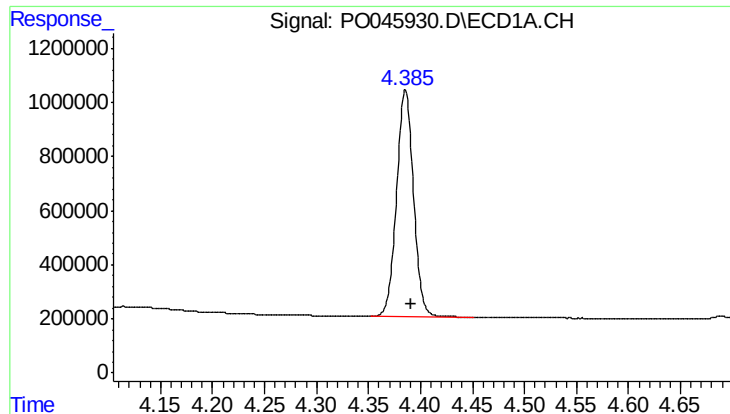


#1 Tetrachloro-m-xylene

R.T.: 4.386 min
Delta R.T.: -0.005 min
Response: 9421467
Conc: 48.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-44COMP


Manual Integrations
APPROVED

UGO
6/21/2018 3:15:17 PM

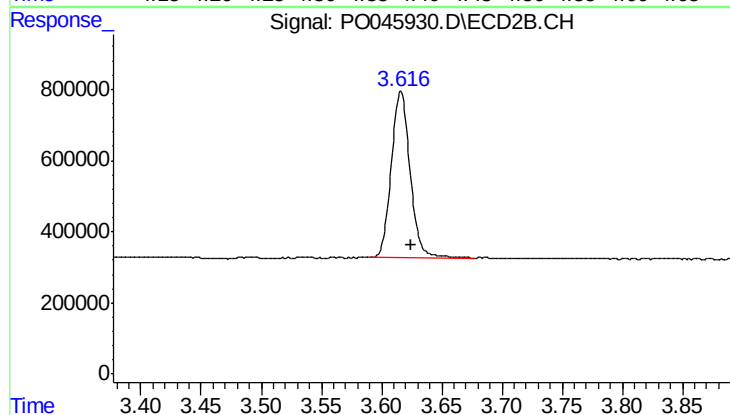


#1 Tetrachloro-m-xylene

R.T.: 3.616 min
Delta R.T.: -0.009 min
Response: 5103550
Conc: 54.46 ng/ml

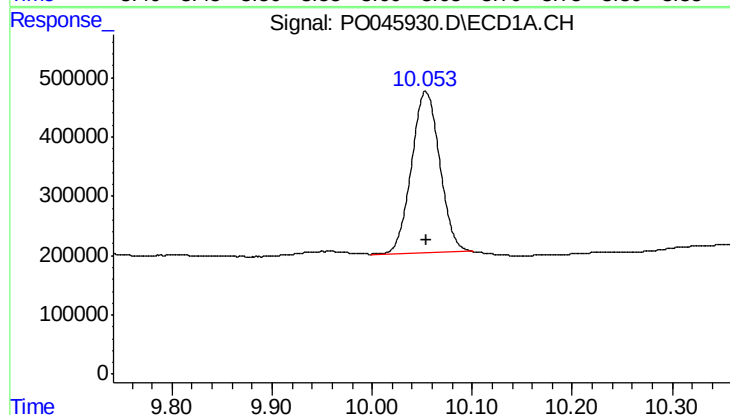


#2 Decachlorobiphenyl

R.T.: 10.053 min
Delta R.T.: -0.001 min
Response: 5347651
Conc: 26.53 ng/ml

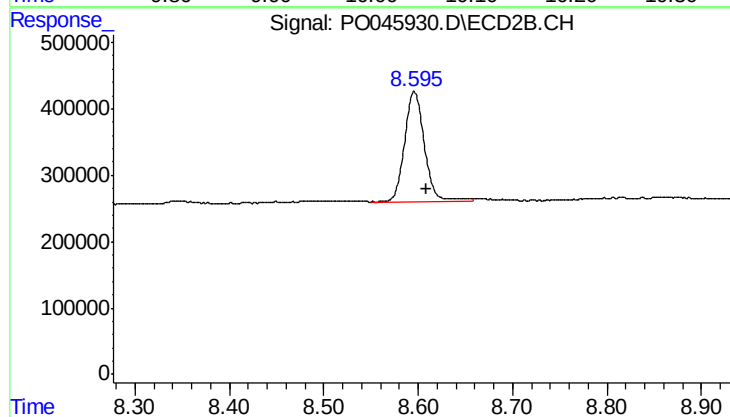

#2 Decachlorobiphenyl

R.T.: 8.596 min
Delta R.T.: -0.012 min
Response: 2418389
Conc: 30.62 ng/ml

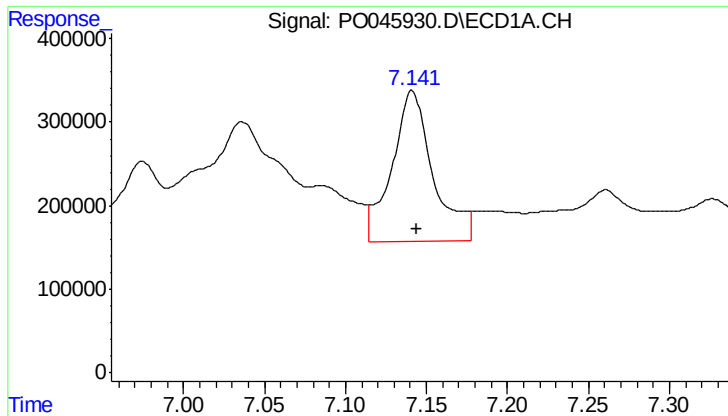


#31 AR-1260-1

R.T.: 7.141 min
Delta R.T.: -0.002 min
Response: 3203488
Conc: 301.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-44COMP


Manual Integrations
APPROVED

UGO
6/21/2018 3:15:17 PM

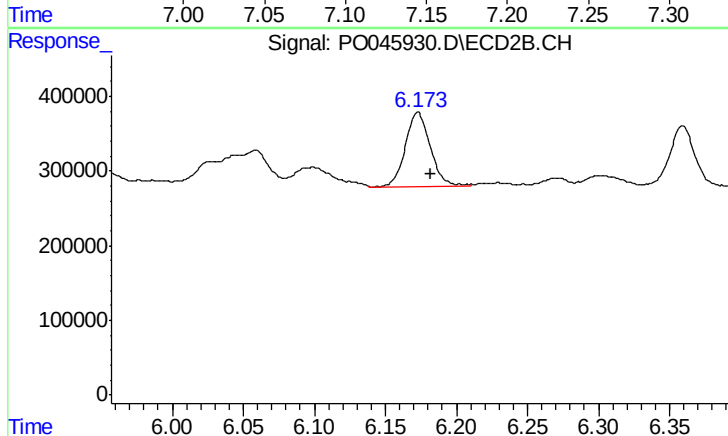


#31 AR-1260-1

R.T.: 6.173 min
Delta R.T.: -0.009 min
Response: 1235629
Conc: 222.72 ng/ml m

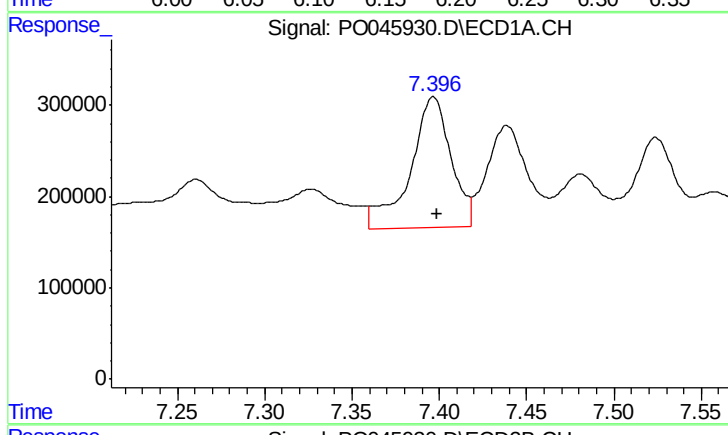


#32 AR-1260-2

R.T.: 7.396 min
Delta R.T.: -0.002 min
Response: 2328822
Conc: 184.95 ng/ml

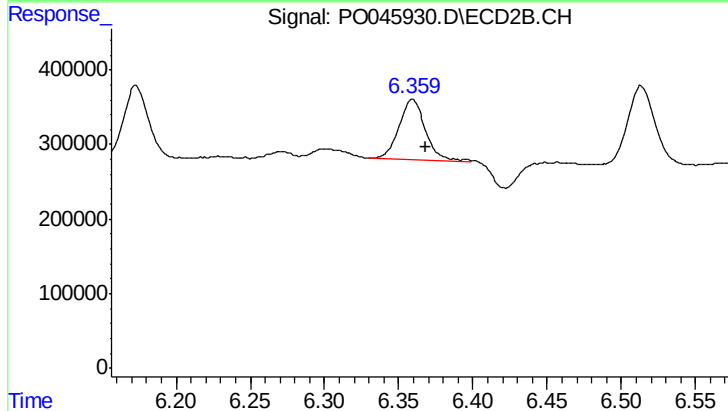

#32 AR-1260-2

R.T.: 6.359 min
Delta R.T.: -0.010 min
Response: 993196
Conc: 143.07 ng/ml m

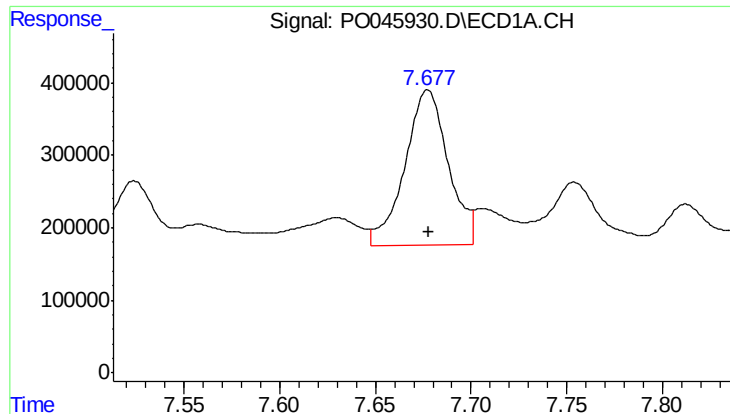


#33 AR-1260-3

R.T.: 7.677 min
Delta R.T.: 0.000 min
Response: 3381188
Conc: 224.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-44COMP


Manual Integrations
APPROVED

UGO
6/21/2018 3:15:17 PM

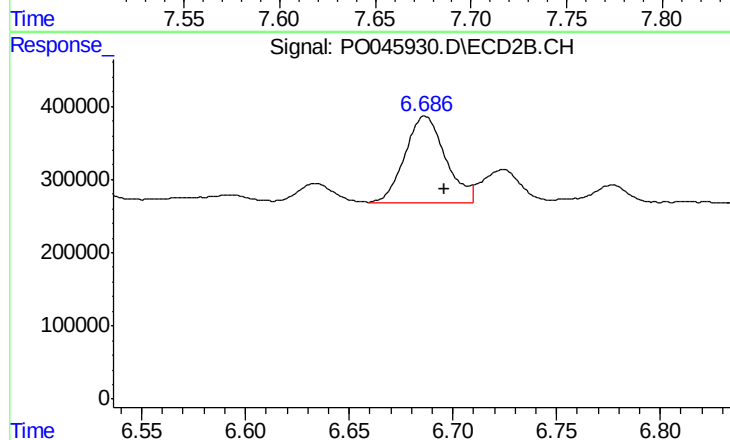


#33 AR-1260-3

R.T.: 6.686 min
Delta R.T.: -0.010 min
Response: 1632369
Conc: 225.48 ng/ml m

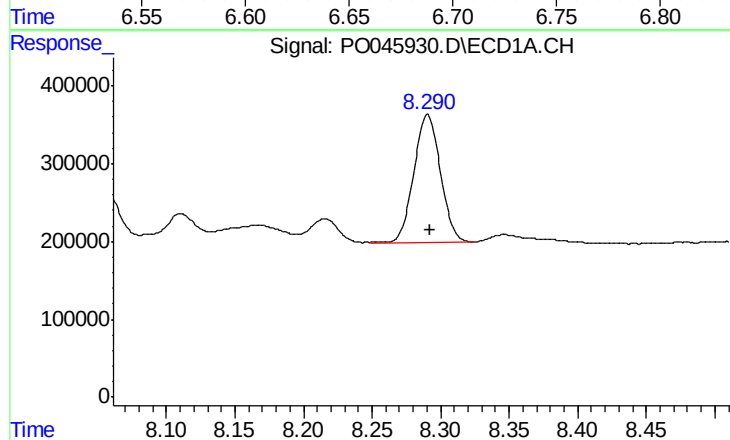


#34 AR-1260-4

R.T.: 8.290 min
Delta R.T.: -0.002 min
Response: 2228766
Conc: 106.62 ng/ml

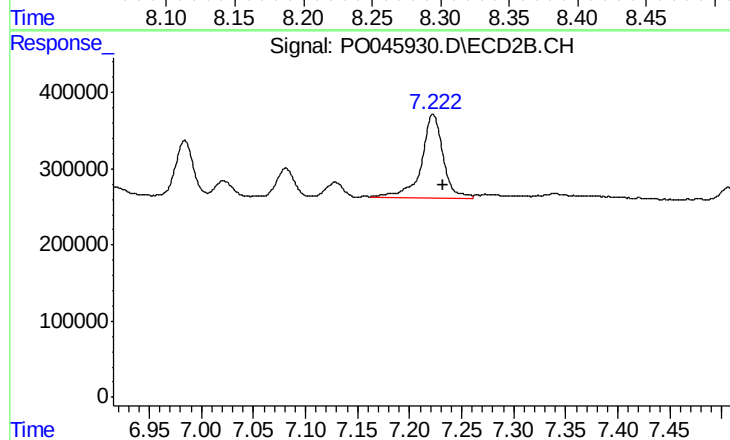

#34 AR-1260-4

R.T.: 7.222 min
Delta R.T.: -0.009 min
Response: 1613630
Conc: 144.62 ng/ml

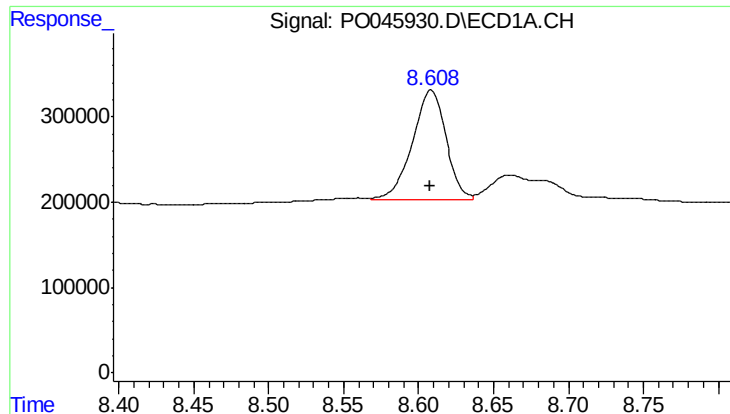


#35 AR-1260-5

R.T.: 8.608 min
Delta R.T.: 0.000 min
Response: 1983686
Conc: 144.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-44COMP

Manual Integrations
APPROVED

UGO
6/21/2018 3:15:17 PM

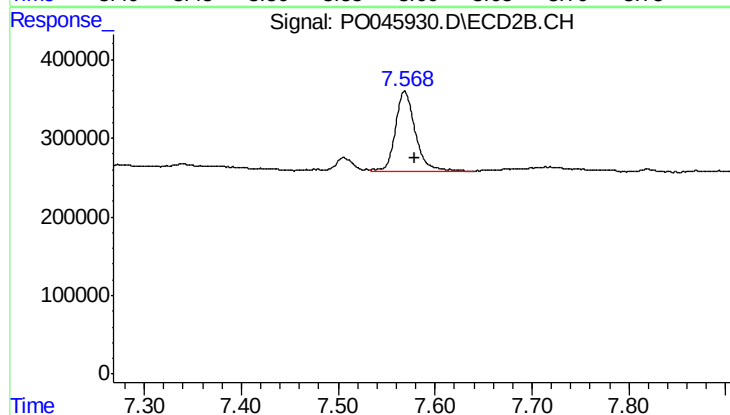

#35 AR-1260-5

R.T.: 7.569 min
Delta R.T.: -0.011 min
Response: 1435860
Conc: 179.90 ng/ml