

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061919\
 Data File : P0057262.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jun 2019 15:47
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 08:01:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.238	3.559	818886	687952	21.390	20.861
2)	SA Decachlor...	9.796	8.486	822771	504236	16.763	14.141
Target Compounds							
20)	L4 AR-1242-5	0.000	5.440	0	54688	N.D.	46.257 #
25)	L5 AR-1248-5	0.000	5.440	0	54688	N.D.	33.043 #
26)	L6 AR-1254-1	0.000	5.440	0	54688	N.D.	20.678 #
29)	L6 AR-1254-4	0.000	6.270	0	48083	N.D.	21.886 #
32)	L7 AR-1260-2	0.000	6.270	0	48083	N.D.	19.507 #
40)	L8 AR-1262-5	0.000	8.037	0	10623	N.D.	4.575 #
44)	L9 AR-1268-4	0.000	8.037	0	10623	N.D.	4.551 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061919\
Data File : PO057262.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jun 2019 15:47
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 08:01:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

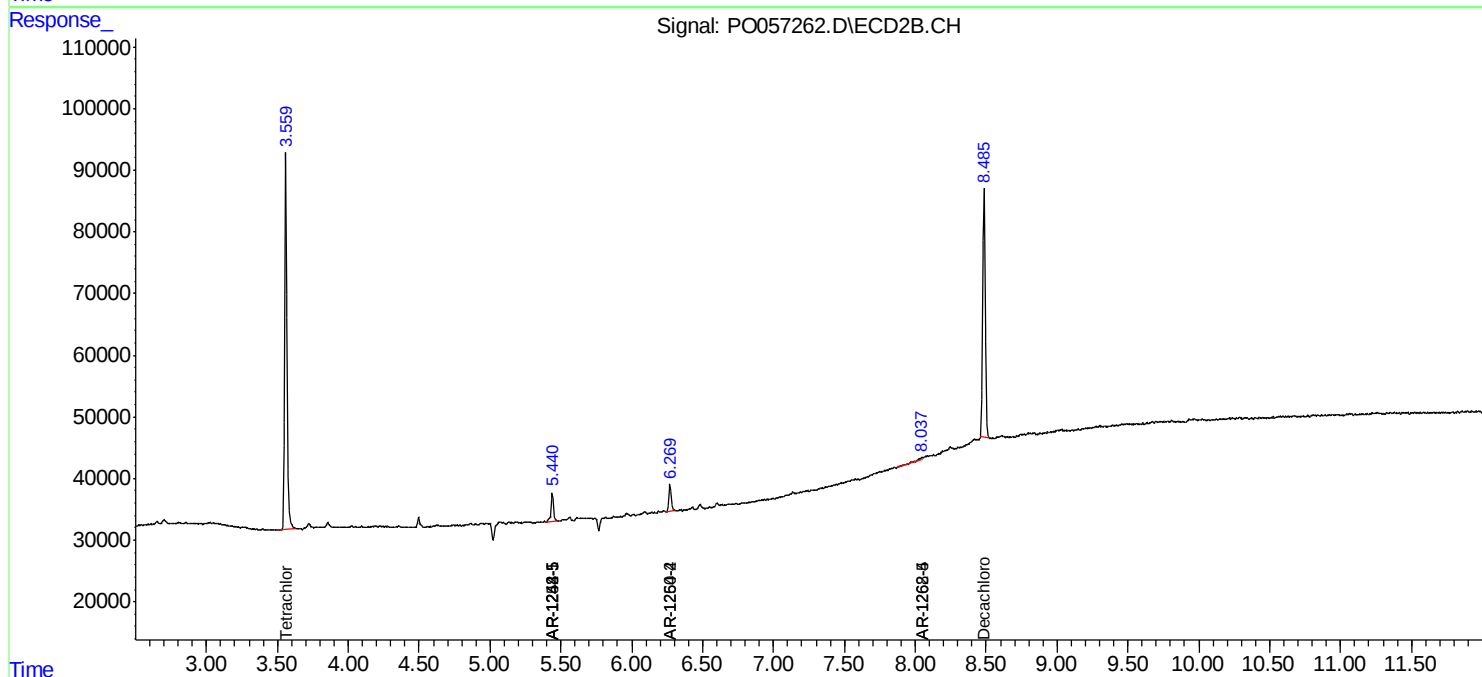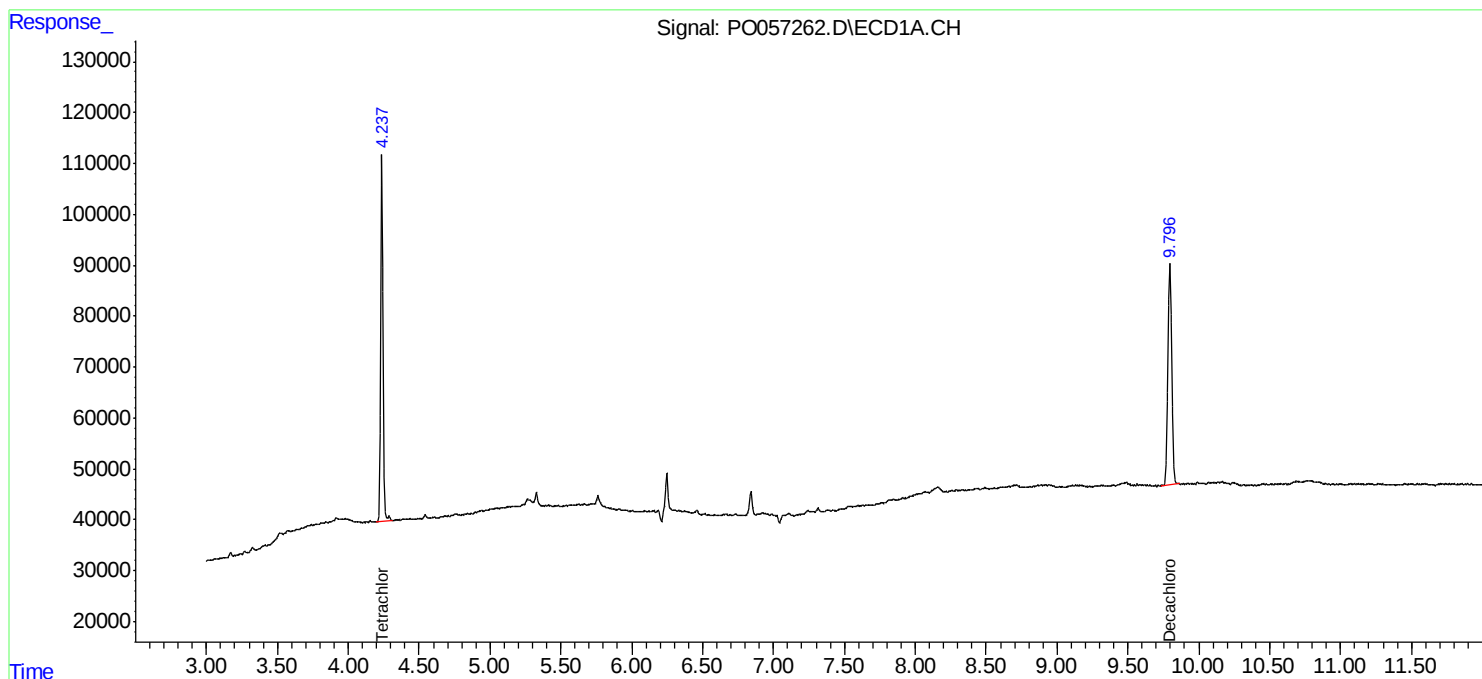


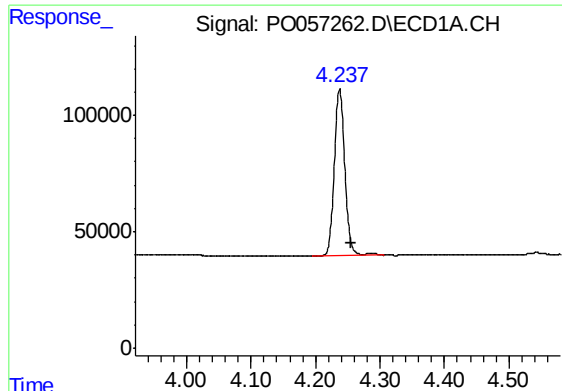

#1 Tetrachloro-m-xylene


R.T.: 4.238 min
Delta R.T.: -0.018 min
Response: 818886
Conc: 21.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

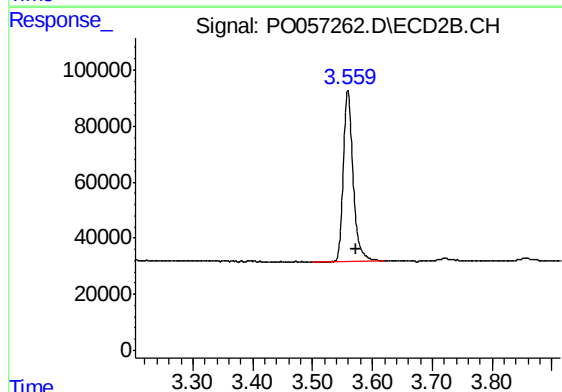


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: -0.014 min
Response: 687952
Conc: 20.86 ng/ml

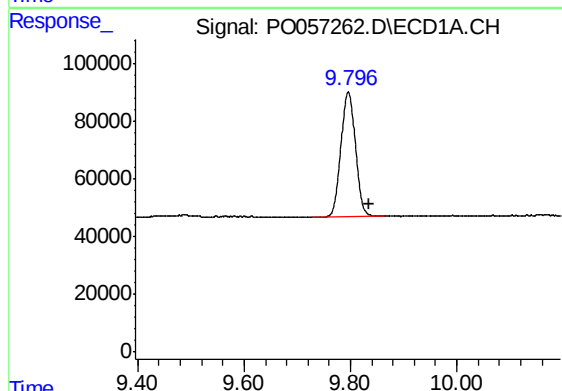


#2 Decachlorobiphenyl

R.T.: 9.796 min
Delta R.T.: -0.040 min
Response: 822771
Conc: 16.76 ng/ml

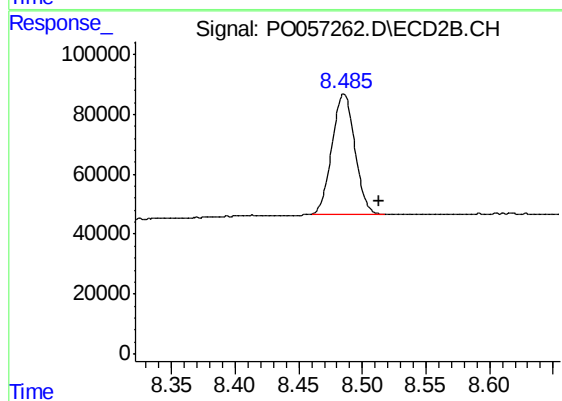

#2 Decachlorobiphenyl


R.T.: 8.486 min
Delta R.T.: -0.027 min
Response: 504236
Conc: 14.14 ng/ml

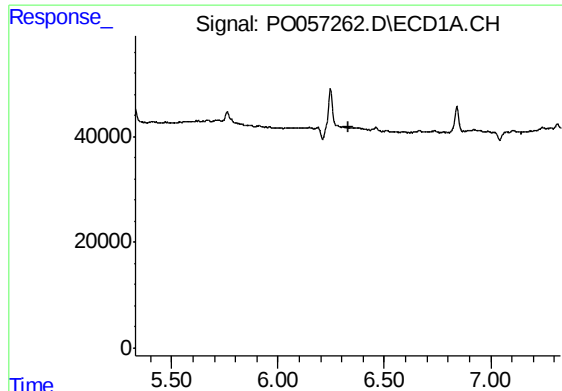

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.329 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

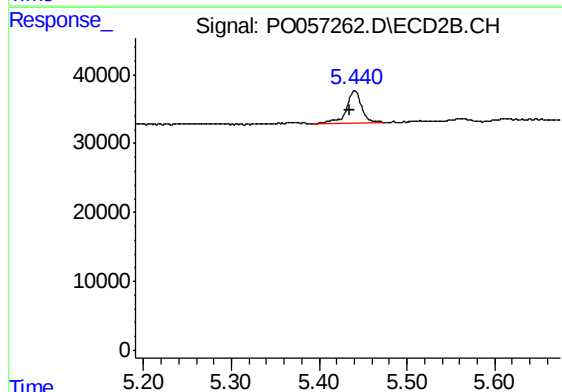


#20 AR-1242-5

R.T.: 5.440 min
Delta R.T.: 0.005 min
Response: 54688
Conc: 46.26 ng/ml

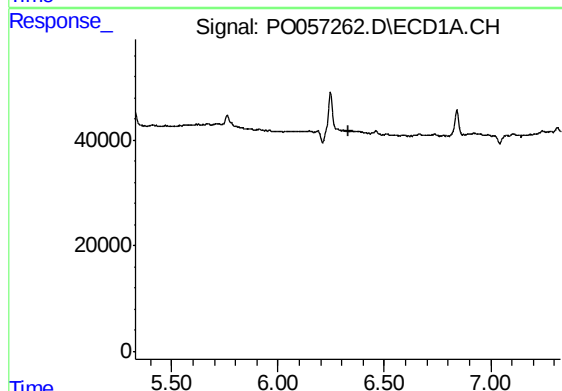


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.329 min
Response: 0
Conc: N.D.

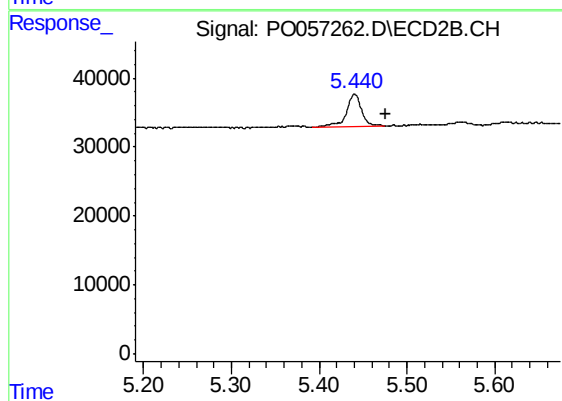

#25 AR-1248-5


R.T.: 5.440 min
Delta R.T.: -0.035 min
Response: 54688
Conc: 33.04 ng/ml

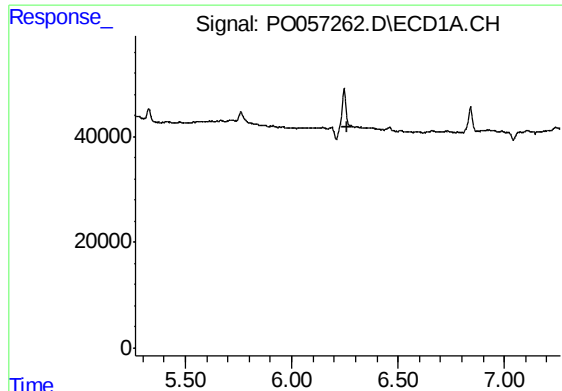

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

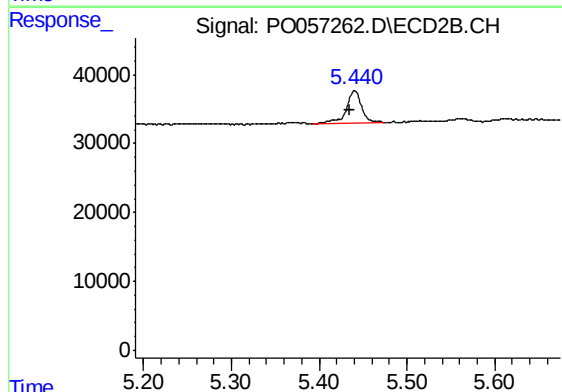


#26 AR-1254-1

R.T.: 5.440 min
Delta R.T.: 0.006 min
Response: 54688
Conc: 20.68 ng/ml

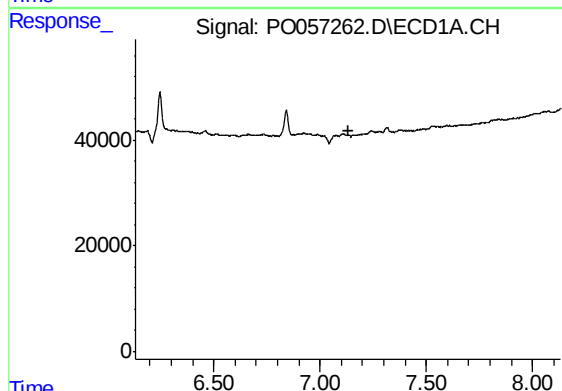


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T.: 7.131 min
Response: 0
Conc: N.D.

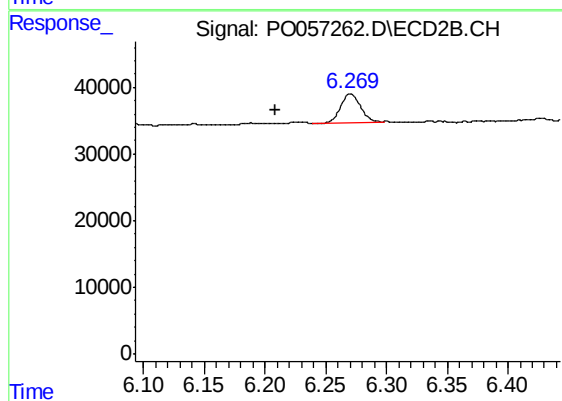

#29 AR-1254-4


R.T.: 6.270 min
Delta R.T.: 0.062 min
Response: 48083
Conc: 21.89 ng/ml

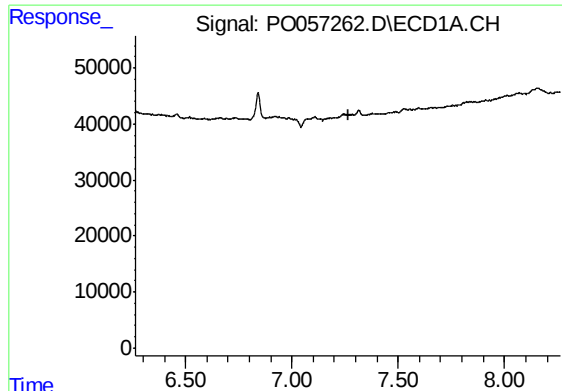

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

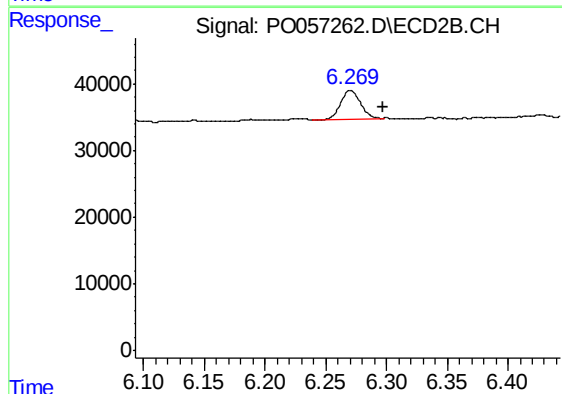


#32 AR-1260-2

R.T.: 6.270 min
Delta R.T.: -0.028 min
Response: 48083
Conc: 19.51 ng/ml

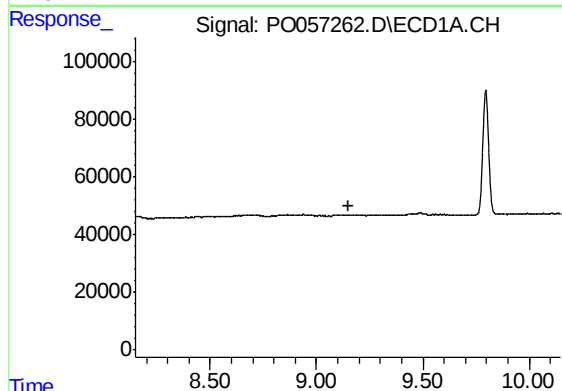


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.148 min
Response: 0
Conc: N.D.

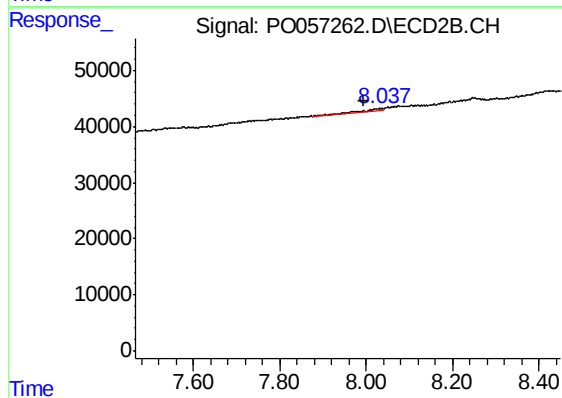

#40 AR-1262-5


R.T.: 8.037 min
Delta R.T.: 0.043 min
Response: 10623
Conc: 4.57 ng/ml

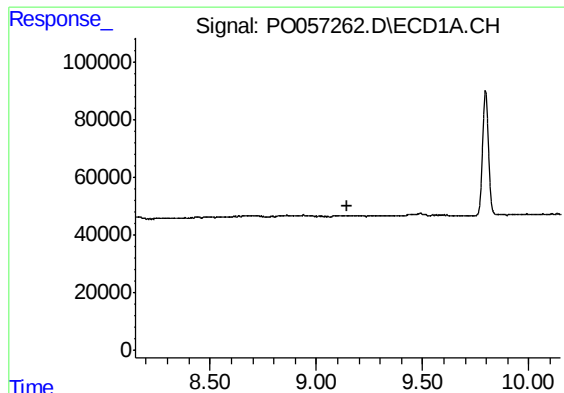

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.148 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

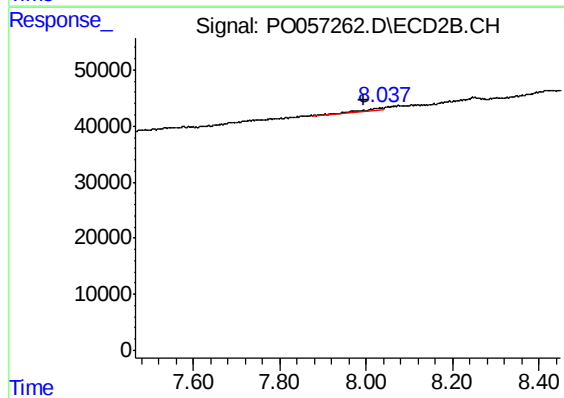

#44 AR-1268-4

R.T.: 8.037 min
Delta R.T.: 0.044 min
Response: 10623
Conc: 4.55 ng/ml