

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061919\
 Data File : P0057291.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2019 00:59
 Operator : SM/SJ
 Sample : K3417-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONTROL-HOUSE-BRICKS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 08:14:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.234	3.559	1083104	834501	28.292	25.304
2)	SA Decachlor...	9.791	8.483	966434	644374	19.689	18.072
Target Compounds							
3)	L1 AR-1016-1	0.000	4.620	0	11204	N.D.	8.903 #
4)	L1 AR-1016-2	0.000	4.620	0	11204	N.D.	6.219 #
5)	L1 AR-1016-3	0.000	4.837	0	211620	N.D.	214.637 #
6)	L1 AR-1016-4	0.000	4.837	0	211620	N.D.	255.629 #
7)	L1 AR-1016-5	0.000	5.104	0	40807	N.D.	38.041 #
10)	L2 AR-1221-3	4.690	3.972	1112657	828031	752.776	691.725
11)	L3 AR-1232-1	4.690	3.972	1112657	828031	944.222	921.711
12)	L3 AR-1232-2	0.000	4.620	0	11204	N.D.	11.528 #
13)	L3 AR-1232-3	0.000	4.837	0	211620	N.D.	404.402 #
14)	L3 AR-1232-4	0.000	4.925	0	53313	N.D.	108.209 #
15)	L3 AR-1232-5	0.000	5.104	0	40807	N.D.	72.449 #
16)	L4 AR-1242-1	0.000	4.620	0	11204	N.D.	9.046 #
17)	L4 AR-1242-2	0.000	4.620	0	11204	N.D.	6.230 #
18)	L4 AR-1242-3	0.000	4.837	0	211620	N.D.	215.257 #
19)	L4 AR-1242-4	0.000	4.925	0	53313	N.D.	54.787 #
20)	L4 AR-1242-5	0.000	5.440	0	216277	N.D.	182.934 #
21)	L5 AR-1248-1	0.000	4.620	0	11204	N.D.	11.964 #
22)	L5 AR-1248-2	0.000	4.837	0	211620	N.D.	166.572 #
23)	L5 AR-1248-3	0.000	4.925	0	53313	N.D.	40.825 #
24)	L5 AR-1248-4	0.000	5.104	0	40807	N.D.	25.768 #
25)	L5 AR-1248-5	0.000	5.440	0	216277	N.D.	130.676 #
26)	L6 AR-1254-1	0.000	5.440	0	216277	N.D.	81.777 #
27)	L6 AR-1254-2	6.458	5.561	467170	77328	120.278	35.870 #
28)	L6 AR-1254-3	0.000	5.962	0	278341	N.D.	76.027 #
29)	L6 AR-1254-4	7.073	6.189	296772	141499	98.601	64.408 #
30)	L6 AR-1254-5	0.000	6.636	0	248192	N.D.	78.288 #
31)	L7 AR-1260-1	6.953	6.093	941055	334039	366.715	166.988 #
32)	L7 AR-1260-2	0.000	6.306	0	329886	N.D.	133.830 #
33)	L7 AR-1260-3	0.000	6.427	0	158568	N.D.	70.687 #
34)	L7 AR-1260-4	0.000	6.892	0	153298	N.D.	82.373 #
35)	L7 AR-1260-5	0.000	7.137	0	472443	N.D.	109.556 #
36)	L8 AR-1262-1	0.000	6.636	0	248192	N.D.	59.461 #
37)	L8 AR-1262-2	0.000	7.137	0	472443	N.D.	68.763 #
38)	L8 AR-1262-3	0.000	7.414	0	138180	N.D.	46.786 #
39)	L8 AR-1262-4	0.000	7.480	0	232205	N.D.	44.564 #
40)	L8 AR-1262-5	0.000	7.972	0	58996	N.D.	25.406 #
41)	L9 AR-1268-1	0.000	7.414	0	138180	N.D.	18.510 #
42)	L9 AR-1268-2	0.000	7.480	0	232205	N.D.	33.253 #
43)	L9 AR-1268-3	0.000	7.680	0	11192	N.D.	1.886 #
44)	L9 AR-1268-4	0.000	7.972	0	58996	N.D.	25.274 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061919\
Data File : P0057291.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2019 00:59
Operator : SM/SJ
Sample : K3417-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 08:14:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	0.000	8.247	0	48482	N.D.	2.801 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061919\
Data File : PO057291.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2019 00:59
Operator : SM/SJ
Sample : K3417-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 08:14:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

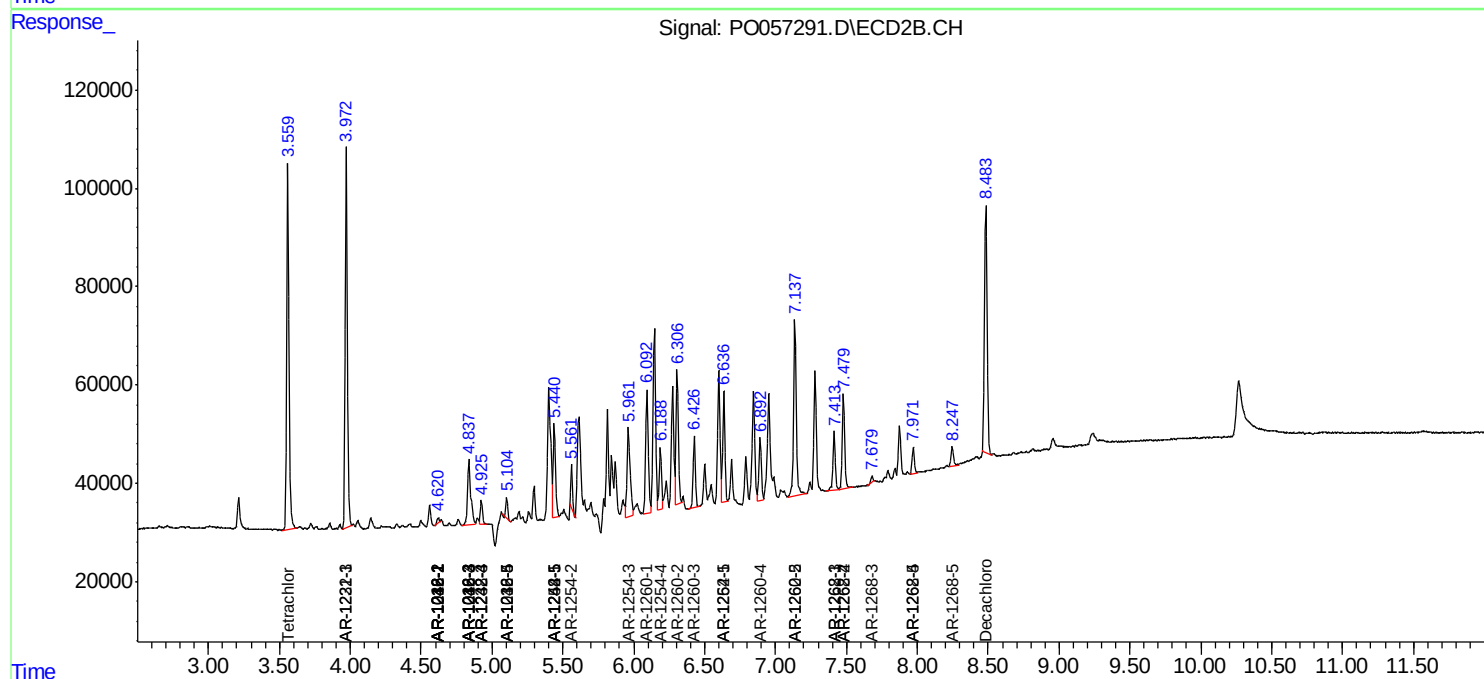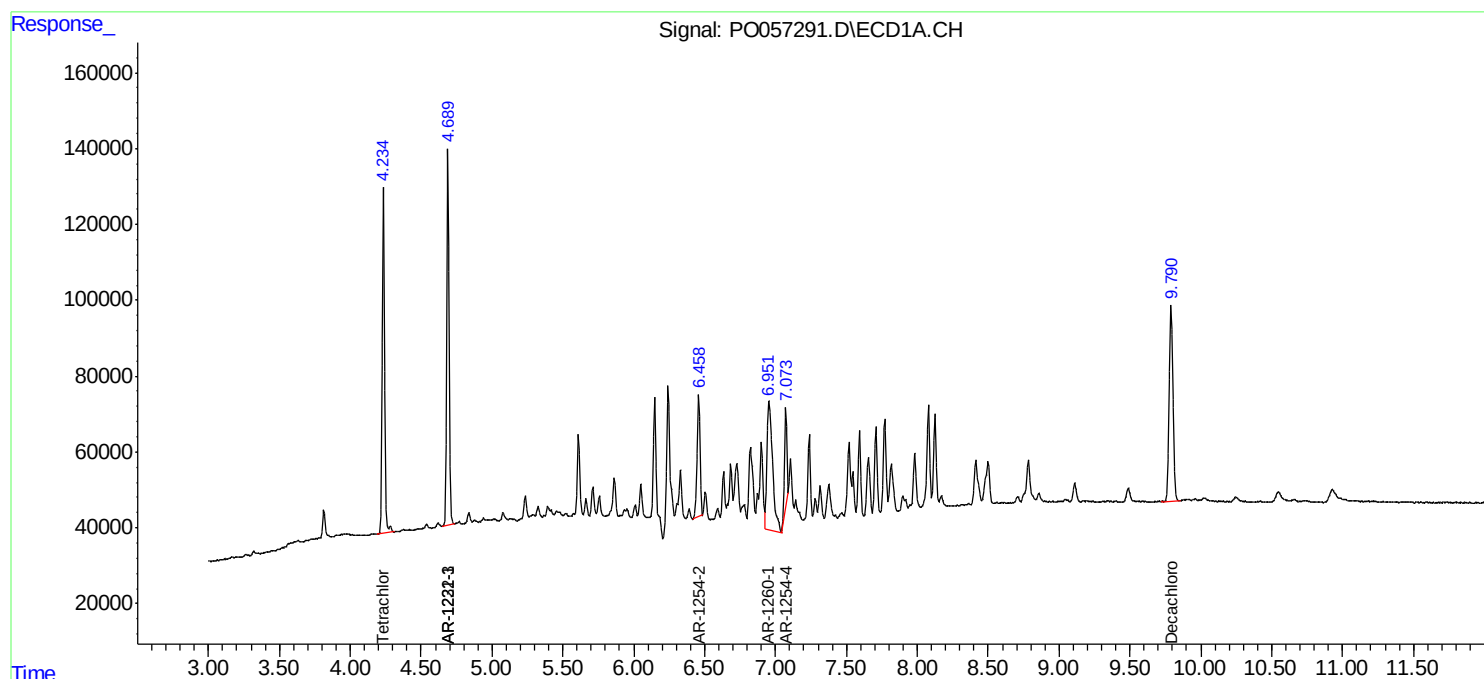




#1 Tetrachloro-m-xylene


R.T.: 4.234 min
Delta R.T.: -0.022 min
Response: 1083104
Conc: 28.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

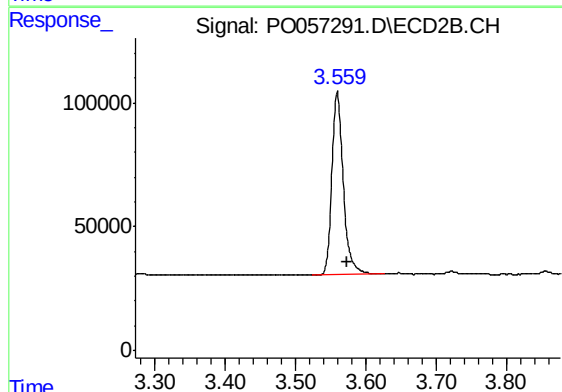


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: -0.014 min
Response: 834501
Conc: 25.30 ng/ml




#2 Decachlorobiphenyl

R.T.: 9.791 min
Delta R.T.: -0.046 min
Response: 966434
Conc: 19.69 ng/ml

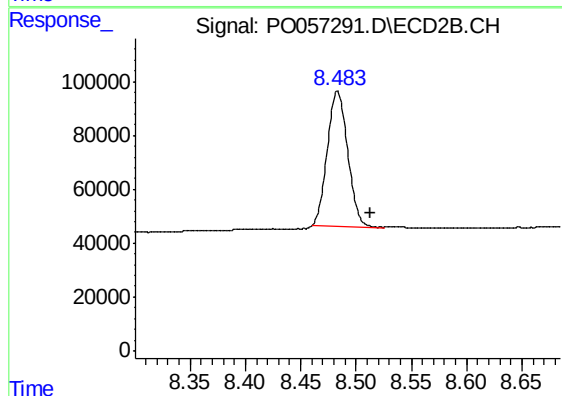

#2 Decachlorobiphenyl


R.T.: 8.483 min
Delta R.T.: -0.030 min
Response: 644374
Conc: 18.07 ng/ml

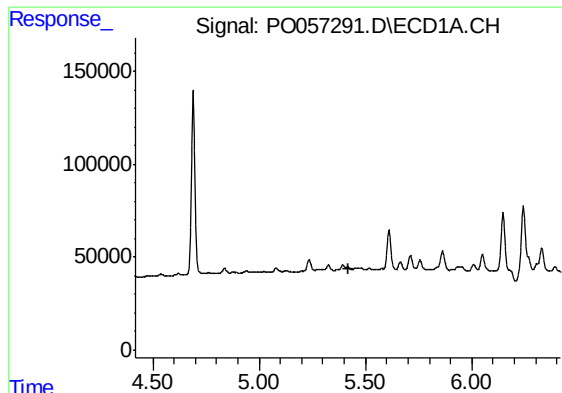

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

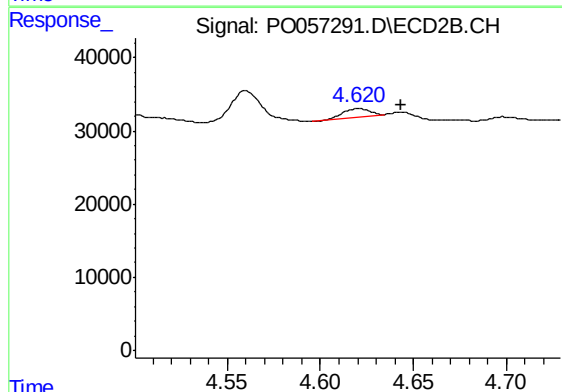


#3 AR-1016-1

R.T.: 4.620 min
Delta R.T.: -0.023 min
Response: 11204
Conc: 8.90 ng/ml

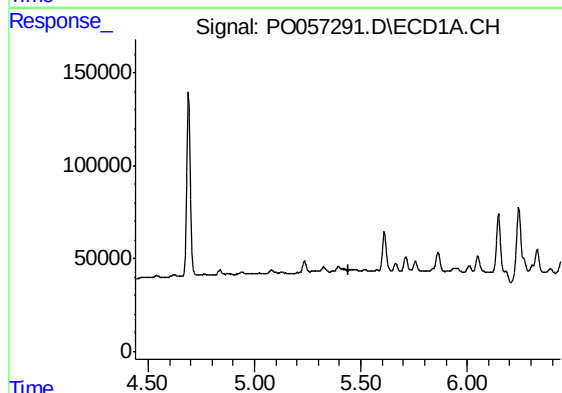


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.440 min
Response: 0
Conc: N.D.

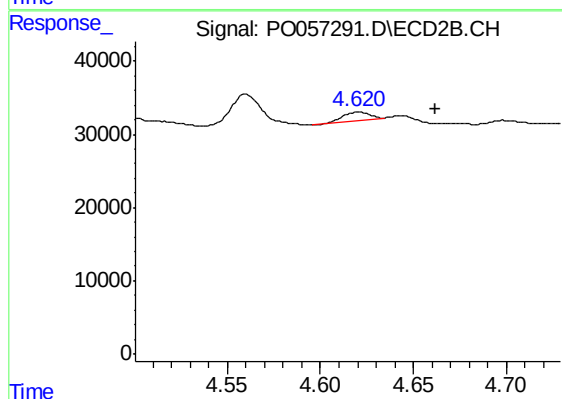

#4 AR-1016-2


R.T.: 4.620 min
Delta R.T.: -0.042 min
Response: 11204
Conc: 6.22 ng/ml



#5 AR-1016-3


R.T.: 0.000 min
Exp R.T. : 5.500 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

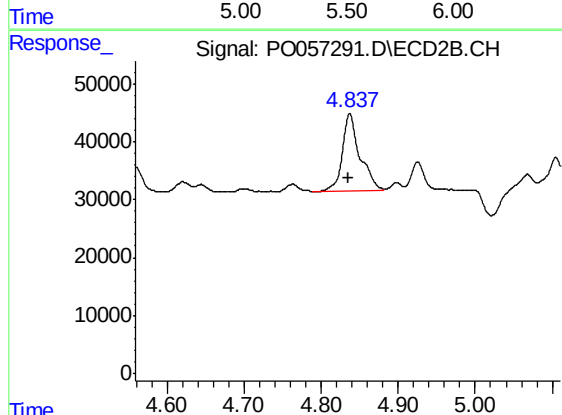


#5 AR-1016-3

R.T.: 4.837 min
Delta R.T.: 0.000 min
Response: 211620
Conc: 214.64 ng/ml

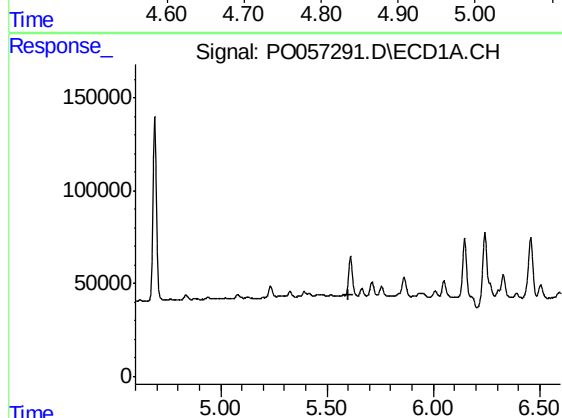


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.599 min
Response: 0
Conc: N.D.

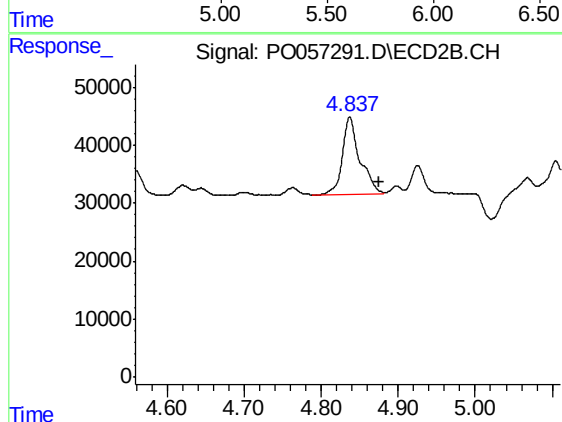

#6 AR-1016-4


R.T.: 4.837 min
Delta R.T.: -0.039 min
Response: 211620
Conc: 255.63 ng/ml

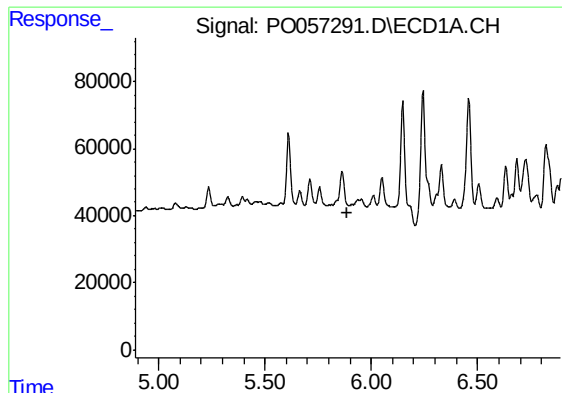

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.890 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

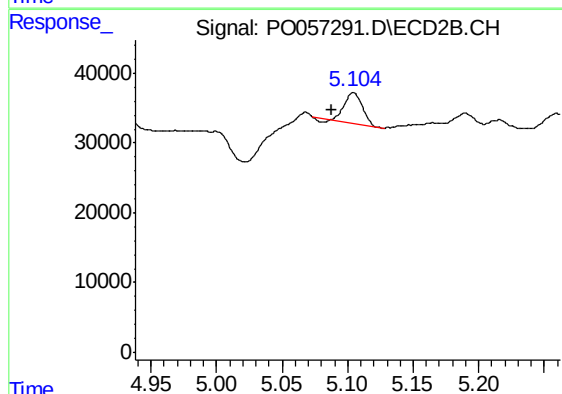


#7 AR-1016-5

R.T.: 5.104 min
Delta R.T.: 0.016 min
Response: 40807
Conc: 38.04 ng/ml

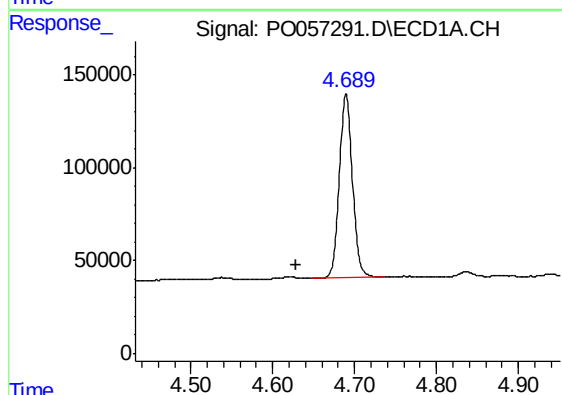


#10 AR-1221-3

R.T.: 4.690 min
Delta R.T.: 0.061 min
Response: 1112657
Conc: 752.78 ng/ml

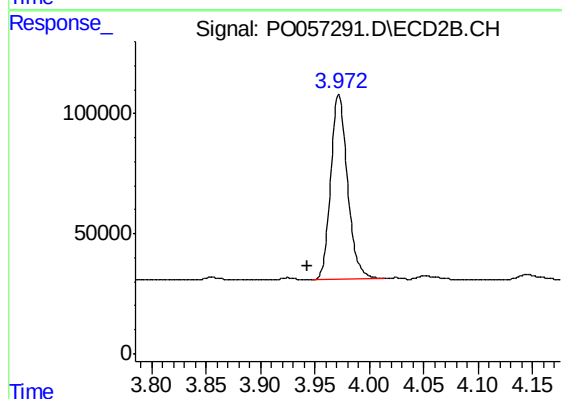

#10 AR-1221-3


R.T.: 3.972 min
Delta R.T.: 0.029 min
Response: 828031
Conc: 691.72 ng/ml



#11 AR-1232-1


R.T.: 4.690 min
Delta R.T.: 0.061 min
Response: 1112657
Conc: 944.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

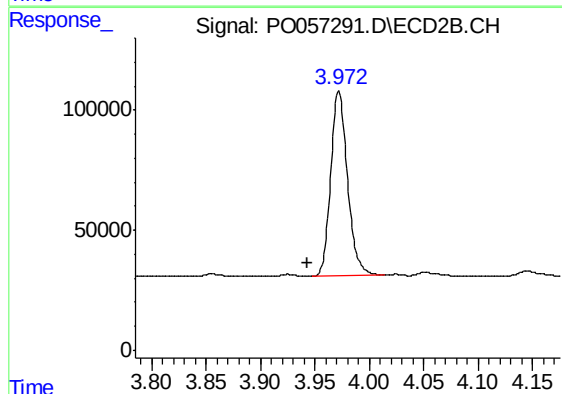


#11 AR-1232-1

R.T.: 3.972 min
Delta R.T.: 0.029 min
Response: 828031
Conc: 921.71 ng/ml




#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.152 min
Response: 0
Conc: N.D.

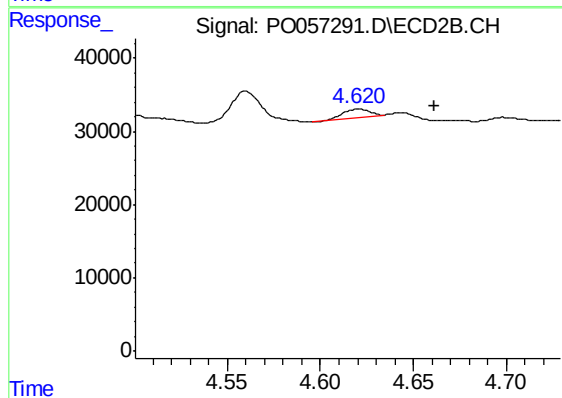

#12 AR-1232-2


R.T.: 4.620 min
Delta R.T.: -0.041 min
Response: 11204
Conc: 11.53 ng/ml



#13 AR-1232-3


R.T.: 0.000 min
Exp R.T. : 5.439 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

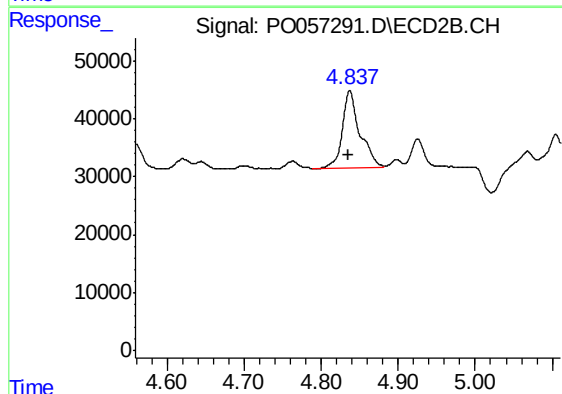


#13 AR-1232-3

R.T.: 4.837 min
Delta R.T.: 0.001 min
Response: 211620
Conc: 404.40 ng/ml




#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.599 min
Response: 0
Conc: N.D.

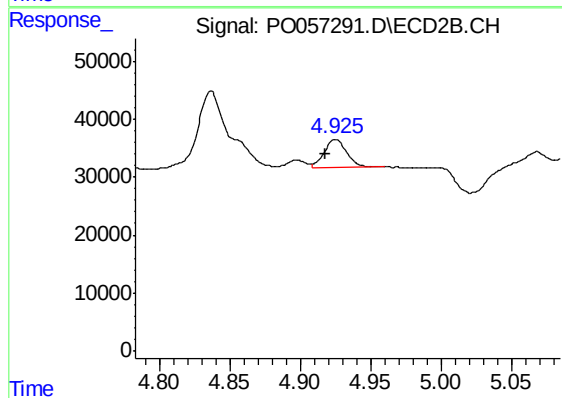

#14 AR-1232-4


R.T.: 4.925 min
Delta R.T.: 0.007 min
Response: 53313
Conc: 108.21 ng/ml

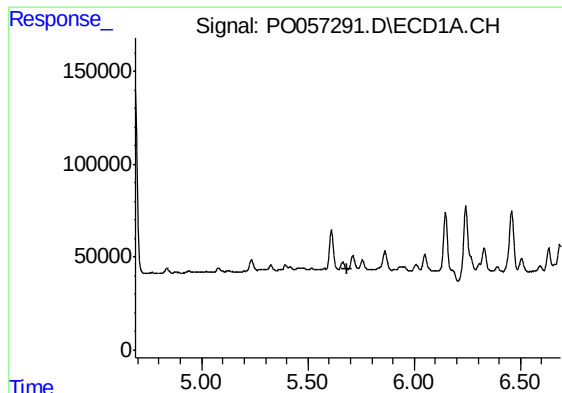

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.688 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

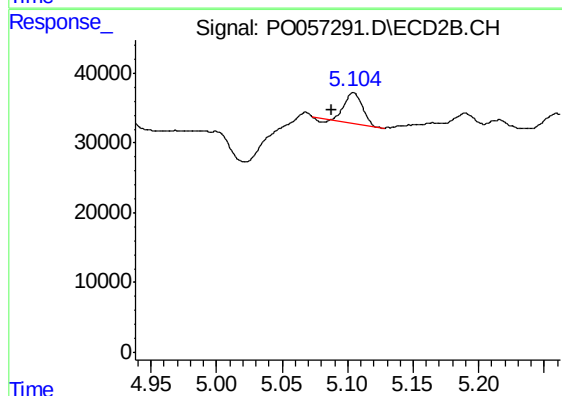


#15 AR-1232-5

R.T.: 5.104 min
Delta R.T.: 0.016 min
Response: 40807
Conc: 72.45 ng/ml

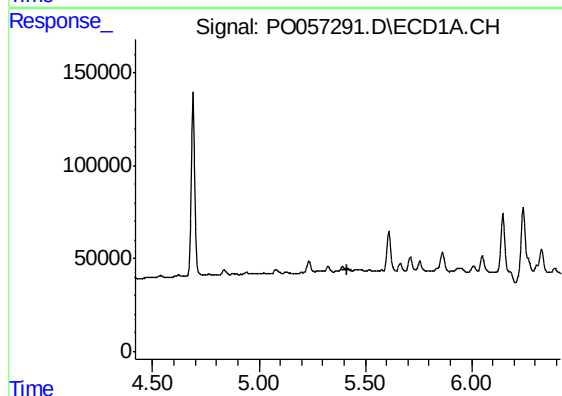


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.418 min
Response: 0
Conc: N.D.

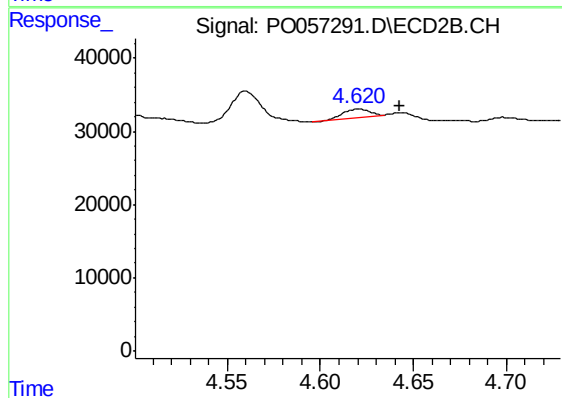

#16 AR-1242-1


R.T.: 4.620 min
Delta R.T.: -0.023 min
Response: 11204
Conc: 9.05 ng/ml



#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

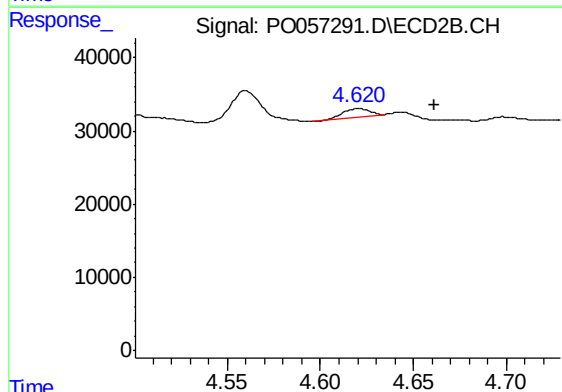


#17 AR-1242-2

R.T.: 4.620 min
Delta R.T.: -0.041 min
Response: 11204
Conc: 6.23 ng/ml




#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.500 min
Response: 0
Conc: N.D.

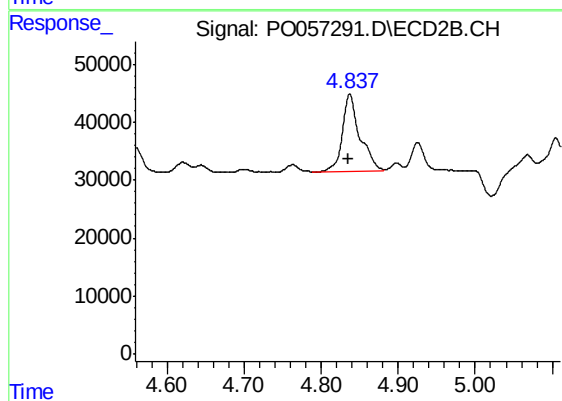

#18 AR-1242-3


R.T.: 4.837 min
Delta R.T.: 0.002 min
Response: 211620
Conc: 215.26 ng/ml

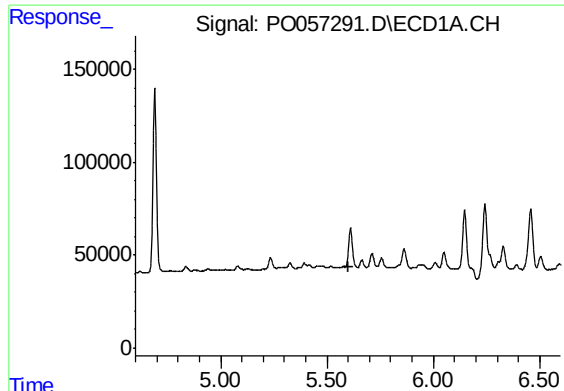

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

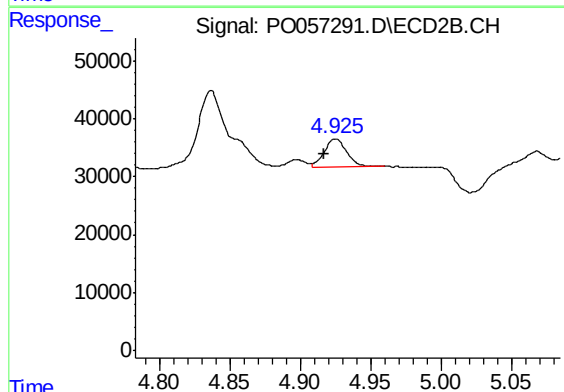


#19 AR-1242-4

R.T.: 4.925 min
Delta R.T.: 0.008 min
Response: 53313
Conc: 54.79 ng/ml

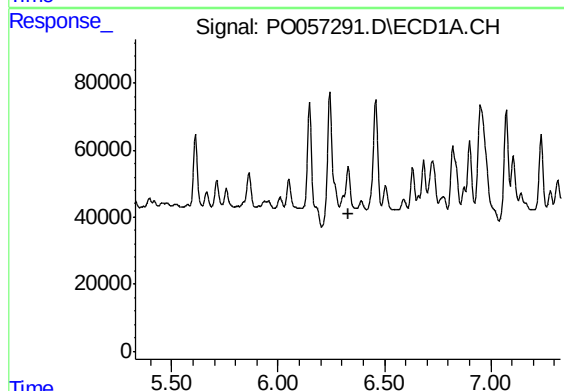


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.329 min
Response: 0
Conc: N.D.

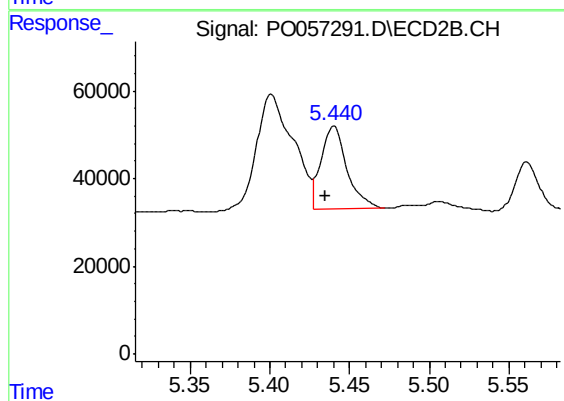

#20 AR-1242-5


R.T.: 5.440 min
Delta R.T.: 0.005 min
Response: 216277
Conc: 182.93 ng/ml

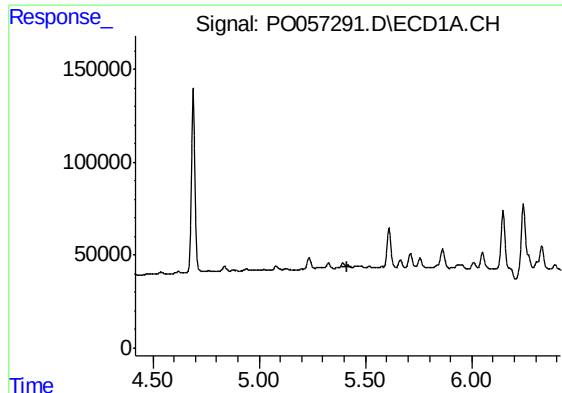

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

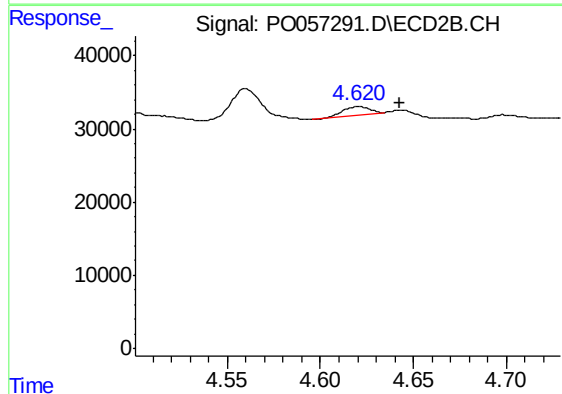


#21 AR-1248-1

R.T.: 4.620 min
Delta R.T.: -0.023 min
Response: 11204
Conc: 11.96 ng/ml

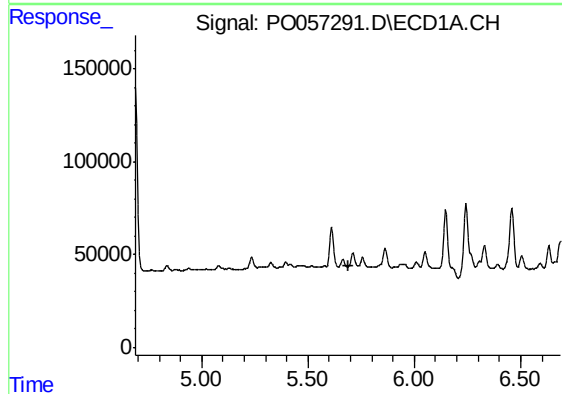


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.688 min
Response: 0
Conc: N.D.

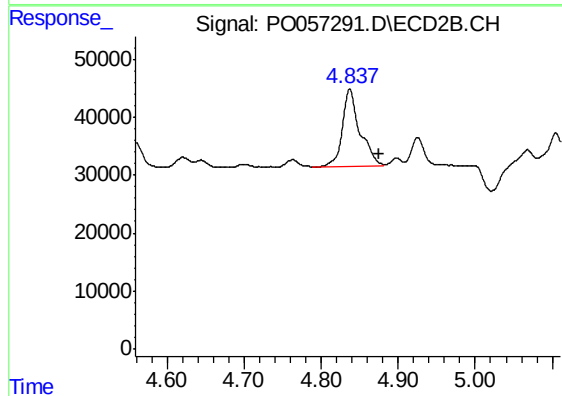

#22 AR-1248-2


R.T.: 4.837 min
Delta R.T.: -0.039 min
Response: 211620
Conc: 166.57 ng/ml



#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.890 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

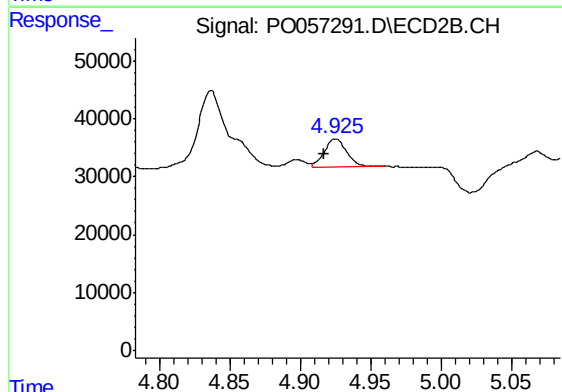


#23 AR-1248-3

R.T.: 4.925 min
Delta R.T.: 0.008 min
Response: 53313
Conc: 40.82 ng/ml

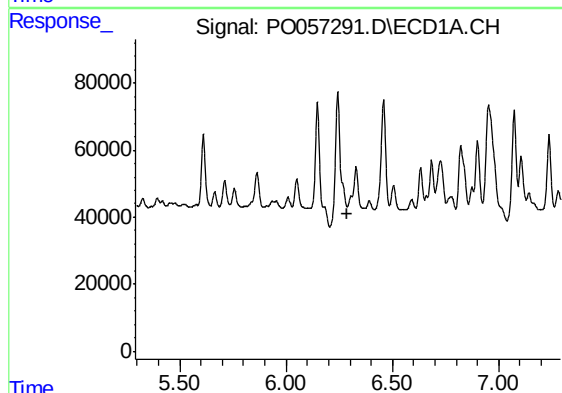


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.291 min
Response: 0
Conc: N.D.

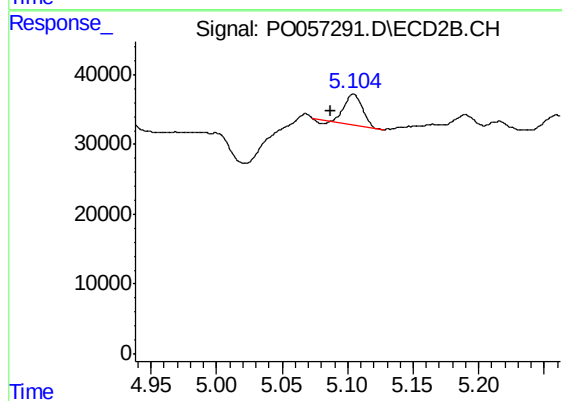

#24 AR-1248-4


R.T.: 5.104 min
Delta R.T.: 0.017 min
Response: 40807
Conc: 25.77 ng/ml



#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.329 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

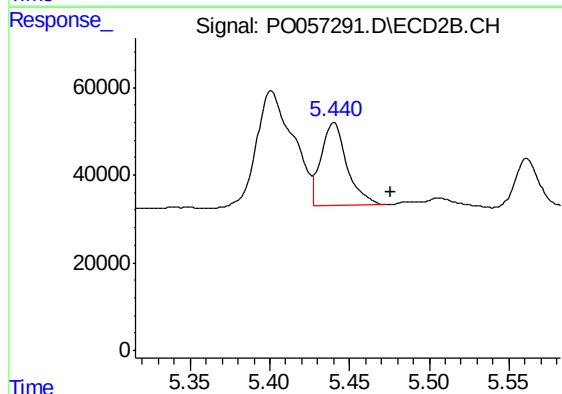


#25 AR-1248-5

R.T.: 5.440 min
Delta R.T.: -0.036 min
Response: 216277
Conc: 130.68 ng/ml




#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.264 min
Response: 0
Conc: N.D.

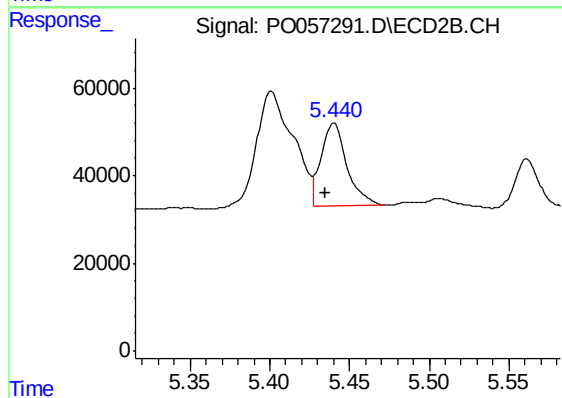

#26 AR-1254-1


R.T.: 5.440 min
Delta R.T.: 0.005 min
Response: 216277
Conc: 81.78 ng/ml



#27 AR-1254-2


R.T.: 6.458 min
Delta R.T.: -0.023 min
Response: 467170
Conc: 120.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

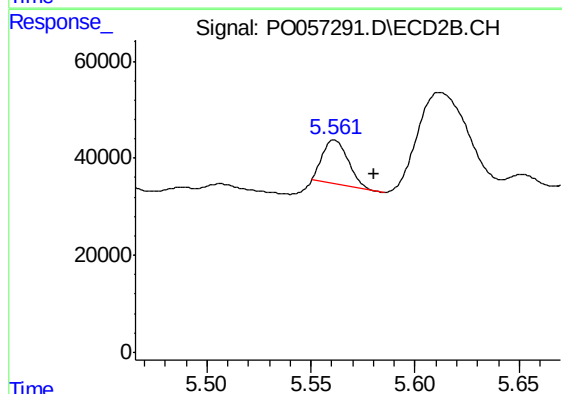


#27 AR-1254-2

R.T.: 5.561 min
Delta R.T.: -0.019 min
Response: 77328
Conc: 35.87 ng/ml

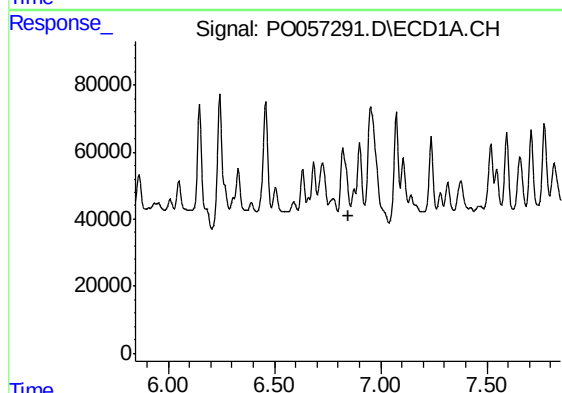


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.846 min
Response: 0
Conc: N.D.

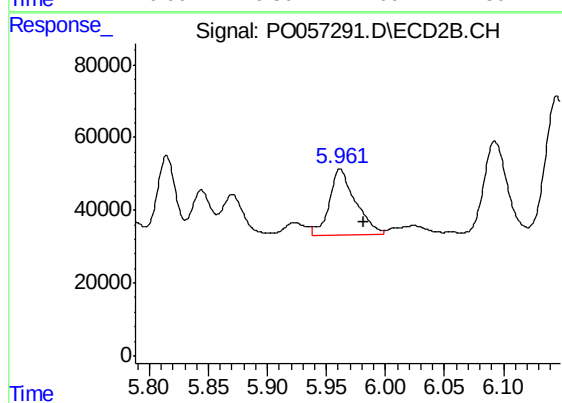

#28 AR-1254-3


R.T.: 5.962 min
Delta R.T.: -0.020 min
Response: 278341
Conc: 76.03 ng/ml



#29 AR-1254-4


R.T.: 7.073 min
Delta R.T.: -0.058 min
Response: 296772
Conc: 98.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

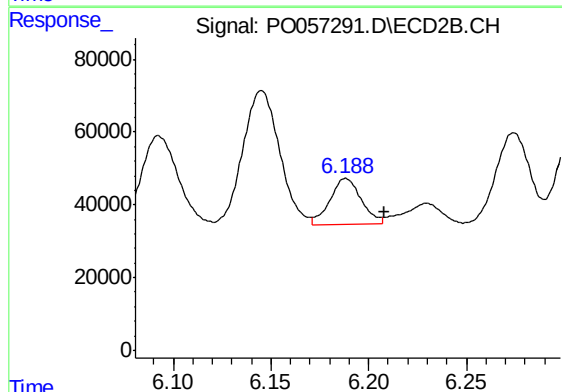


#29 AR-1254-4

R.T.: 6.189 min
Delta R.T.: -0.020 min
Response: 141499
Conc: 64.41 ng/ml




#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.547 min
Response: 0
Conc: N.D.

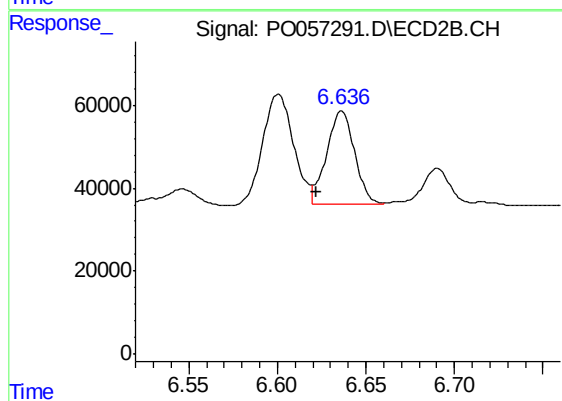

#30 AR-1254-5


R.T.: 6.636 min
Delta R.T.: 0.014 min
Response: 248192
Conc: 78.29 ng/ml



#31 AR-1260-1


R.T.: 6.953 min
Delta R.T.: -0.055 min
Response: 941055
Conc: 366.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

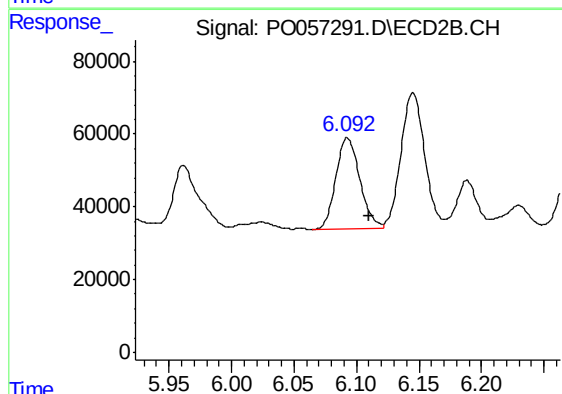


#31 AR-1260-1

R.T.: 6.093 min
Delta R.T.: -0.018 min
Response: 334039
Conc: 166.99 ng/ml

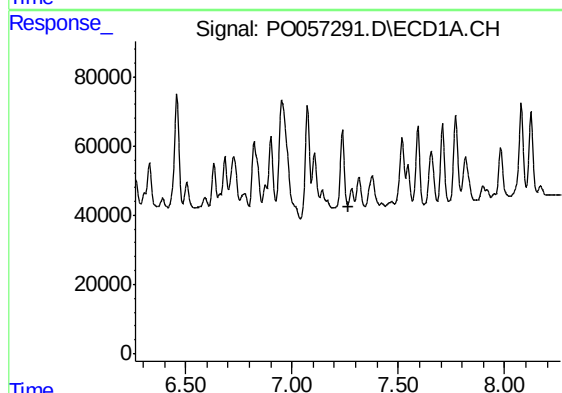


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.264 min
Response: 0
Conc: N.D.

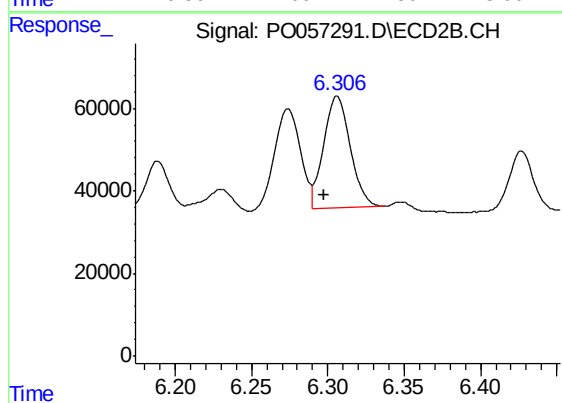

#32 AR-1260-2


R.T.: 6.306 min
Delta R.T.: 0.009 min
Response: 329886
Conc: 133.83 ng/ml



#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.620 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

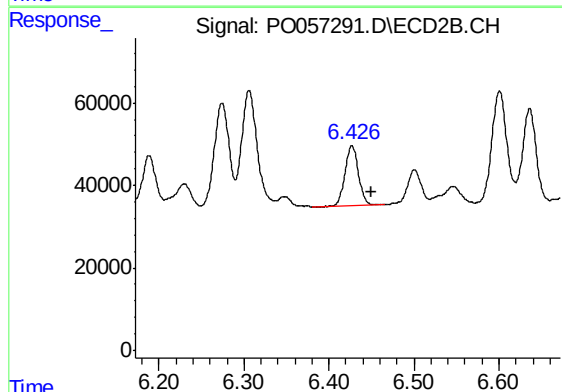


#33 AR-1260-3

R.T.: 6.427 min
Delta R.T.: -0.023 min
Response: 158568
Conc: 70.69 ng/ml




#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.845 min
Response: 0
Conc: N.D.

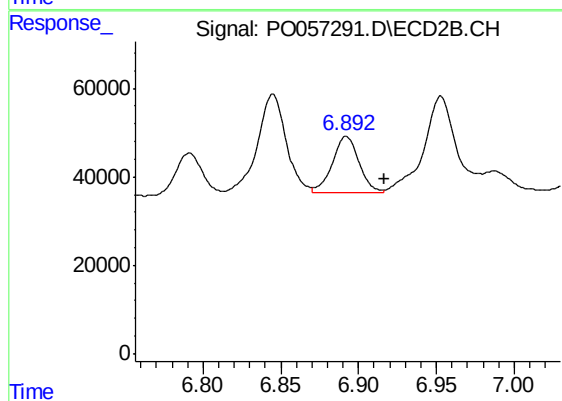

#34 AR-1260-4


R.T.: 6.892 min
Delta R.T.: -0.025 min
Response: 153298
Conc: 82.37 ng/ml



#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.153 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

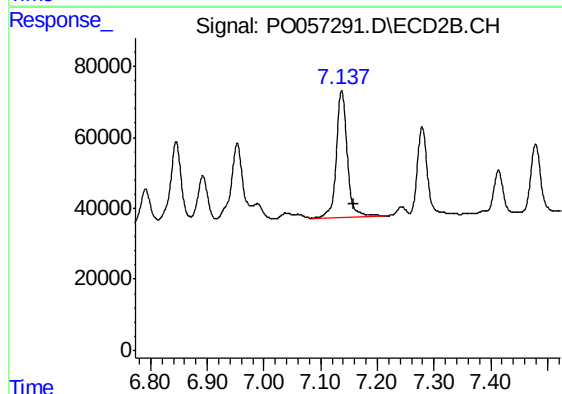


#35 AR-1260-5

R.T.: 7.137 min
Delta R.T.: -0.021 min
Response: 472443
Conc: 109.56 ng/ml




#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.620 min
Response: 0
Conc: N.D.

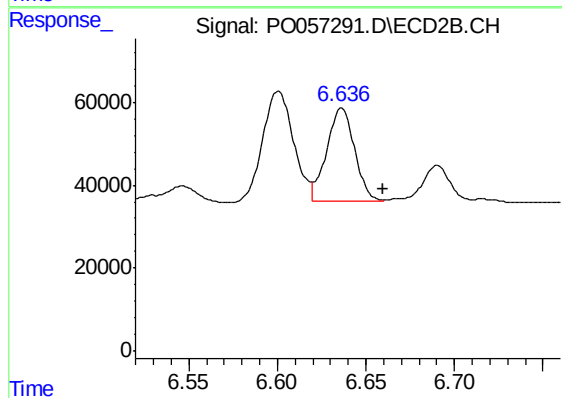

#36 AR-1262-1


R.T.: 6.636 min
Delta R.T.: -0.024 min
Response: 248192
Conc: 59.46 ng/ml



#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.154 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

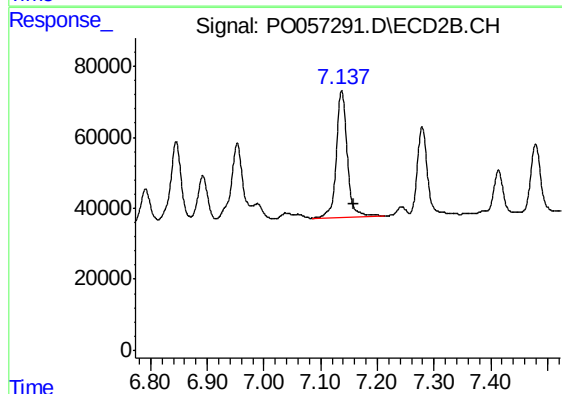


#37 AR-1262-2

R.T.: 7.137 min
Delta R.T.: -0.021 min
Response: 472443
Conc: 68.76 ng/ml




#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.445 min
Response: 0
Conc: N.D.

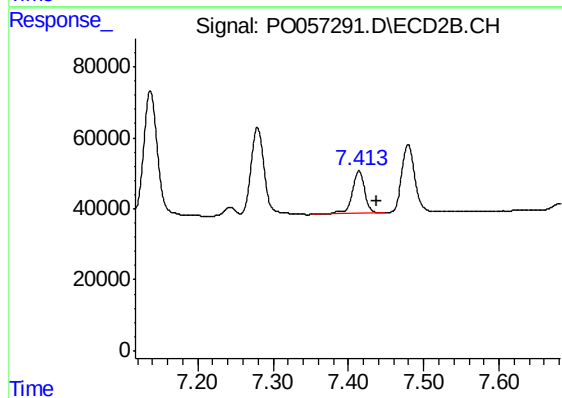

#38 AR-1262-3


R.T.: 7.414 min
Delta R.T.: -0.024 min
Response: 138180
Conc: 46.79 ng/ml



#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

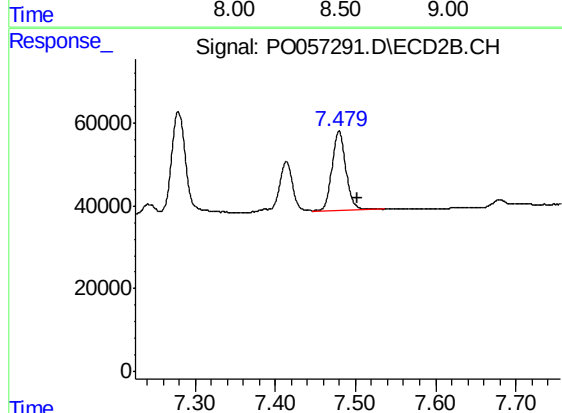


#39 AR-1262-4

R.T.: 7.480 min
Delta R.T.: -0.023 min
Response: 232205
Conc: 44.56 ng/ml

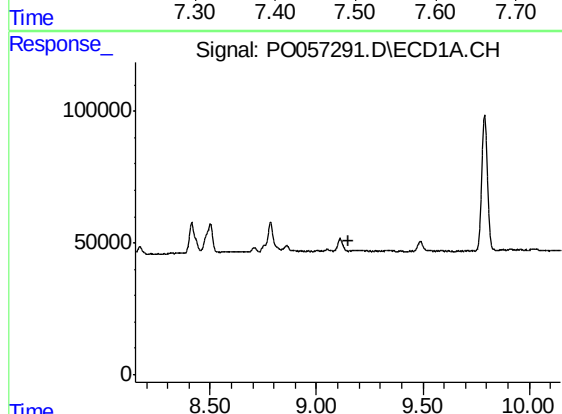


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.148 min
Response: 0
Conc: N.D.

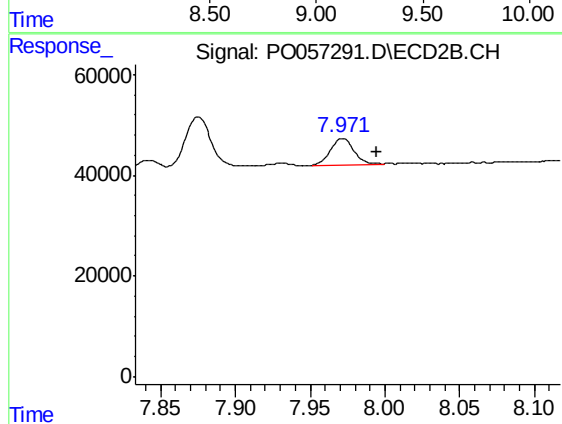

#40 AR-1262-5


R.T.: 7.972 min
Delta R.T.: -0.023 min
Response: 58996
Conc: 25.41 ng/ml



#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.444 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

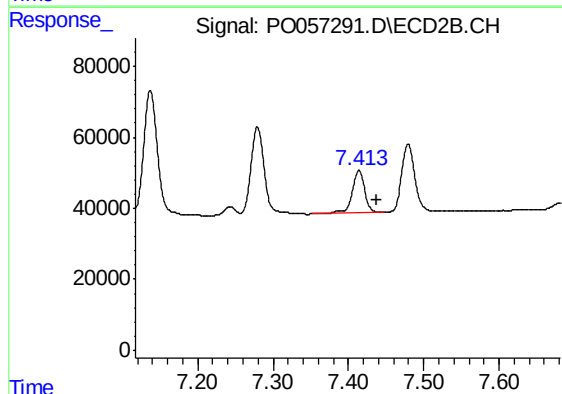


#41 AR-1268-1

R.T.: 7.414 min
Delta R.T.: -0.023 min
Response: 138180
Conc: 18.51 ng/ml




#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.534 min
Response: 0
Conc: N.D.

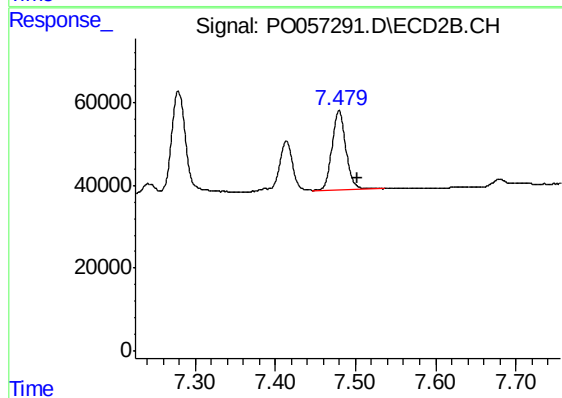

#42 AR-1268-2


R.T.: 7.480 min
Delta R.T.: -0.023 min
Response: 232205
Conc: 33.25 ng/ml



#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

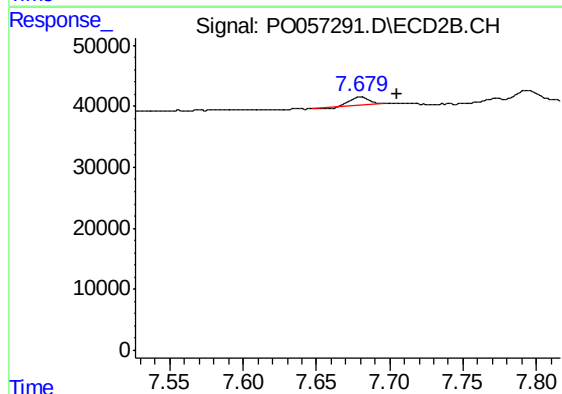


#43 AR-1268-3

R.T.: 7.680 min
Delta R.T.: -0.025 min
Response: 11192
Conc: 1.89 ng/ml




#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.148 min
Response: 0
Conc: N.D.

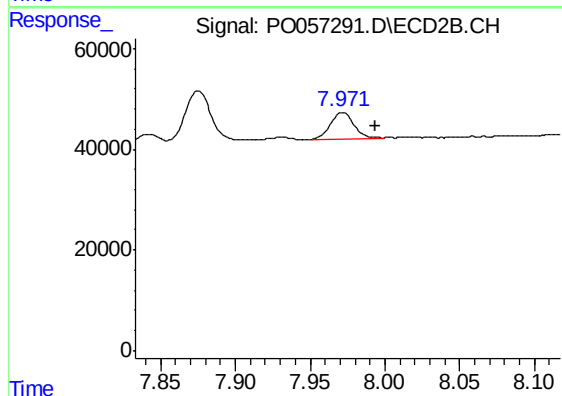

#44 AR-1268-4


R.T.: 7.972 min
Delta R.T.: -0.022 min
Response: 58996
Conc: 25.27 ng/ml

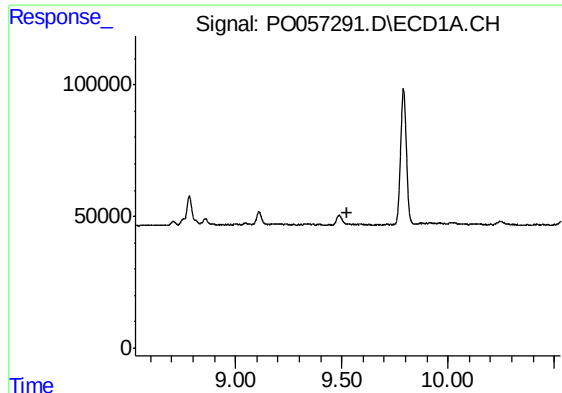

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS

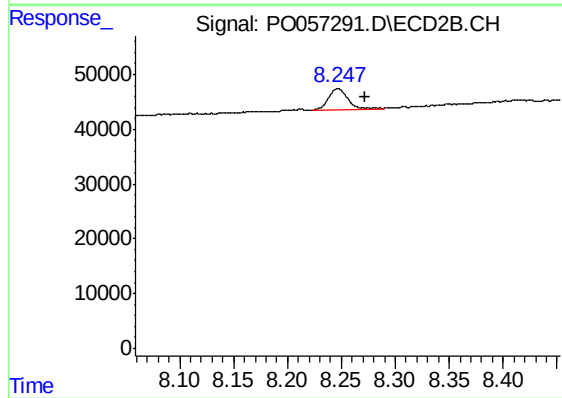

#45 AR-1268-5

R.T.: 8.247 min
Delta R.T.: -0.025 min
Response: 48482
Conc: 2.80 ng/ml