

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061919\
 Data File : P0057269.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jun 2019 17:55
 Operator : SM/SJ
 Sample : K3163-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU-03-061719-A

Manual Integrations
 APPROVED

Ankita
 6/20/2019 11:57:58 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 08:04:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.235	3.559	1071634	794018	27.992	24.077m
2) SA Decachlor...	9.795	8.485	1049981	660578	21.392	18.526m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061919\
Data File : P0057269.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jun 2019 17:55
Operator : SM/SJ
Sample : K3163-09
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SU-03-061719-A


Manual Integrations
APPROVED

Ankita
6/20/2019 11:57:58 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 08:04:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

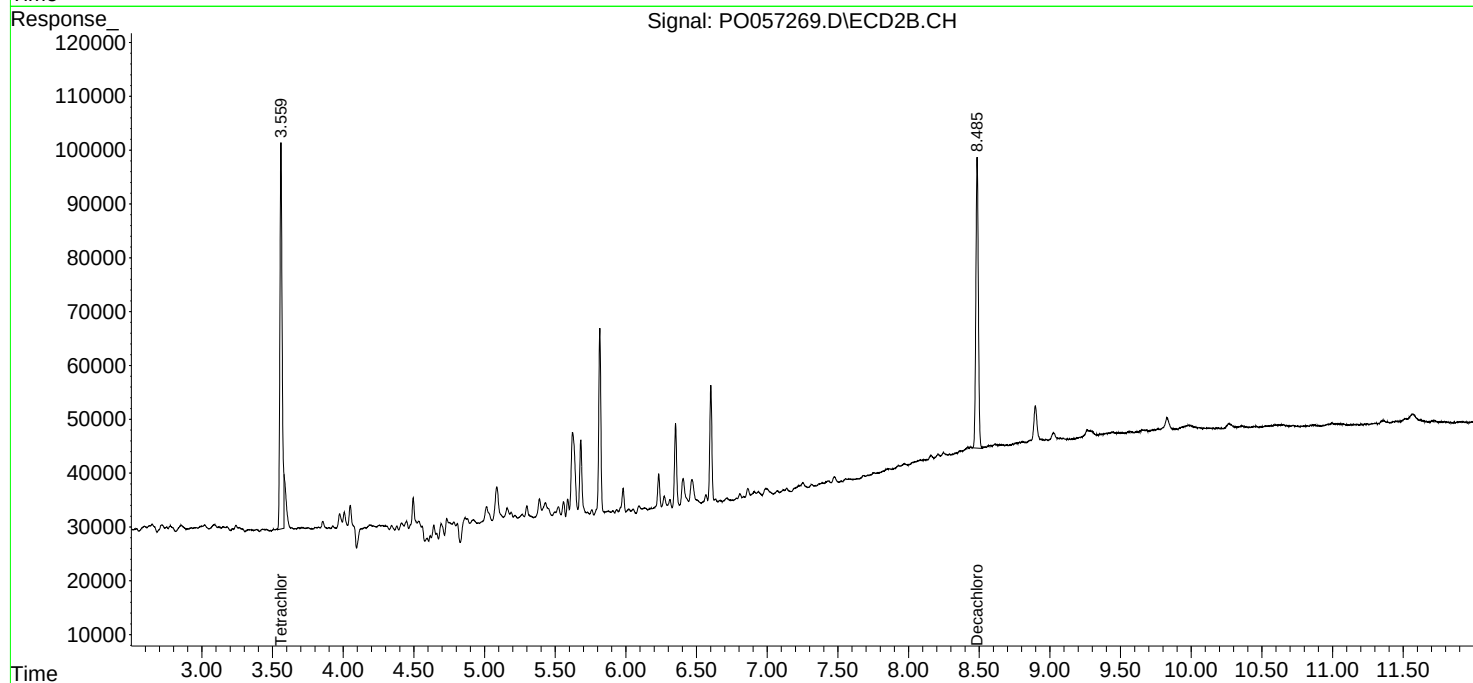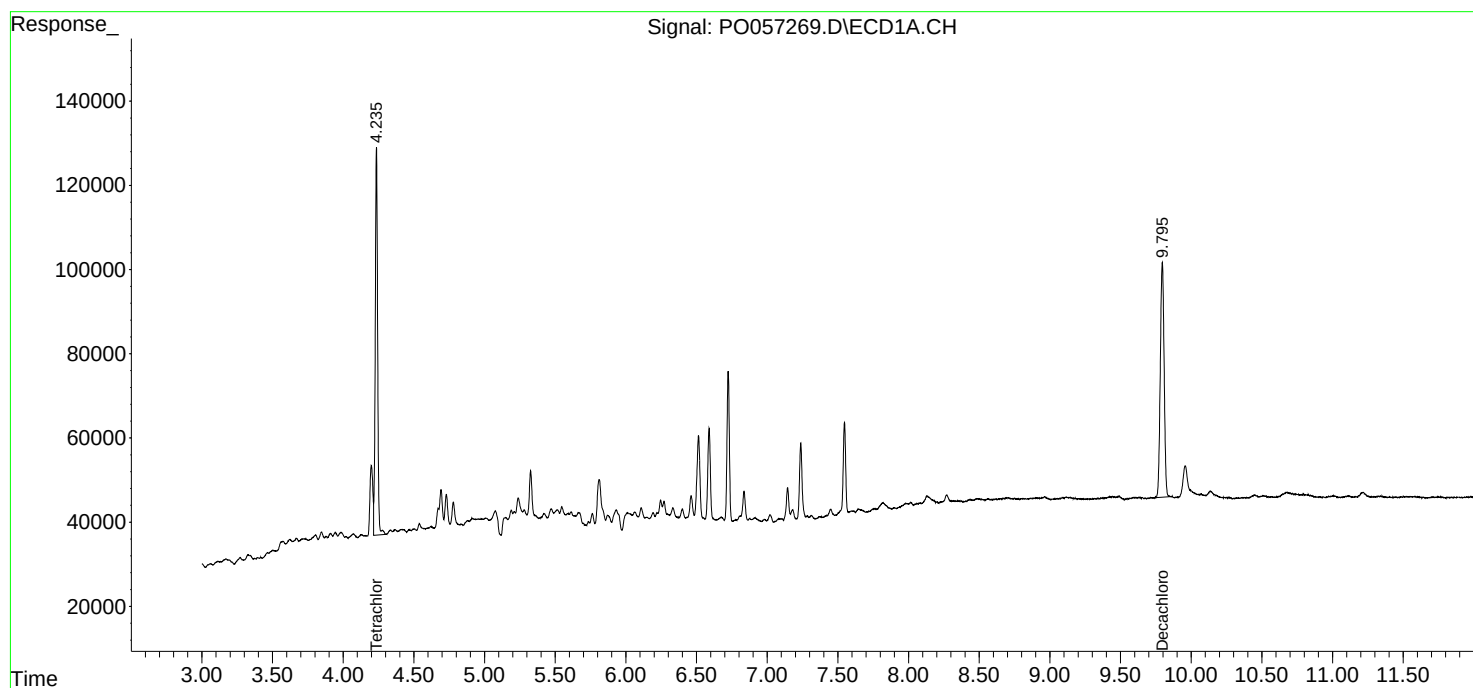

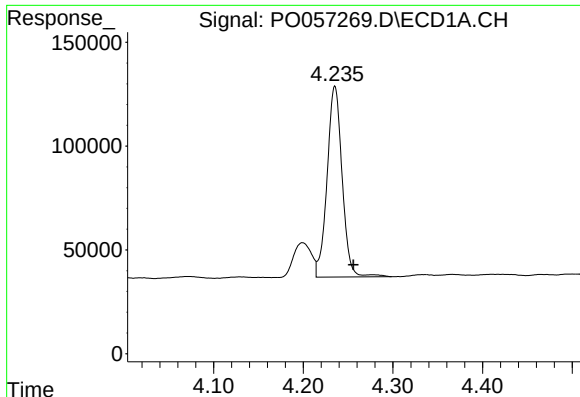


#1 Tetrachloro-m-xylene

R.T.: 4.235 min
Delta R.T.: -0.021 min
Response: 1071634
Conc: 27.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU-03-061719-A


Manual Integrations
APPROVED

Ankita
6/20/2019 11:57:58 AM

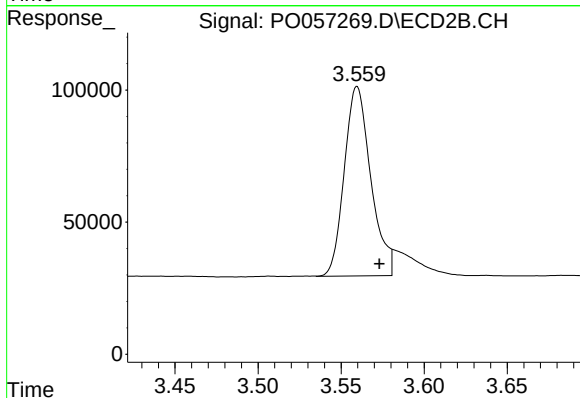


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: -0.014 min
Response: 794018
Conc: 24.08 ng/ml m

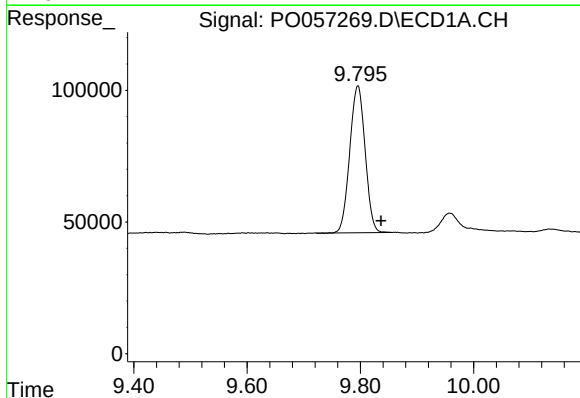

#2 Decachlorobiphenyl

R.T.: 9.795 min
Delta R.T.: -0.041 min
Response: 1049981
Conc: 21.39 ng/ml

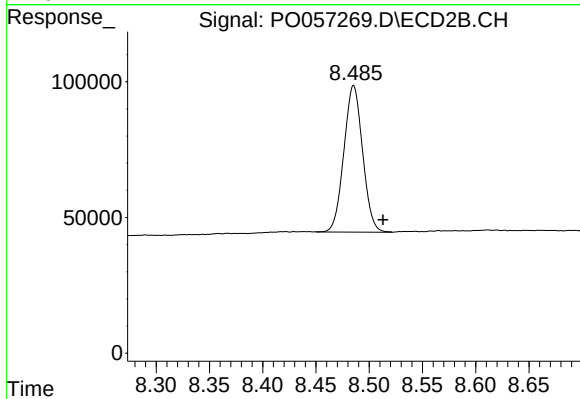

#2 Decachlorobiphenyl

R.T.: 8.485 min
Delta R.T.: -0.028 min
Response: 660578
Conc: 18.53 ng/ml m