

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061919\
 Data File : P0057276.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jun 2019 20:45
 Operator : SM/SJ
 Sample : K3157-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-01-061719-A

Manual Integrations
 APPROVED

Ankita
 6/20/2019 12:39:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 08:08:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.235	3.560	1383892	1113009	36.149m	33.750
2) SA Decachlor...	9.793	8.484	1137044	742773	23.165	20.831m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061919\
Data File : PO057276.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jun 2019 20:45
Operator : SM/SJ
Sample : K3157-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-01-061719-A


Manual Integrations
APPROVED

Ankita
6/20/2019 12:39:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 08:08:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

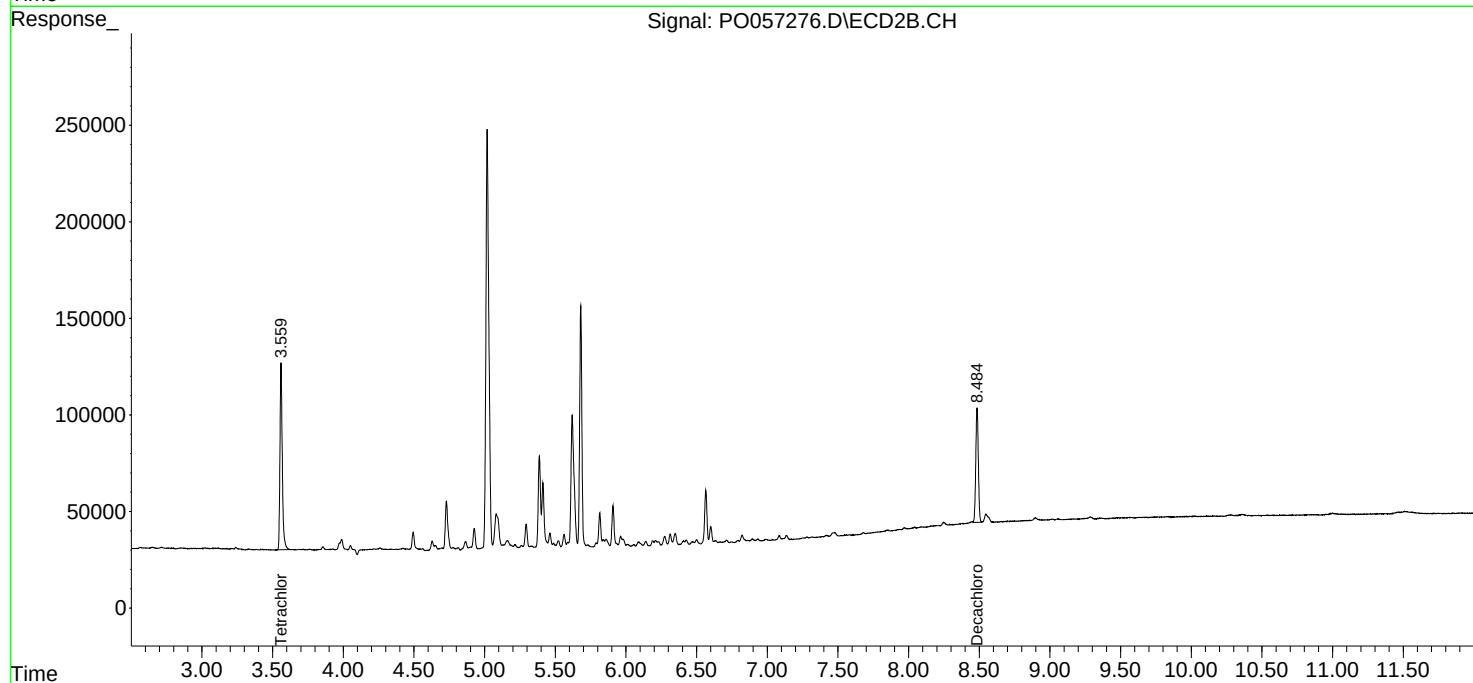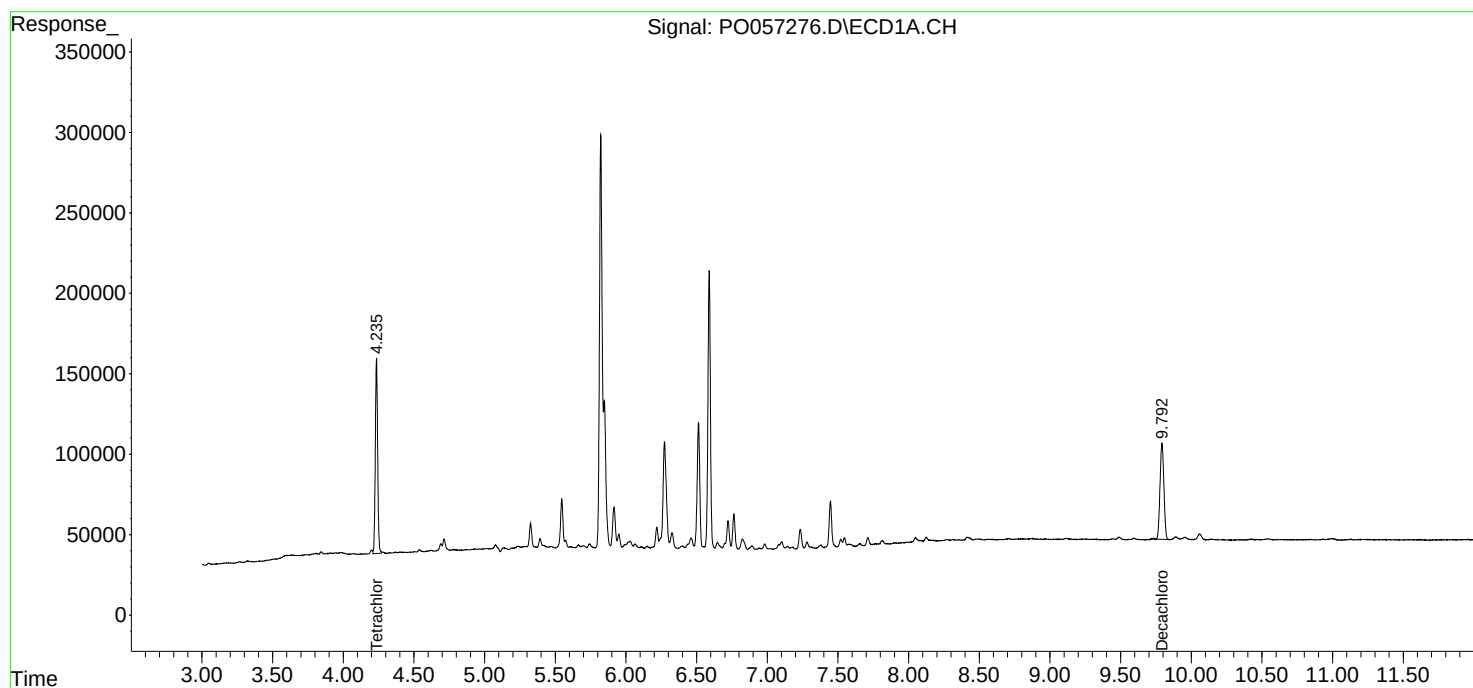

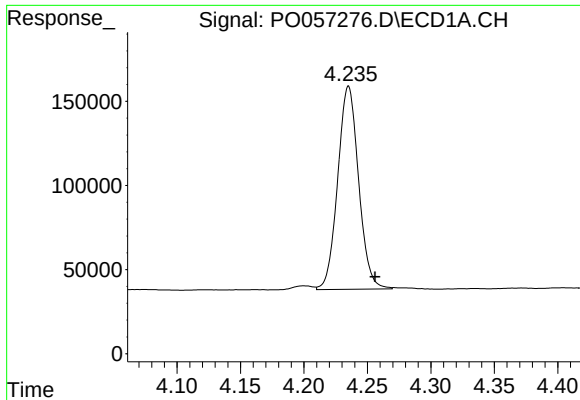


#1 Tetrachloro-m-xylene

R.T.: 4.235 min
Delta R.T.: -0.021 min
Response: 1383892
Conc: 36.15 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-01-061719-A


Manual Integrations
APPROVED

Ankita
6/20/2019 12:39:22 PM

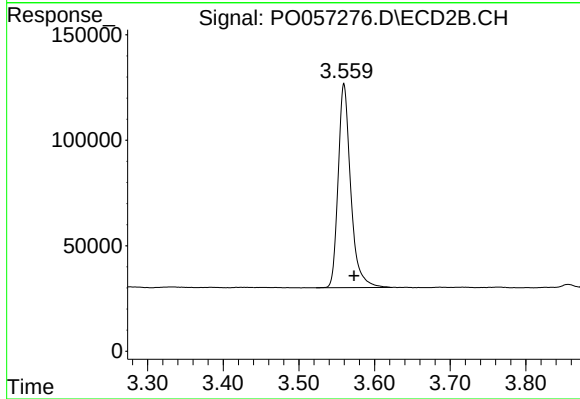


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: -0.013 min
Response: 1113009
Conc: 33.75 ng/ml

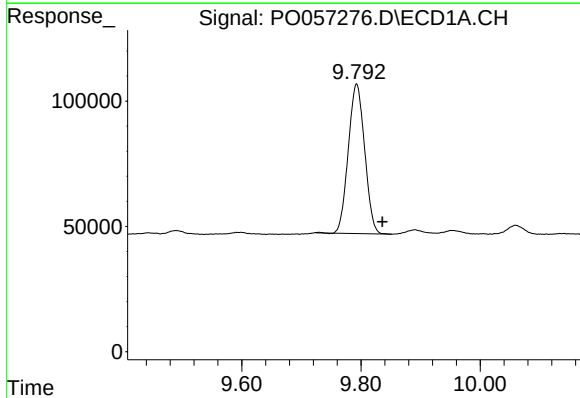

#2 Decachlorobiphenyl

R.T.: 9.793 min
Delta R.T.: -0.044 min
Response: 1137044
Conc: 23.17 ng/ml

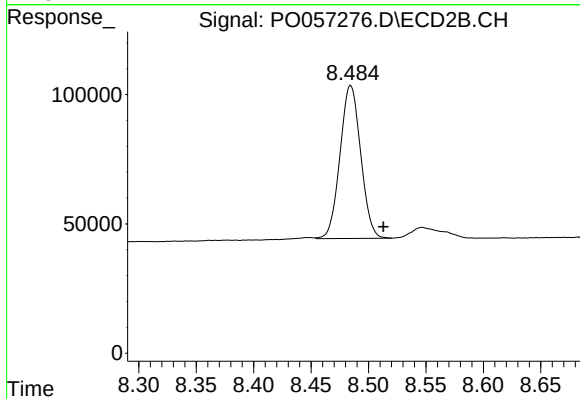

#2 Decachlorobiphenyl

R.T.: 8.484 min
Delta R.T.: -0.029 min
Response: 742773
Conc: 20.83 ng/ml m