

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061919\
 Data File : P0057290.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2019 00:42
 Operator : SM/SJ
 Sample : K3419-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-A

Manual Integrations
 APPROVED

Ankita
 6/20/2019 12:40:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 08:14:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.235	3.559	1220931	979066	31.892	29.688
2) SA Decachlor...	9.793	8.484	1090865	765661	22.225	21.473m
Target Compounds						
31) L7 AR-1260-1	6.982	6.089	1178328	898704	459.176	449.266
32) L7 AR-1260-2	7.237	6.276	1308332	1227149	432.626m	497.837
33) L7 AR-1260-3	7.593	6.427	858806	995094	356.491	443.599
34) L7 AR-1260-4	7.818	6.894	937907	723220	358.088	388.615m
35) L7 AR-1260-5	8.126	7.136	1784551	1792385	373.174	415.642

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061919\
Data File : P0057290.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2019 00:42
Operator : SM/SJ
Sample : K3419-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-A


Manual Integrations
APPROVED

Ankita
6/20/2019 12:40:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 08:14:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

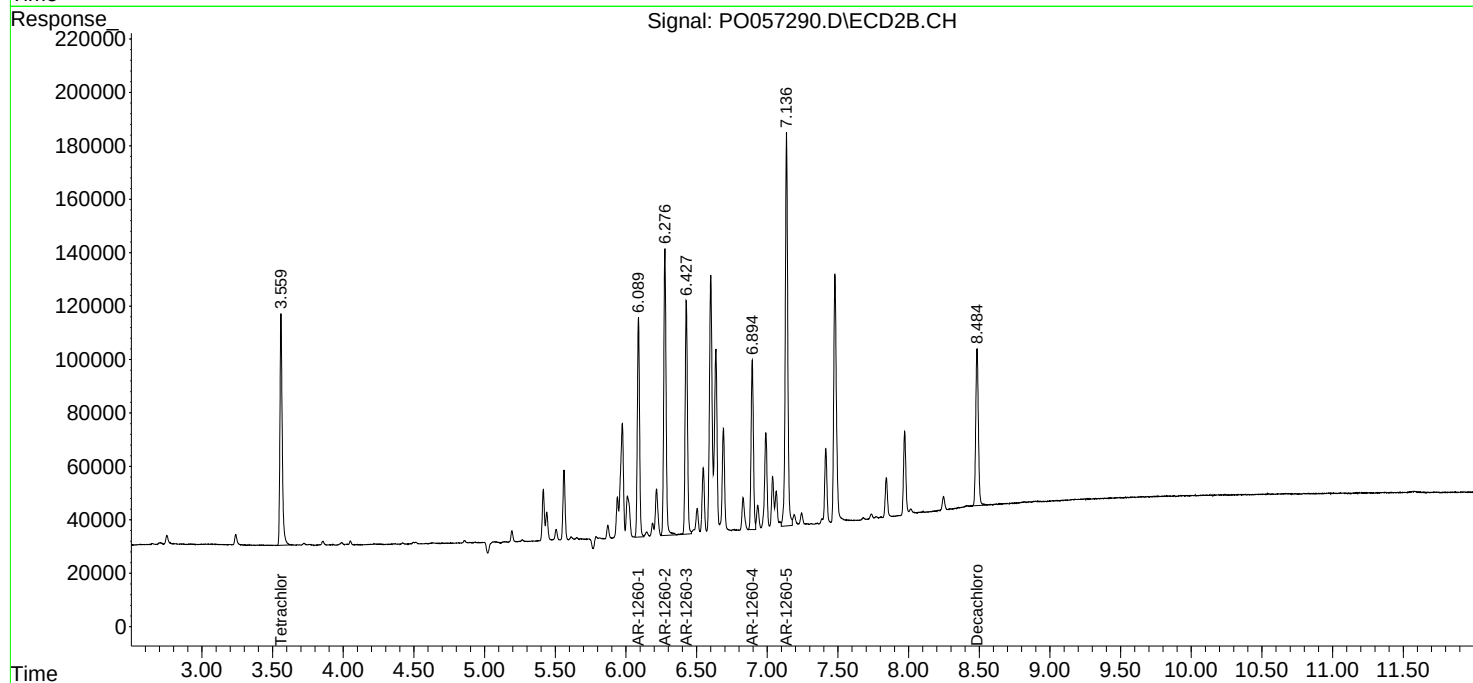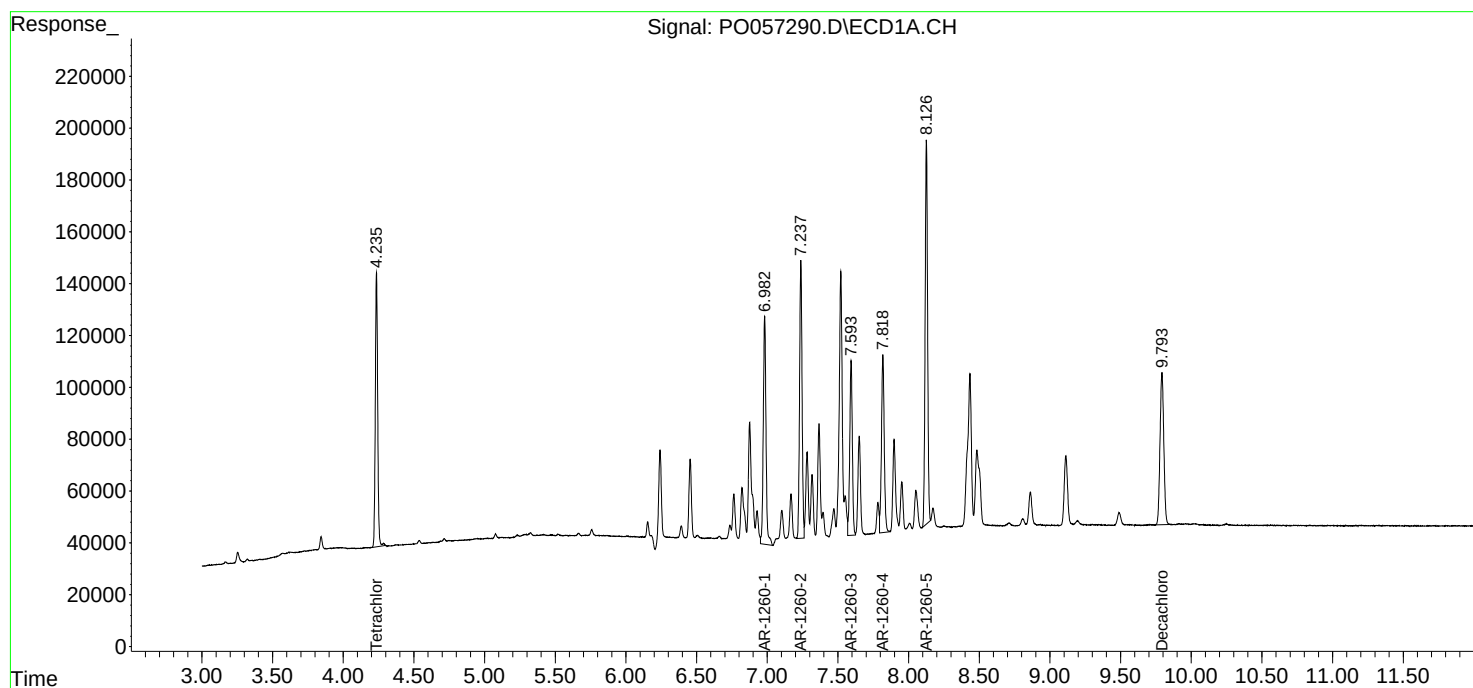

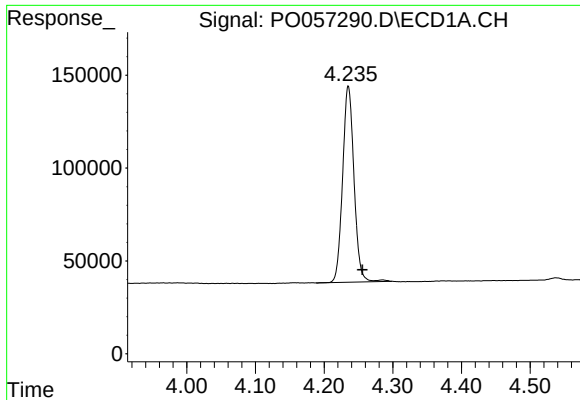


#1 Tetrachloro-m-xylene

R.T.: 4.235 min
Delta R.T.: -0.021 min
Response: 1220931
Conc: 31.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-A


Manual Integrations
APPROVED

Ankita
6/20/2019 12:40:13 PM

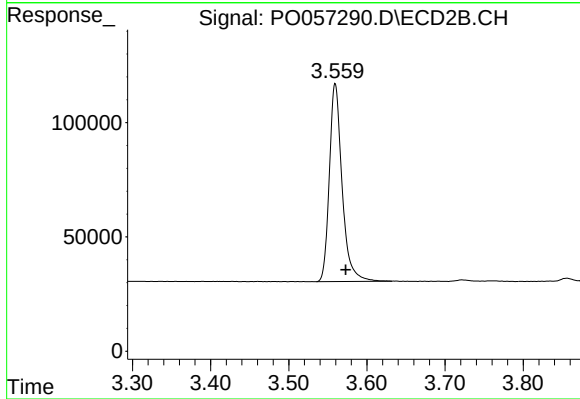


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: -0.014 min
Response: 979066
Conc: 29.69 ng/ml

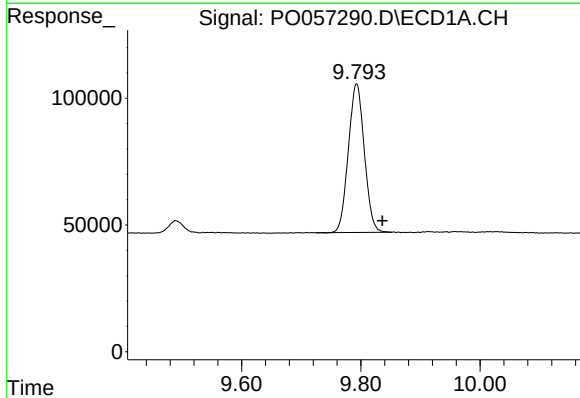


#2 Decachlorobiphenyl

R.T.: 9.793 min
Delta R.T.: -0.043 min
Response: 1090865
Conc: 22.22 ng/ml

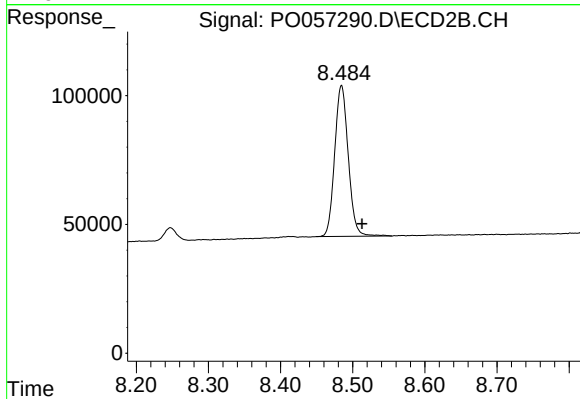

#2 Decachlorobiphenyl

R.T.: 8.484 min
Delta R.T.: -0.029 min
Response: 765661
Conc: 21.47 ng/ml m

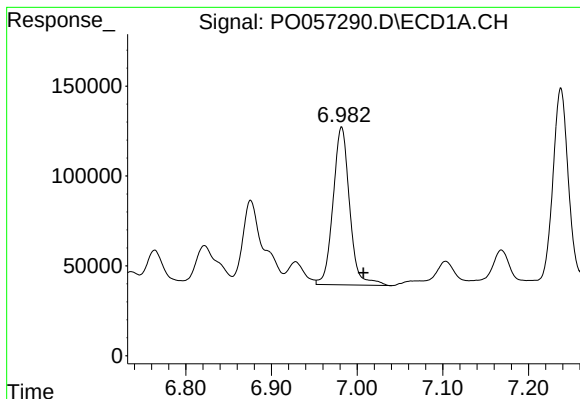


#31 AR-1260-1

R.T.: 6.982 min
Delta R.T.: -0.026 min
Response: 1178328
Conc: 459.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-A


Manual Integrations
APPROVED

Ankita
6/20/2019 12:40:13 PM

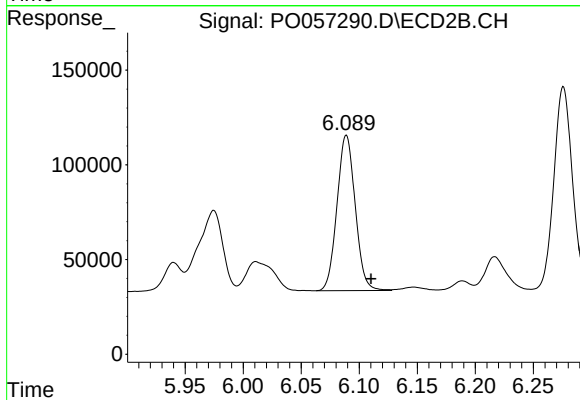


#31 AR-1260-1

R.T.: 6.089 min
Delta R.T.: -0.021 min
Response: 898704
Conc: 449.27 ng/ml

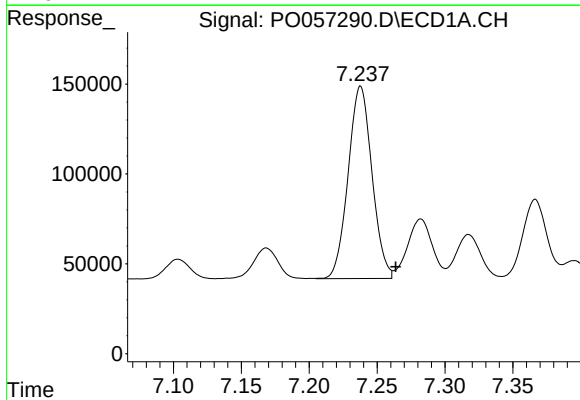


#32 AR-1260-2

R.T.: 7.237 min
Delta R.T.: -0.026 min
Response: 1308332
Conc: 432.63 ng/ml m

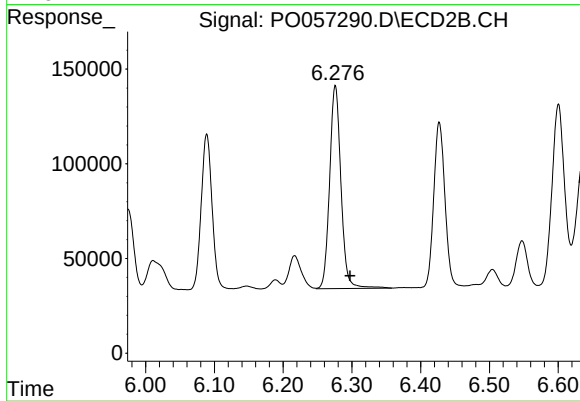

#32 AR-1260-2

R.T.: 6.276 min
Delta R.T.: -0.022 min
Response: 1227149
Conc: 497.84 ng/ml

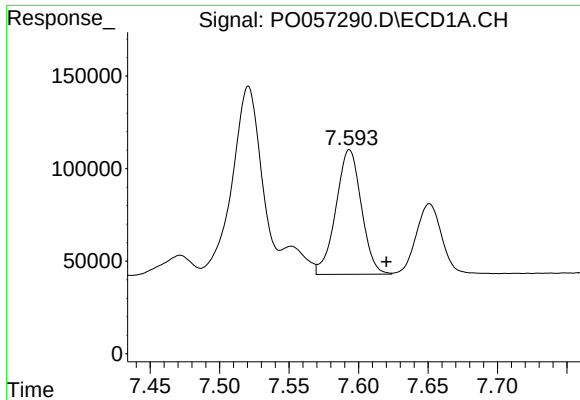


#33 AR-1260-3

R.T.: 7.593 min
Delta R.T.: -0.027 min
Response: 858806
Conc: 356.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-A


Manual Integrations
APPROVED

Ankita
6/20/2019 12:40:13 PM

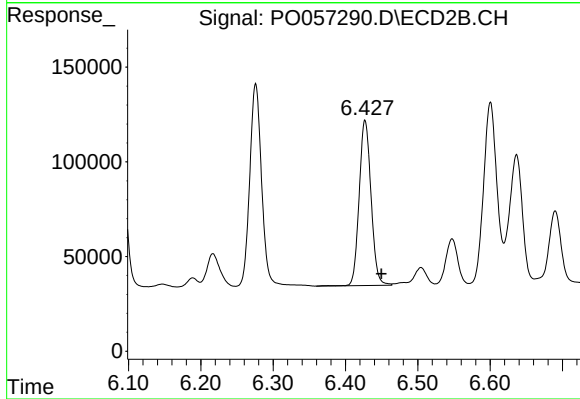


#33 AR-1260-3

R.T.: 6.427 min
Delta R.T.: -0.023 min
Response: 995094
Conc: 443.60 ng/ml

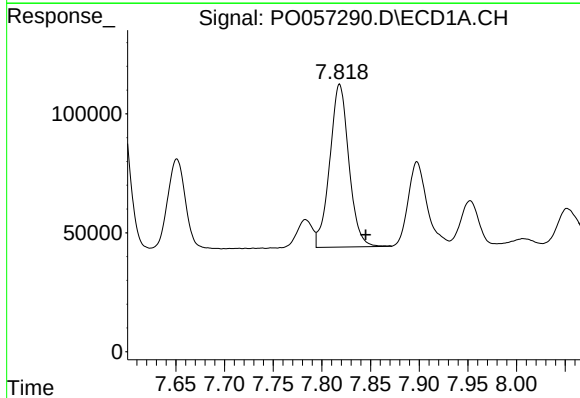


#34 AR-1260-4

R.T.: 7.818 min
Delta R.T.: -0.027 min
Response: 937907
Conc: 358.09 ng/ml

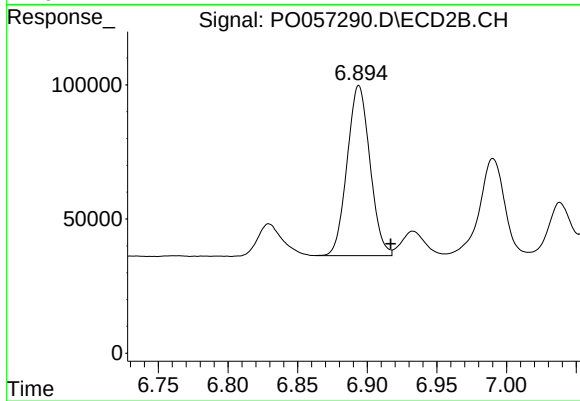

#34 AR-1260-4

R.T.: 6.894 min
Delta R.T.: -0.023 min
Response: 723220
Conc: 388.61 ng/ml m

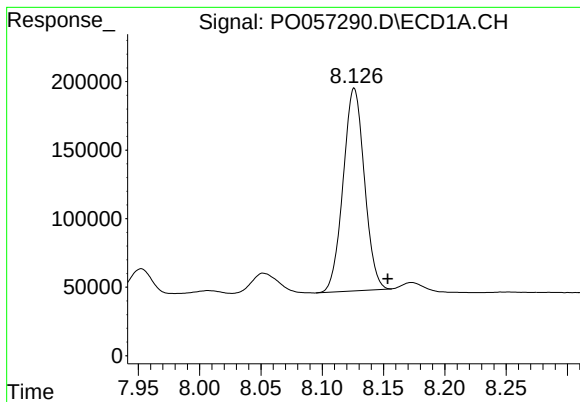


#35 AR-1260-5

R.T.: 8.126 min
Delta R.T.: -0.027 min
Response: 1784551
Conc: 373.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-A

Manual Integrations
APPROVED

Ankita
6/20/2019 12:40:13 PM

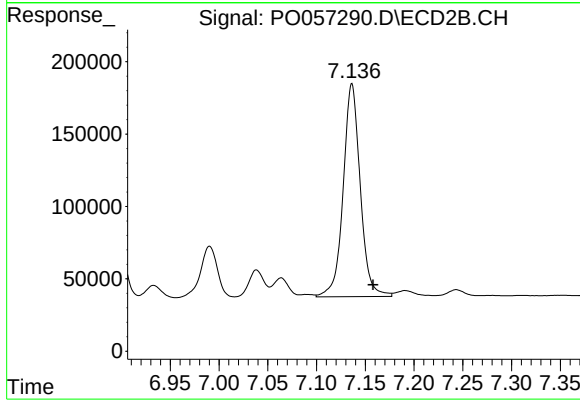

#35 AR-1260-5

R.T.: 7.136 min
Delta R.T.: -0.022 min
Response: 1792385
Conc: 415.64 ng/ml