

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061919\
 Data File : P0057291.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2019 00:59
 Operator : SM/SJ
 Sample : K3417-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONTROL-HOUSE-BRICKS

Manual Integrations
 APPROVED

Ankita
 6/20/2019 12:40:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 08:14:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.234	3.559	1061609	834501	27.730m	25.304
2)	SA Decachlor...	9.791	8.483	966434	671334	19.689	18.828m
Target Compounds							
26)	L6 AR-1254-1	6.243	5.409	485196	148030	176.260m	55.972m#
27)	L6 AR-1254-2	6.458	5.561	467170	114675	120.278	53.194m#
28)	L6 AR-1254-3	6.821	5.962	237389	278341	57.571m	76.027 #
29)	L6 AR-1254-4	7.105	6.189	184024	141499	61.141m	64.408
30)	L6 AR-1254-5	7.545	6.600	149368	333381	39.666m	105.160m#
31)	L7 AR-1260-1	6.973	6.093	165208	334039	64.379m	166.988 #
32)	L7 AR-1260-2	7.237	6.274	278503	304984	92.093m	123.728m#
33)	L7 AR-1260-3	7.592	6.427	291684	158568	121.078m	70.687 #
34)	L7 AR-1260-4	7.816	6.892	222445	153298	84.928m	82.373
35)	L7 AR-1260-5	8.124	7.137	302846	472443	63.329m	109.556 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061919\
Data File : P0057291.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2019 00:59
Operator : SM/SJ
Sample : K3417-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS


Manual Integrations
APPROVED

Ankita
6/20/2019 12:40:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 08:14:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

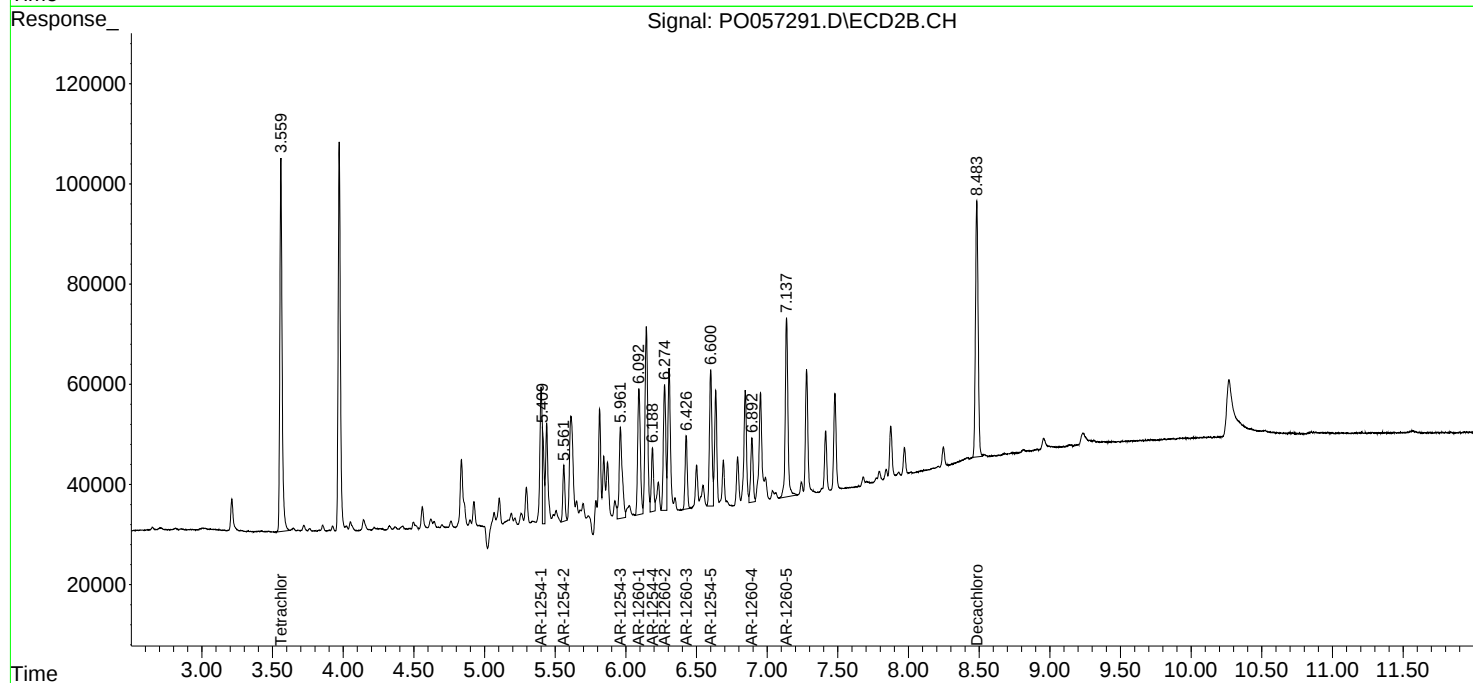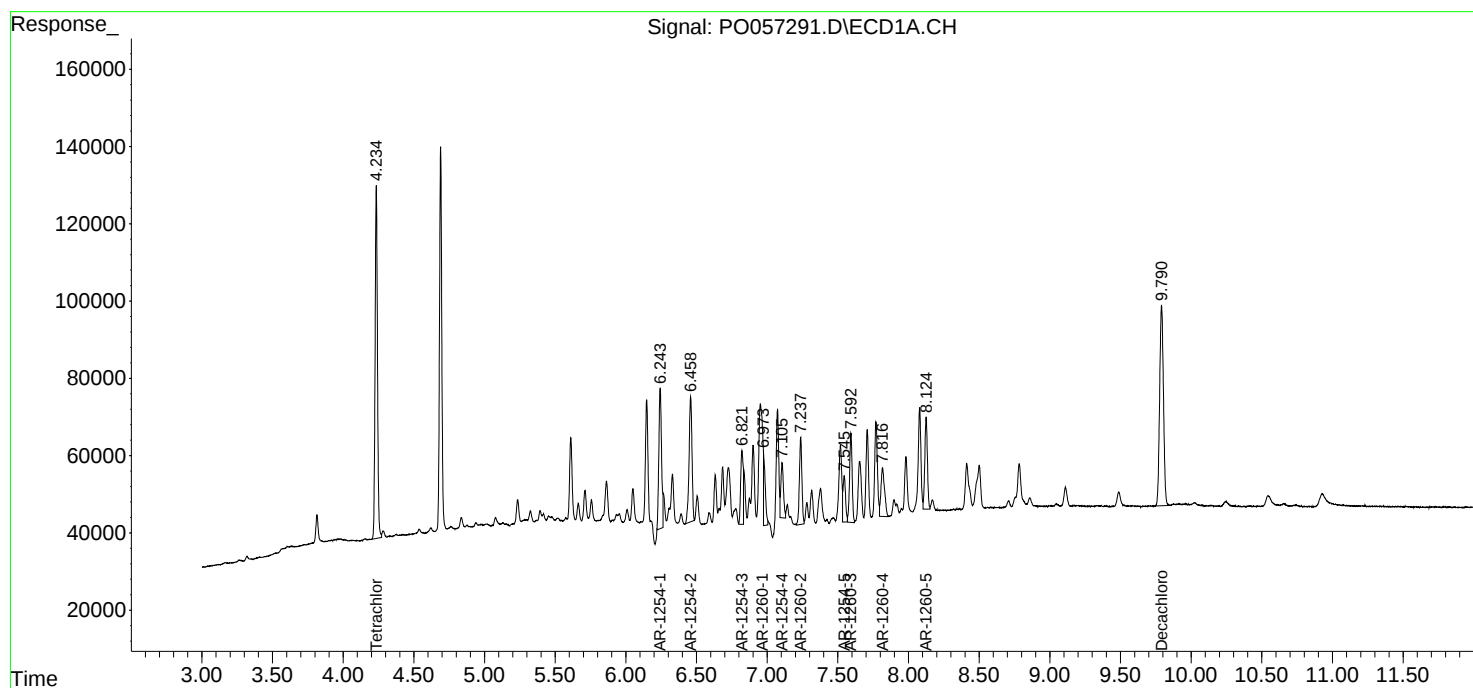

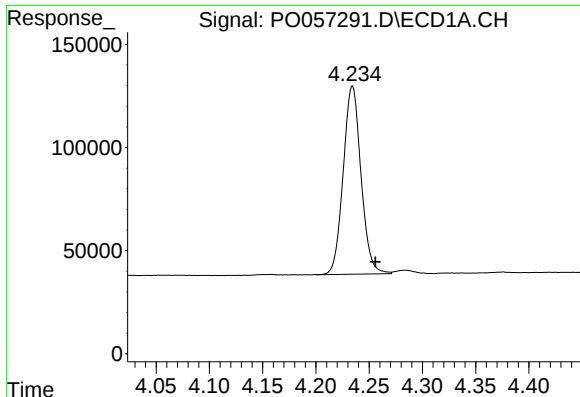


#1 Tetrachloro-m-xylene

R.T.: 4.234 min
Delta R.T.: -0.022 min
Response: 1061609
Conc: 27.73 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS


Manual Integrations
APPROVED

Ankita
6/20/2019 12:40:16 PM

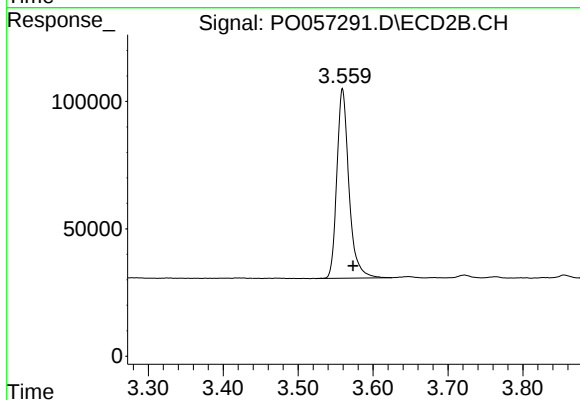


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: -0.014 min
Response: 834501
Conc: 25.30 ng/ml

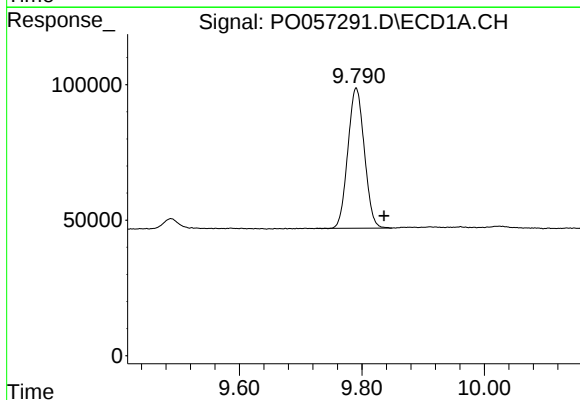


#2 Decachlorobiphenyl

R.T.: 9.791 min
Delta R.T.: -0.046 min
Response: 966434
Conc: 19.69 ng/ml

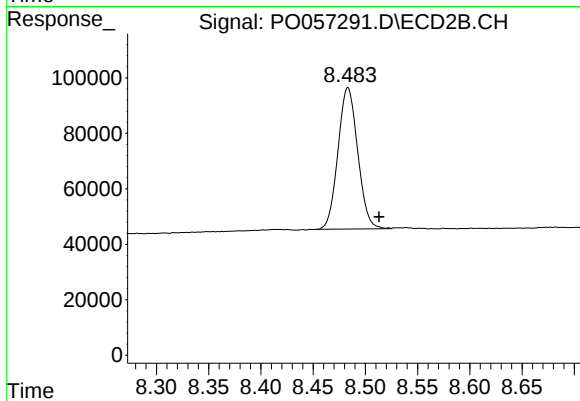

#2 Decachlorobiphenyl

R.T.: 8.483 min
Delta R.T.: -0.030 min
Response: 671334
Conc: 18.83 ng/ml m

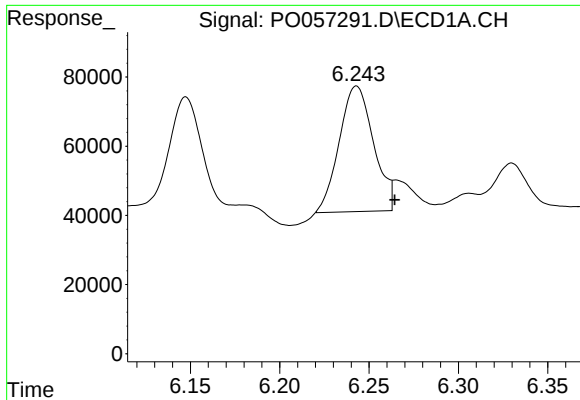


#26 AR-1254-1

R.T.: 6.243 min
Delta R.T.: -0.022 min
Response: 485196
Conc: 176.26 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS


Manual Integrations
APPROVED

Ankita
6/20/2019 12:40:16 PM

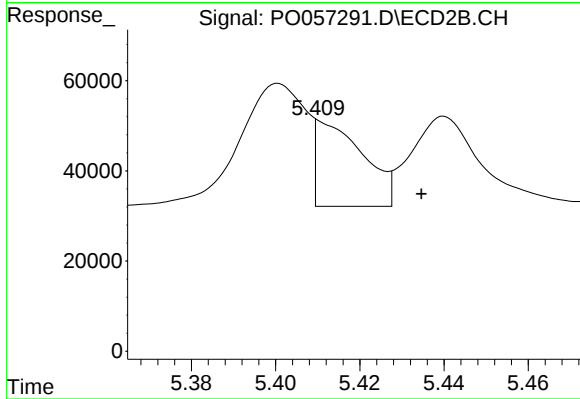


#26 AR-1254-1

R.T.: 5.409 min
Delta R.T.: -0.025 min
Response: 148030
Conc: 55.97 ng/ml m

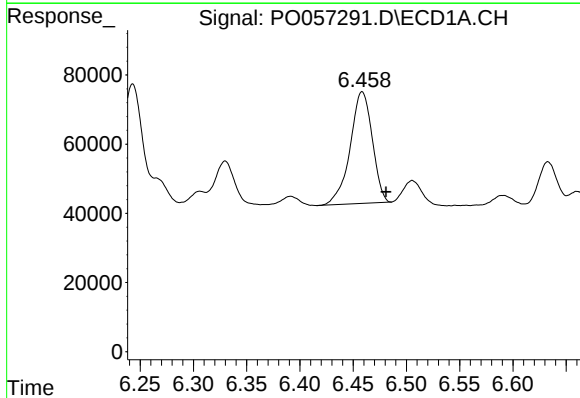


#27 AR-1254-2

R.T.: 6.458 min
Delta R.T.: -0.023 min
Response: 467170
Conc: 120.28 ng/ml

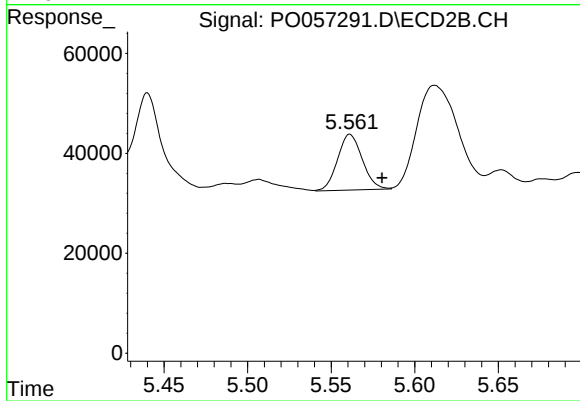

#27 AR-1254-2

R.T.: 5.561 min
Delta R.T.: -0.020 min
Response: 114675
Conc: 53.19 ng/ml m

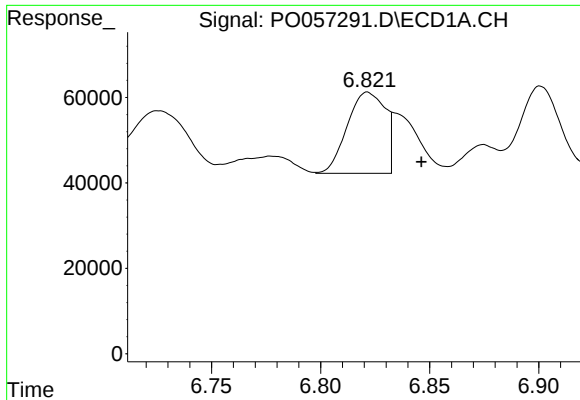


#28 AR-1254-3

R.T.: 6.821 min
Delta R.T.: -0.025 min
Response: 237389
Conc: 57.57 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS


Manual Integrations
APPROVED

Ankita
6/20/2019 12:40:16 PM

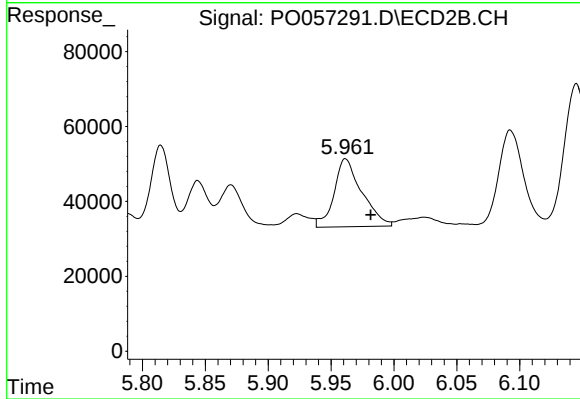


#28 AR-1254-3

R.T.: 5.962 min
Delta R.T.: -0.020 min
Response: 278341
Conc: 76.03 ng/ml

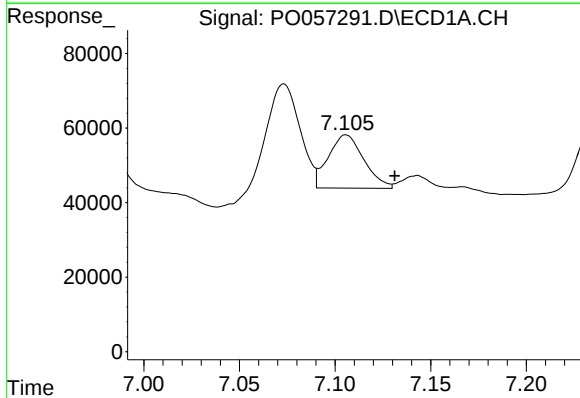


#29 AR-1254-4

R.T.: 7.105 min
Delta R.T.: -0.026 min
Response: 184024
Conc: 61.14 ng/ml m

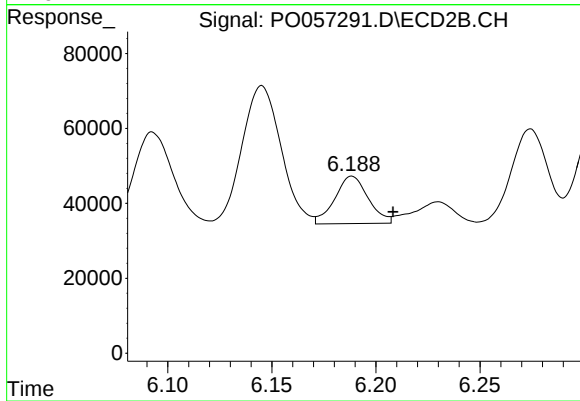

#29 AR-1254-4

R.T.: 6.189 min
Delta R.T.: -0.020 min
Response: 141499
Conc: 64.41 ng/ml

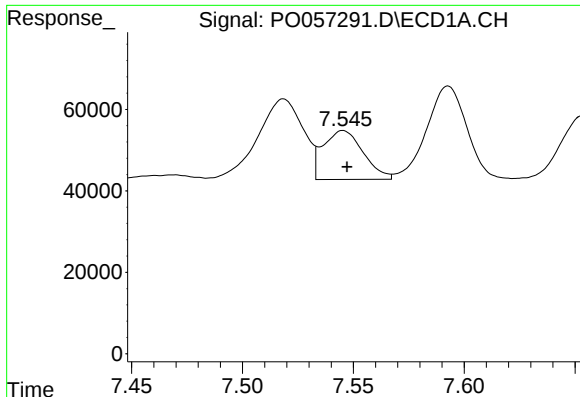


#30 AR-1254-5

R.T.: 7.545 min
Delta R.T.: -0.002 min
Response: 149368
Conc: 39.67 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS


Manual Integrations
APPROVED

Ankita
6/20/2019 12:40:16 PM

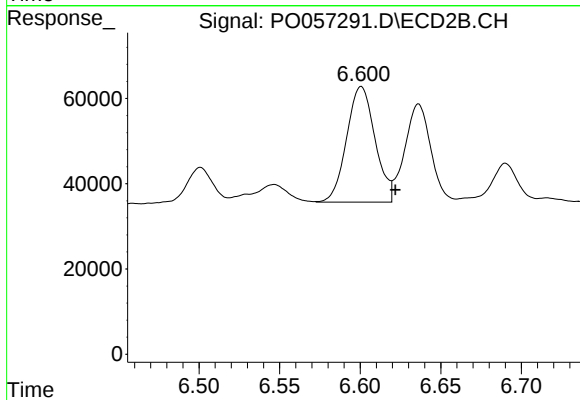


#30 AR-1254-5

R.T.: 6.600 min
Delta R.T.: -0.022 min
Response: 333381
Conc: 105.16 ng/ml m

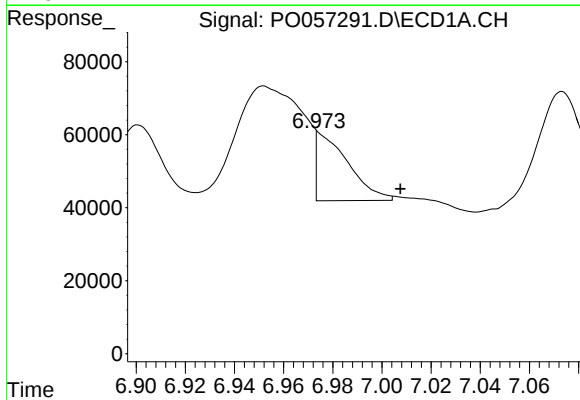


#31 AR-1260-1

R.T.: 6.973 min
Delta R.T.: -0.034 min
Response: 165208
Conc: 64.38 ng/ml m

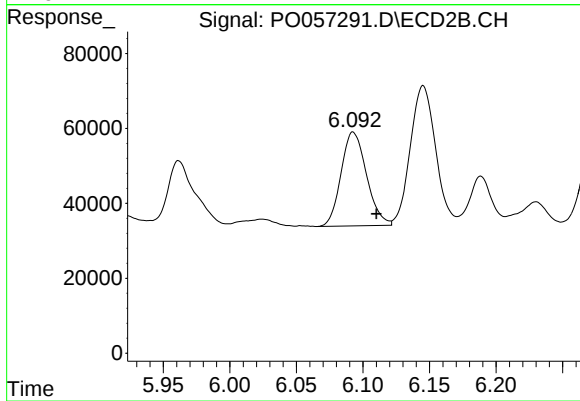

#31 AR-1260-1

R.T.: 6.093 min
Delta R.T.: -0.018 min
Response: 334039
Conc: 166.99 ng/ml

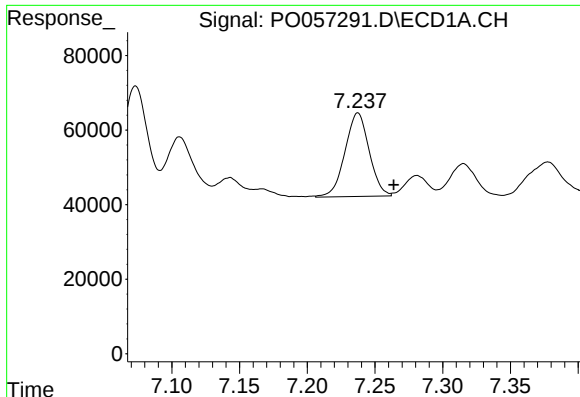


#32 AR-1260-2

R.T.: 7.237 min
Delta R.T.: -0.027 min
Response: 278503
Conc: 92.09 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS


Manual Integrations
APPROVED

Ankita
6/20/2019 12:40:16 PM

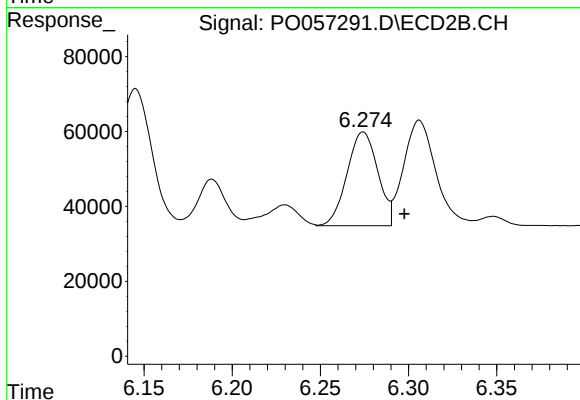


#32 AR-1260-2

R.T.: 6.274 min
Delta R.T.: -0.024 min
Response: 304984
Conc: 123.73 ng/ml m

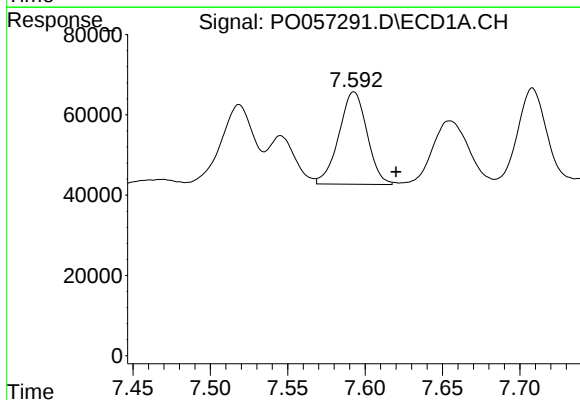


#33 AR-1260-3

R.T.: 7.592 min
Delta R.T.: -0.028 min
Response: 291684
Conc: 121.08 ng/ml m

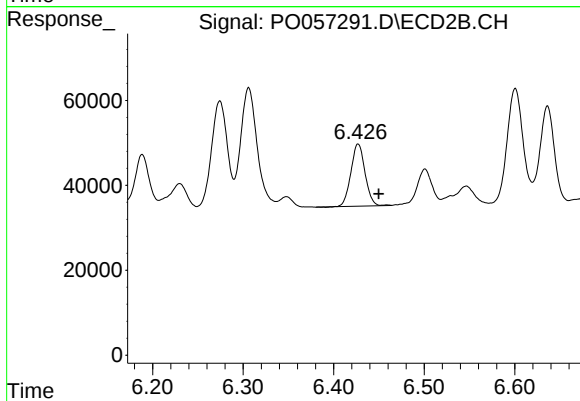

#33 AR-1260-3

R.T.: 6.427 min
Delta R.T.: -0.023 min
Response: 158568
Conc: 70.69 ng/ml

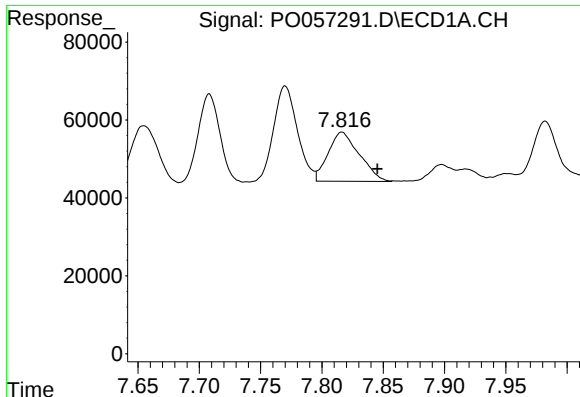


#34 AR-1260-4

R.T.: 7.816 min
Delta R.T.: -0.029 min
Response: 222445
Conc: 84.93 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS


Manual Integrations
APPROVED

Ankita
6/20/2019 12:40:16 PM

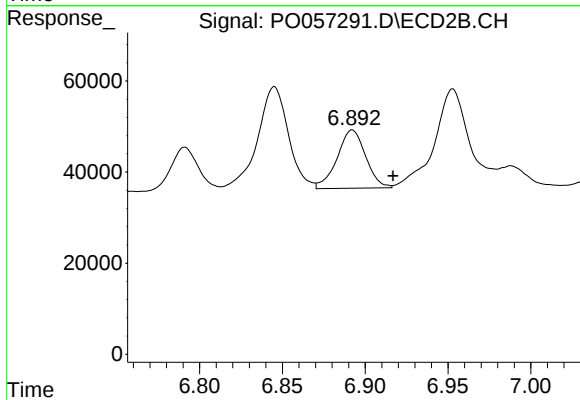


#34 AR-1260-4

R.T.: 6.892 min
Delta R.T.: -0.025 min
Response: 153298
Conc: 82.37 ng/ml

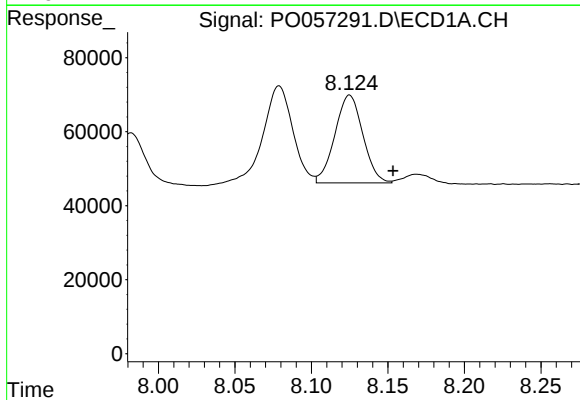

#35 AR-1260-5

R.T.: 8.124 min
Delta R.T.: -0.029 min
Response: 302846
Conc: 63.33 ng/ml m

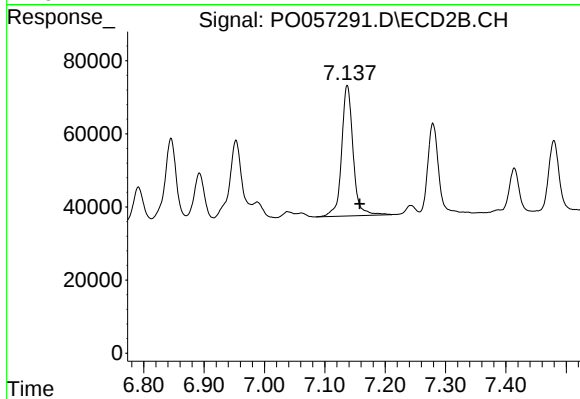

#35 AR-1260-5

R.T.: 7.137 min
Delta R.T.: -0.021 min
Response: 472443
Conc: 109.56 ng/ml