

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061920\
 Data File : P0069053.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jun 2020 13:40
 Operator : DD\AJ
 Sample : L3055-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AMITY-ST-ENTRANCE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 14:29:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 19 05:15:02 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.405	3.564	707609	799007	23.919	20.759
2) SA Decachlor...	10.069	8.771	929922	1029593	19.579	18.914
Target Compounds						
28) L6 AR-1254-3	0.000	6.191	0	170483	N.D.	49.442 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061920\
Data File : P0069053.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jun 2020 13:40
Operator : DD\AJ
Sample : L3055-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AMITY-ST-ENTRANCE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 14:29:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 19 05:15:02 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

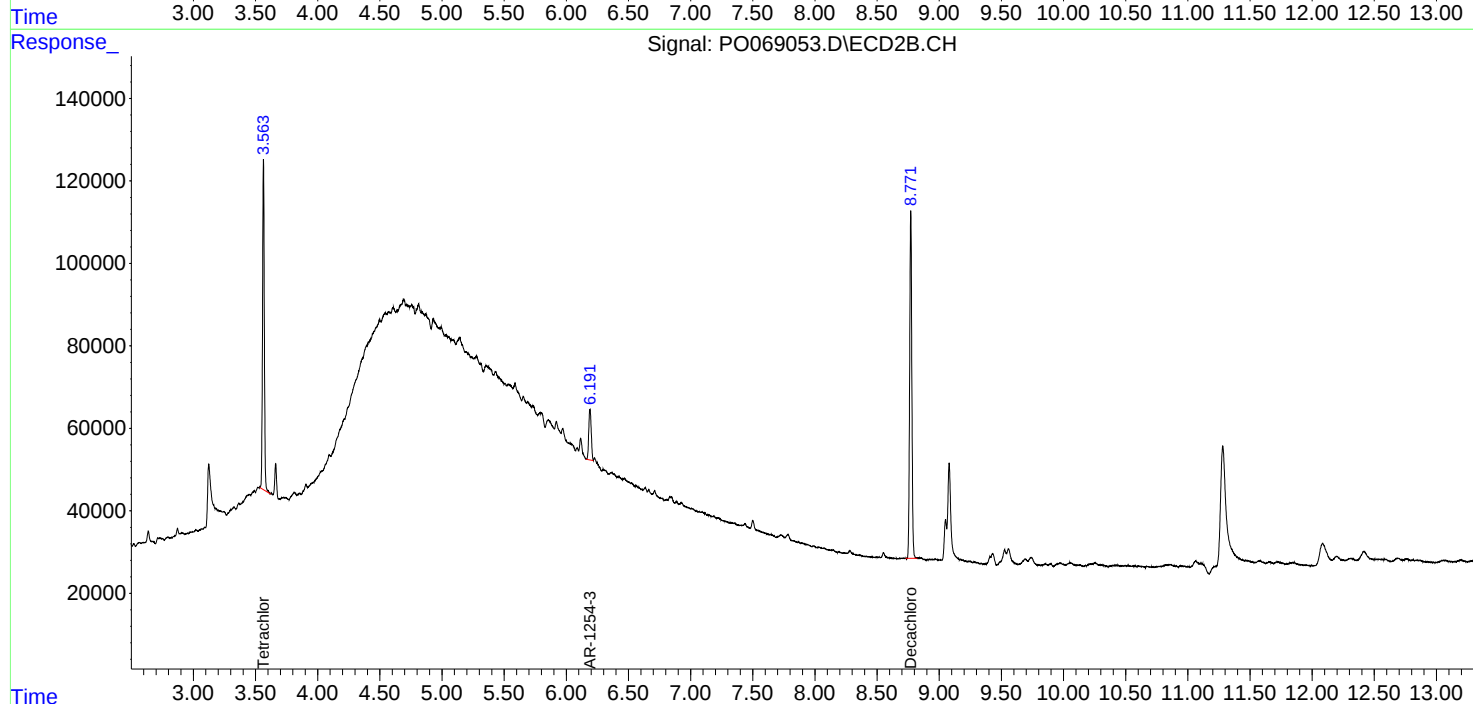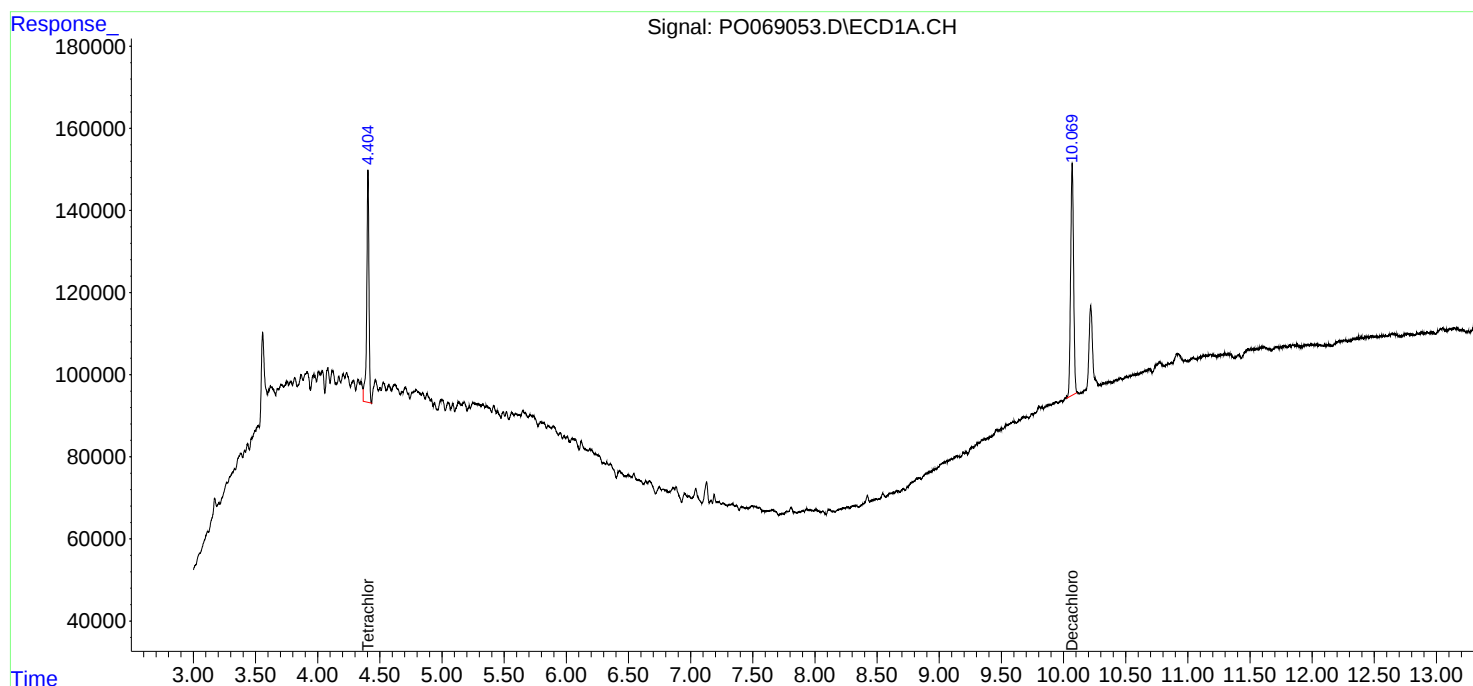


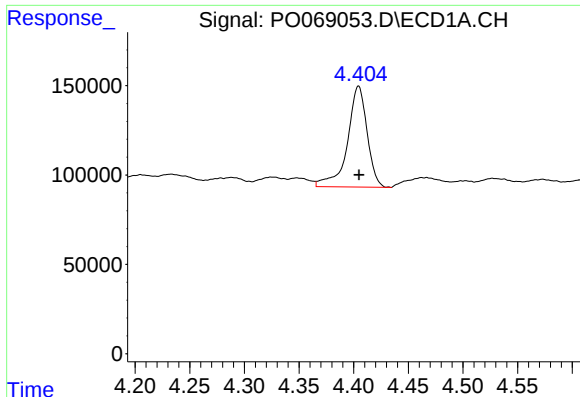

#1 Tetrachloro-m-xylene


R.T.: 4.405 min
Delta R.T.: 0.000 min
Response: 707609
Conc: 23.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
AMITY-ST-ENTRANCE

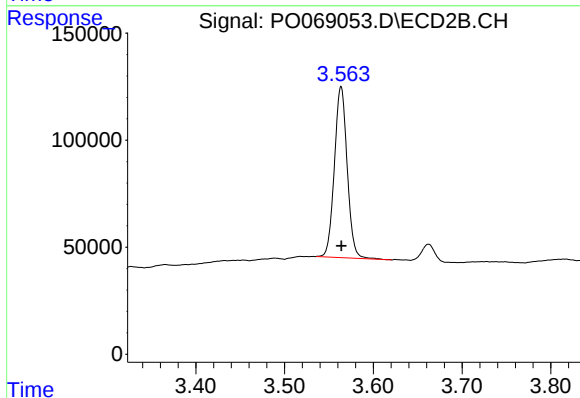


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 799007
Conc: 20.76 ng/ml

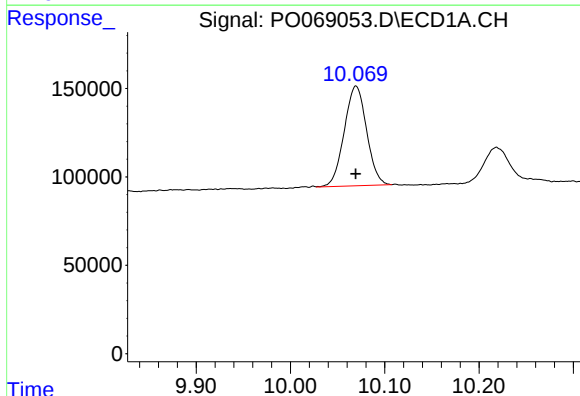


#2 Decachlorobiphenyl

R.T.: 10.069 min
Delta R.T.: 0.000 min
Response: 929922
Conc: 19.58 ng/ml

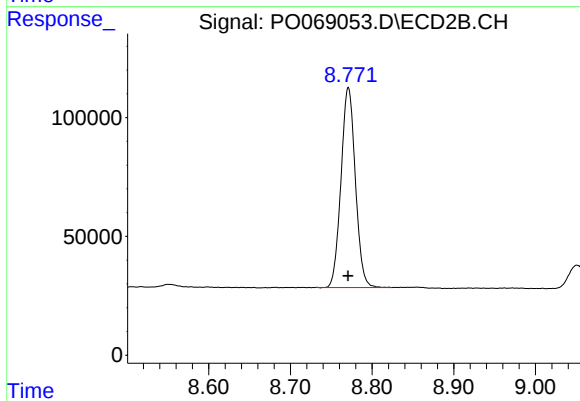

#2 Decachlorobiphenyl


R.T.: 8.771 min
Delta R.T.: 0.000 min
Response: 1029593
Conc: 18.91 ng/ml

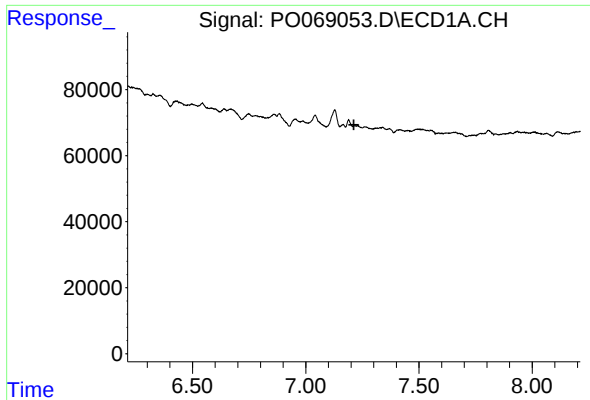

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 7.213 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
AMITY-ST-ENTRANCE

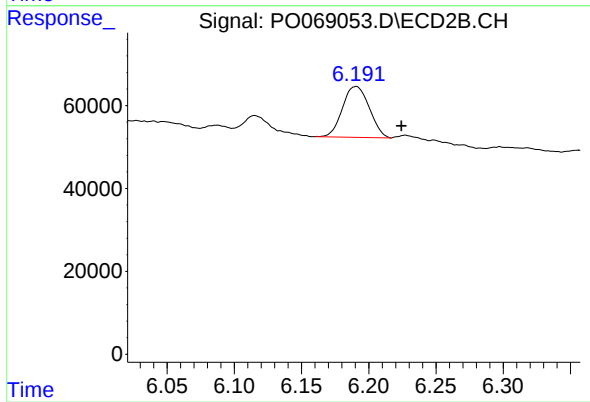

#28 AR-1254-3

R.T.: 6.191 min
Delta R.T.: -0.033 min
Response: 170483
Conc: 49.44 ng/ml