

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061920\
 Data File : P0069067.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jun 2020 17:40
 Operator : DD\AJ
 Sample : L3051-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SLUDGE-BOX

Manual Integrations
 APPROVED

Sohil
 6/22/2020 4:27:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 00:14:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 19 05:15:02 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.405	3.565	552184	734552	18.665	19.085
2) SA Decachlor...	10.070	8.771	868308	1082023	18.282m	19.877

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061920\
Data File : P0069067.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jun 2020 17:40
Operator : DD\AJ
Sample : L3051-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SLUDGE-BOX


Manual Integrations
APPROVED

Sohil
6/22/2020 4:27:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 00:14:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 19 05:15:02 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

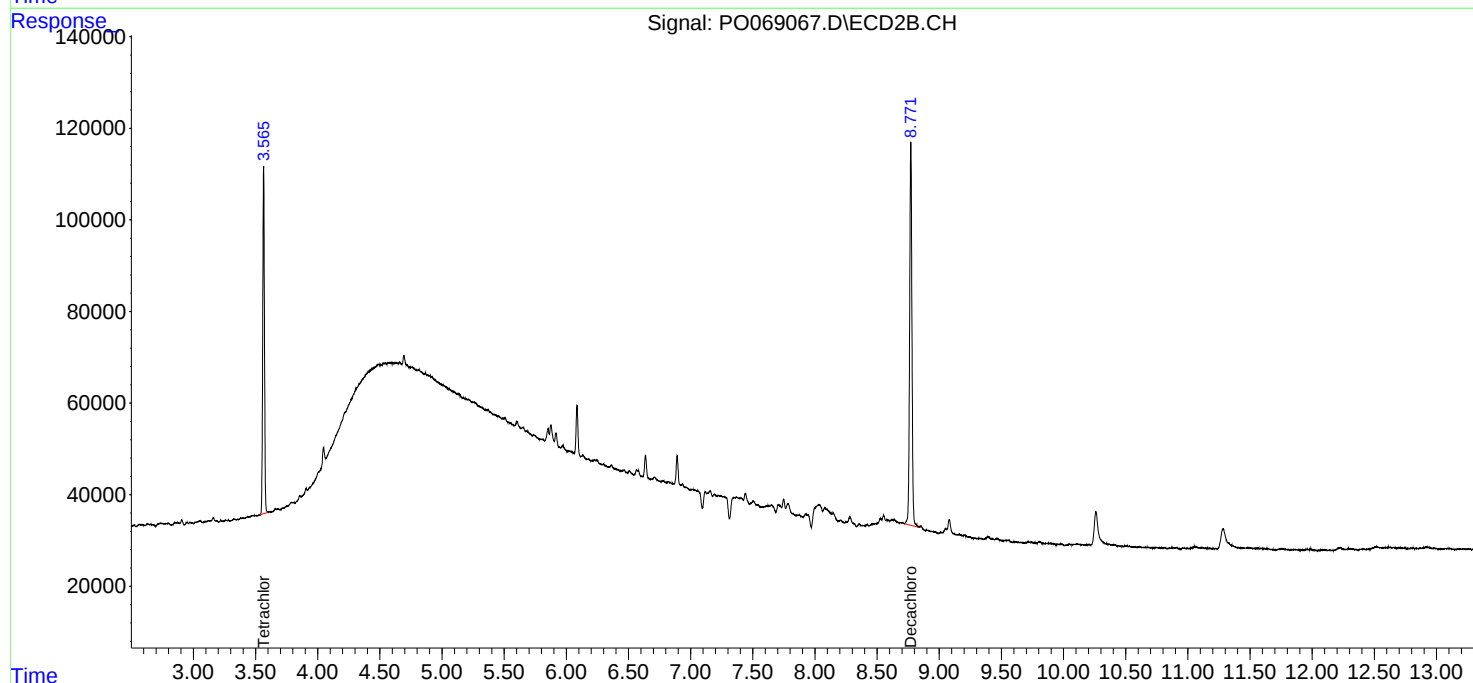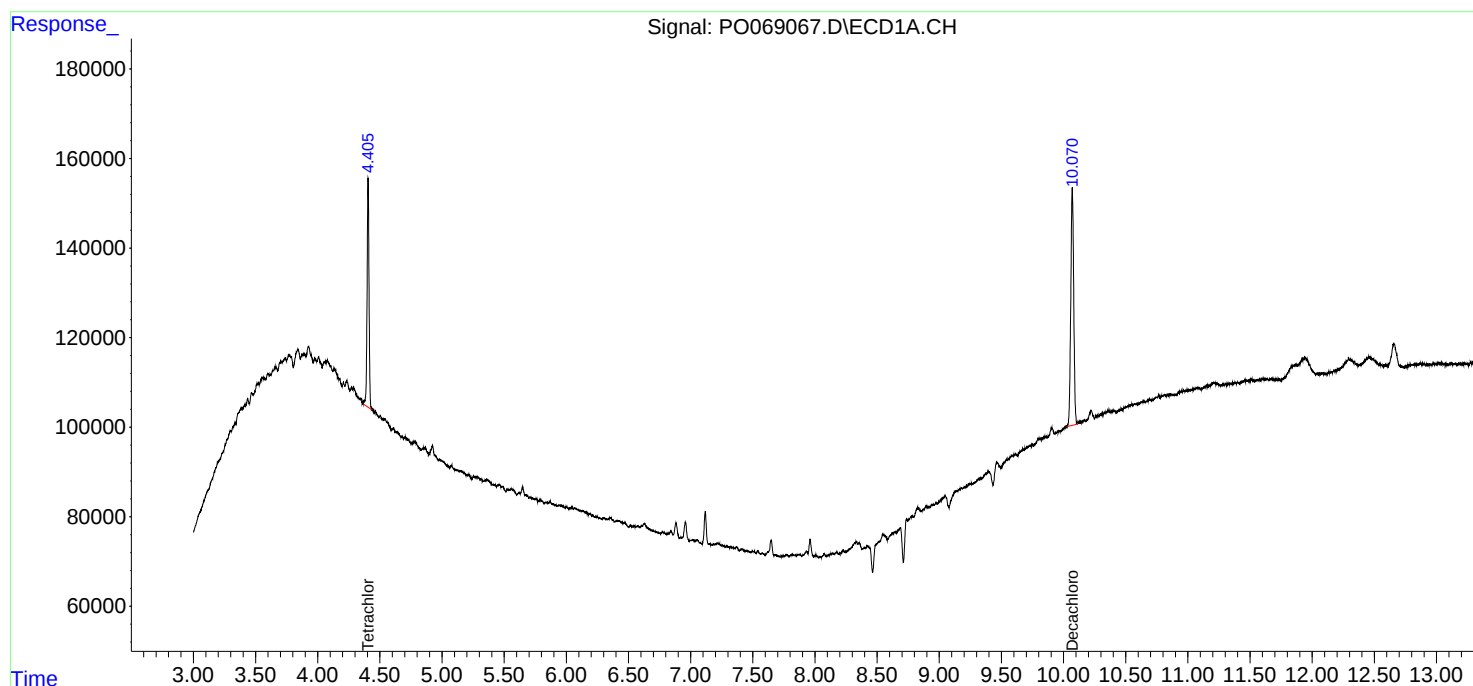

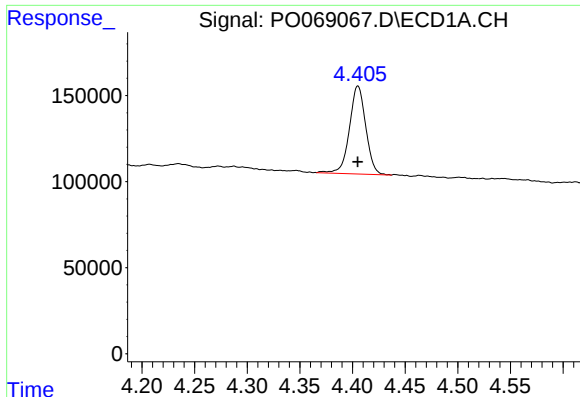


#1 Tetrachloro-m-xylene

R.T.: 4.405 min
Delta R.T.: 0.000 min
Response: 552184
Conc: 18.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
SLUDGE-BOX


Manual Integrations
APPROVED

Sohil
6/22/2020 4:27:50 PM

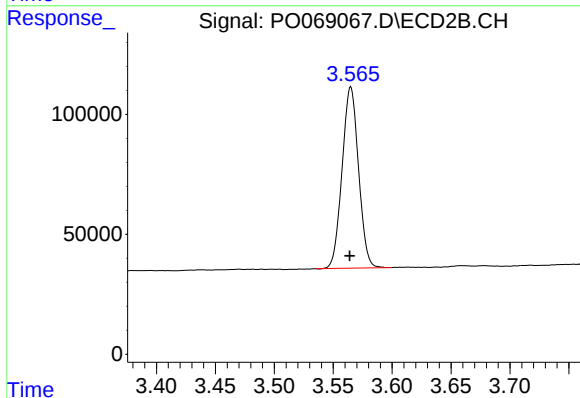


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 734552
Conc: 19.08 ng/ml

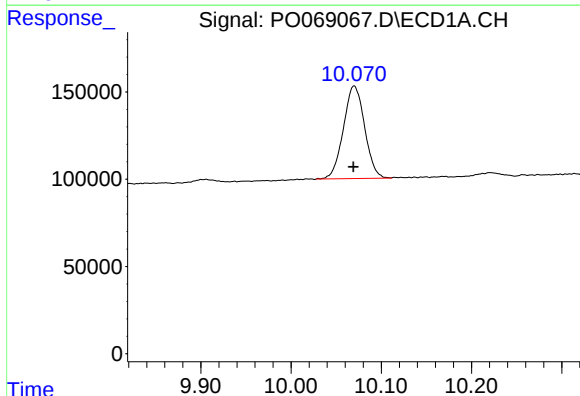

#2 Decachlorobiphenyl

R.T.: 10.070 min
Delta R.T.: 0.000 min
Response: 868308
Conc: 18.28 ng/ml m

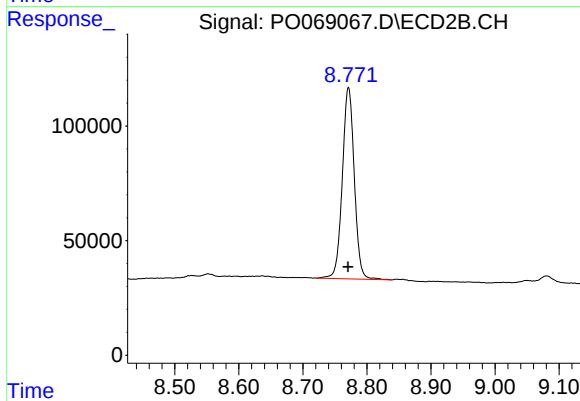

#2 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: 0.000 min
Response: 1082023
Conc: 19.88 ng/ml