

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0062018\
Data File : P0045971.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 13:20
Operator : SM/UA
Sample : J3567-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-5-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 13:33:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.380	3.609	11046070	5551819	23.100	22.084
2) SA Decachlor...	10.049	8.587	8022850	3058594	19.140	19.530

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062018\
Data File : P0045971.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 13:20
Operator : SM/UA
Sample : J3567-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-5-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 13:33:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

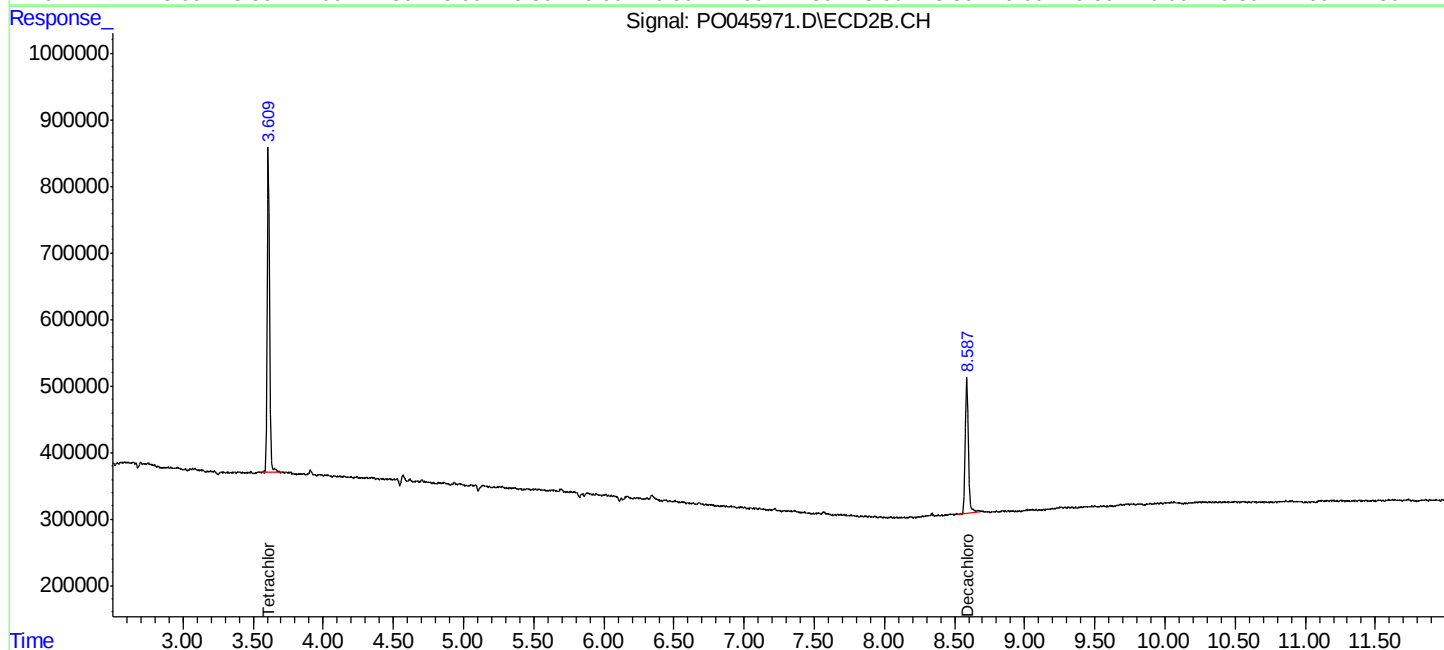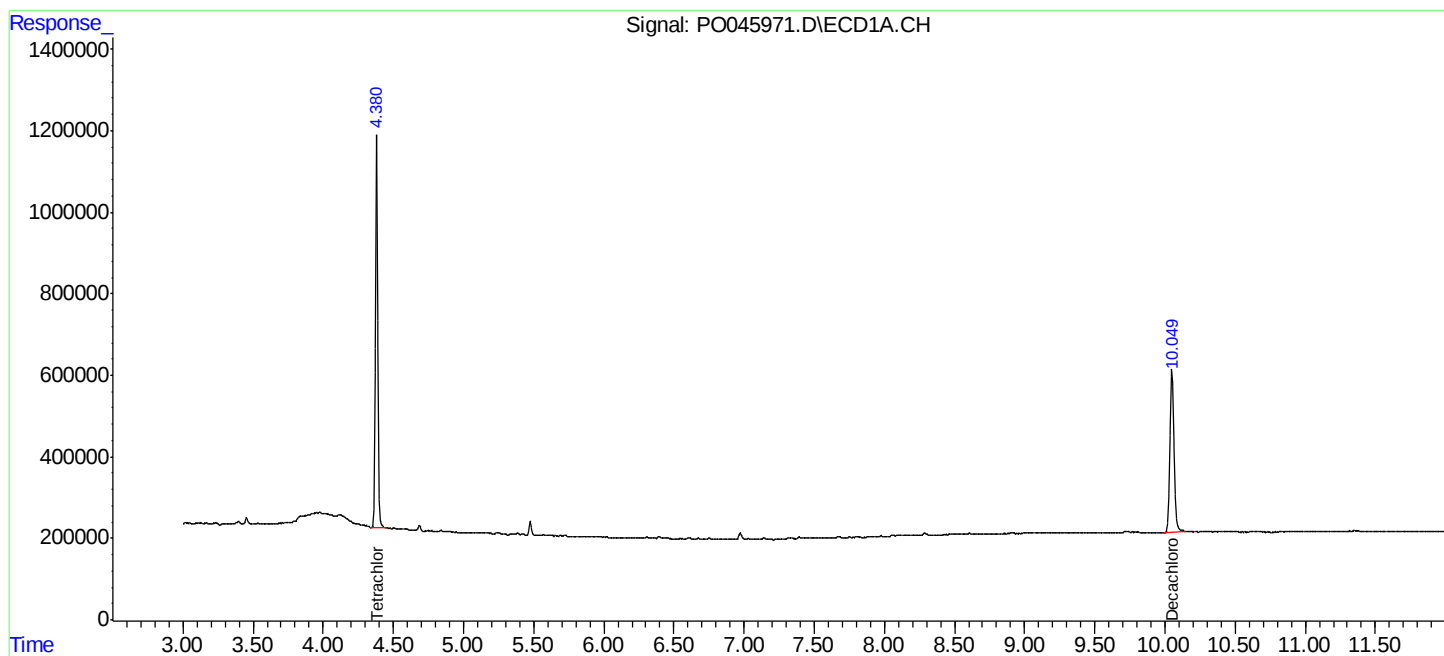


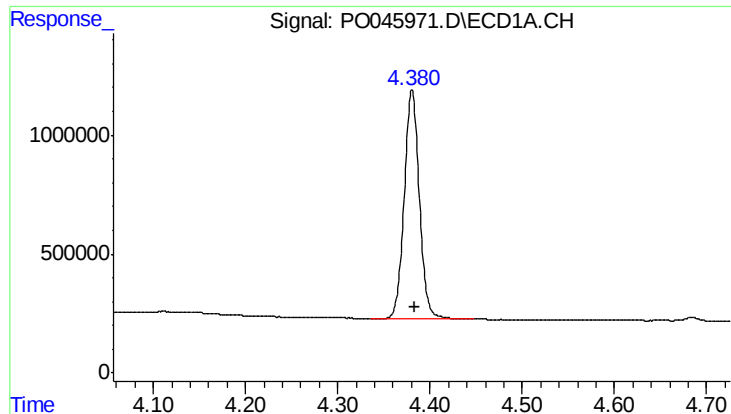

#1 Tetrachloro-m-xylene


R.T.: 4.380 min
Delta R.T.: -0.003 min
Response: 11046070
Conc: 23.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-5-D

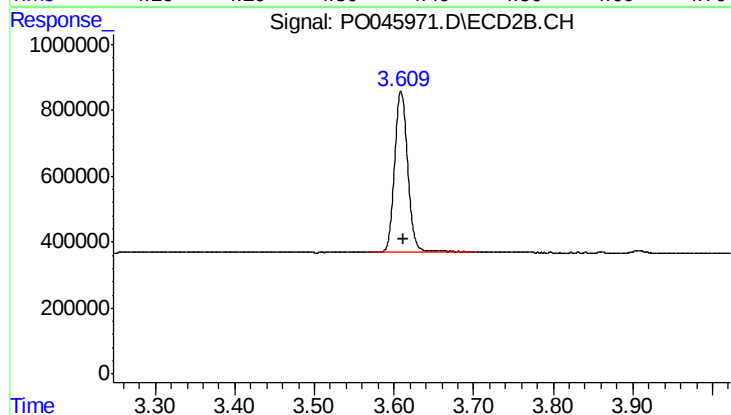


#1 Tetrachloro-m-xylene

R.T.: 3.609 min
Delta R.T.: -0.003 min
Response: 5551819
Conc: 22.08 ng/ml

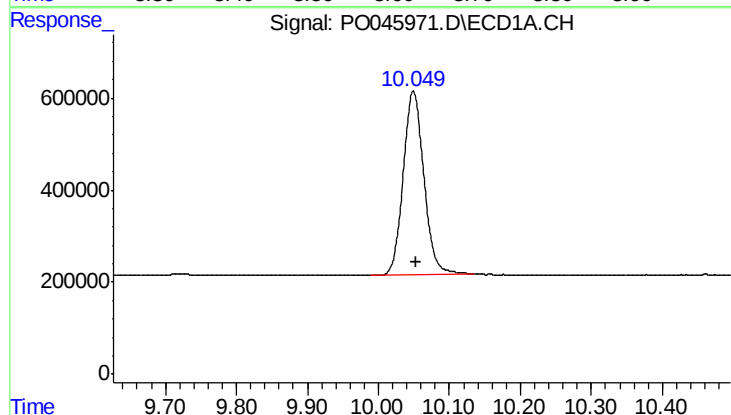

#2 Decachlorobiphenyl

R.T.: 10.049 min
Delta R.T.: -0.004 min
Response: 8022850
Conc: 19.14 ng/ml

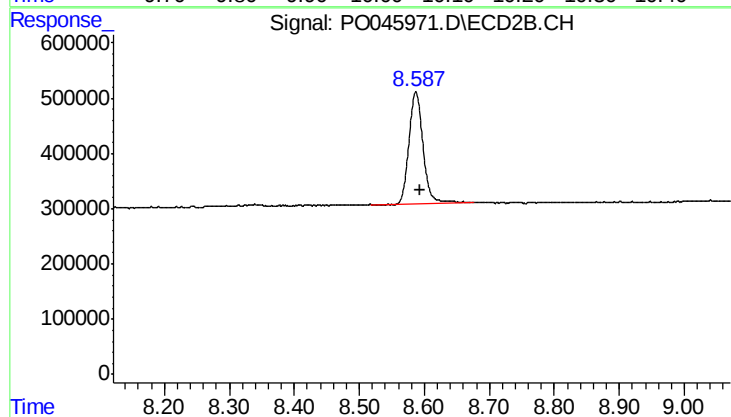

#2 Decachlorobiphenyl

R.T.: 8.587 min
Delta R.T.: -0.006 min
Response: 3058594
Conc: 19.53 ng/ml