

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0062018\
 Data File : P0045983.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2018 16:33
 Operator : SM/UA
 Sample : J3471-04RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 #2RE

Manual Integrations
 APPROVED

Sohil
 6/23/2018 1:37:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 16:51:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 20 03:39:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.384	3.613	7889635	4274836	16.499	17.004
2) SA Decachlor...	10.057	8.591	3479139	1409578	8.300	9.000m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062018\
Data File : P0045983.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 16:33
Operator : SM/UA
Sample : J3471-04RE
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
#2RE


Manual Integrations
APPROVED

Sohil
6/23/2018 1:37:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 16:51:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

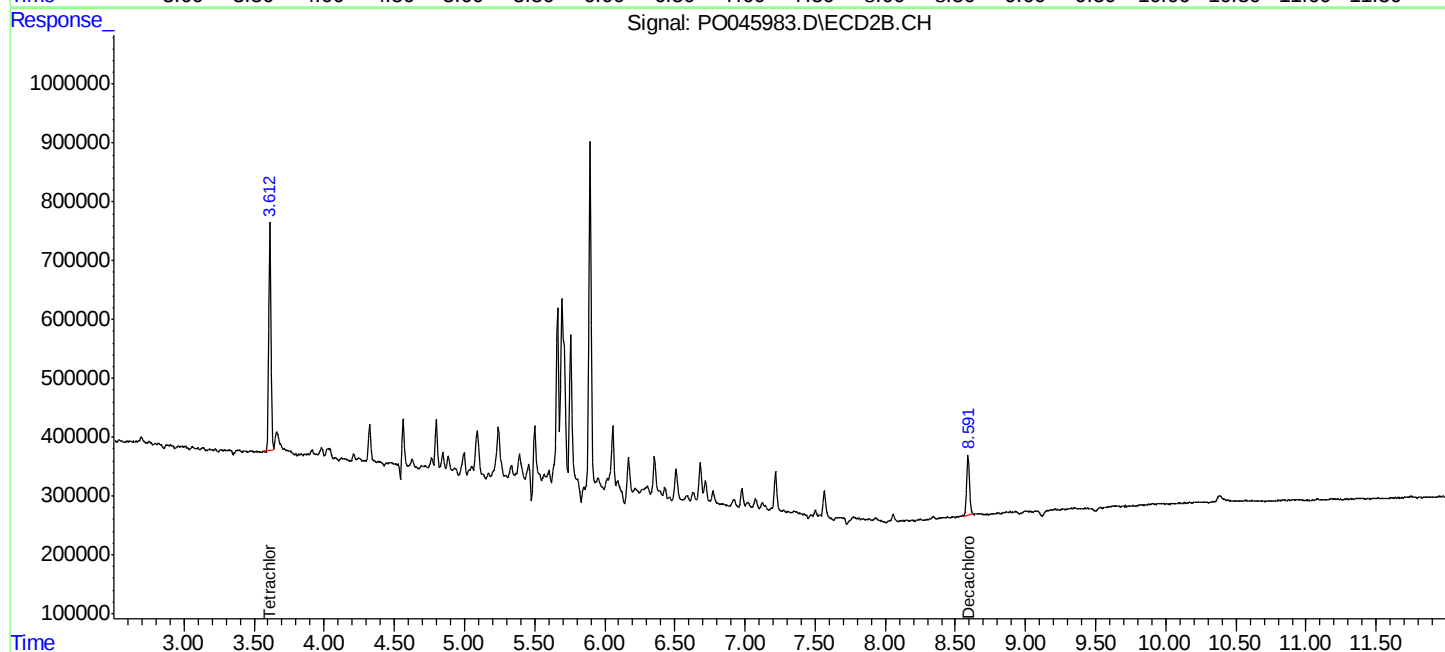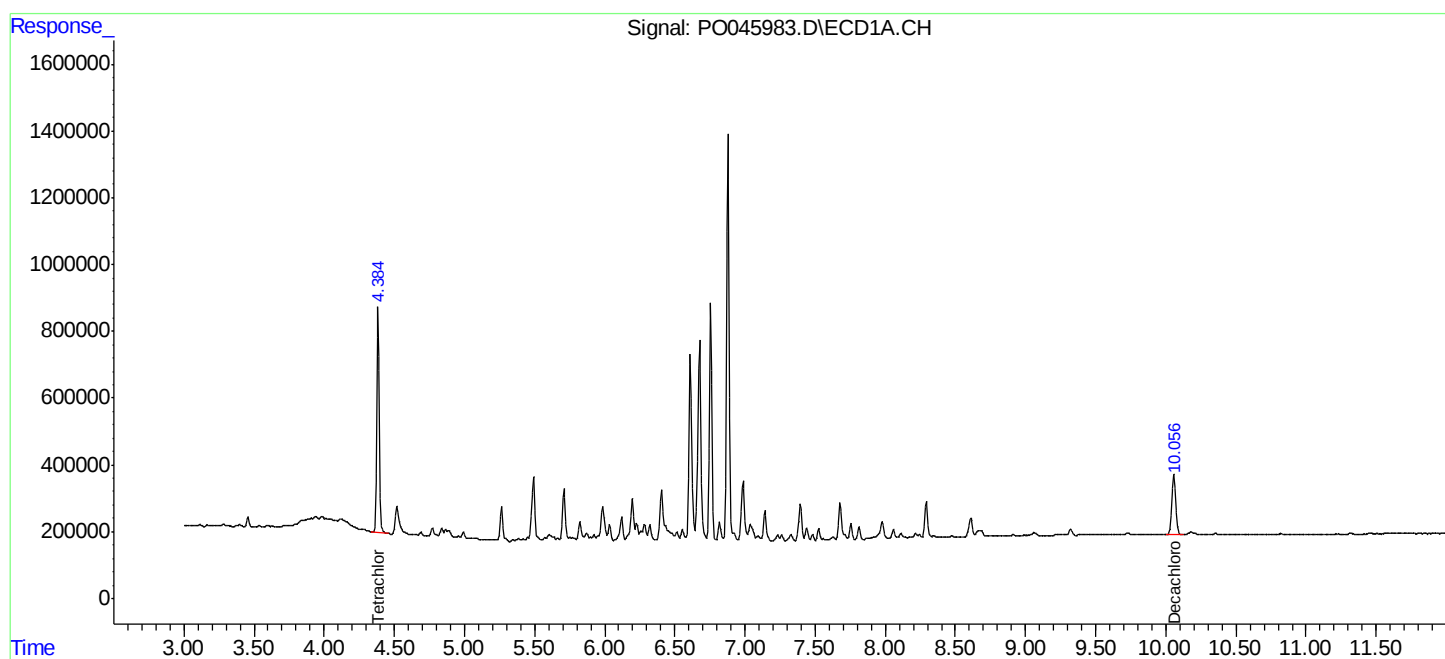

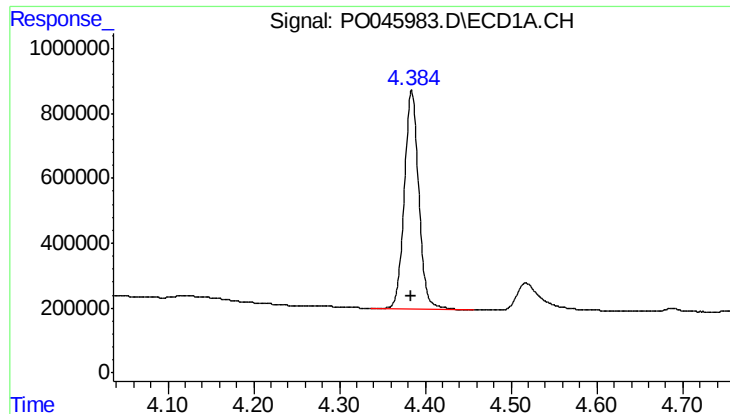


#1 Tetrachloro-m-xylene

R.T.: 4.384 min
Delta R.T.: 0.000 min
Response: 7889635
Conc: 16.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
#2RE


Manual Integrations
APPROVED

Sohil
6/23/2018 1:37:19 AM

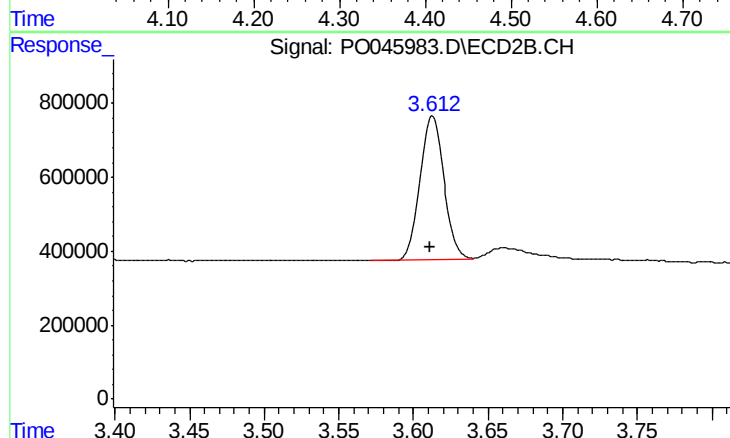


#1 Tetrachloro-m-xylene

R.T.: 3.613 min
Delta R.T.: 0.000 min
Response: 4274836
Conc: 17.00 ng/ml

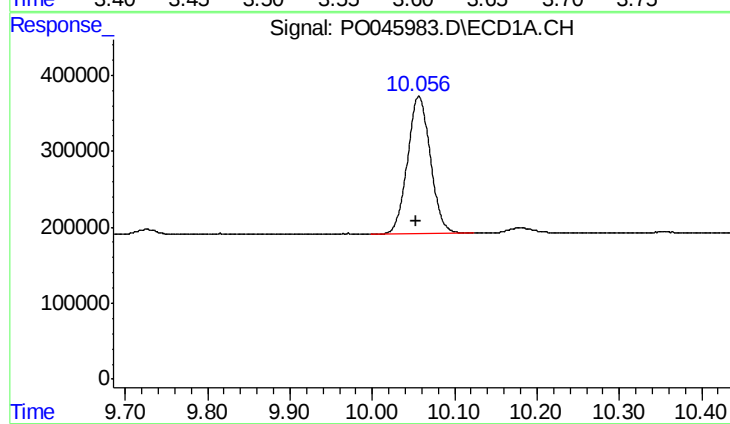

#2 Decachlorobiphenyl

R.T.: 10.057 min
Delta R.T.: 0.003 min
Response: 3479139
Conc: 8.30 ng/ml

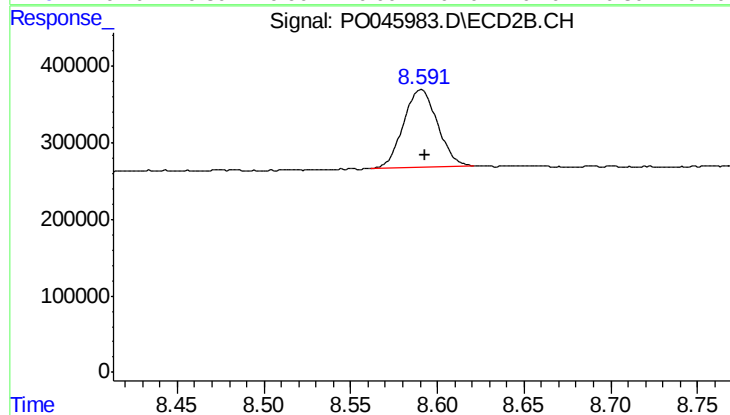

#2 Decachlorobiphenyl

R.T.: 8.591 min
Delta R.T.: -0.002 min
Response: 1409578
Conc: 9.00 ng/ml m