

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062118\
Data File : P0046010.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 11:22
Operator : SM/UA
Sample : J3575-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-11-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 11:39:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.382	3.611	10683268	5374866	22.341	21.380
2) SA Decachlor...	10.055	8.589	5972111	2372208	14.248	15.147

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062118\
Data File : P0046010.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 11:22
Operator : SM/UA
Sample : J3575-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-11-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 11:39:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

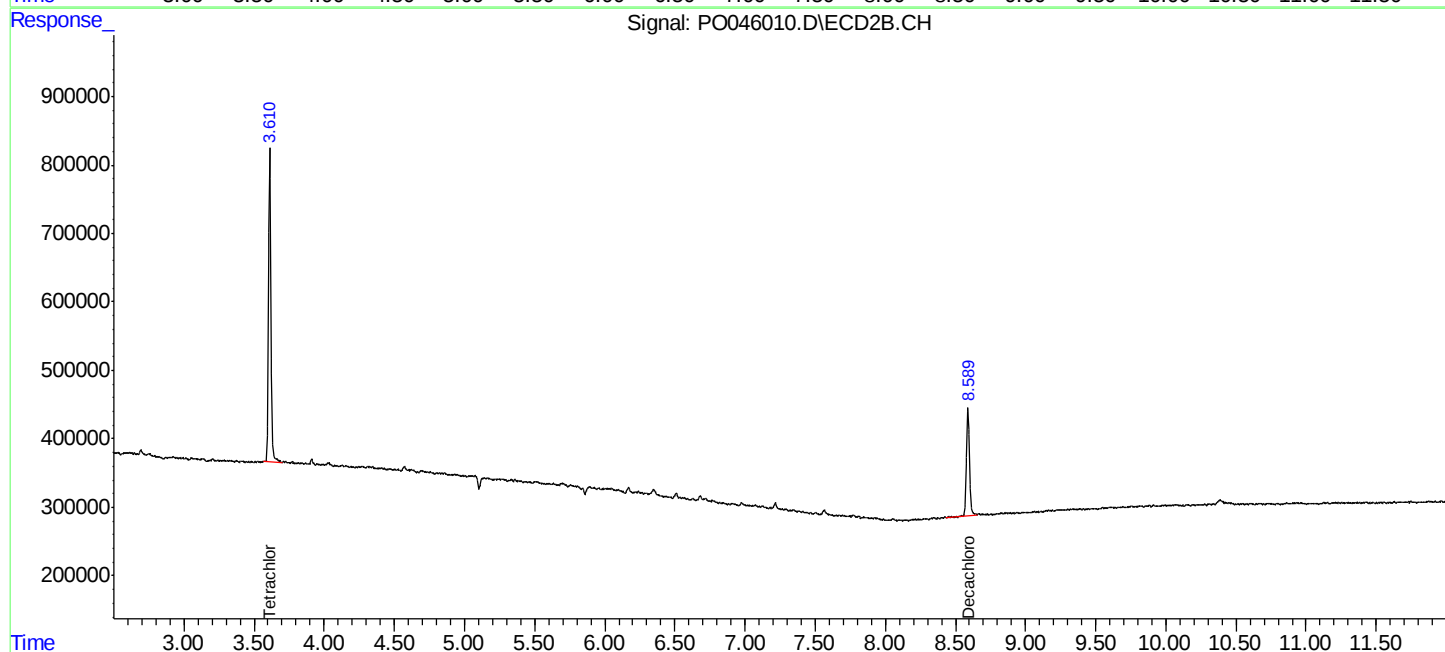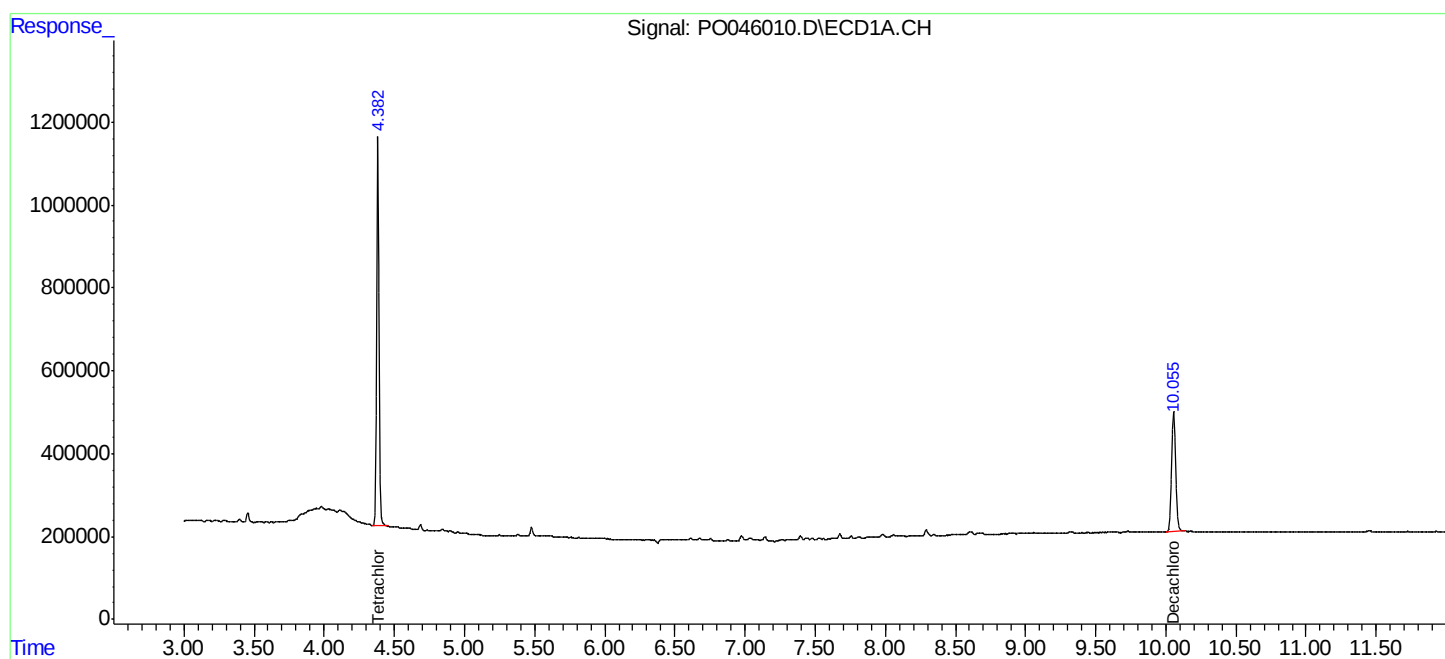


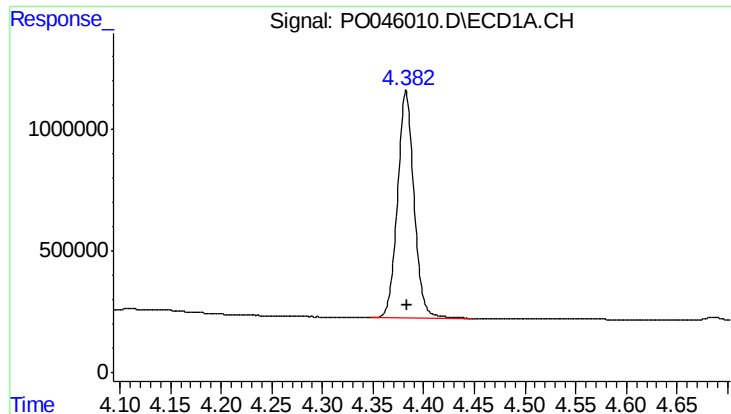

#1 Tetrachloro-m-xylene


R.T.: 4.382 min
Delta R.T.: -0.001 min
Response: 10683268
Conc: 22.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-11-S

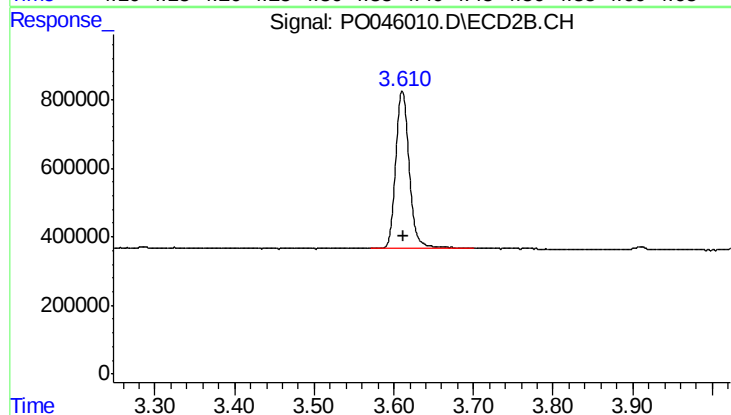


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: 0.000 min
Response: 5374866
Conc: 21.38 ng/ml

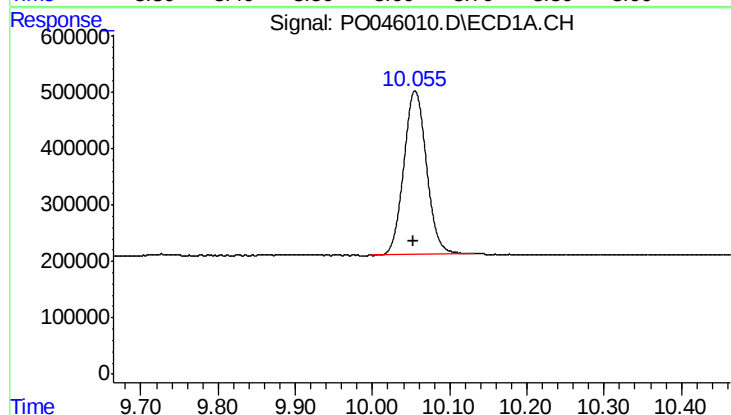

#2 Decachlorobiphenyl

R.T.: 10.055 min
Delta R.T.: 0.002 min
Response: 5972111
Conc: 14.25 ng/ml

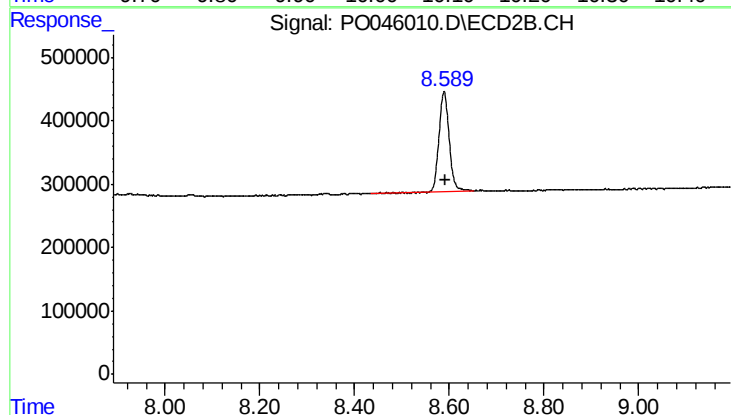

#2 Decachlorobiphenyl

R.T.: 8.589 min
Delta R.T.: -0.004 min
Response: 2372208
Conc: 15.15 ng/ml