

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0062118\
 Data File : P0046030.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 17:19
 Operator : SM/UA
 Sample : J3584-19
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 17:35:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 20 03:39:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.383	3.611	9702434	4700177	20.290	18.696
2) SA Decachlor...	10.055	8.587	5734219	2362974	13.680	15.088
Target Compounds						
7) L1 AR-1016-5	0.000	5.499	0	448171	N.D.	69.702 #
12) L3 AR-1232-2	5.479	4.625	1184313	267238	150.826	63.268 #
22) L5 AR-1248-2	0.000	5.275	0	350619	N.D.	45.802 #
23) L5 AR-1248-3	0.000	5.499	0	448171	N.D.	39.077 #
24) L5 AR-1248-4	0.000	5.536	0	340783	N.D.	40.288 #
26) L6 AR-1254-1	0.000	5.499	0	448171	N.D.	34.991 #
27) L6 AR-1254-2	0.000	5.660	0	288064	N.D.	26.090 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062118\
Data File : P0046030.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 17:19
Operator : SM/UA
Sample : J3584-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
TP-1-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 17:35:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

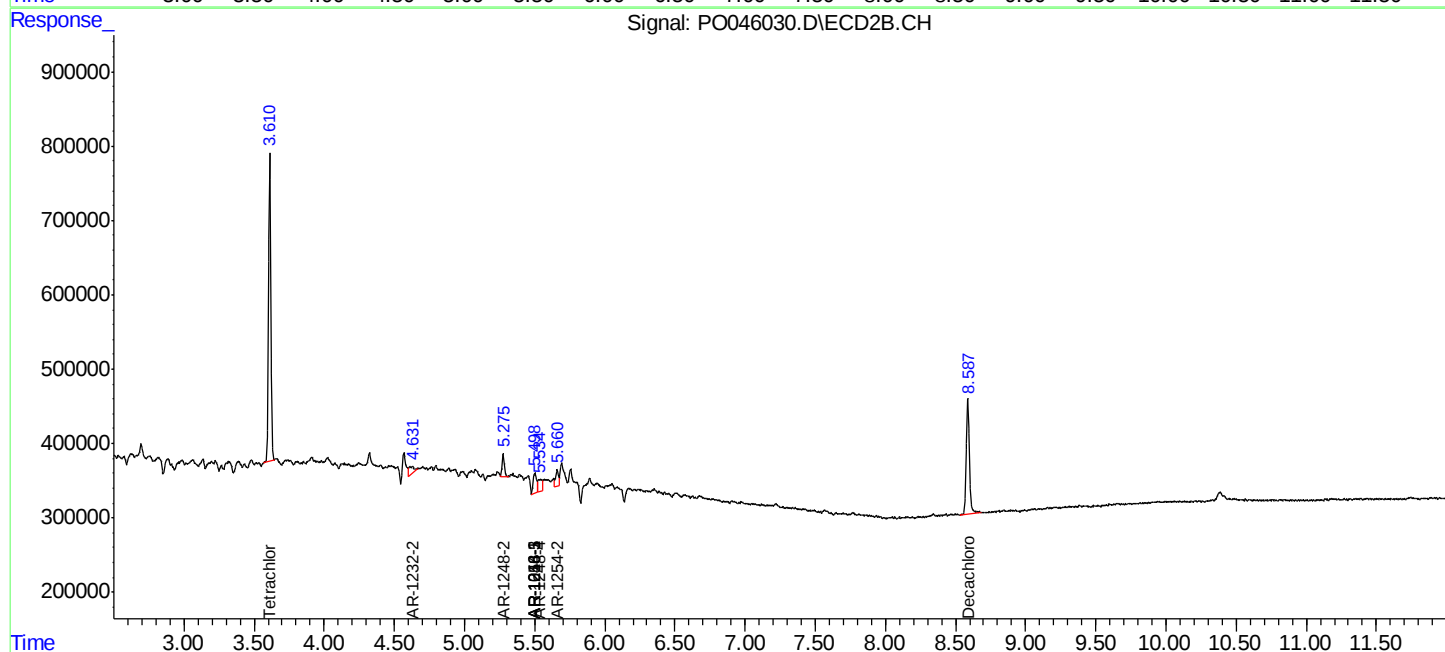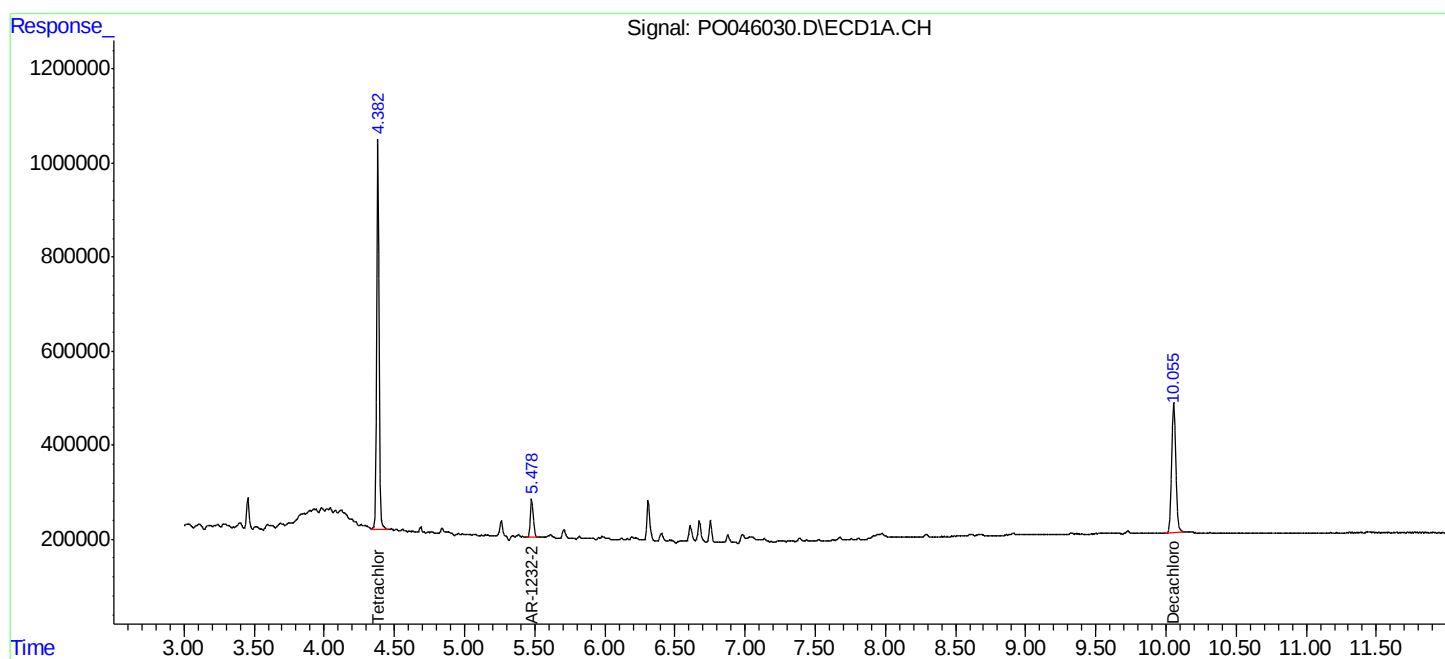


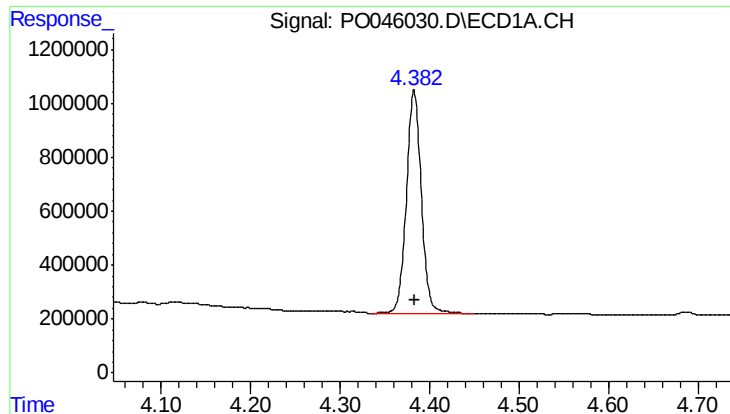

#1 Tetrachloro-m-xylene


R.T.: 4.383 min
Delta R.T.: -0.001 min
Response: 9702434
Conc: 20.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1-S

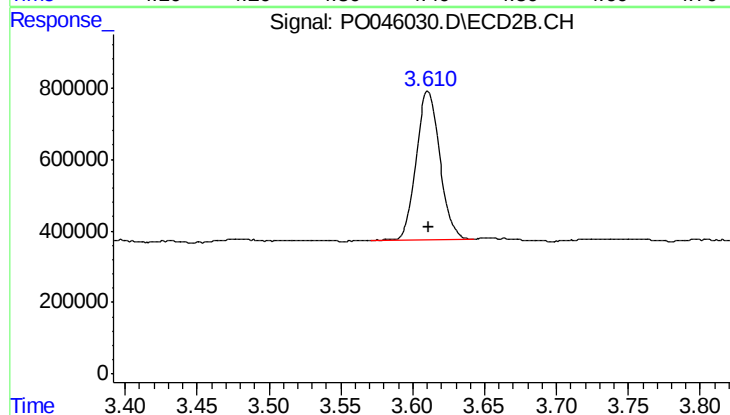


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: 0.000 min
Response: 4700177
Conc: 18.70 ng/ml

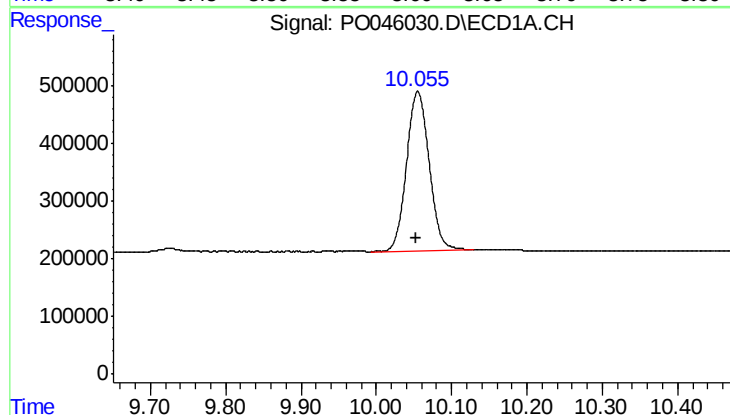


#2 Decachlorobiphenyl

R.T.: 10.055 min
Delta R.T.: 0.002 min
Response: 5734219
Conc: 13.68 ng/ml

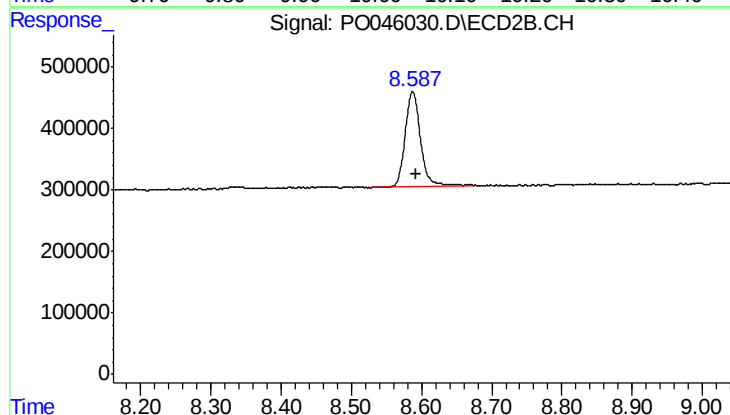

#2 Decachlorobiphenyl


R.T.: 8.587 min
Delta R.T.: -0.006 min
Response: 2362974
Conc: 15.09 ng/ml

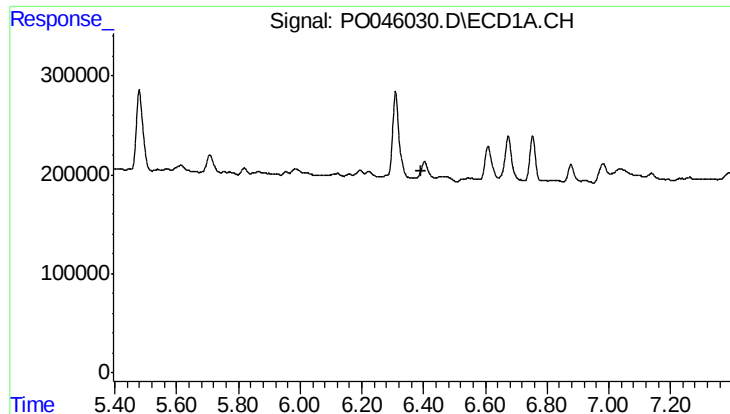

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-1-S

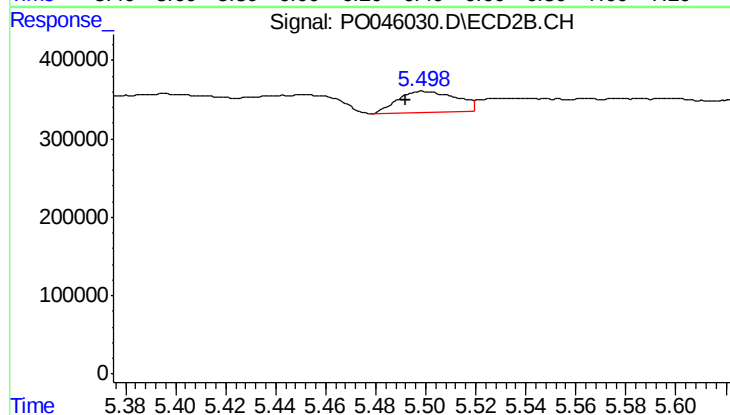


#7 AR-1016-5

R.T.: 5.499 min
Delta R.T.: 0.006 min
Response: 448171
Conc: 69.70 ng/ml

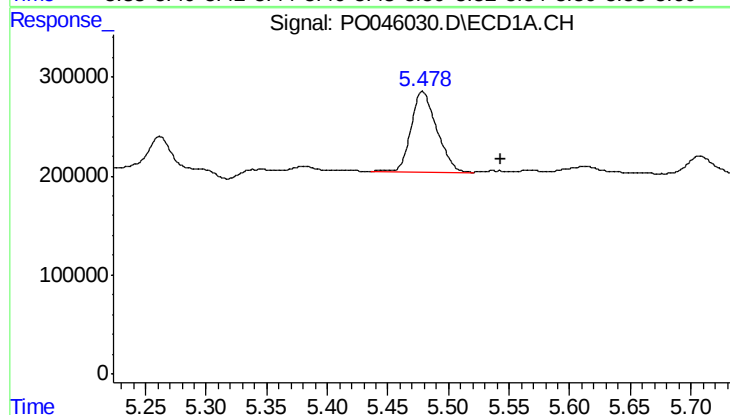


#12 AR-1232-2

R.T.: 5.479 min
Delta R.T.: -0.064 min
Response: 1184313
Conc: 150.83 ng/ml

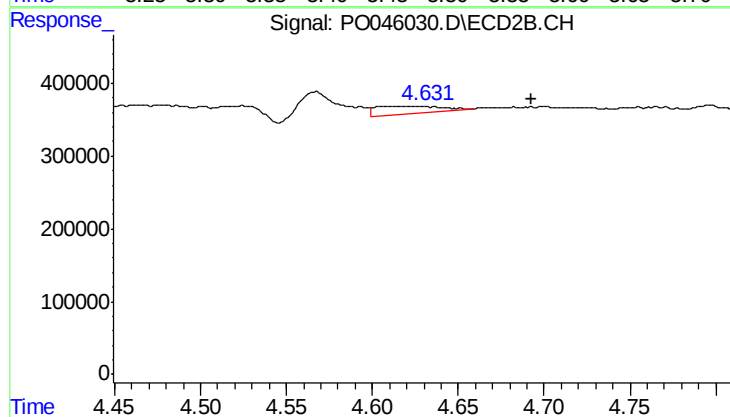

#12 AR-1232-2


R.T.: 4.625 min
Delta R.T.: -0.068 min
Response: 267238
Conc: 63.27 ng/ml

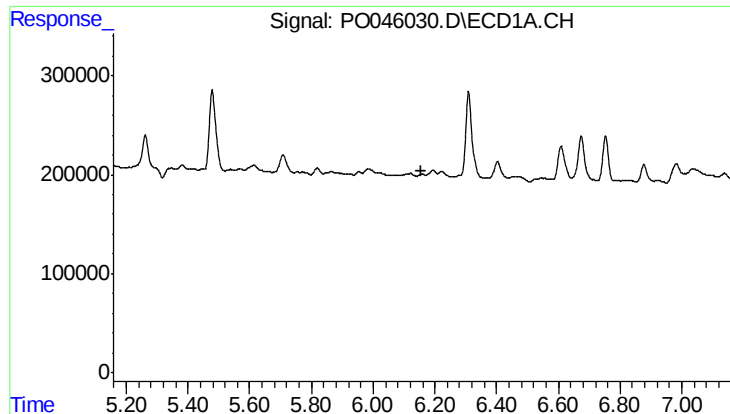

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 6.158 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-1-S

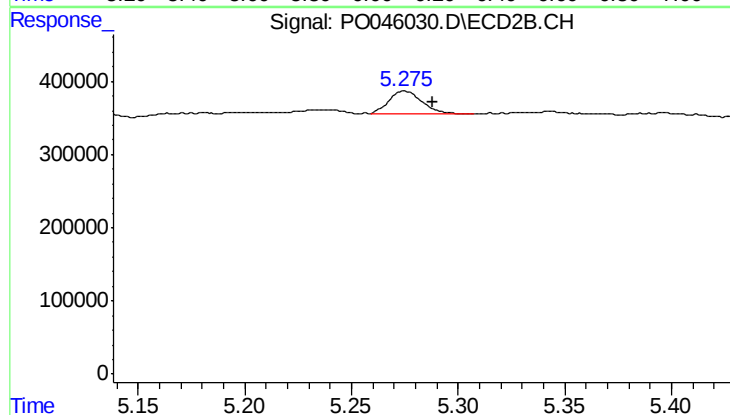


#22 AR-1248-2

R.T.: 5.275 min
Delta R.T.: -0.014 min
Response: 350619
Conc: 45.80 ng/ml

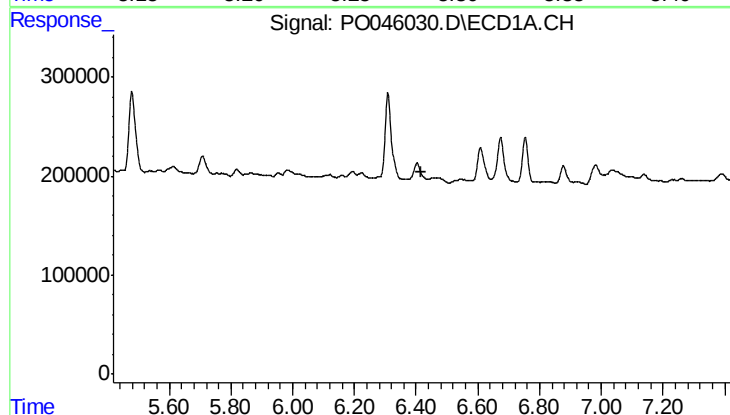


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 6.419 min
Response: 0
Conc: N.D.

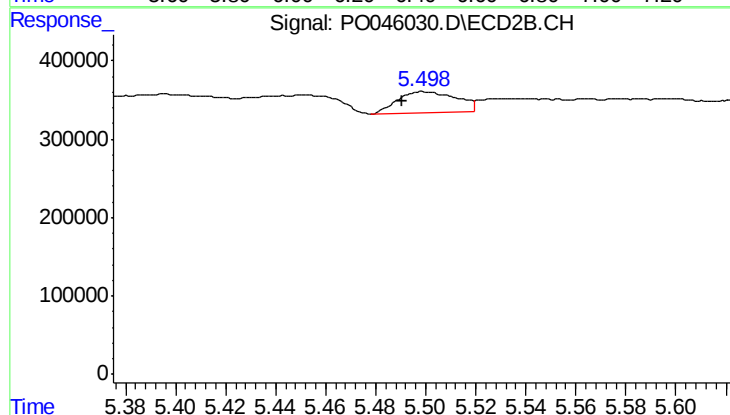

#23 AR-1248-3


R.T.: 5.499 min
Delta R.T.: 0.008 min
Response: 448171
Conc: 39.08 ng/ml

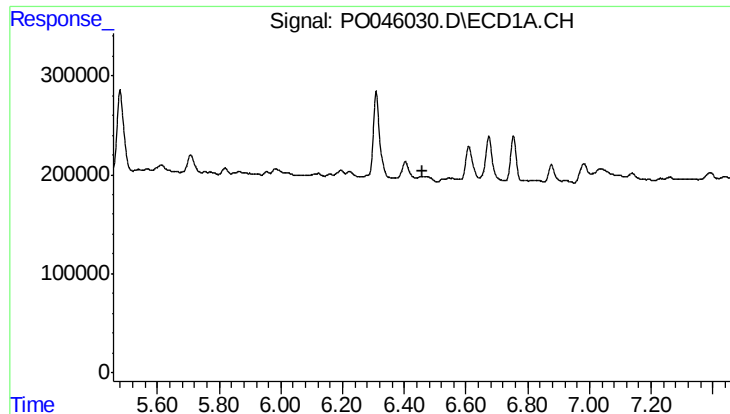

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 6.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-1-S

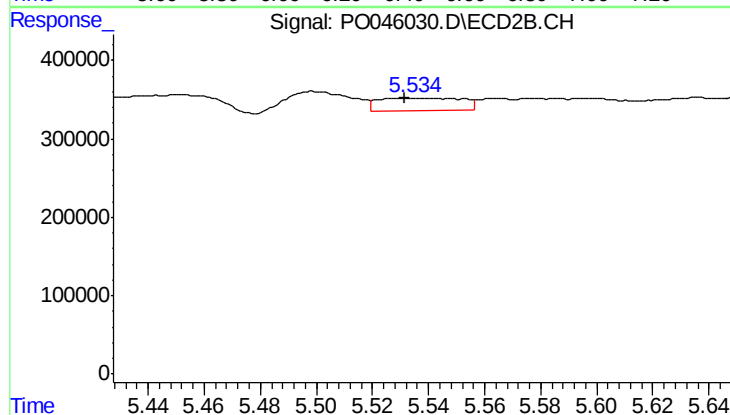


#24 AR-1248-4

R.T.: 5.536 min
Delta R.T.: 0.004 min
Response: 340783
Conc: 40.29 ng/ml

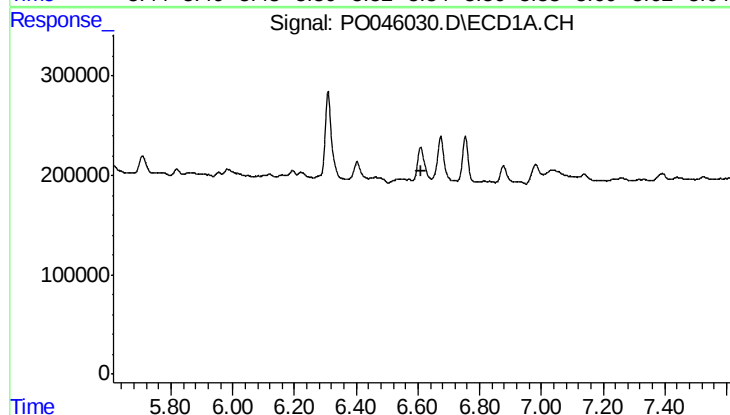


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.613 min
Response: 0
Conc: N.D.

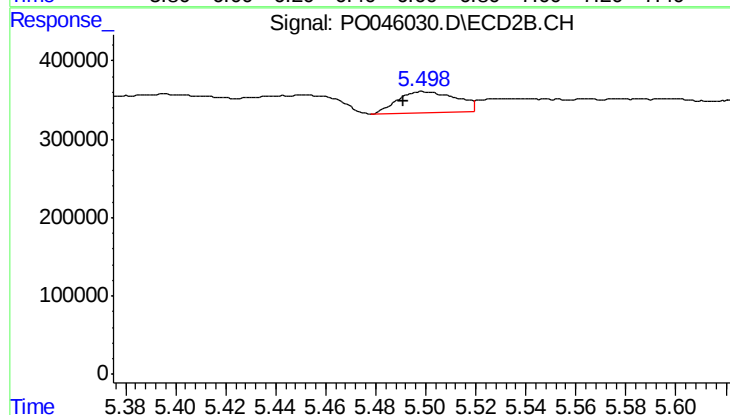

#26 AR-1254-1


R.T.: 5.499 min
Delta R.T.: 0.008 min
Response: 448171
Conc: 34.99 ng/ml

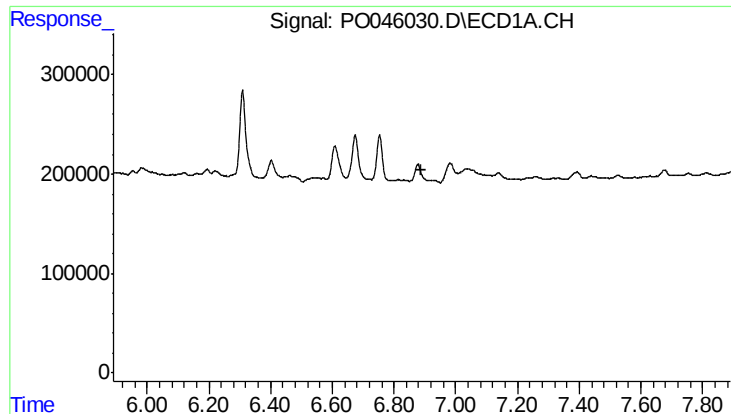

#27 AR-1254-2

R.T.: 0.000 min
Exp R.T.: 6.890 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-1-S

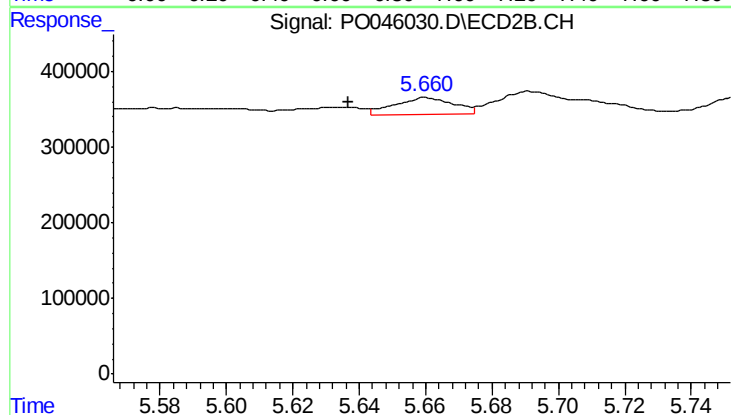

#27 AR-1254-2

R.T.: 5.660 min
Delta R.T.: 0.023 min
Response: 288064
Conc: 26.09 ng/ml