

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0062118\
 Data File : P0046055.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2018 00:02
 Operator : SM/UA
 Sample : J3603-21
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 26KV-TP-8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 02:29:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 20 03:39:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.382	3.610	7268259	3517328	15.199	13.991
2) SA Decachlor...	10.056	8.587	2574401	1153478	6.142	7.365
Target Compounds						
7) L1 AR-1016-5	0.000	5.497	0	233992	N.D.	36.392 #
23) L5 AR-1248-3	0.000	5.497	0	233992	N.D.	20.402 #
24) L5 AR-1248-4	0.000	5.544	0	152599	N.D.	18.041 #
25) L5 AR-1248-5	0.000	6.031	0	759008	N.D.	135.257 #
26) L6 AR-1254-1	0.000	5.497	0	233992	N.D.	18.269 #
28) L6 AR-1254-3	0.000	6.031	0	759008	N.D.	42.456 #
29) L6 AR-1254-4	0.000	6.242	0	40193	N.D.	3.620 #
31) L7 AR-1260-1	0.000	6.176	0	439938	N.D.	36.278 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062118\
Data File : P0046055.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2018 00:02
Operator : SM/UA
Sample : J3603-21
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
26KV-TP-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 02:29:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

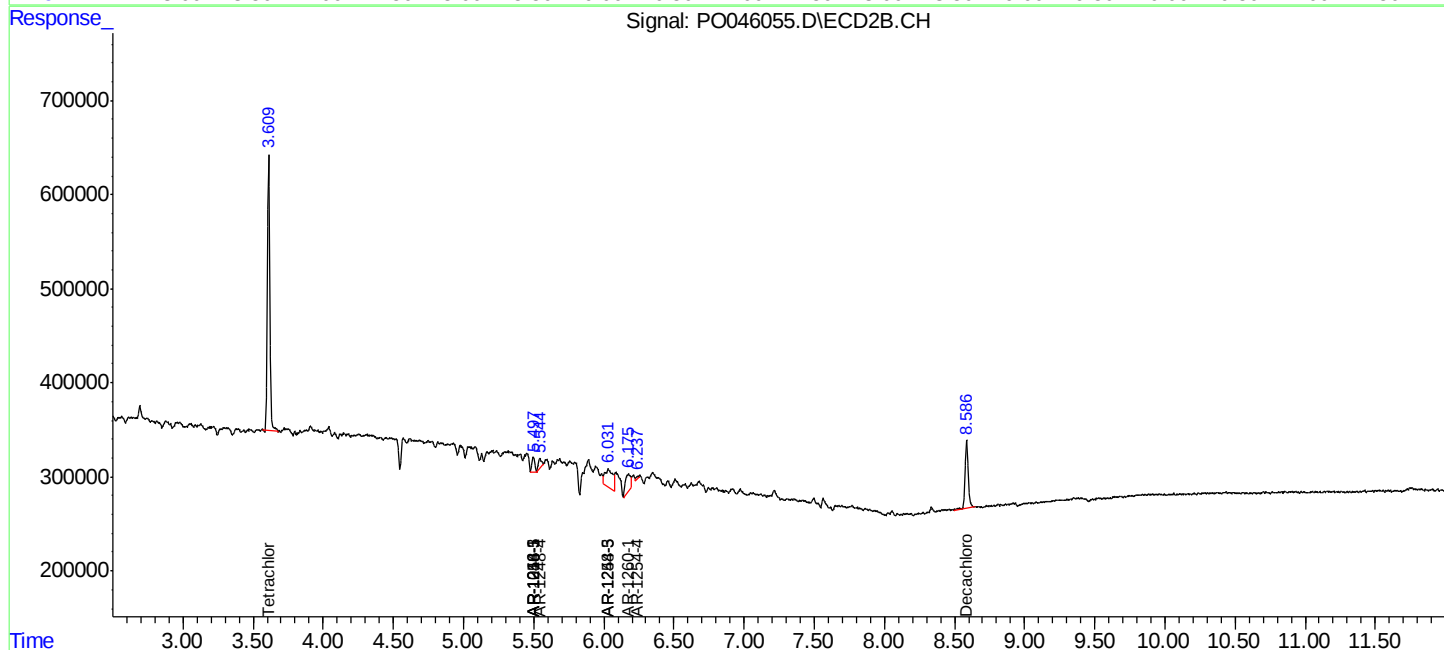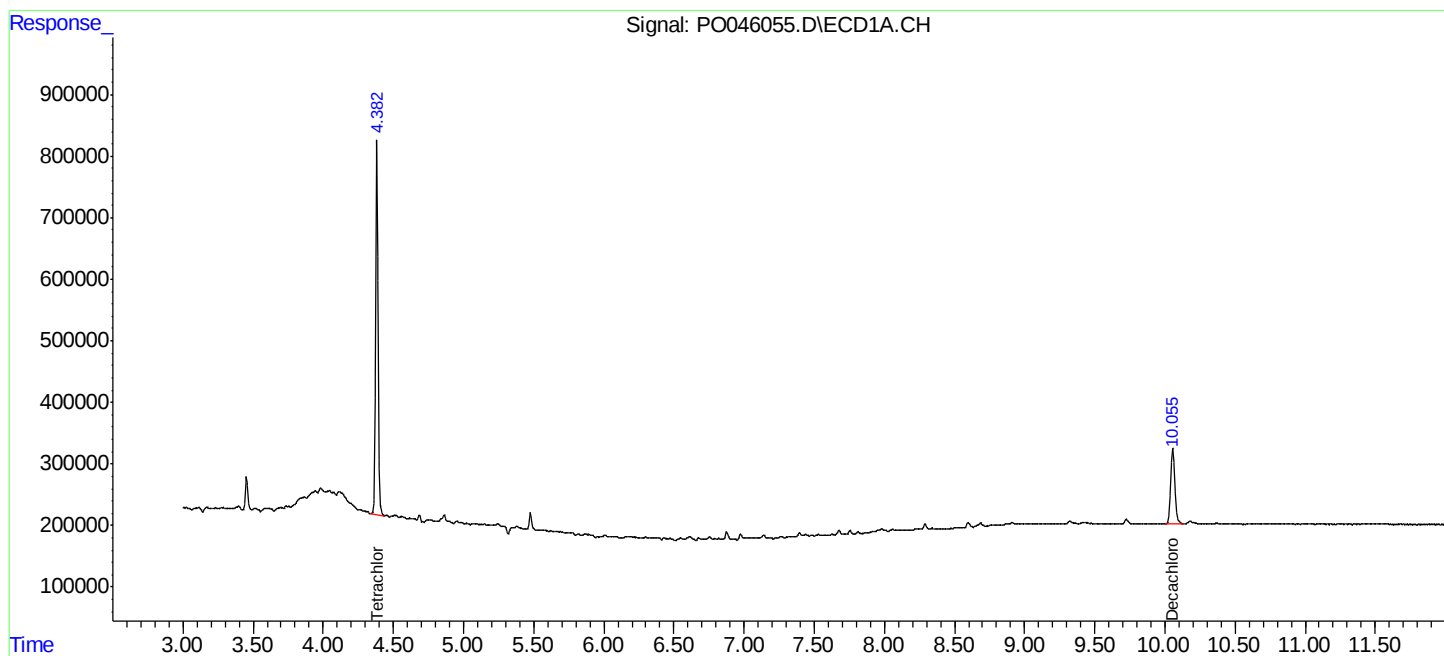


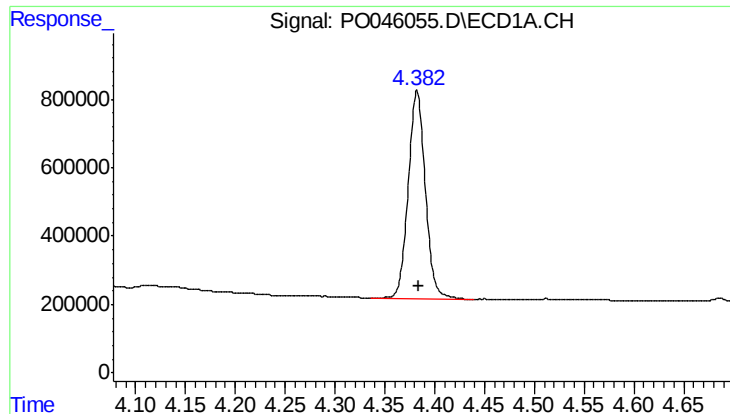

#1 Tetrachloro-m-xylene


R.T.: 4.382 min
Delta R.T.: -0.001 min
Response: 7268259
Conc: 15.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
26KV-TP-8

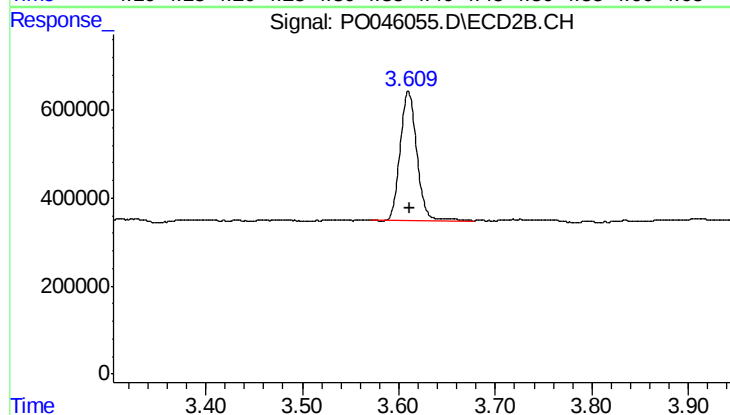


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: -0.002 min
Response: 3517328
Conc: 13.99 ng/ml

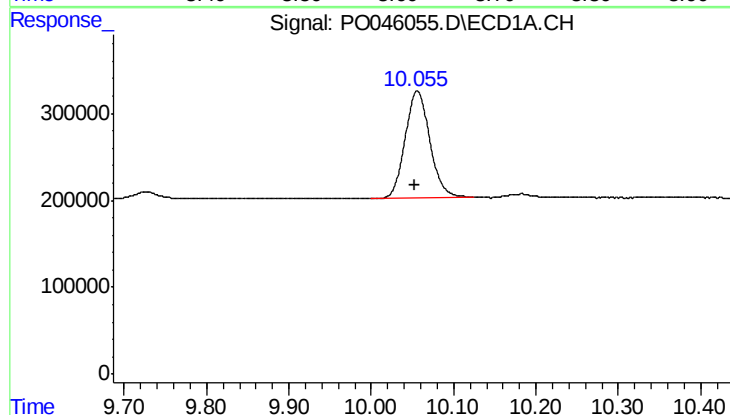


#2 Decachlorobiphenyl

R.T.: 10.056 min
Delta R.T.: 0.002 min
Response: 2574401
Conc: 6.14 ng/ml

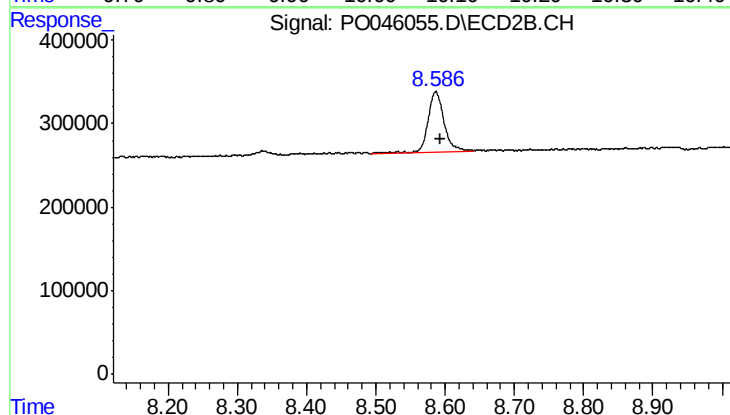

#2 Decachlorobiphenyl


R.T.: 8.587 min
Delta R.T.: -0.006 min
Response: 1153478
Conc: 7.37 ng/ml

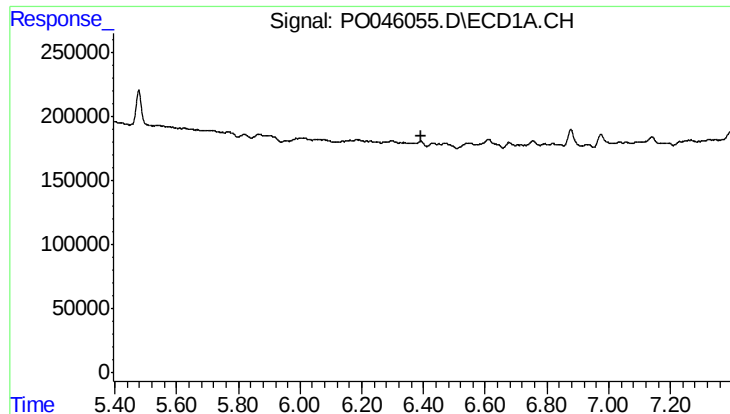

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
26KV-TP-8

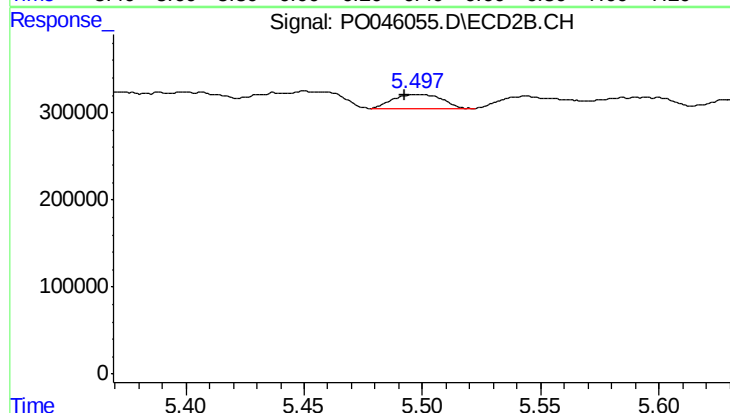


#7 AR-1016-5

R.T.: 5.497 min
Delta R.T.: 0.005 min
Response: 233992
Conc: 36.39 ng/ml

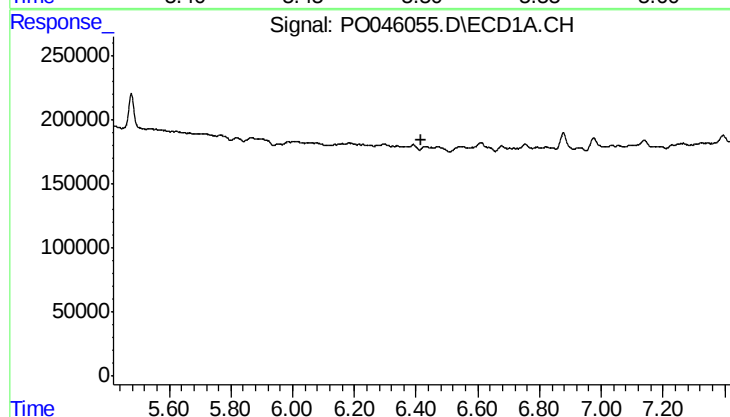


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 6.419 min
Response: 0
Conc: N.D.

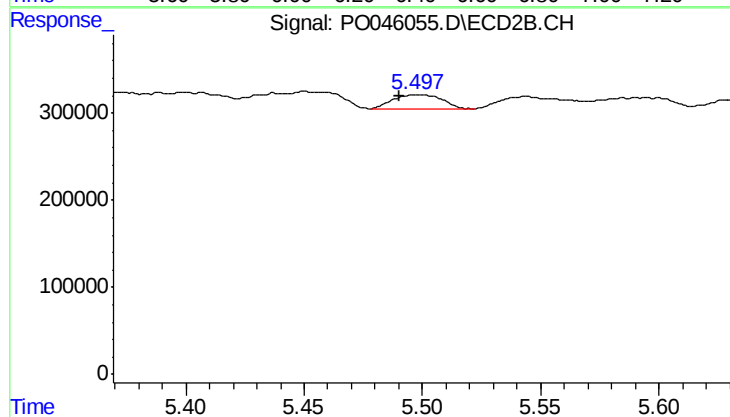

#23 AR-1248-3


R.T.: 5.497 min
Delta R.T.: 0.007 min
Response: 233992
Conc: 20.40 ng/ml

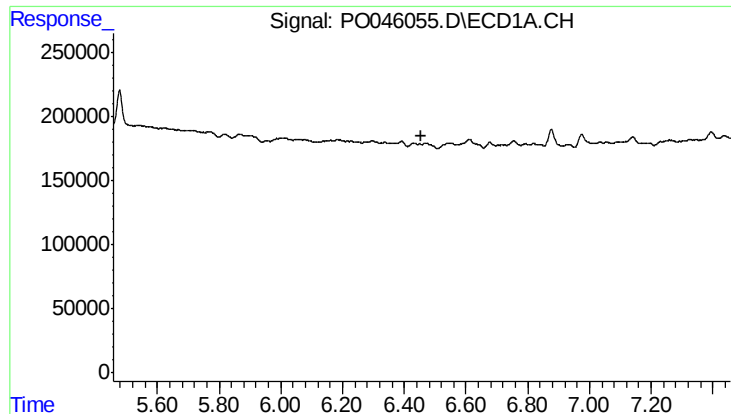

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 6.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
26KV-TP-8

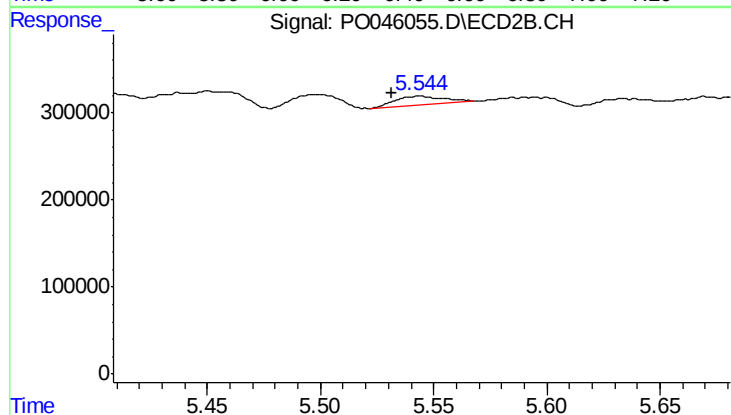


#24 AR-1248-4

R.T.: 5.544 min
Delta R.T.: 0.012 min
Response: 152599
Conc: 18.04 ng/ml

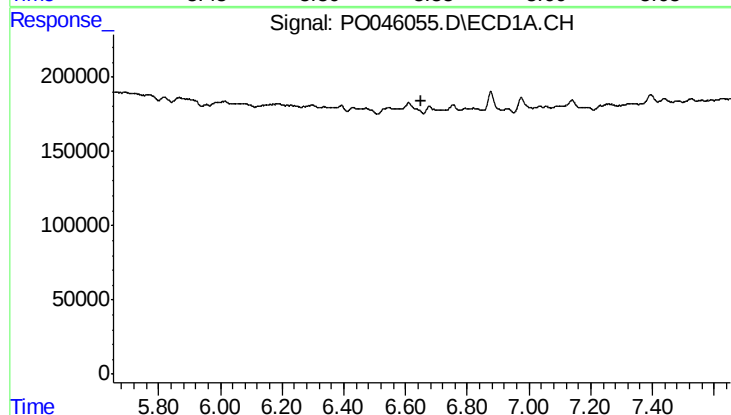


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 6.653 min
Response: 0
Conc: N.D.

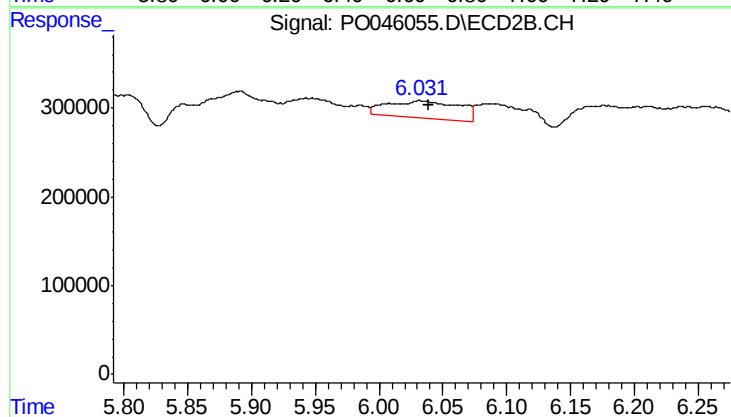

#25 AR-1248-5


R.T.: 6.031 min
Delta R.T.: -0.008 min
Response: 759008
Conc: 135.26 ng/ml

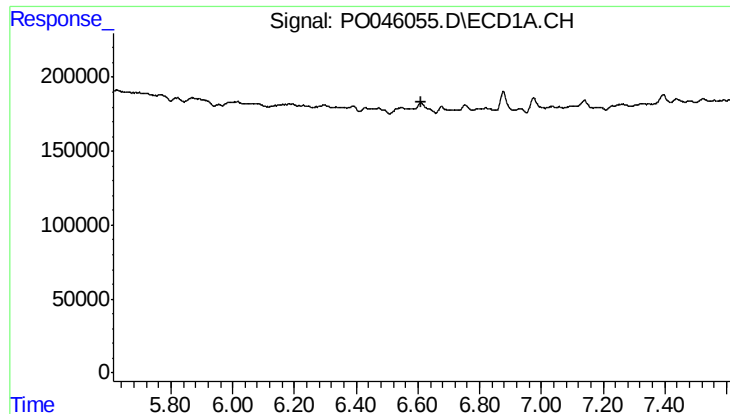

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.613 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
26KV-TP-8

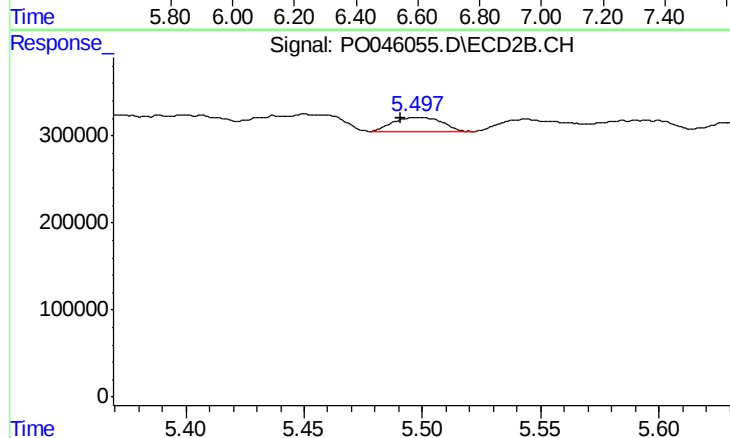


#26 AR-1254-1

R.T.: 5.497 min
Delta R.T.: 0.006 min
Response: 233992
Conc: 18.27 ng/ml

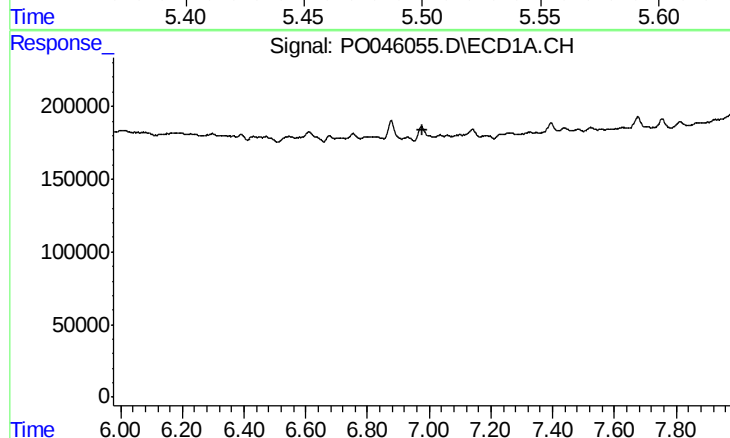


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 6.977 min
Response: 0
Conc: N.D.

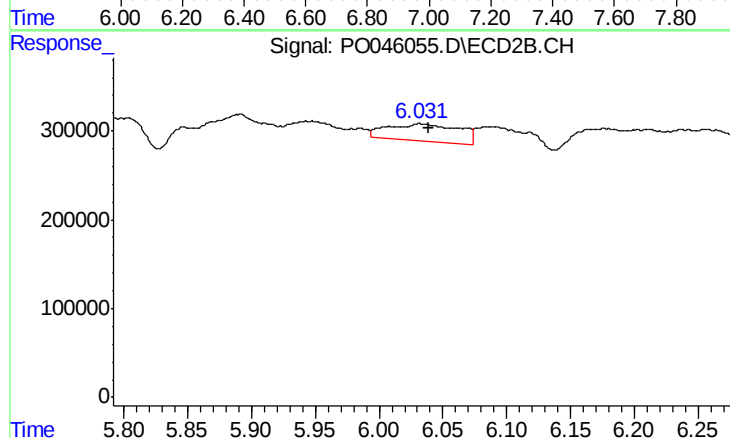

#28 AR-1254-3


R.T.: 6.031 min
Delta R.T.: -0.009 min
Response: 759008
Conc: 42.46 ng/ml

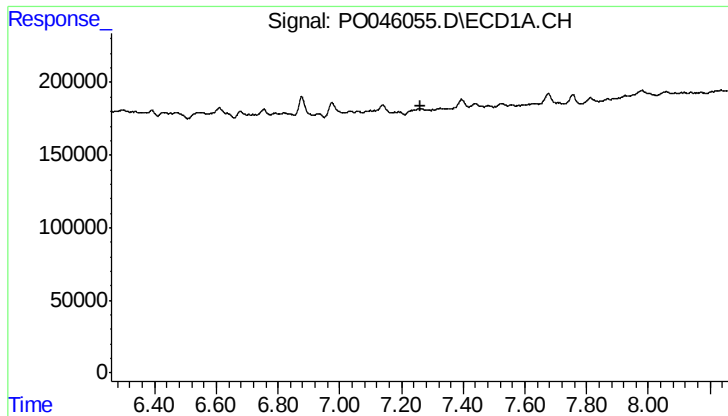

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.260 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
26KV-TP-8

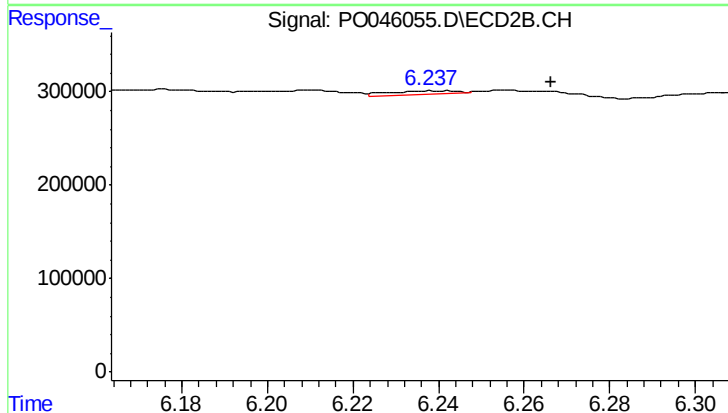


#29 AR-1254-4

R.T.: 6.242 min
Delta R.T.: -0.024 min
Response: 40193
Conc: 3.62 ng/ml

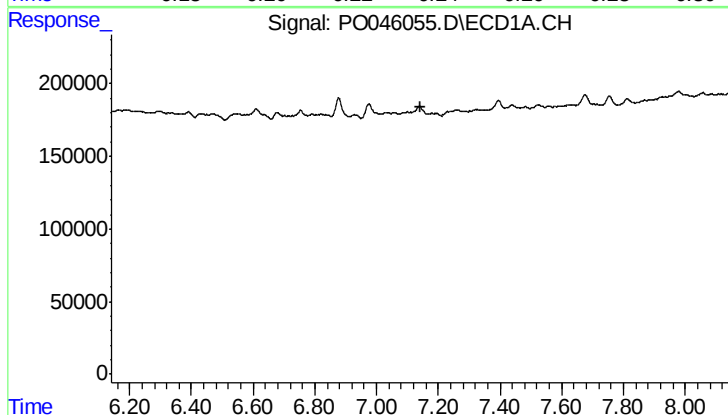

#31 AR-1260-1

R.T.: 0.000 min
Exp R.T.: 7.141 min
Response: 0
Conc: N.D.

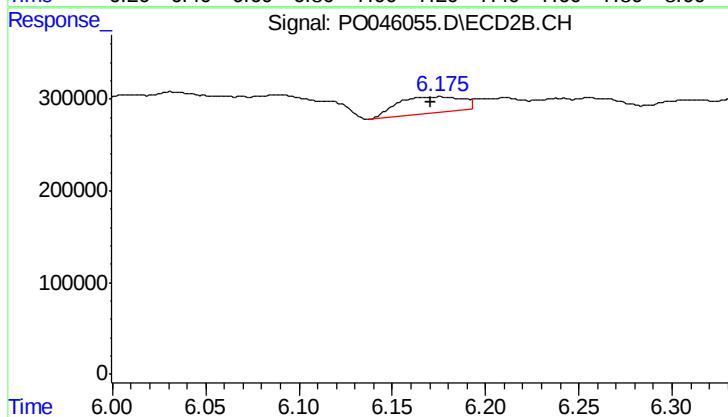

#31 AR-1260-1

R.T.: 6.176 min
Delta R.T.: 0.006 min
Response: 439938
Conc: 36.28 ng/ml