

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062118\
 Data File : P0046020.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 14:02
 Operator : SM/UA
 Sample : J3518-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EPE-106-7(65-67)

Manual Integrations
 APPROVED

UGO
 6/22/2018 3:44:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 14:15:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 20 03:39:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.382	3.610	4270033	2336752	8.930	9.295
2) SA Decachlor...	10.058	8.587	2161514	954422	5.157	6.094m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\PO062118\
Data File : PO046020.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 14:02
Operator : SM/UA
Sample : J3518-03
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EPE-106-7(65-67)


Manual Integrations
APPROVED

UGO
6/22/2018 3:44:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 14:15:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

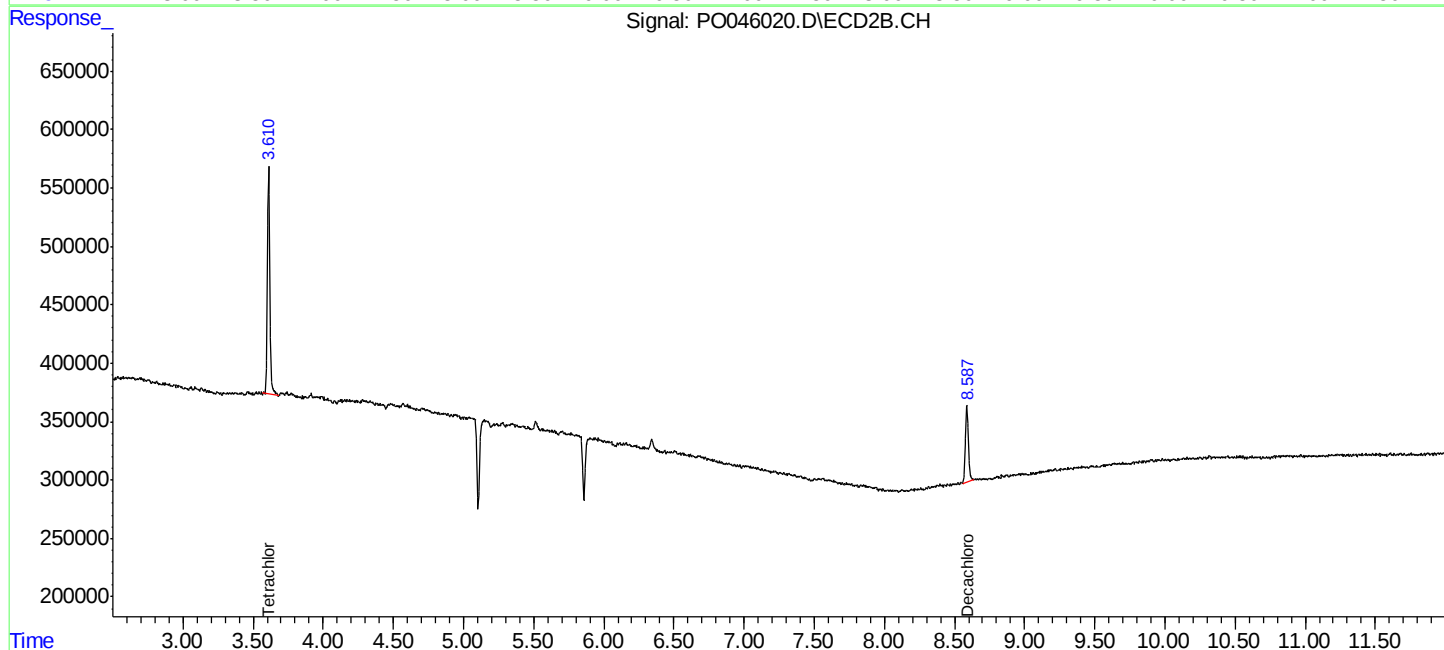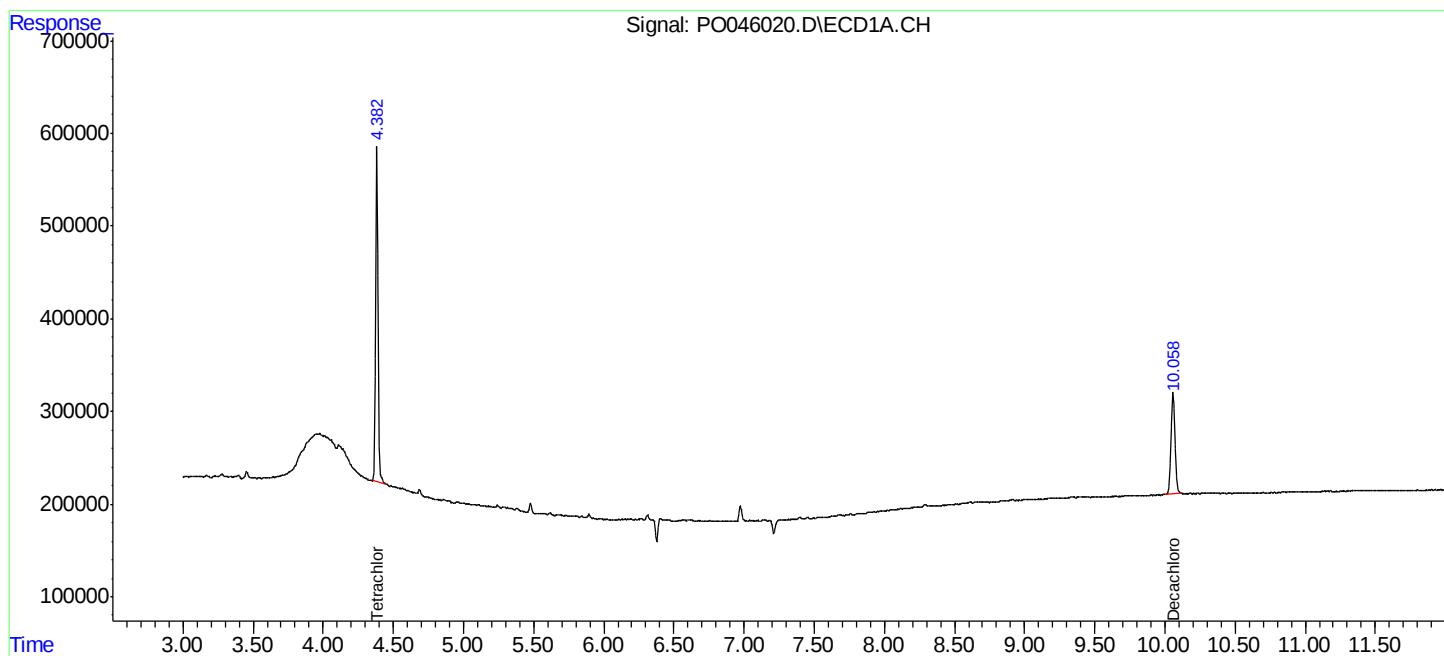

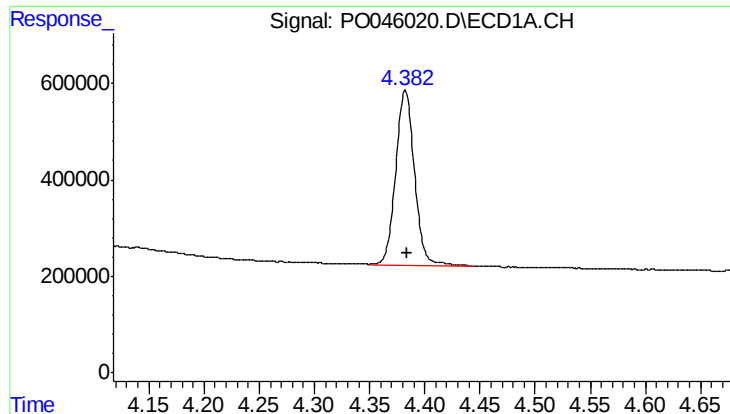


#1 Tetrachloro-m-xylene

R.T.: 4.382 min
Delta R.T.: -0.001 min
Response: 4270033
Conc: 8.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
EPE-106-7(65-67)


Manual Integrations
APPROVED

UGO
6/22/2018 3:44:43 PM

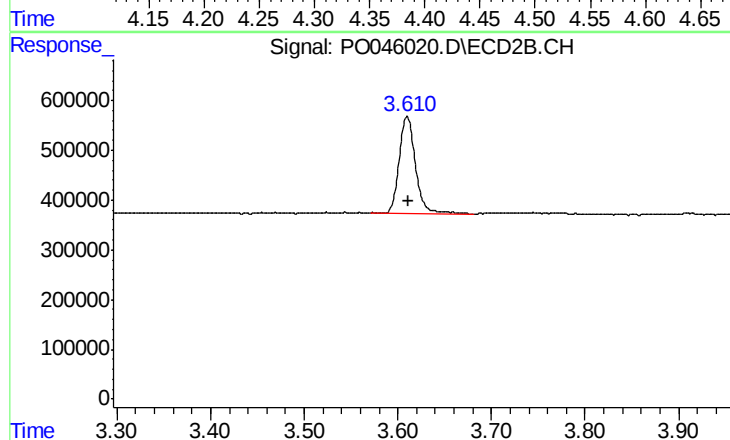


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: -0.002 min
Response: 2336752
Conc: 9.30 ng/ml

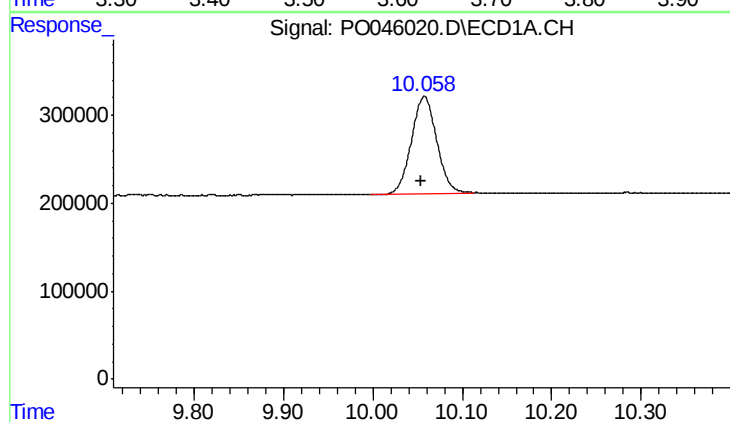

#2 Decachlorobiphenyl

R.T.: 10.058 min
Delta R.T.: 0.004 min
Response: 2161514
Conc: 5.16 ng/ml

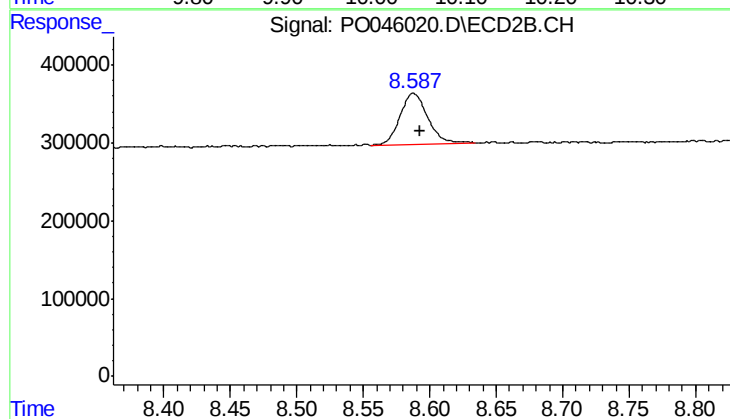

#2 Decachlorobiphenyl

R.T.: 8.587 min
Delta R.T.: -0.006 min
Response: 954422
Conc: 6.09 ng/ml m