

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062118\
Data File : P0046030.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 17:19
Operator : SM/UA
Sample : J3584-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-1-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 17:38:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.383	3.611	9702434	4700177	20.290	18.696
2) SA Decachlor...	10.055	8.587	5734219	2362974	13.680	15.088

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062118\
Data File : P0046030.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 17:19
Operator : SM/UA
Sample : J3584-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-1-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 17:38:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

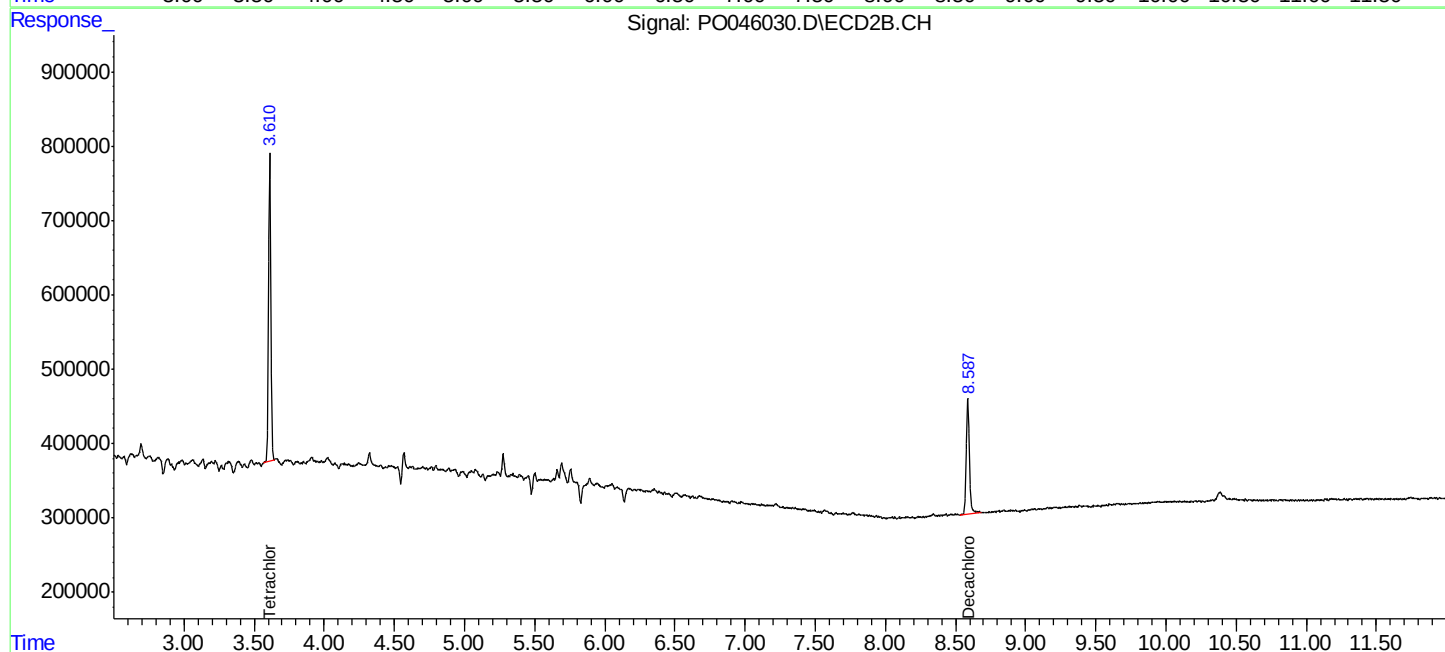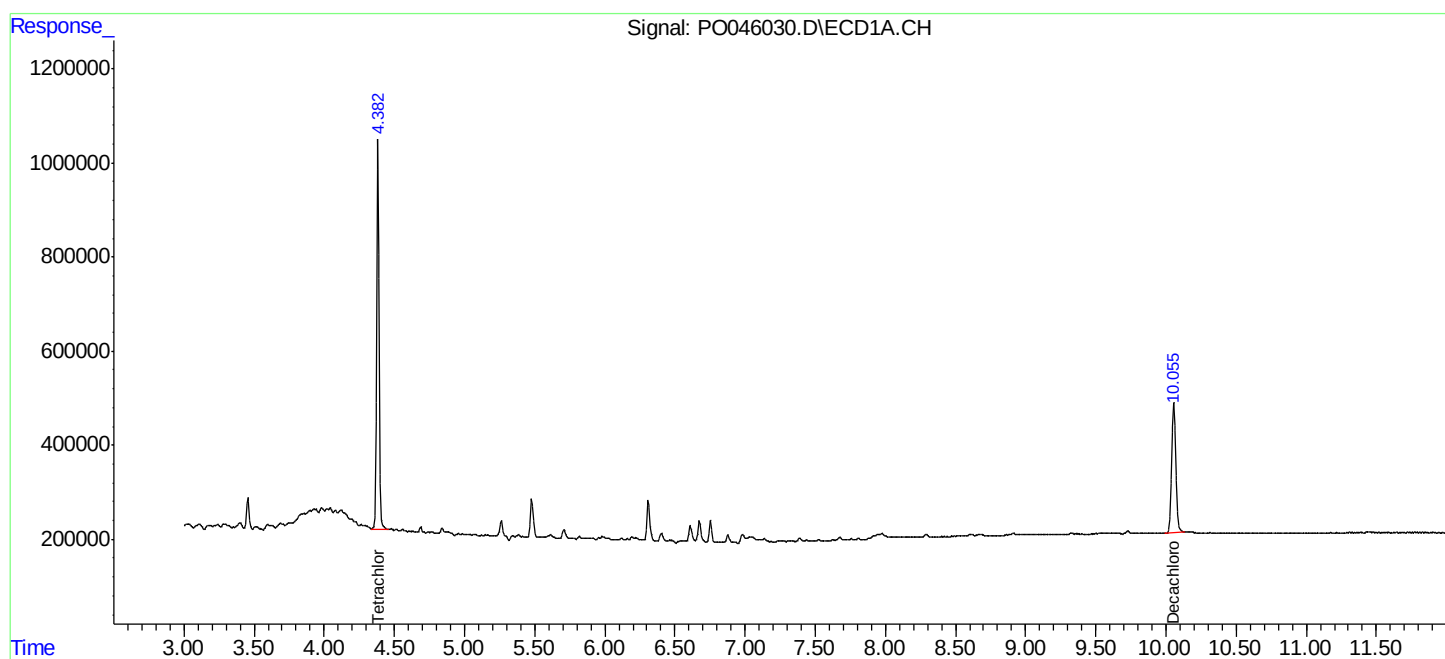


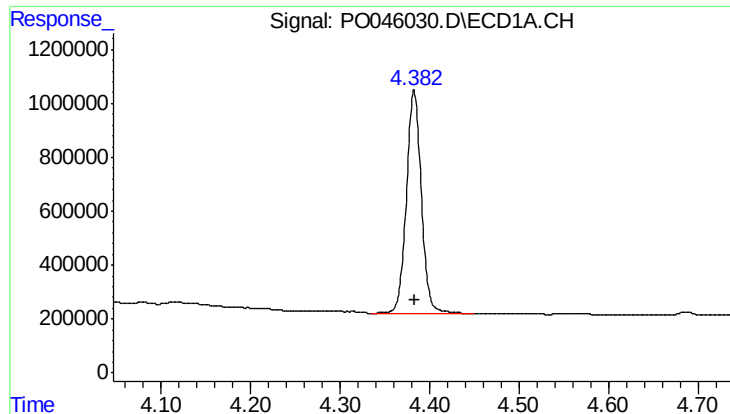

#1 Tetrachloro-m-xylene


R.T.: 4.383 min
Delta R.T.: -0.001 min
Response: 9702434
Conc: 20.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1-S

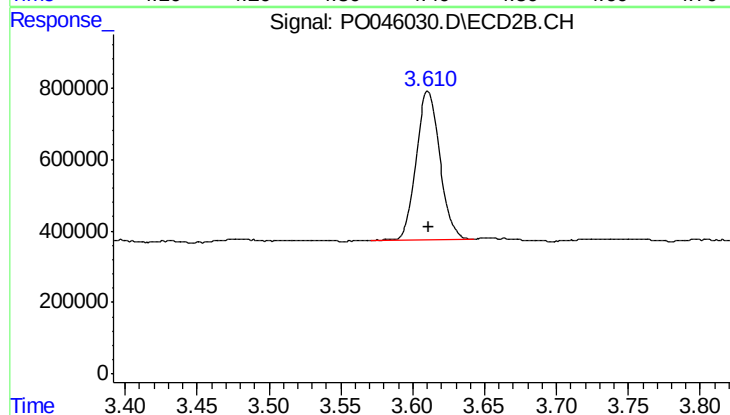


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: 0.000 min
Response: 4700177
Conc: 18.70 ng/ml

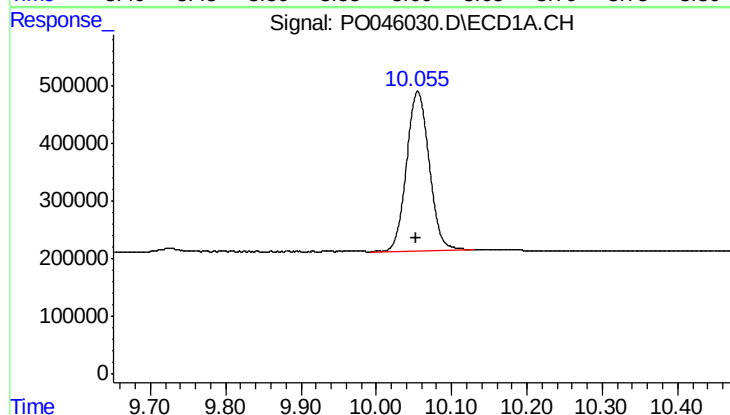

#2 Decachlorobiphenyl

R.T.: 10.055 min
Delta R.T.: 0.002 min
Response: 5734219
Conc: 13.68 ng/ml

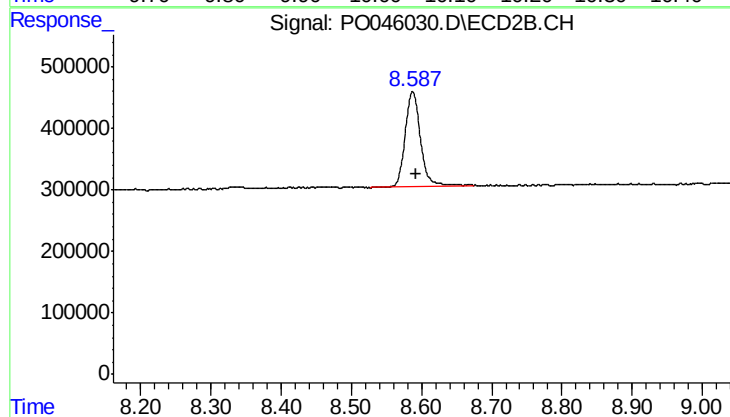

#2 Decachlorobiphenyl

R.T.: 8.587 min
Delta R.T.: -0.006 min
Response: 2362974
Conc: 15.09 ng/ml