

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062118\
Data File : P0046040.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 20:02
Operator : SM/UA
Sample : J3245-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CL-02-061918-B

Manual Integrations
APPROVED

UGO
6/22/2018 3:44:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 03:54:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.384	3.613	7883937	4602328	16.487	18.307
2)	SA Decachlor...	10.056	8.588	4886914	1525500	11.659	9.741m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062118\
Data File : P0046040.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 20:02
Operator : SM/UA
Sample : J3245-11
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-02-061918-B


Manual Integrations
APPROVED

UGO
6/22/2018 3:44:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 03:54:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

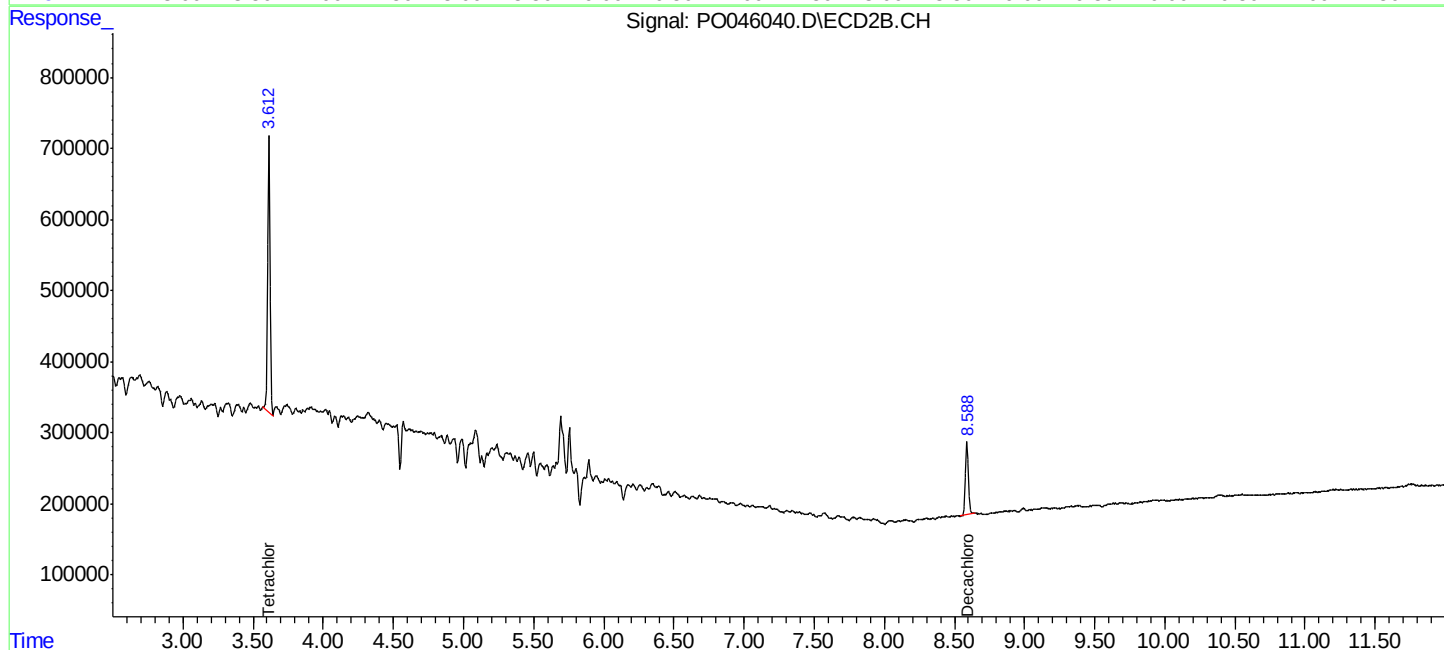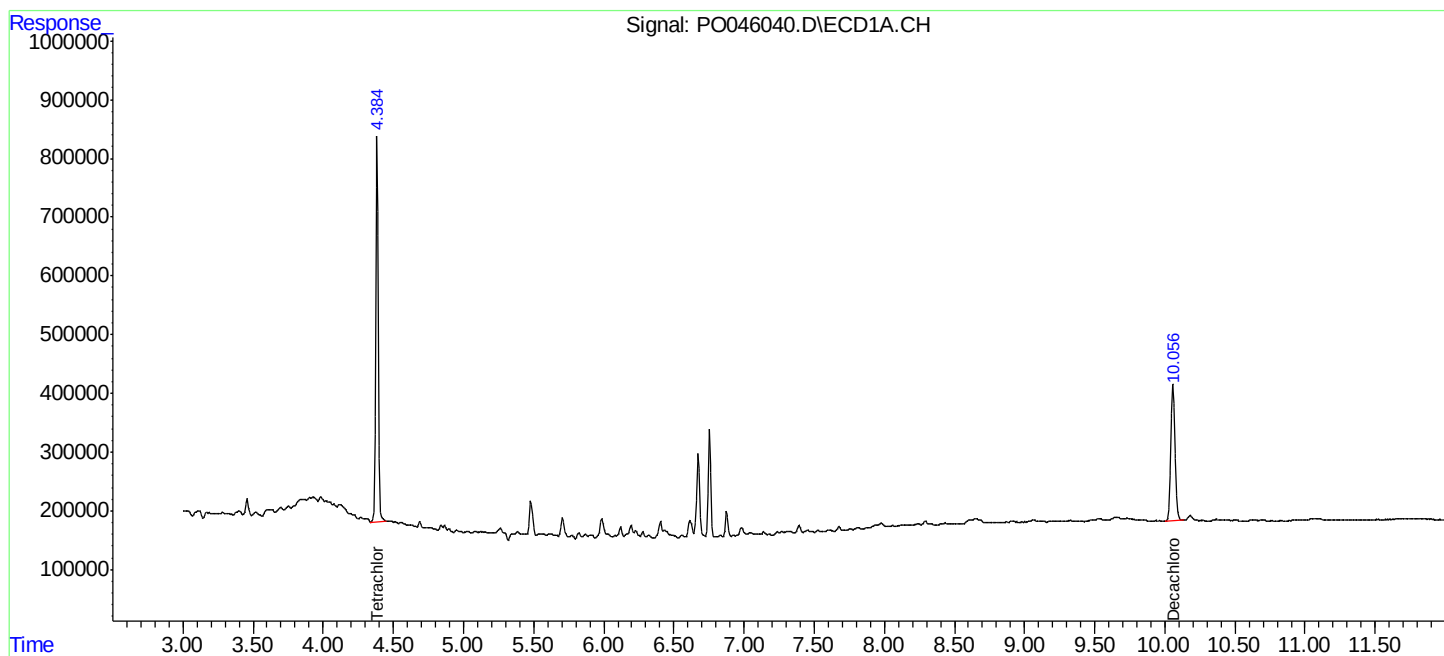

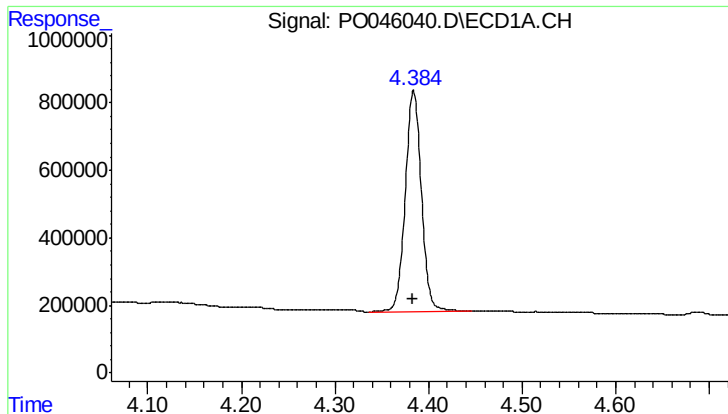


#1 Tetrachloro-m-xylene

R.T.: 4.384 min
Delta R.T.: 0.000 min
Response: 7883937
Conc: 16.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-02-061918-B


Manual Integrations
APPROVED

UGO
6/22/2018 3:44:01 PM

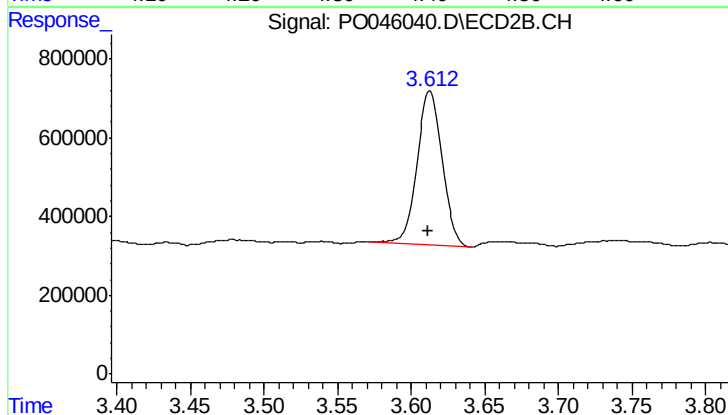


#1 Tetrachloro-m-xylene

R.T.: 3.613 min
Delta R.T.: 0.000 min
Response: 4602328
Conc: 18.31 ng/ml

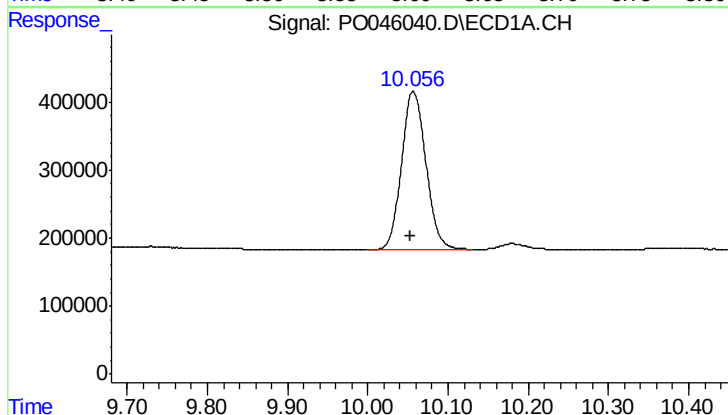

#2 Decachlorobiphenyl

R.T.: 10.056 min
Delta R.T.: 0.003 min
Response: 4886914
Conc: 11.66 ng/ml

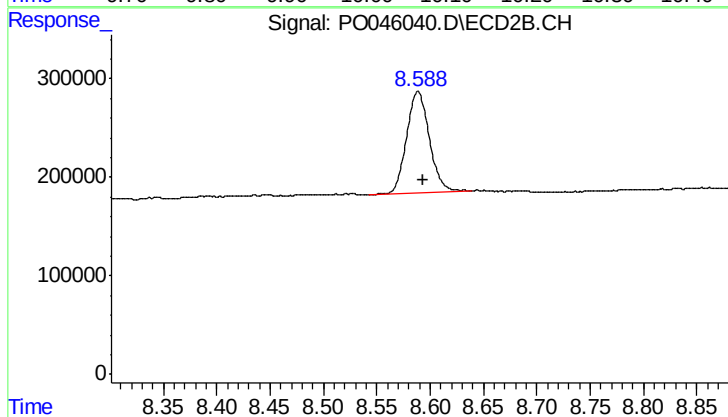

#2 Decachlorobiphenyl

R.T.: 8.588 min
Delta R.T.: -0.005 min
Response: 1525500
Conc: 9.74 ng/ml m