

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0062118\
 Data File : P0046041.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 20:18
 Operator : SM/UA
 Sample : J3245-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-061918-C

Manual Integrations
 APPROVED

UGO
 6/22/2018 3:43:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 04:01:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 20 03:39:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.386	3.613	7674088	4631559	16.048	18.423
2) SA Decachlor...	10.060	8.590	4865755	1564446	11.608	9.989m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062118\
Data File : P0046041.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 20:18
Operator : SM/UA
Sample : J3245-13
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-02-061918-C


Manual Integrations
APPROVED

UGO
6/22/2018 3:43:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 04:01:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

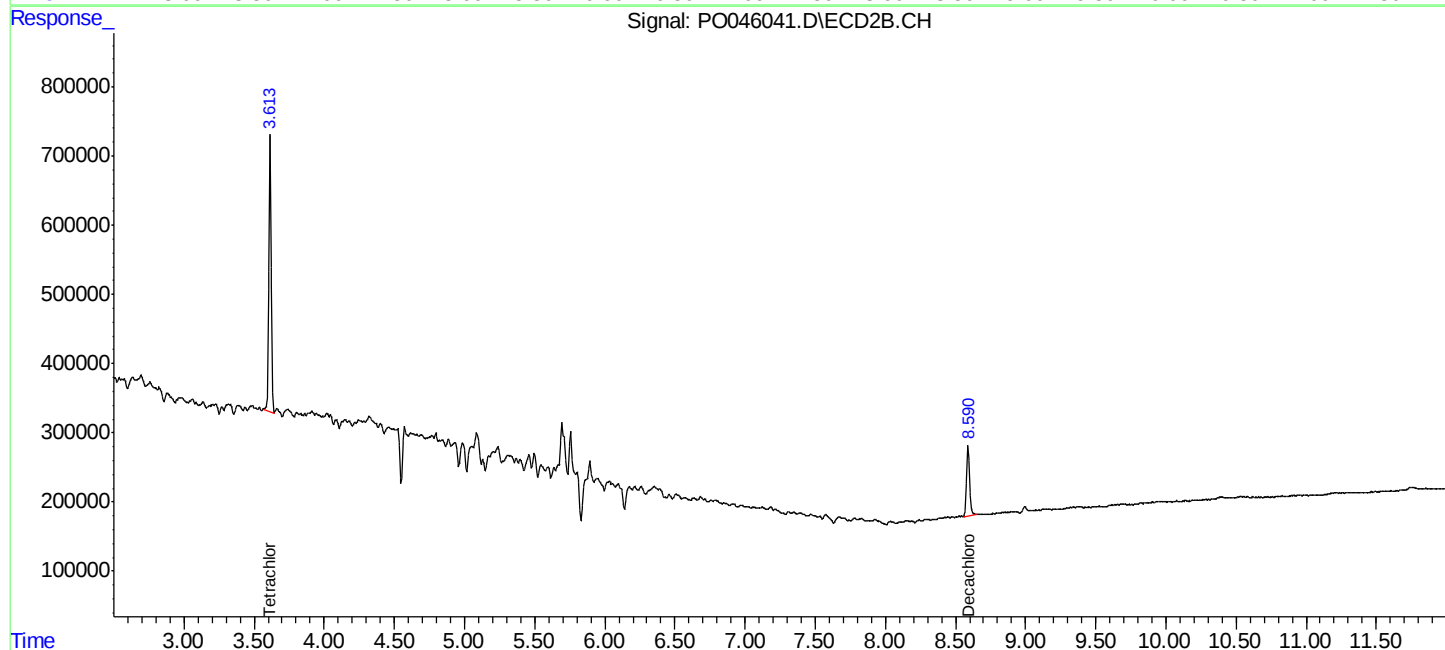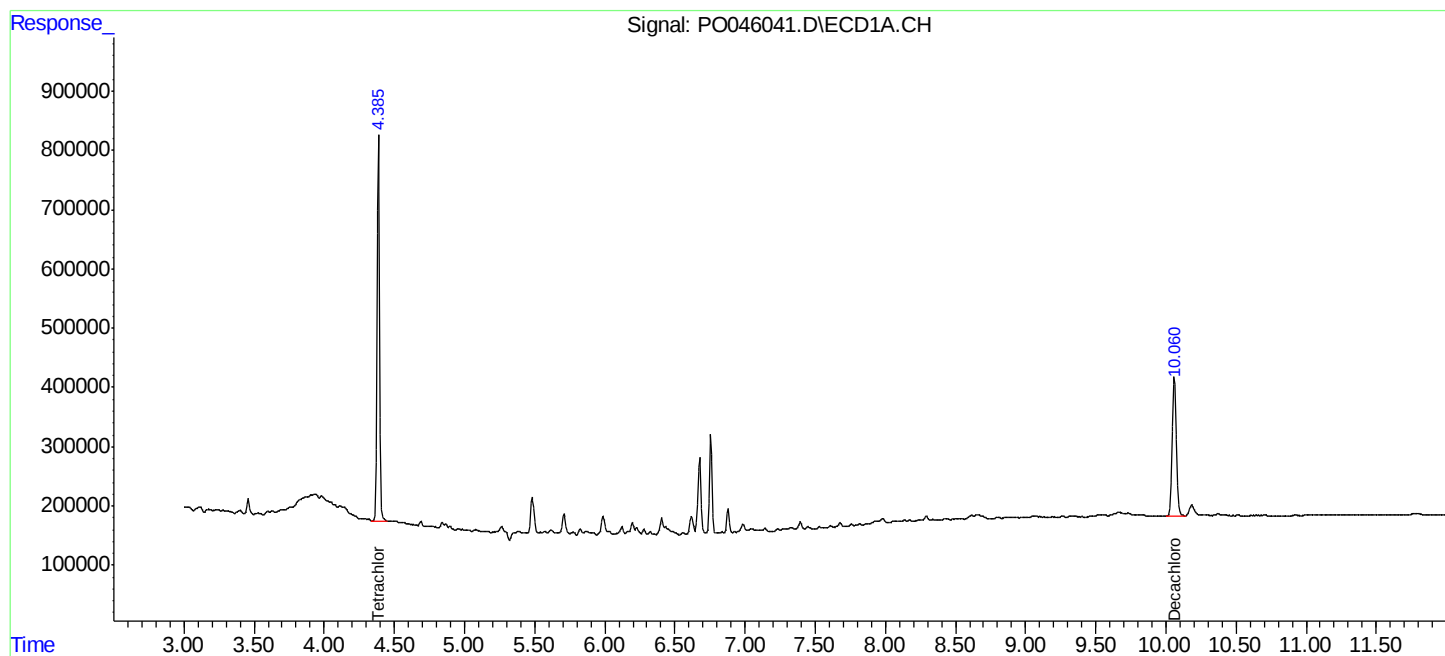

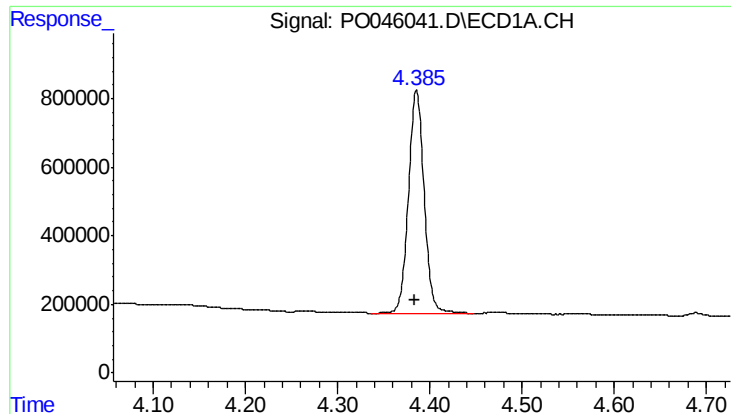


#1 Tetrachloro-m-xylene

R.T.: 4.386 min
Delta R.T.: 0.002 min
Response: 7674088
Conc: 16.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-02-061918-C


Manual Integrations
APPROVED

UGO
6/22/2018 3:43:58 PM

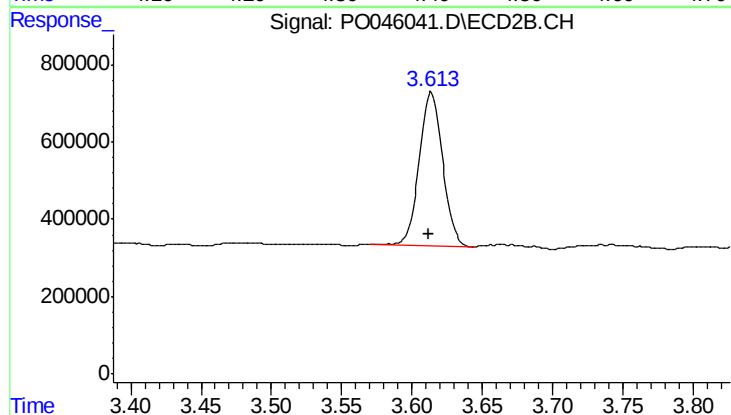


#1 Tetrachloro-m-xylene

R.T.: 3.613 min
Delta R.T.: 0.002 min
Response: 4631559
Conc: 18.42 ng/ml

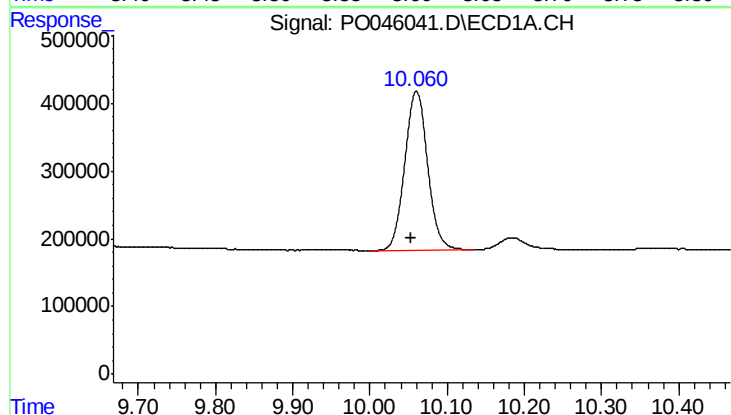

#2 Decachlorobiphenyl

R.T.: 10.060 min
Delta R.T.: 0.007 min
Response: 4865755
Conc: 11.61 ng/ml

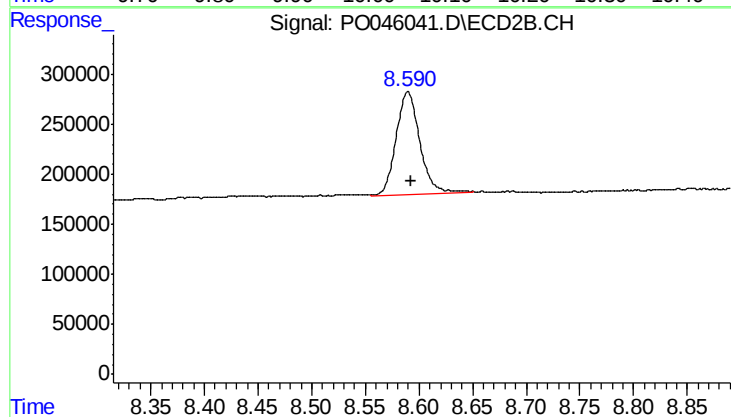

#2 Decachlorobiphenyl

R.T.: 8.590 min
Delta R.T.: -0.004 min
Response: 1564446
Conc: 9.99 ng/ml m