

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0062118\
 Data File : P0046051.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2018 23:30
 Operator : SM/UA
 Sample : J3603-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 26KV-TP-9

Manual Integrations
 APPROVED

UGO
 6/22/2018 3:43:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 13:56:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 20 03:39:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.384	3.611	8003262	3842607	16.737	15.285
2) SA Decachlor...	10.057	8.587	4085467	1752456	9.747	11.190
Target Compounds						
41) L9 AR-1268-1	8.597	7.498	6516609	2950107	102.688	116.939
42) L9 AR-1268-2	8.687	7.562	6940840	4172259	115.129	173.426 #
43) L9 AR-1268-3	8.912	7.769	1629317	977086	32.294	50.132 #
44) L9 AR-1268-4	9.322	8.053	4894722	2419670	255.123	281.376
45) L9 AR-1268-5	9.728	8.338	12313754	4925785	78.277	92.703

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062118\
Data File : P0046051.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2018 23:30
Operator : SM/UA
Sample : J3603-15
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
26KV-TP-9


Manual Integrations
APPROVED

UGO
6/22/2018 3:43:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 13:56:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

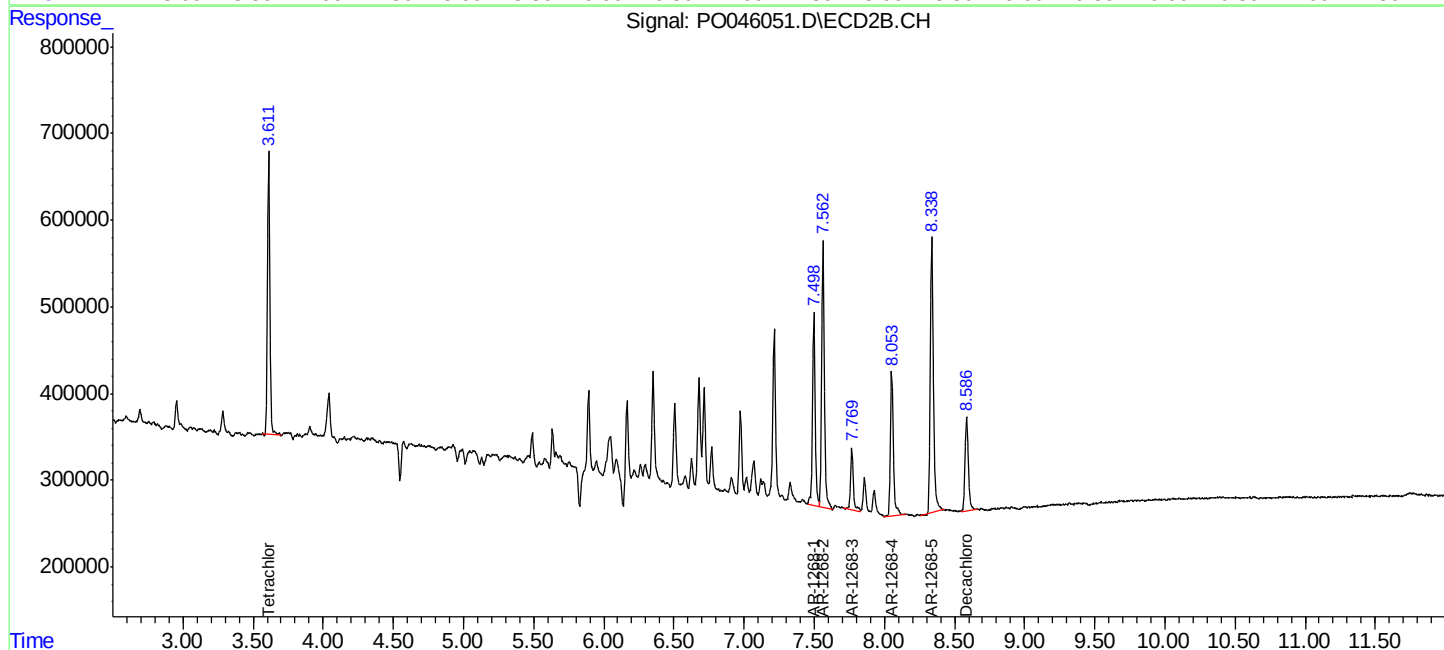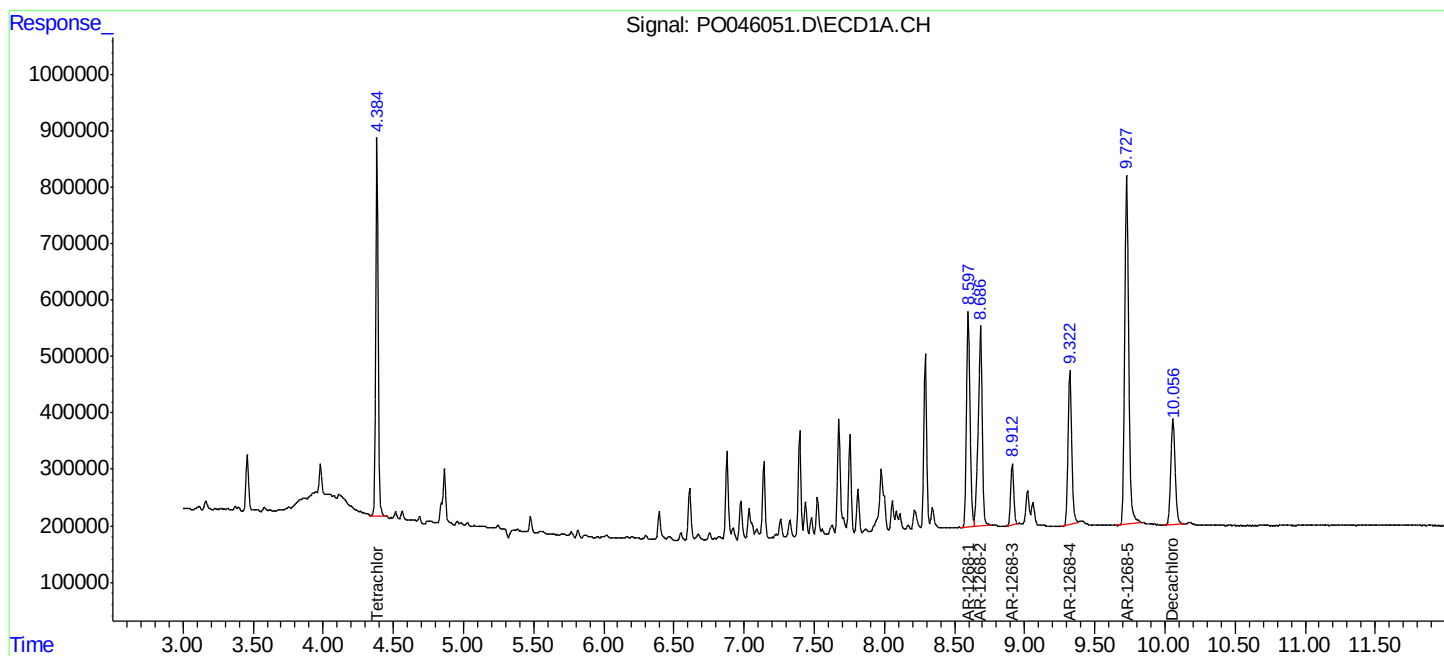

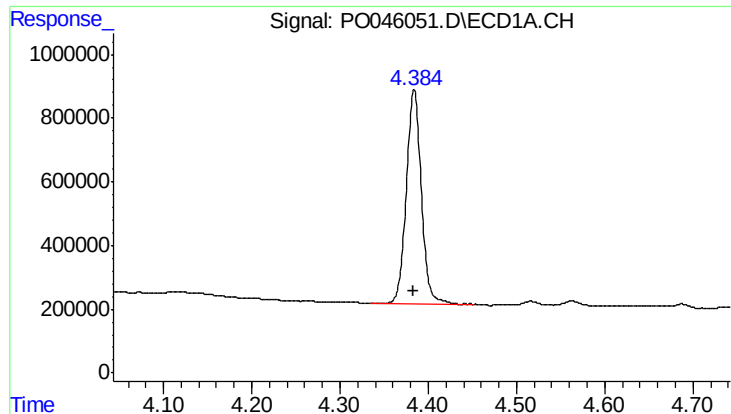


#1 Tetrachloro-m-xylene

R.T.: 4.384 min
Delta R.T.: 0.000 min
Response: 8003262
Conc: 16.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
26KV-TP-9


Manual Integrations
APPROVED

UGO
6/22/2018 3:43:23 PM

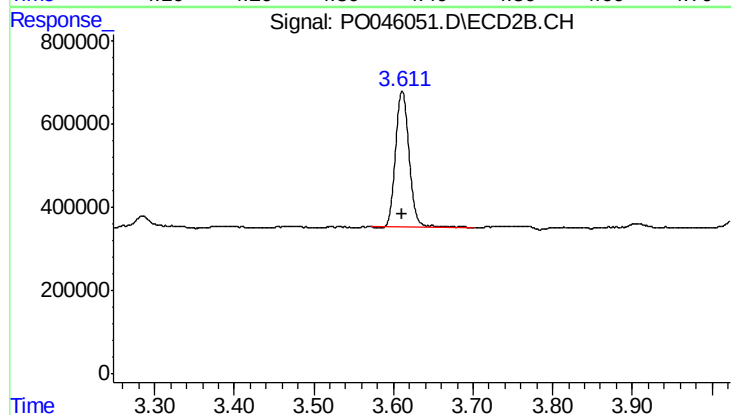


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: 0.000 min
Response: 3842607
Conc: 15.29 ng/ml

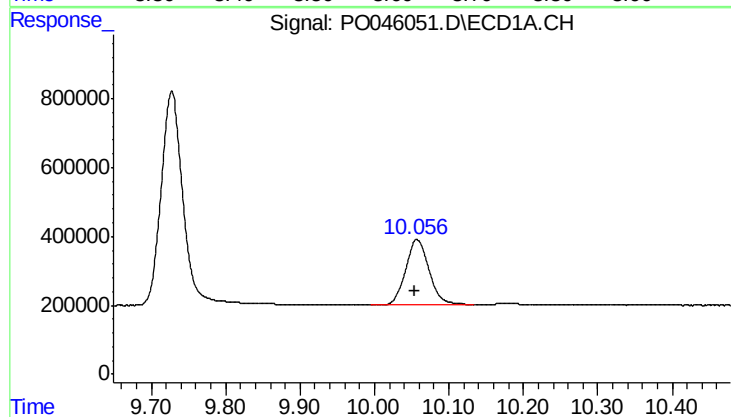


#2 Decachlorobiphenyl

R.T.: 10.057 min
Delta R.T.: 0.003 min
Response: 4085467
Conc: 9.75 ng/ml

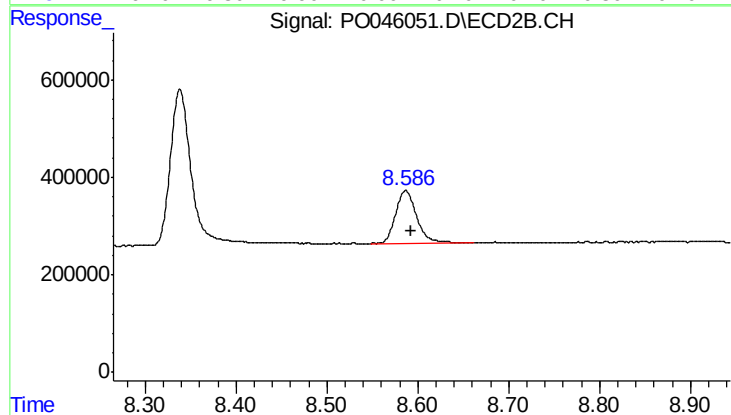

#2 Decachlorobiphenyl

R.T.: 8.587 min
Delta R.T.: -0.006 min
Response: 1752456
Conc: 11.19 ng/ml

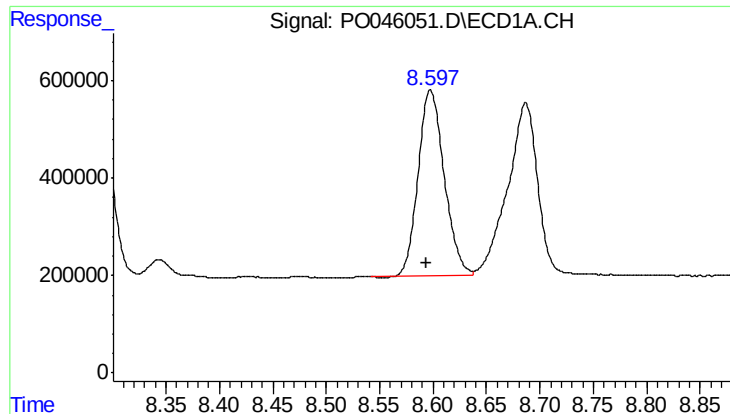


#41 AR-1268-1

R.T.: 8.597 min
Delta R.T.: 0.003 min
Response: 6516609
Conc: 102.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
26KV-TP-9


Manual Integrations
APPROVED

UGO
6/22/2018 3:43:23 PM

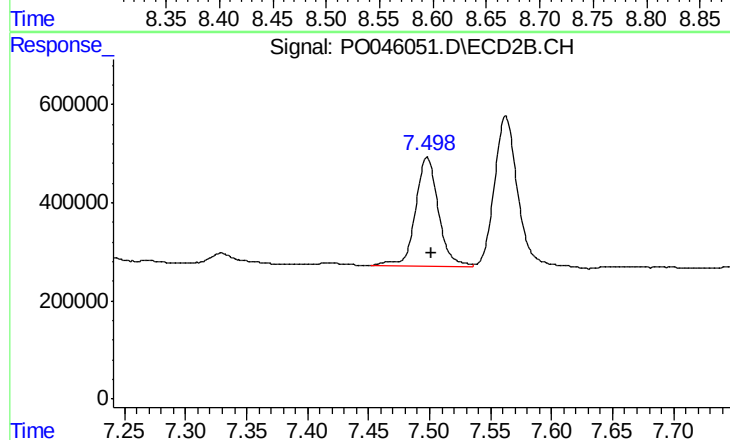


#41 AR-1268-1

R.T.: 7.498 min
Delta R.T.: -0.004 min
Response: 2950107
Conc: 116.94 ng/ml

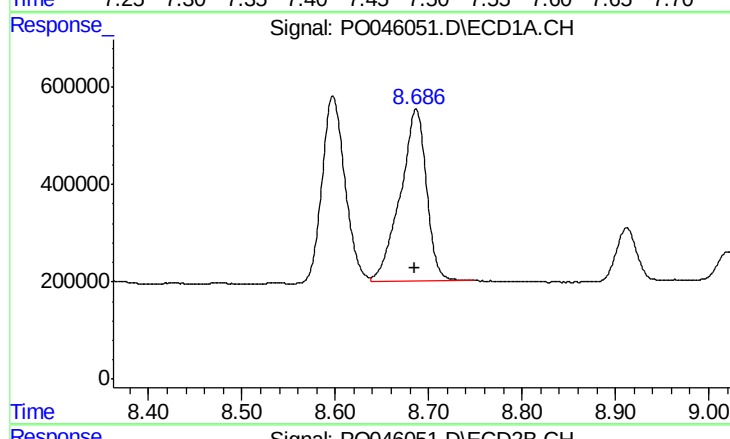


#42 AR-1268-2

R.T.: 8.687 min
Delta R.T.: 0.000 min
Response: 6940840
Conc: 115.13 ng/ml

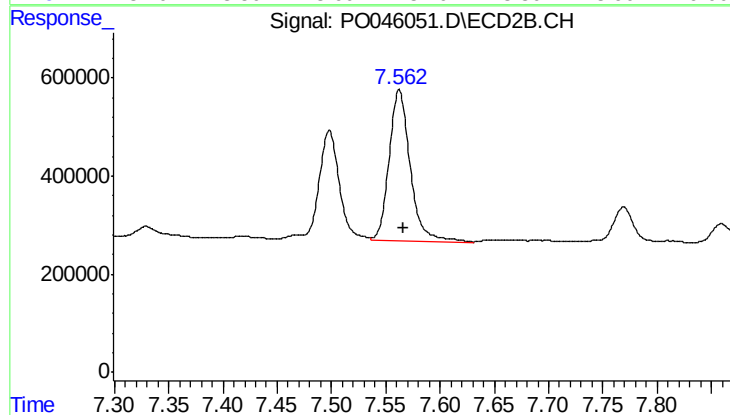

#42 AR-1268-2

R.T.: 7.562 min
Delta R.T.: -0.004 min
Response: 4172259
Conc: 173.43 ng/ml

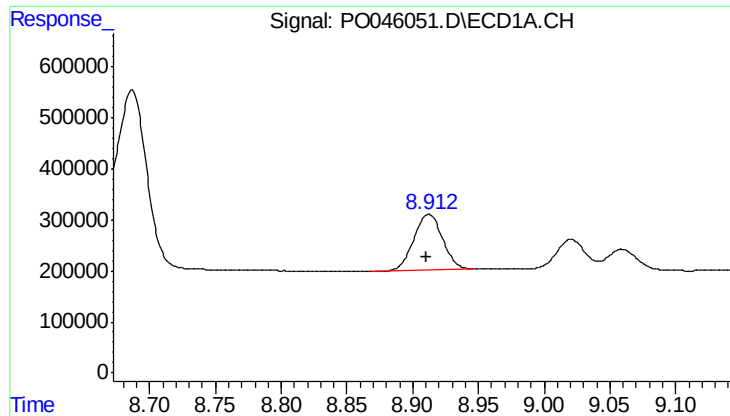


#43 AR-1268-3

R.T.: 8.912 min
Delta R.T.: 0.002 min
Response: 1629317
Conc: 32.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
26KV-TP-9


Manual Integrations
APPROVED

UGO
6/22/2018 3:43:23 PM

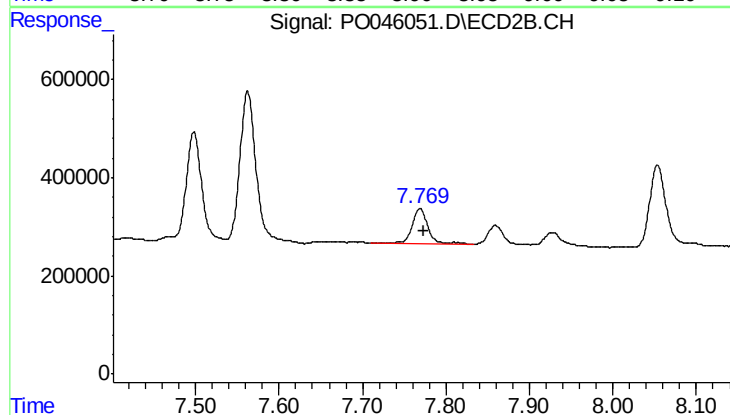


#43 AR-1268-3

R.T.: 7.769 min
Delta R.T.: -0.005 min
Response: 977086
Conc: 50.13 ng/ml

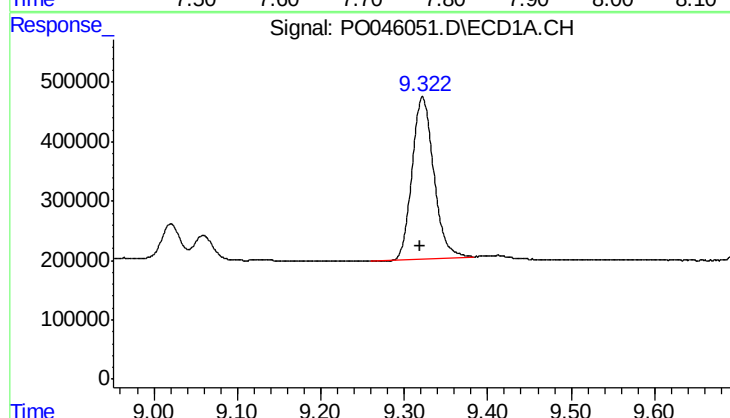


#44 AR-1268-4

R.T.: 9.322 min
Delta R.T.: 0.003 min
Response: 4894722
Conc: 255.12 ng/ml

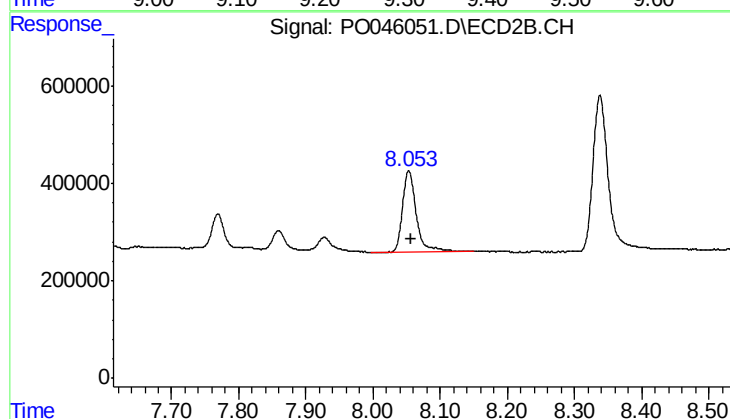

#44 AR-1268-4

R.T.: 8.053 min
Delta R.T.: -0.003 min
Response: 2419670
Conc: 281.38 ng/ml

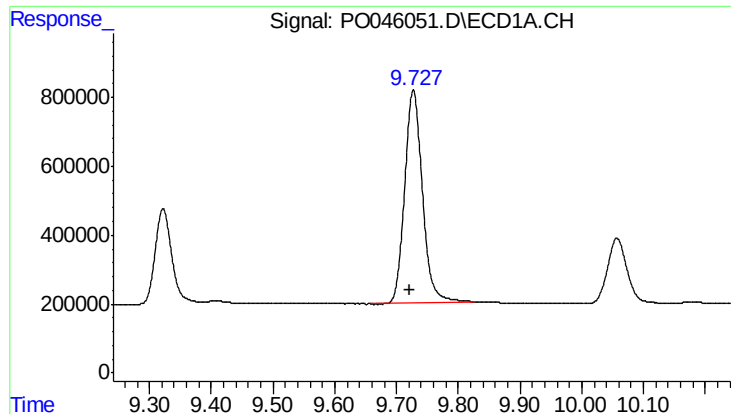


#45 AR-1268-5

R.T.: 9.728 min
Delta R.T.: 0.005 min
Response: 12313754
Conc: 78.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
26KV-TP-9

Manual Integrations
APPROVED

UGO
6/22/2018 3:43:23 PM

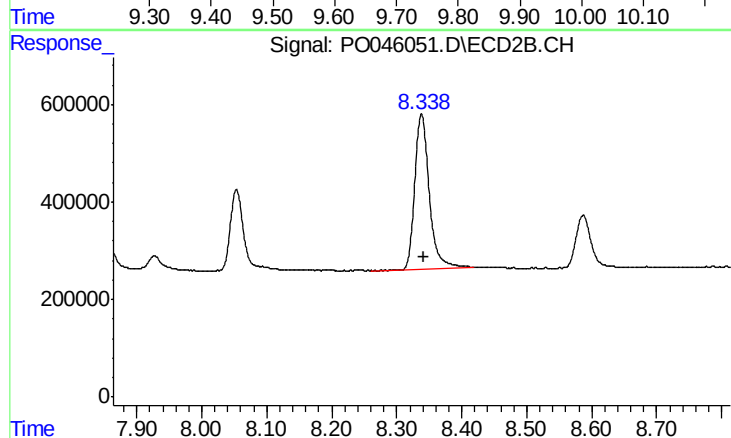

#45 AR-1268-5

R.T.: 8.338 min
Delta R.T.: -0.004 min
Response: 4925785
Conc: 92.70 ng/ml