

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062119\
 Data File : P0057360.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2019 11:58
 Operator : SM/SJ
 Sample : K3458-07DL 2X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 POST-CARTRIDGE-FILTERDL

Manual Integrations
 APPROVED

Ankita
 6/21/2019 5:08:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 12:39:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.232	3.557	346045	274038	9.039	8.310
2)	SA Decachlor...	9.786	8.480	253785	163539	5.170m	4.586m
Target Compounds							
21)	L5 AR-1248-1	5.392	4.622	337508	291906	261.936m	311.693m
22)	L5 AR-1248-2	5.661	4.855	530685	514275	284.871m	404.799m#
23)	L5 AR-1248-3	5.864	4.895	815924	537581	397.749	411.655m
24)	L5 AR-1248-4	6.264	5.066	1238575	689312	535.326m	435.274m
25)	L5 AR-1248-5	6.302	5.453	1396107	1084576	634.772m	655.305m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062119\
Data File : PO057360.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2019 11:58
Operator : SM/SJ
Sample : K3458-07DL 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleID :
POST-CARTRIDGE-FILTERDL


Manual Integrations
APPROVED

Ankita
6/21/2019 5:08:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 12:39:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

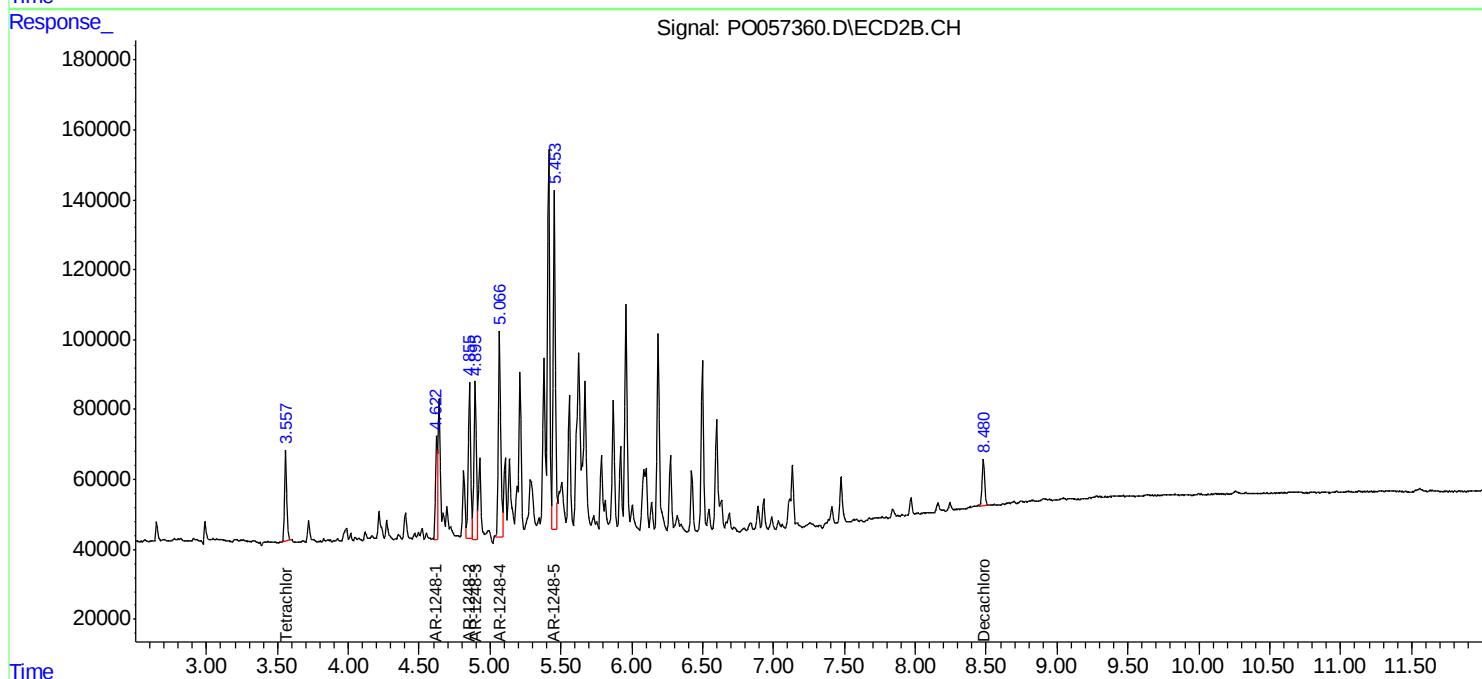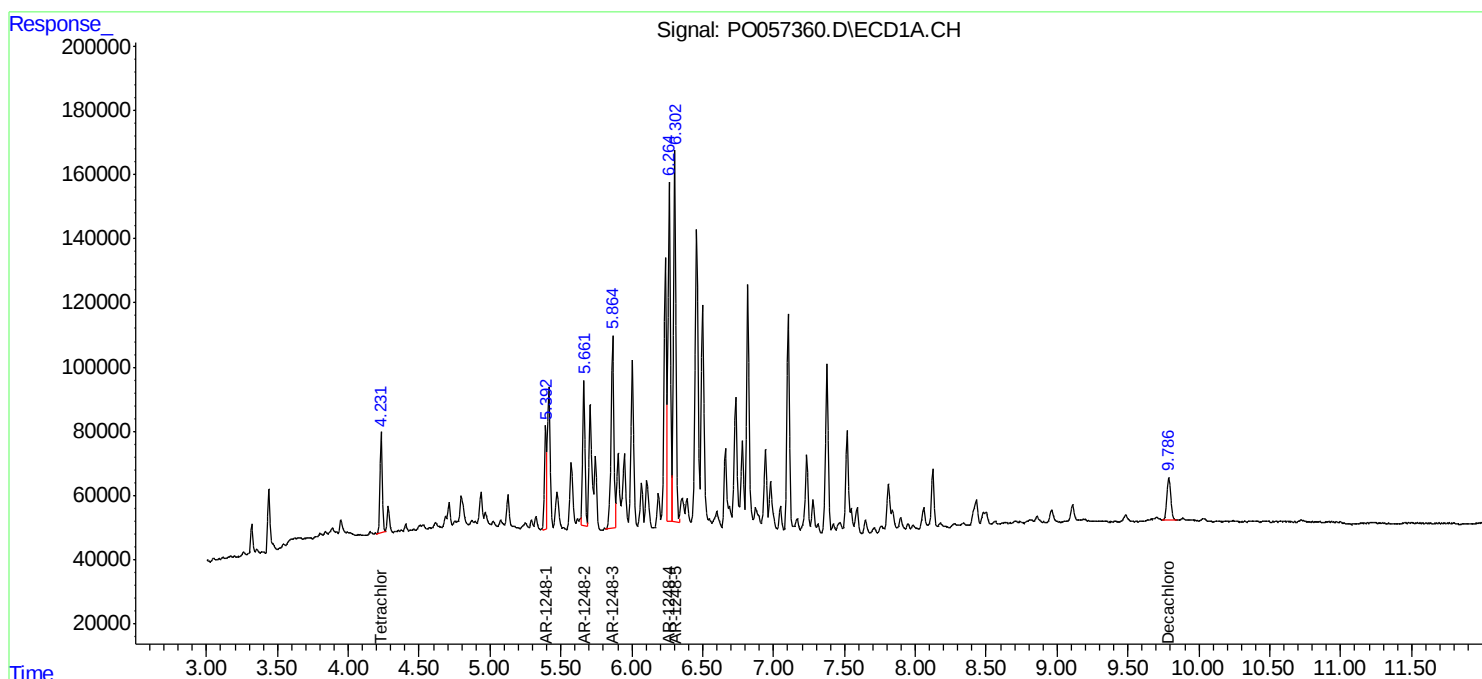

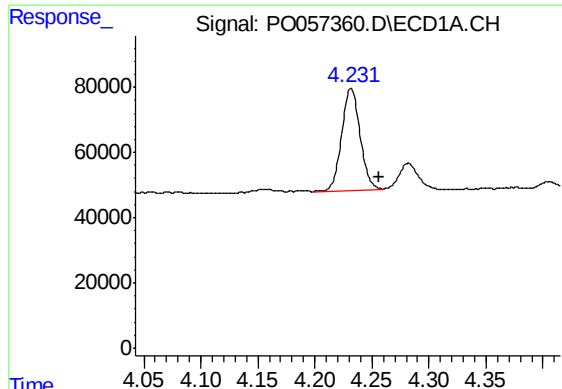


#1 Tetrachloro-m-xylene

R.T.: 4.232 min
Delta R.T.: -0.024 min
Response: 346045
Conc: 9.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
POST-CARTRIDGE-FILTERDL


Manual Integrations
APPROVED

Ankita
6/21/2019 5:08:33 PM

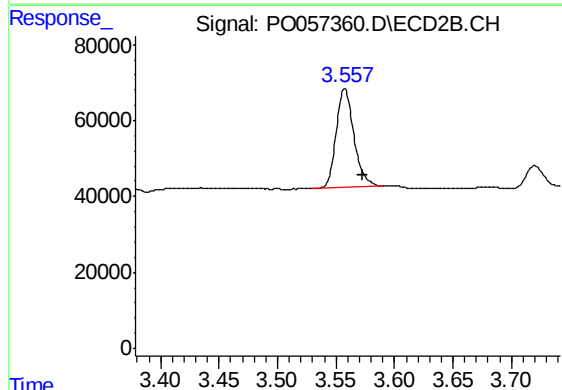


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: -0.016 min
Response: 274038
Conc: 8.31 ng/ml

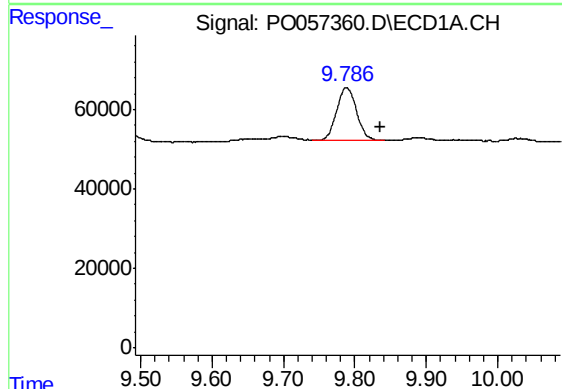


#2 Decachlorobiphenyl

R.T.: 9.786 min
Delta R.T.: -0.050 min
Response: 253785
Conc: 5.17 ng/ml m

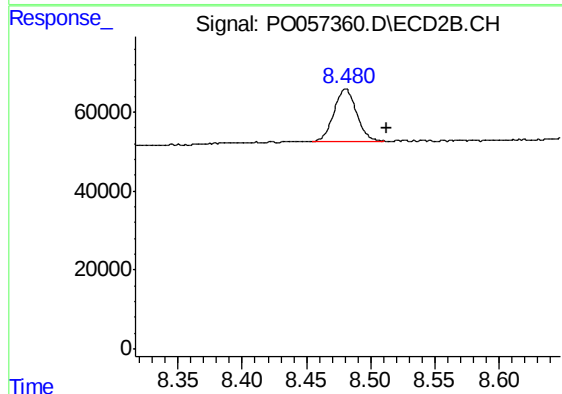

#2 Decachlorobiphenyl

R.T.: 8.480 min
Delta R.T.: -0.033 min
Response: 163539
Conc: 4.59 ng/ml m

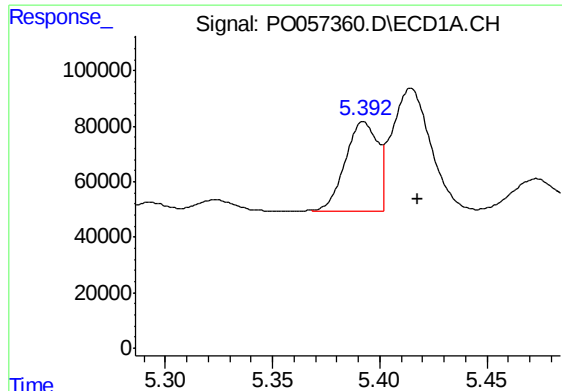


#21 AR-1248-1

R.T.: 5.392 min
Delta R.T.: -0.026 min
Response: 337508
Conc: 261.94 ng/ml m

Instrument :
ECD_O
ClientSampleId :
POST-CARTRIDGE-FILTERDL


Manual Integrations
APPROVED

Ankita
6/21/2019 5:08:33 PM

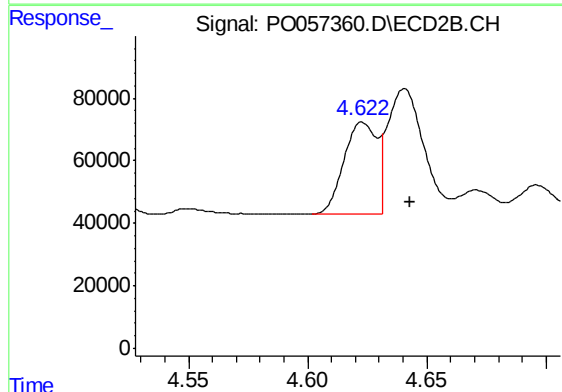


#21 AR-1248-1

R.T.: 4.622 min
Delta R.T.: -0.021 min
Response: 291906
Conc: 311.69 ng/ml m

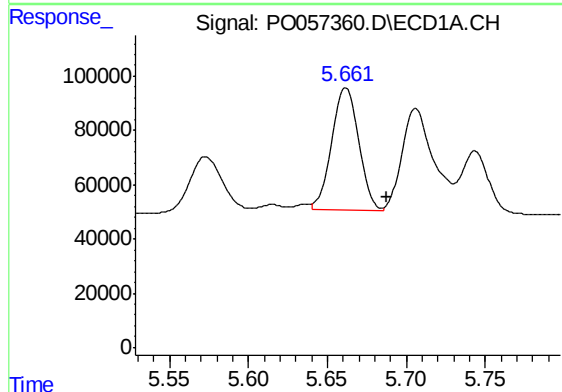


#22 AR-1248-2

R.T.: 5.661 min
Delta R.T.: -0.026 min
Response: 530685
Conc: 284.87 ng/ml m

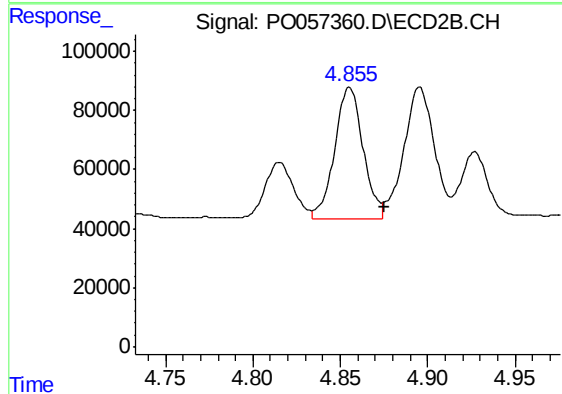

#22 AR-1248-2

R.T.: 4.855 min
Delta R.T.: -0.021 min
Response: 514275
Conc: 404.80 ng/ml m

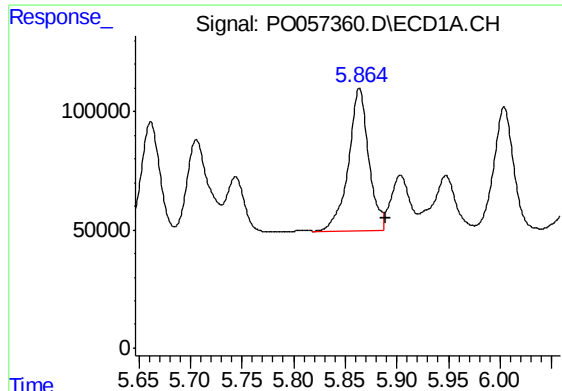


#23 AR-1248-3

R.T.: 5.864 min
Delta R.T.: -0.026 min
Response: 815924
Conc: 397.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
POST-CARTRIDGE-FILTERDL


Manual Integrations
APPROVED

Ankita
6/21/2019 5:08:33 PM

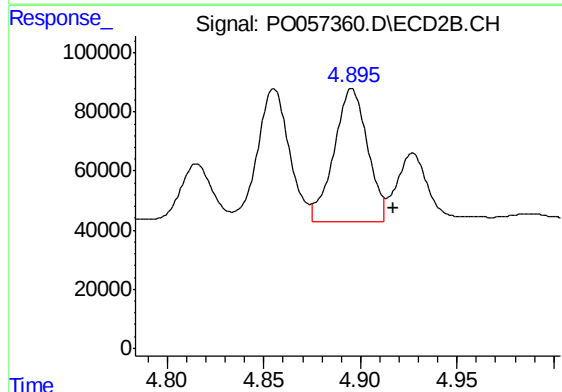


#23 AR-1248-3

R.T.: 4.895 min
Delta R.T.: -0.022 min
Response: 537581
Conc: 411.66 ng/ml m

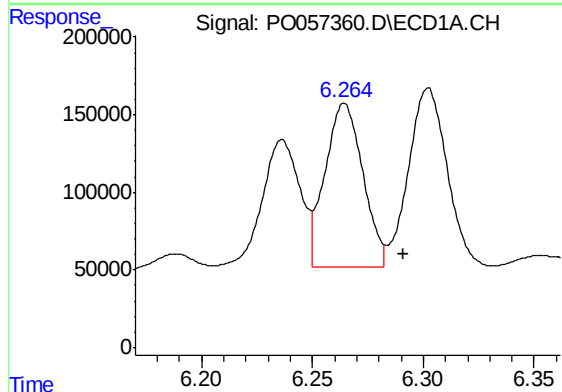


#24 AR-1248-4

R.T.: 6.264 min
Delta R.T.: -0.027 min
Response: 1238575
Conc: 535.33 ng/ml m

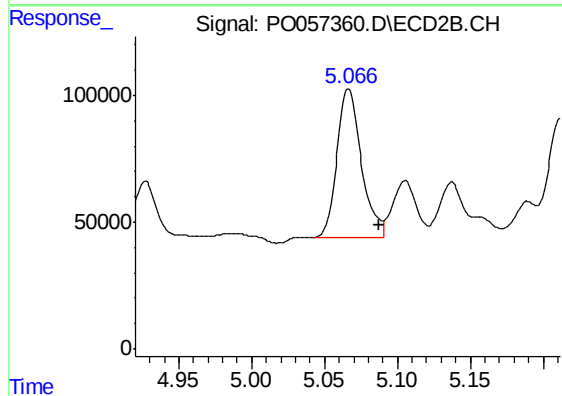

#24 AR-1248-4

R.T.: 5.066 min
Delta R.T.: -0.021 min
Response: 689312
Conc: 435.27 ng/ml m

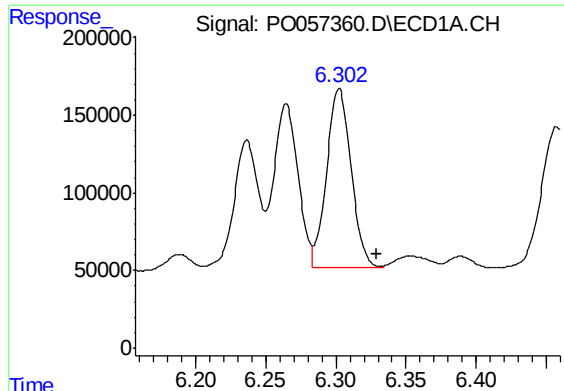


#25 AR-1248-5

R.T.: 6.302 min
Delta R.T.: -0.027 min
Response: 1396107
Conc: 634.77 ng/ml m

Instrument :
ECD_O
ClientSampleId :
POST-CARTRIDGE-FILTERDL

Manual Integrations
APPROVED

Ankita
6/21/2019 5:08:33 PM

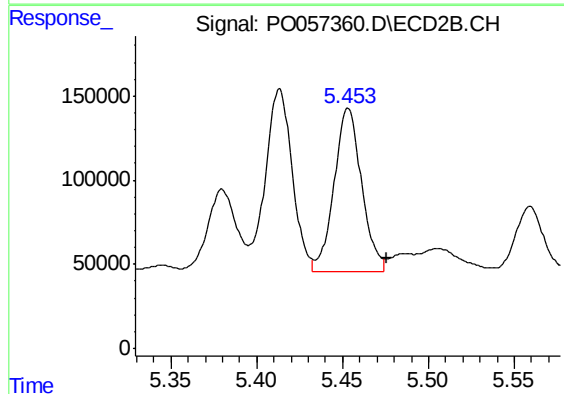

#25 AR-1248-5

R.T.: 5.453 min
Delta R.T.: -0.023 min
Response: 1084576
Conc: 655.30 ng/ml m