

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062119\
 Data File : P0057368.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2019 15:08
 Operator : SM/SJ
 Sample : PB120709BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB120709BL

Manual Integrations
 APPROVED

Ankita
 6/21/2019 5:08:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 15:27:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.231	3.556	825845	637388	21.572	19.327
2)	SA Decachlor...	9.787	8.478	871255	597544	17.750	16.758m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062119\
Data File : PO057368.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2019 15:08
Operator : SM/SJ
Sample : PB120709BL
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB120709BL


Manual Integrations
APPROVED

Ankita
6/21/2019 5:08:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 15:27:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

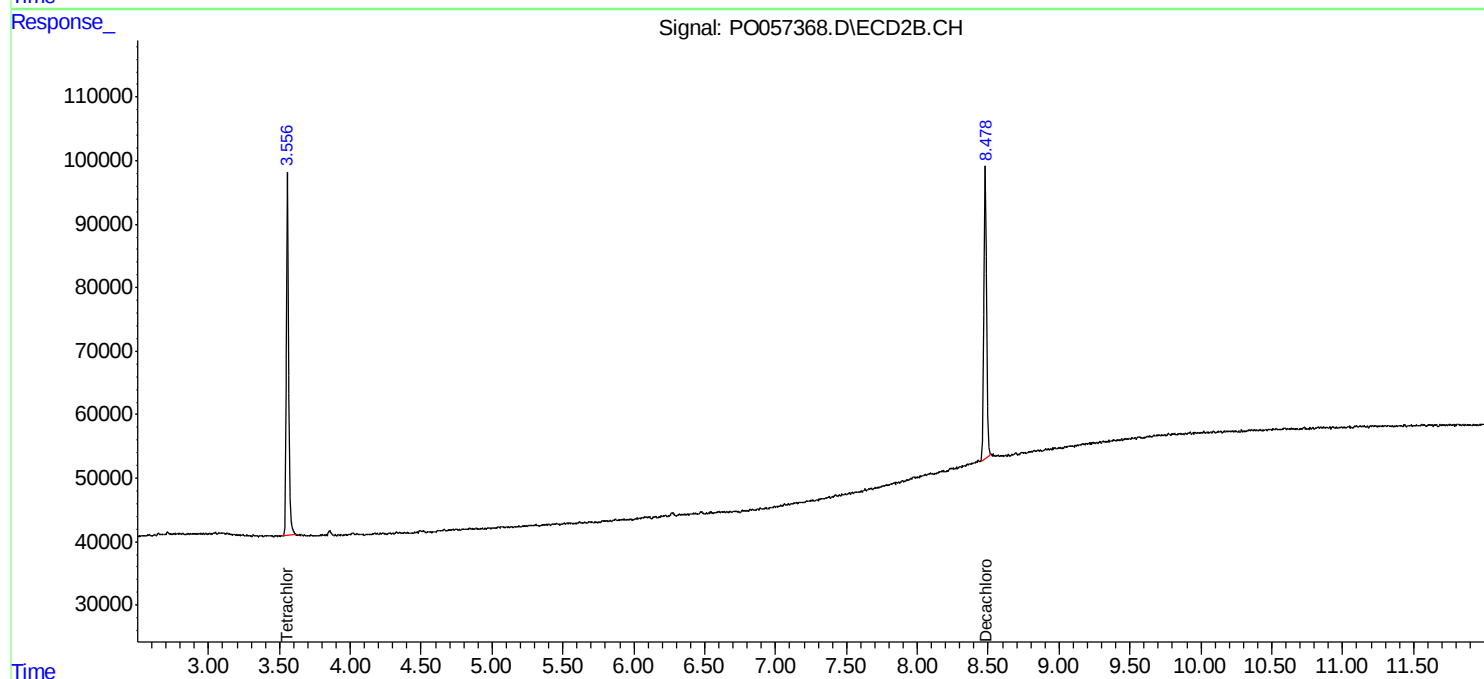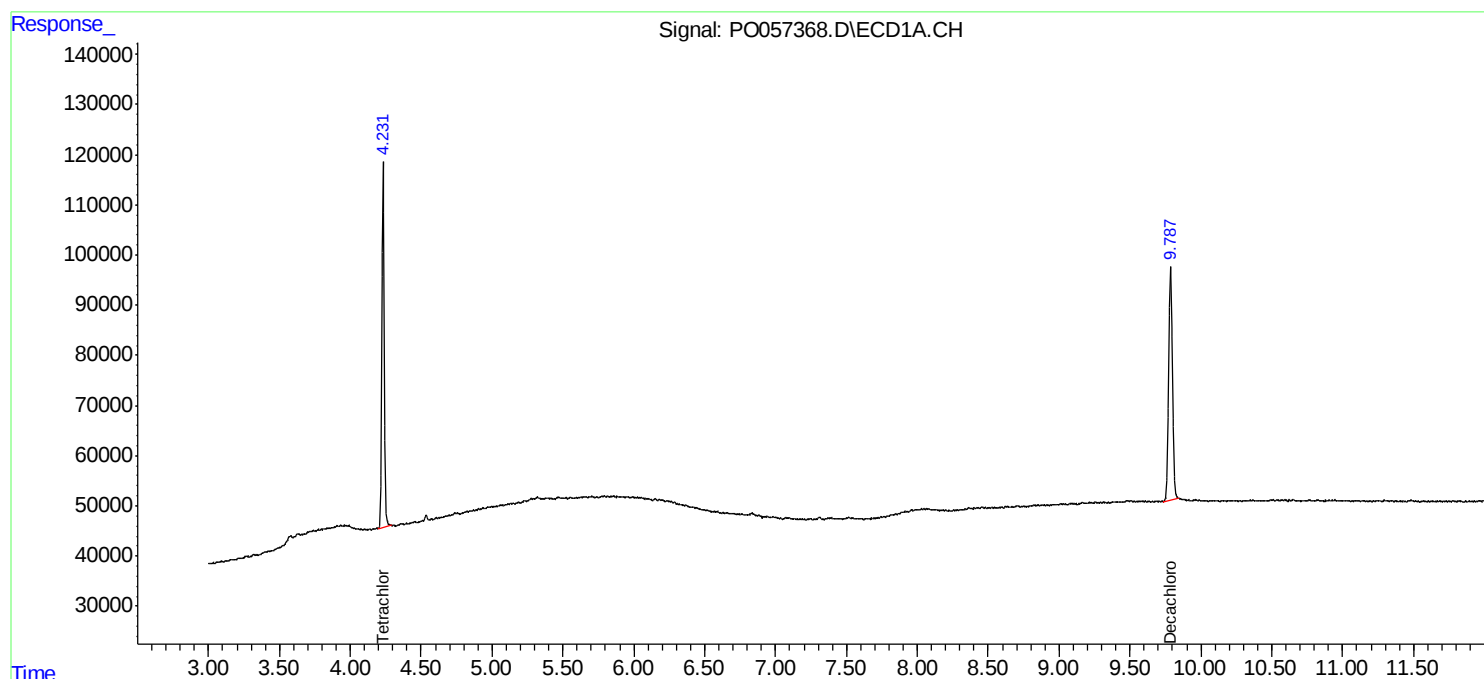

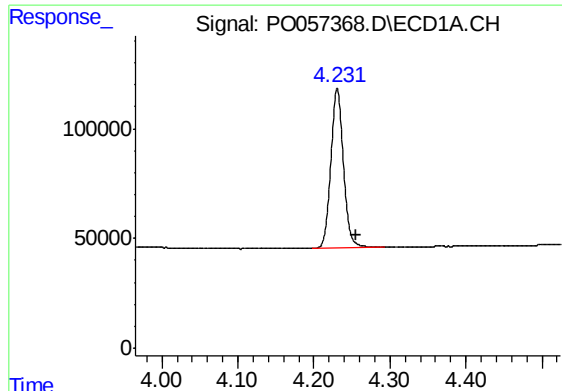


#1 Tetrachloro-m-xylene

R.T.: 4.231 min
Delta R.T.: -0.025 min
Response: 825845
Conc: 21.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB120709BL


Manual Integrations
APPROVED

Ankita
6/21/2019 5:08:48 PM

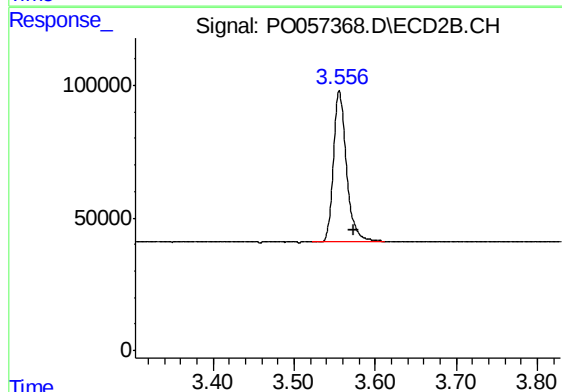


#1 Tetrachloro-m-xylene

R.T.: 3.556 min
Delta R.T.: -0.017 min
Response: 637388
Conc: 19.33 ng/ml

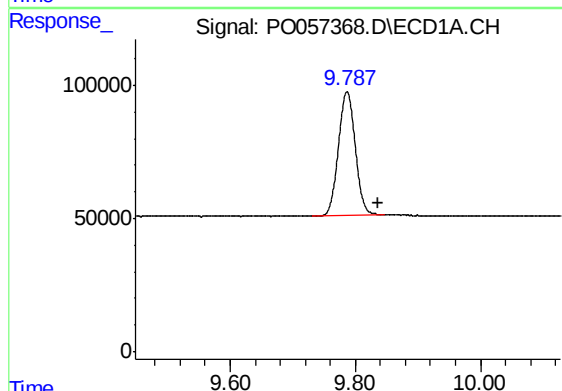

#2 Decachlorobiphenyl

R.T.: 9.787 min
Delta R.T.: -0.049 min
Response: 871255
Conc: 17.75 ng/ml

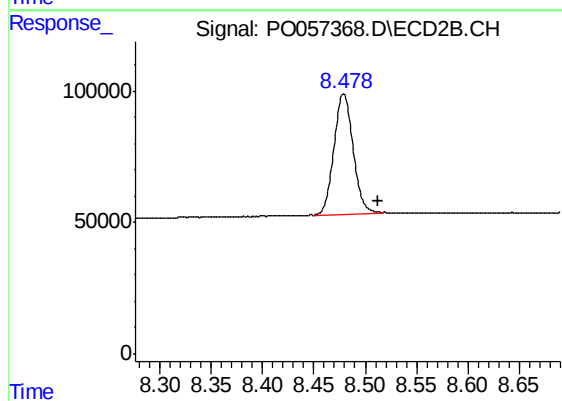

#2 Decachlorobiphenyl

R.T.: 8.478 min
Delta R.T.: -0.035 min
Response: 597544
Conc: 16.76 ng/ml m