

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062119\
 Data File : P0057372.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2019 16:17
 Operator : SM/SJ
 Sample : K3417-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONTROL-HOUSE-BRICKS

Manual Integrations
 APPROVED

Ankita
 6/24/2019 8:39:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 16:32:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.232	3.557	883611	696056	23.081	21.106
2)	SA Decachlor...	9.787	8.479	973170	678567	19.827	19.031m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062119\
Data File : PO057372.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2019 16:17
Operator : SM/SJ
Sample : K3417-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS


Manual Integrations
APPROVED

Ankita
6/24/2019 8:39:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 16:32:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

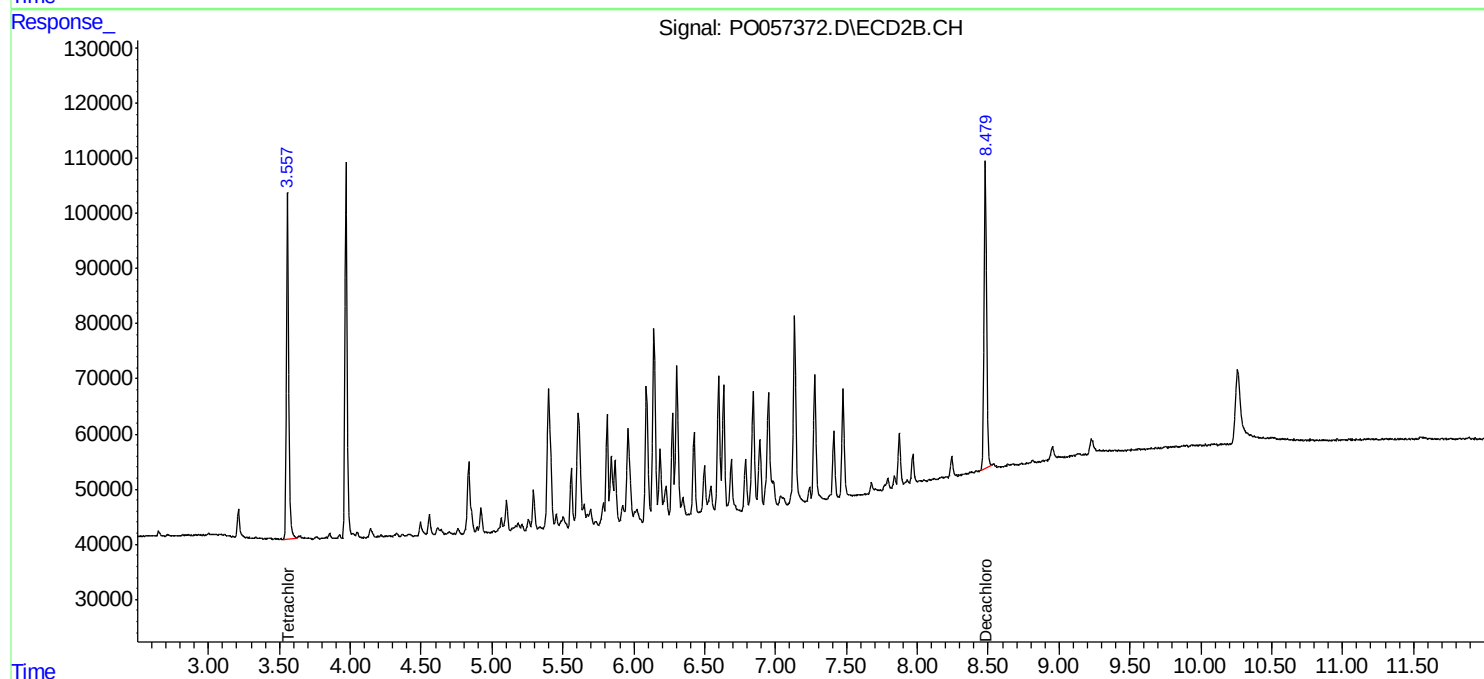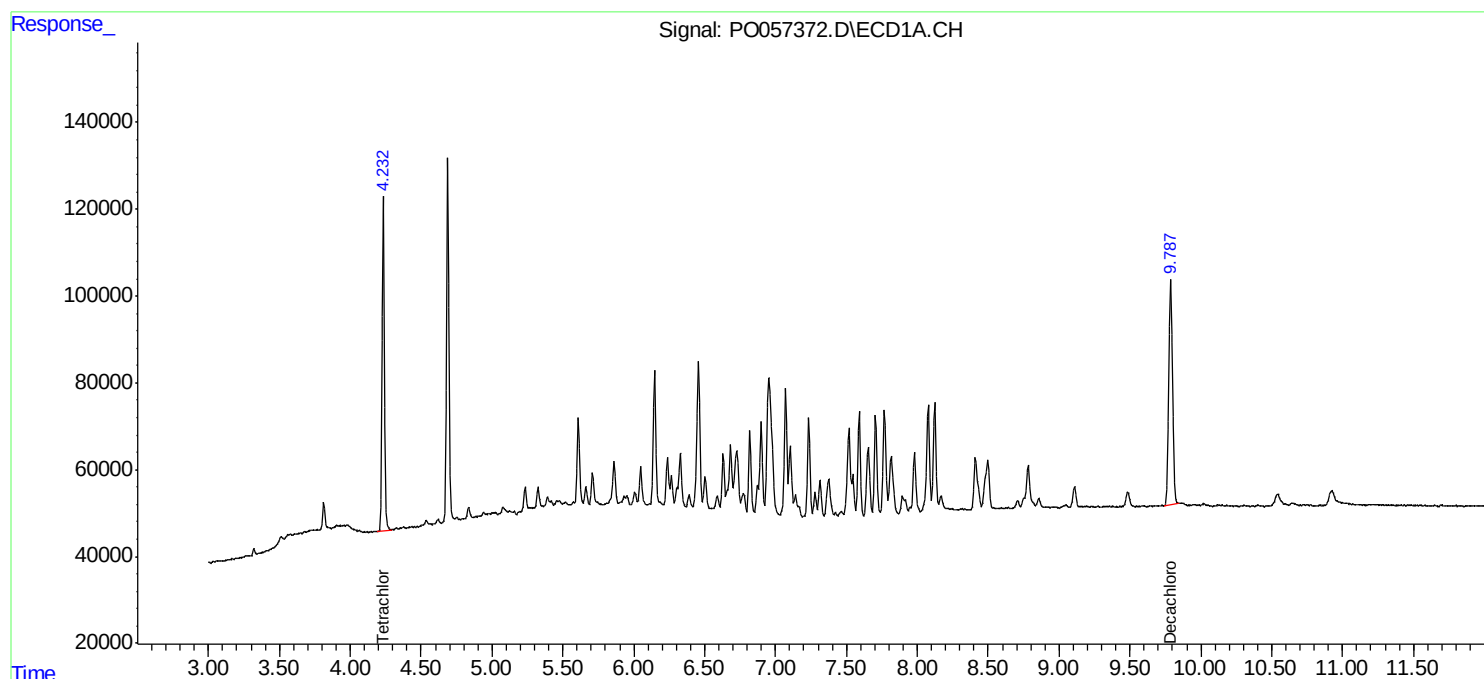

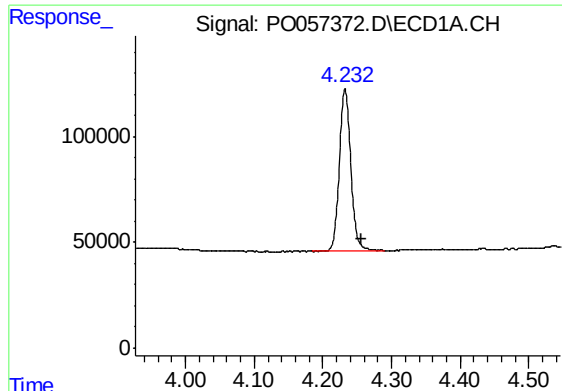


#1 Tetrachloro-m-xylene

R.T.: 4.232 min
Delta R.T.: -0.024 min
Response: 883611
Conc: 23.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-BRICKS


Manual Integrations
APPROVED

Ankita
6/24/2019 8:39:51 AM

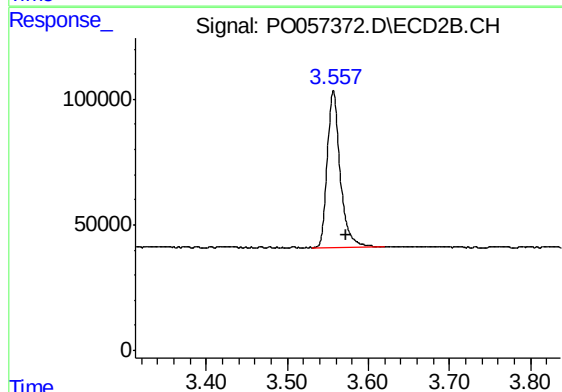


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: -0.016 min
Response: 696056
Conc: 21.11 ng/ml

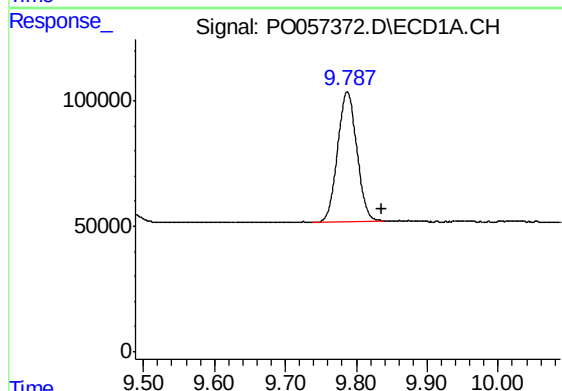

#2 Decachlorobiphenyl

R.T.: 9.787 min
Delta R.T.: -0.049 min
Response: 973170
Conc: 19.83 ng/ml

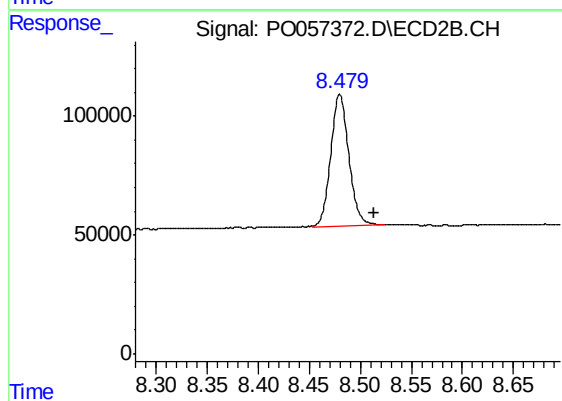

#2 Decachlorobiphenyl

R.T.: 8.479 min
Delta R.T.: -0.034 min
Response: 678567
Conc: 19.03 ng/ml m