

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
 Data File : PP062555.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2018 20:40
 Operator : UA/AJ
 Sample : J3529-10MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TPTW-04MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 16:52:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 20 14:06:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.075	4.101	8806210	14844627	95.442	62.340 #
2) SA Decachlor...	8.346	8.930	3381755	9124371	23.310	57.829 #
Target Compounds						
3) L1 Aroclor-1...	4.552	4.474	3214873	8946342	1400.518	2200.222 #
4) L1 Aroclor-1...	4.982	4.939	8544978	5845560	3228.961	1939.310 #
5) L1 Aroclor-1...	5.061	5.191	4496018	2940828	2473.910	478.270 #
6) L1 Aroclor-1...	5.333	5.291	4289407	11112479	3519.495	2798.229
7) L1 Aroclor-1...	5.372	5.522	4866637	10065563	3215.657	2424.973
8) L2 Aroclor-1...	4.190	4.366	23450932	7884210	19968.610	2473.818 #
9) L2 Aroclor-1...	4.280	4.421	4516391	6748617	3732.679	3348.329
10) L2 Aroclor-1...	4.330	4.474	2268997	8946342	482.489	1238.875 #
11) L3 Aroclor-1...	4.552	4.939	3214873	5845560	2502.314	3568.902 #
12) L3 Aroclor-1...	4.982	5.191	8544978	2940828	5828.253	935.677 #
13) L3 Aroclor-1...	5.061	5.291	4496018	11112479	4372.623	5379.963
14) L3 Aroclor-1...	5.333	5.522	4289407	10065563	6724.253	4781.802 #
15) L3 Aroclor-1...	5.372	5.870	4866637	2742710	5673.045	1130.082 #
16) L4 Aroclor-1...	4.552	4.790	3214873	7114479	1566.282	1165.779 #
17) L4 Aroclor-1...	4.916	5.112	3070562	5388396	667.903	711.603
18) L4 Aroclor-1...	4.982	5.291	8544978	11112479	3983.592	3690.965
19) L4 Aroclor-1...	5.298	5.522	2317342	10065563	1135.133	3022.175 #
20) L4 Aroclor-1...	5.602	5.638	9393475	2209329	5286.028	458.715 #
21) L5 Aroclor-1...	5.298	5.522	2317342	10065563	679.799	1636.502 #
22) L5 Aroclor-1...	5.333	5.638	4289407	2209329	2227.689	303.554 #
23) L5 Aroclor-1...	5.602	5.819	9393475	12747370	3103.598	1812.738 #
24) L5 Aroclor-1...	5.602	5.870	9393475	2742710	3045.223	346.299 #
25) L5 Aroclor-1...	5.778	6.053	21977760	12567540	7453.997	1700.505 #
26) L6 Aroclor-1...	5.778	5.870	21977760	2742710	4765.292	376.471 #
27) L6 Aroclor-1...	5.918	5.991	2832836	4518120	848.734	582.876 #
28) L6 Aroclor-1...	6.060	6.372	1520569	4742474	250.603	365.528 #
29) L6 Aroclor-1...	6.276	6.679	5419213	9609239	923.054	1865.821 #
30) L6 Aroclor-1...	6.632	6.943	3520232	16133090	463.228	1494.569 #
31) L7 Aroclor-1...	6.198	6.500	5445056	6763098	1527.761	822.590 #
32) L7 Aroclor-1...	6.632	6.639	3520232	6571858	384.153	715.717 #
33) L7 Aroclor-1...	6.702	6.986	5152720	15993275	781.197	2440.601 #
34) L7 Aroclor-1...	6.900	7.243	10012483	18457610	1932.392	2515.234 #
35) L7 Aroclor-1...	7.137	7.460	10212224	13772249	553.644	870.918 #
36) L8 Aroclor-1...	6.198	6.679	5445056	9609239	1634.270	1178.946 #
37) L8 Aroclor-1...	6.425	6.807	35484903	14537709	5289.769	3088.041 #
38) L8 Aroclor-1...	6.702	7.064	5152720	23580420	445.339	2138.920 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
 Data File : PP026555.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2018 20:40
 Operator : UA/AJ
 Sample : J3529-10MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TPTW-04MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 16:52:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 20 14:06:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
39) L8	Aroclor-1...	6.900	7.310	10012483	10343585	1238.299	1035.012
40) L8	Aroclor-1...	7.137	7.460	10212224	13772249	386.145	653.667 #
41) L9	Aroclor-1...	7.451	7.805	41479073	23503305	1528.272	1141.476 #
42) L9	Aroclor-1...	7.451	7.805	41479073	23503305	2007.836	1251.283 #
43) L9	Aroclor-1...	7.601	8.050	8776121	18770227	476.172	1216.026 #
44) L9	Aroclor-1...	7.923	8.290	7114038	17929678	864.211	2418.211 #
45) L9	Aroclor-1...	8.149	8.640	5393637	12313116	89.995	219.219 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP062018\
Data File : PP026555.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 20:40
Operator : UA/AJ
Sample : J3529-10MSD
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 16:52:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP062018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 14:06:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPEST1 Signal #2 Phase: ZB-CLPEST2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

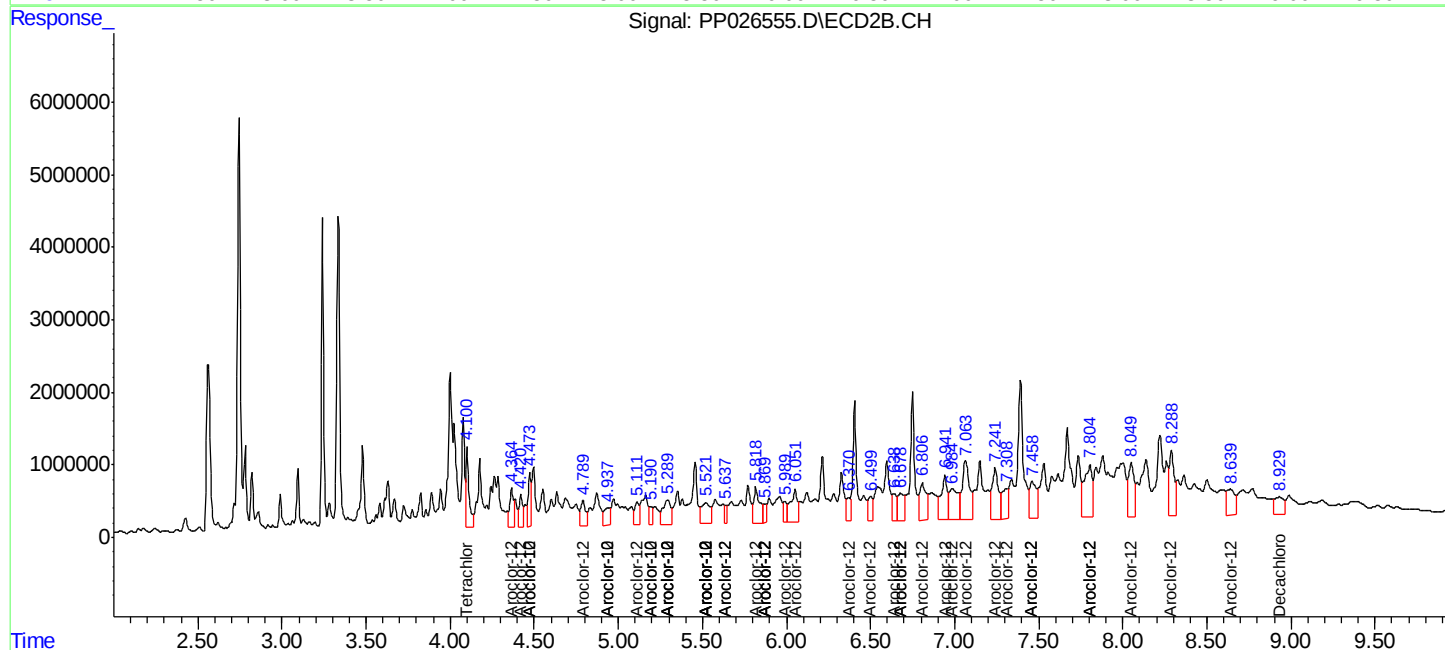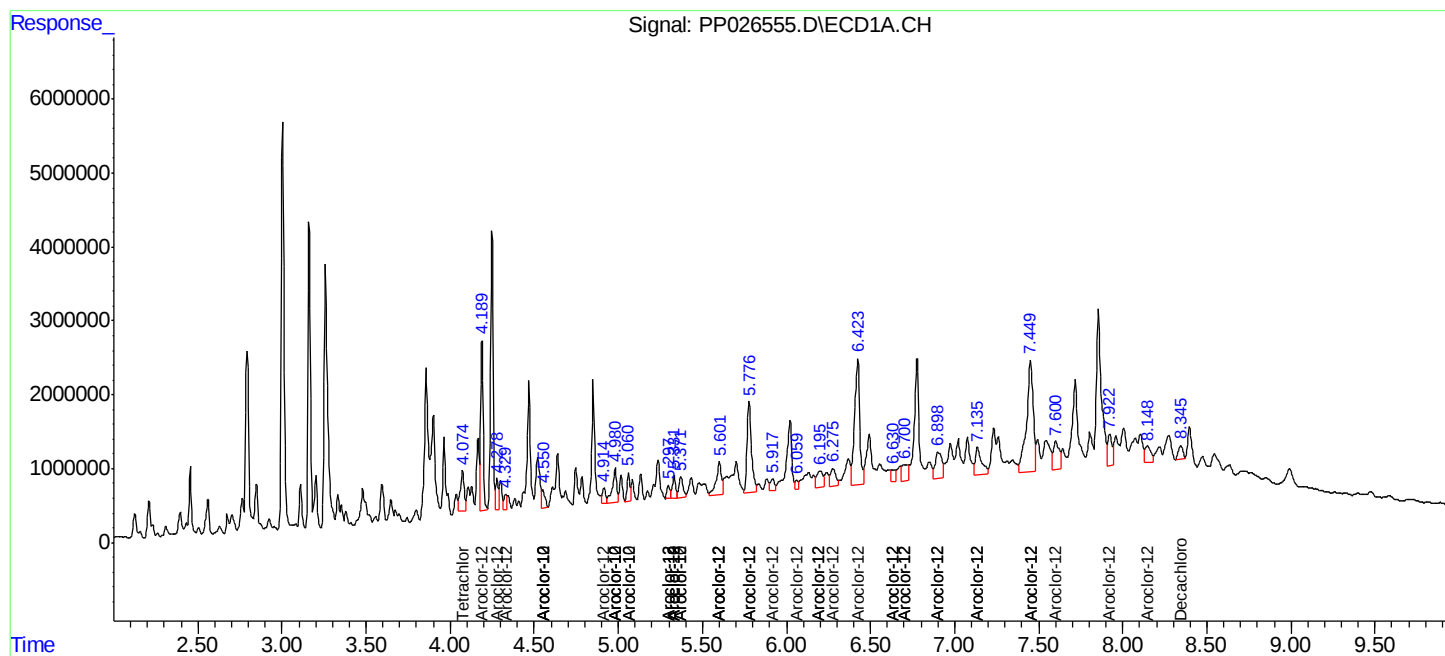


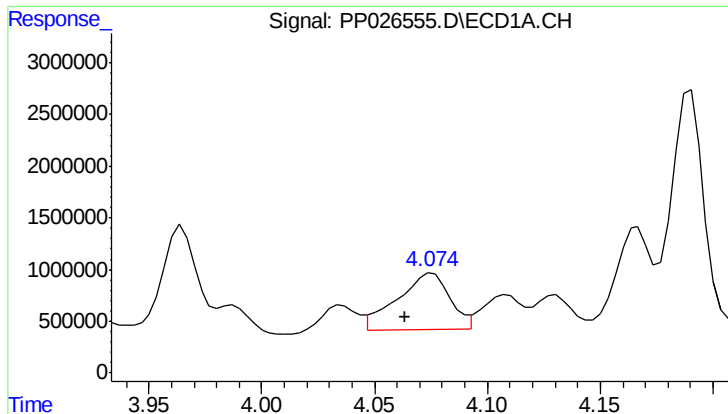

#1 Tetrachloro-m-xylene


R.T.: 4.075 min
Delta R.T.: 0.012 min
Response: 8806210
Conc: 95.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

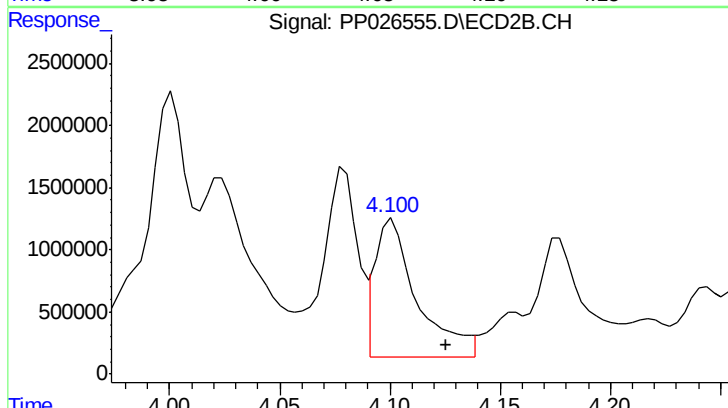


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: -0.024 min
Response: 14844627
Conc: 62.34 ng/ml

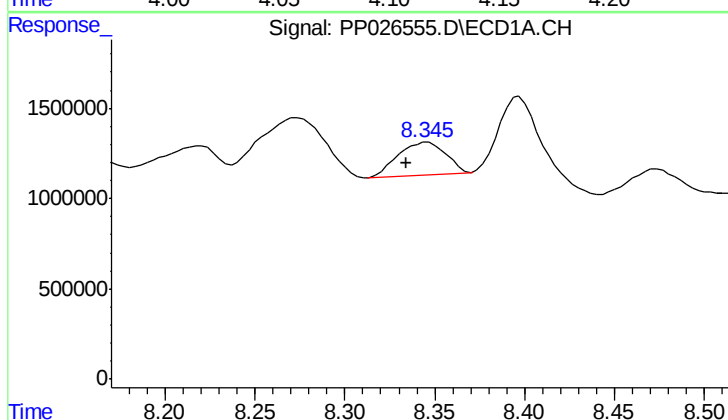


#2 Decachlorobiphenyl

R.T.: 8.346 min
Delta R.T.: 0.012 min
Response: 3381755
Conc: 23.31 ng/ml

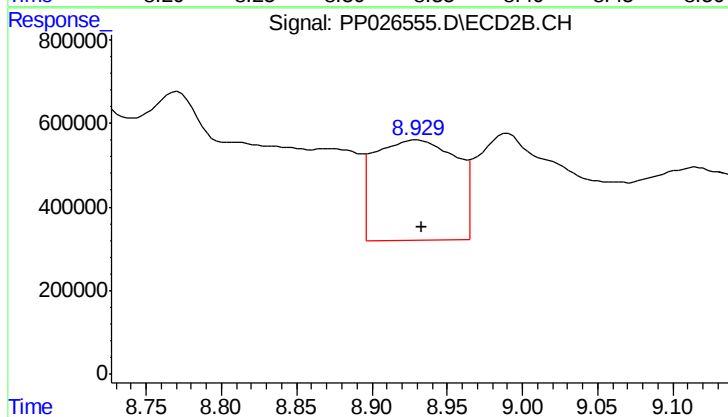

#2 Decachlorobiphenyl


R.T.: 8.930 min
Delta R.T.: -0.003 min
Response: 9124371
Conc: 57.83 ng/ml

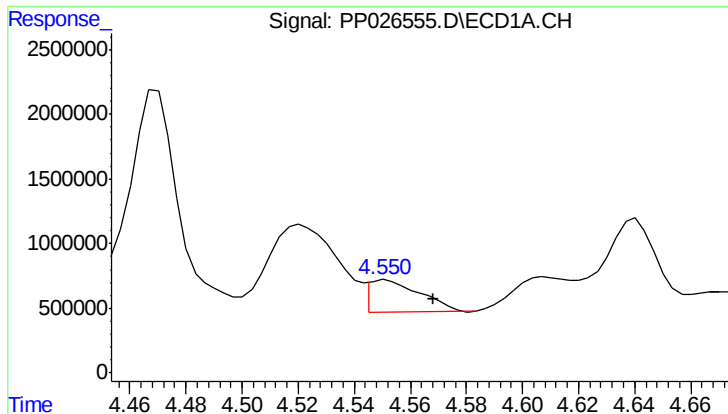

#3 Aroclor-1016-1


R.T.: 4.552 min
Delta R.T.: -0.017 min
Response: 3214873
Conc: 1400.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

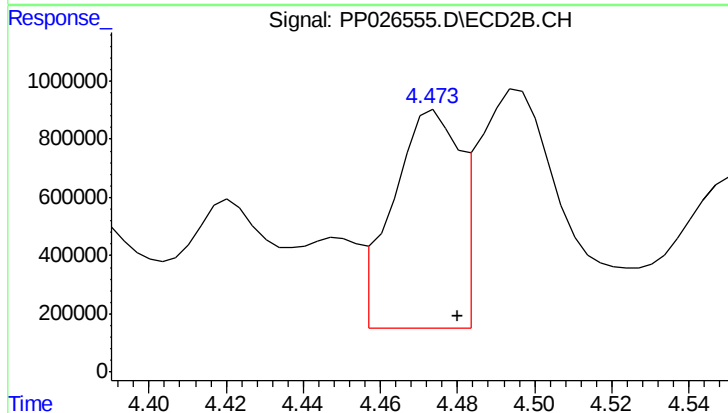


#3 Aroclor-1016-1

R.T.: 4.474 min
Delta R.T.: -0.006 min
Response: 8946342
Conc: 2200.22 ng/ml

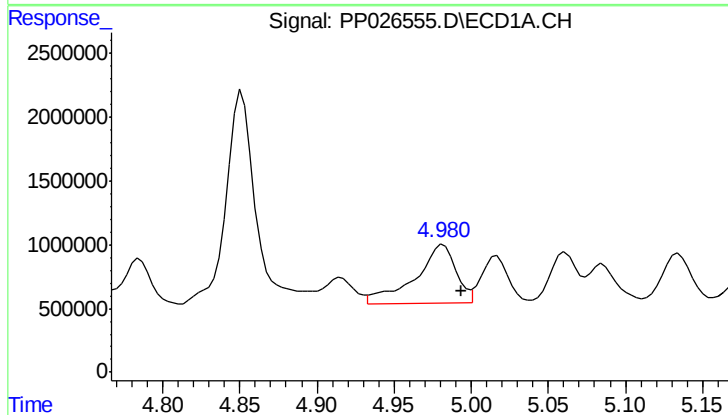


#4 Aroclor-1016-2

R.T.: 4.982 min
Delta R.T.: -0.012 min
Response: 8544978
Conc: 3228.96 ng/ml

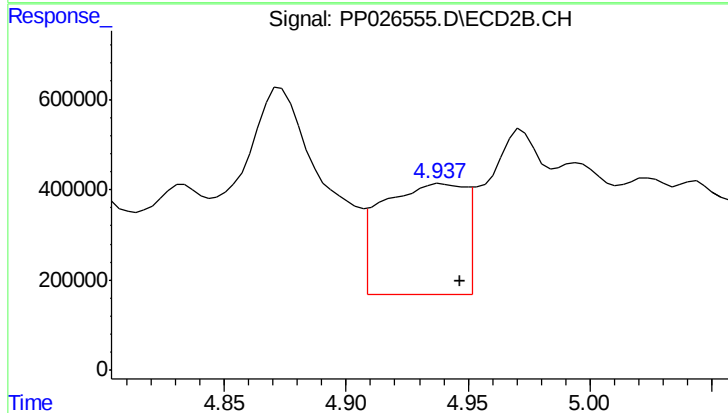

#4 Aroclor-1016-2


R.T.: 4.939 min
Delta R.T.: -0.008 min
Response: 5845560
Conc: 1939.31 ng/ml

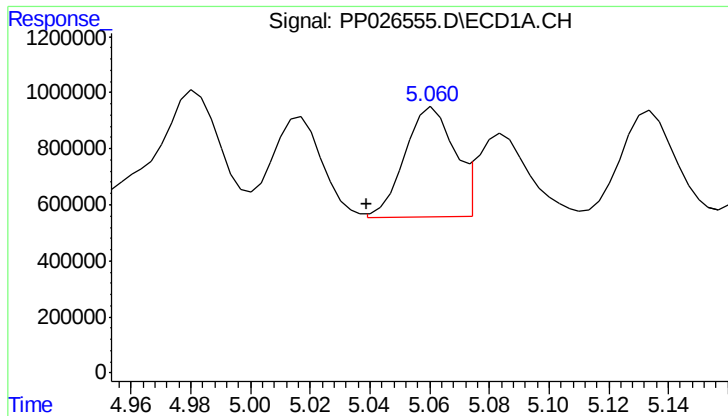

#5 Aroclor-1016-3


R.T.: 5.061 min
Delta R.T.: 0.022 min
Response: 4496018
Conc: 2473.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

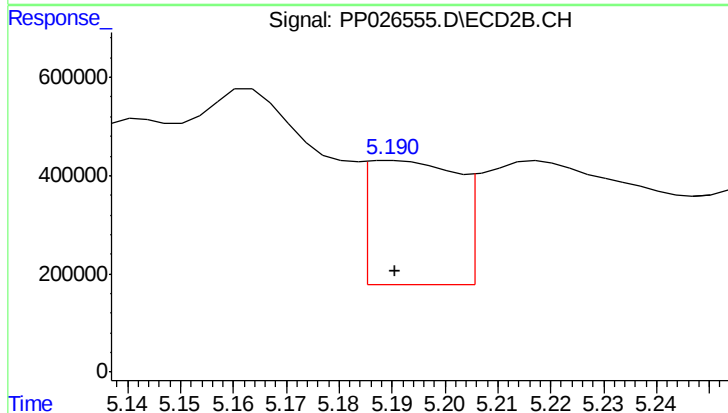


#5 Aroclor-1016-3

R.T.: 5.191 min
Delta R.T.: 0.000 min
Response: 2940828
Conc: 478.27 ng/ml

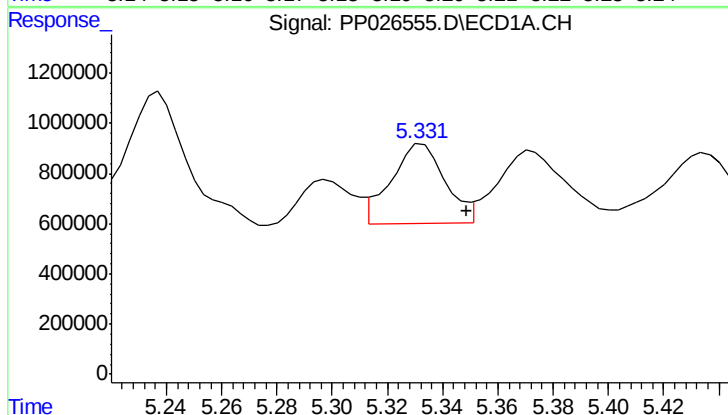


#6 Aroclor-1016-4

R.T.: 5.333 min
Delta R.T.: -0.016 min
Response: 4289407
Conc: 3519.50 ng/ml

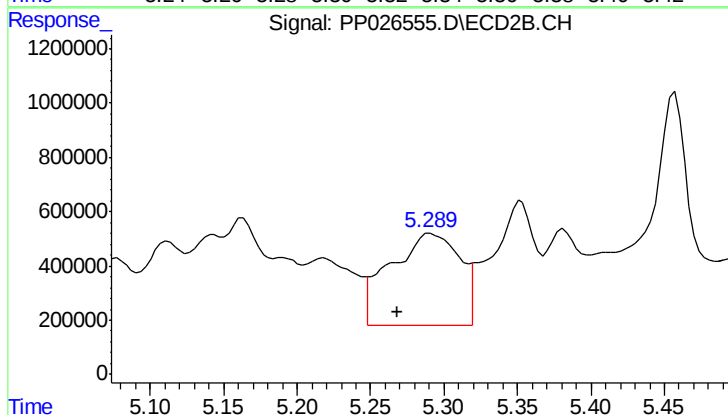

#6 Aroclor-1016-4


R.T.: 5.291 min
Delta R.T.: 0.022 min
Response: 11112479
Conc: 2798.23 ng/ml

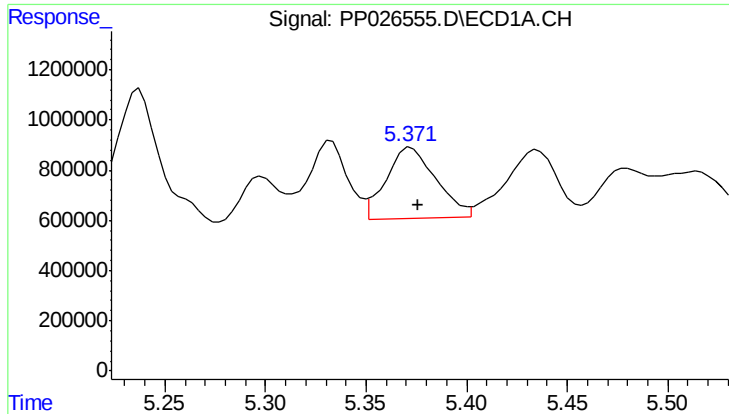

#7 Aroclor-1016-5


R.T.: 5.372 min
Delta R.T.: -0.003 min
Response: 4866637
Conc: 3215.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

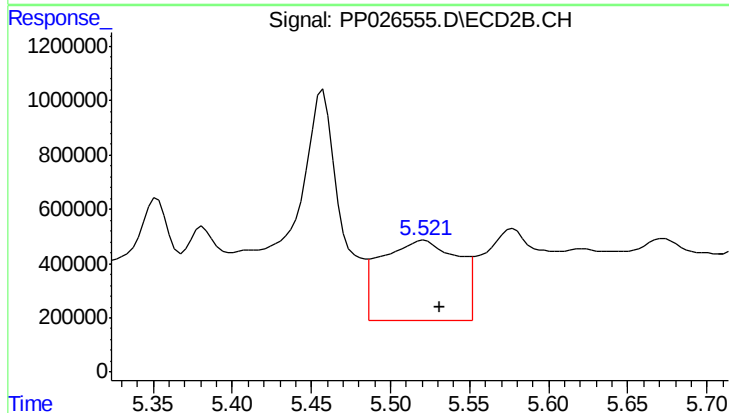


#7 Aroclor-1016-5

R.T.: 5.522 min
Delta R.T.: -0.009 min
Response: 10065563
Conc: 2424.97 ng/ml

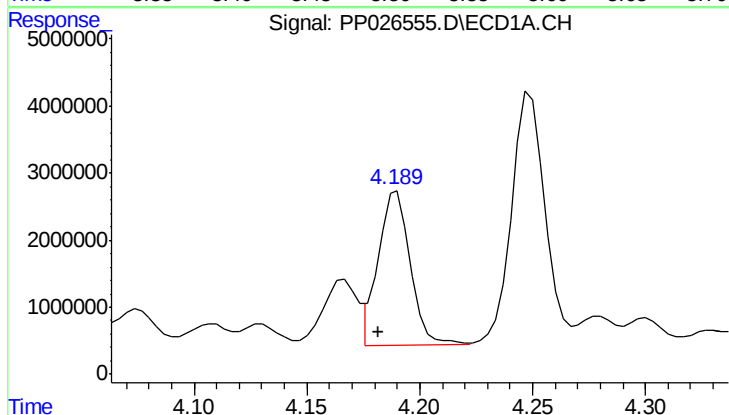


#8 Aroclor-1221-1

R.T.: 4.190 min
Delta R.T.: 0.008 min
Response: 23450932
Conc: 19968.61 ng/ml

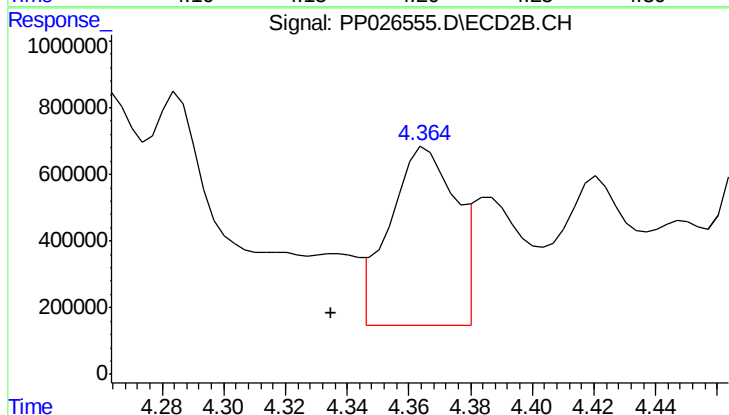

#8 Aroclor-1221-1


R.T.: 4.366 min
Delta R.T.: 0.031 min
Response: 7884210
Conc: 2473.82 ng/ml

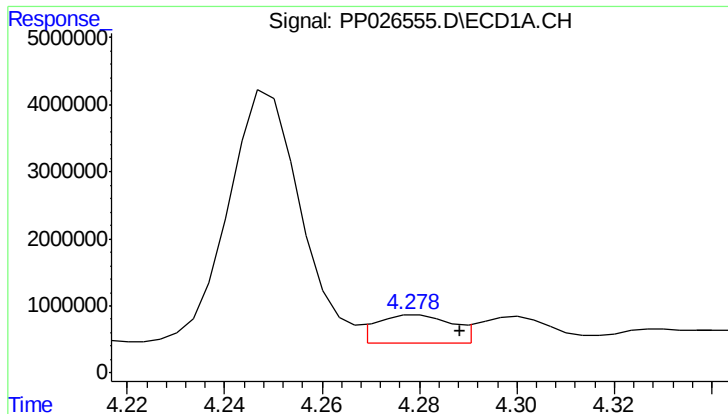

#9 Aroclor-1221-2


R.T.: 4.280 min
Delta R.T.: -0.009 min
Response: 4516391
Conc: 3732.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

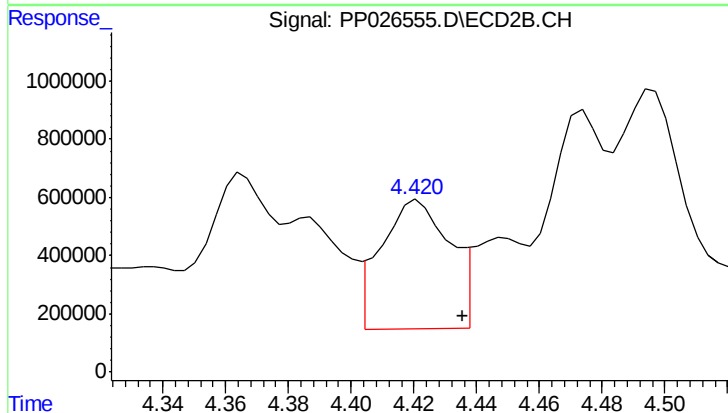


#9 Aroclor-1221-2

R.T.: 4.421 min
Delta R.T.: -0.014 min
Response: 6748617
Conc: 3348.33 ng/ml

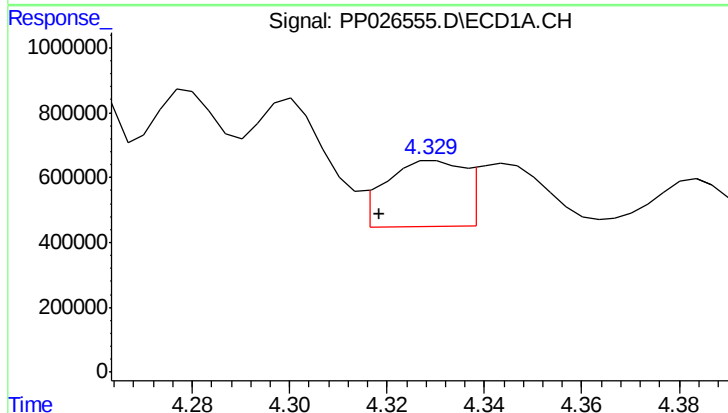


#10 Aroclor-1221-3

R.T.: 4.330 min
Delta R.T.: 0.012 min
Response: 2268997
Conc: 482.49 ng/ml

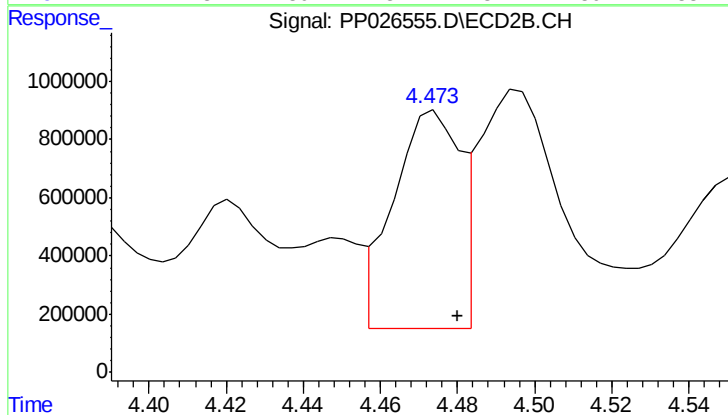

#10 Aroclor-1221-3


R.T.: 4.474 min
Delta R.T.: -0.006 min
Response: 8946342
Conc: 1238.87 ng/ml

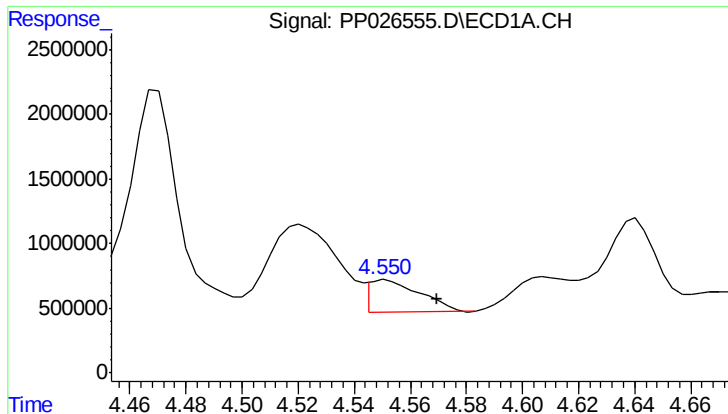

#11 Aroclor-1232-1


R.T.: 4.552 min
Delta R.T.: -0.018 min
Response: 3214873
Conc: 2502.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

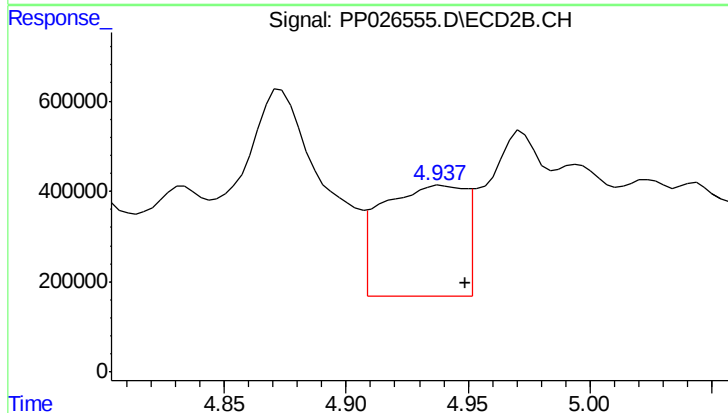


#11 Aroclor-1232-1

R.T.: 4.939 min
Delta R.T.: -0.010 min
Response: 5845560
Conc: 3568.90 ng/ml

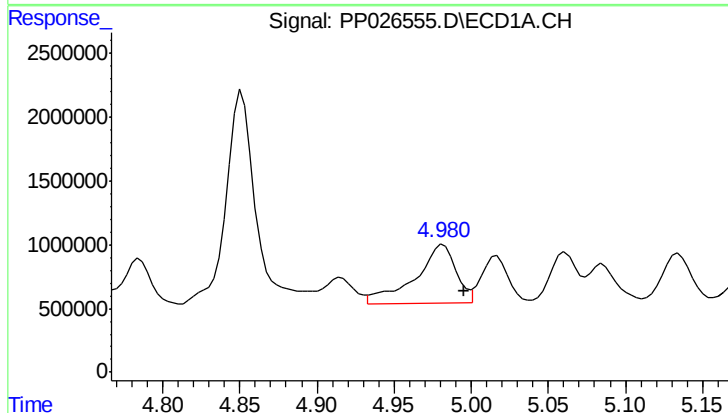


#12 Aroclor-1232-2

R.T.: 4.982 min
Delta R.T.: -0.014 min
Response: 8544978
Conc: 5828.25 ng/ml

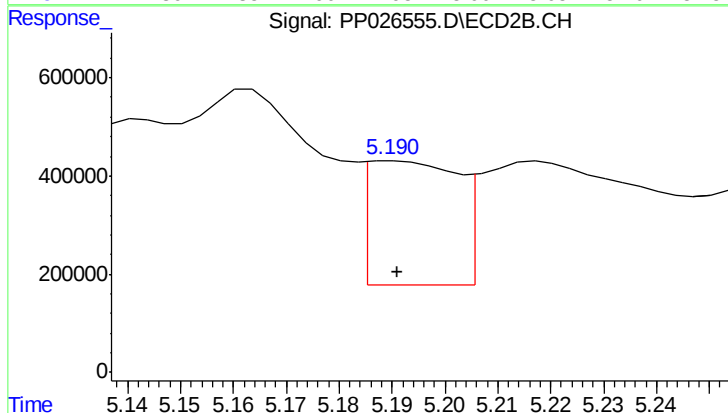

#12 Aroclor-1232-2


R.T.: 5.191 min
Delta R.T.: 0.000 min
Response: 2940828
Conc: 935.68 ng/ml

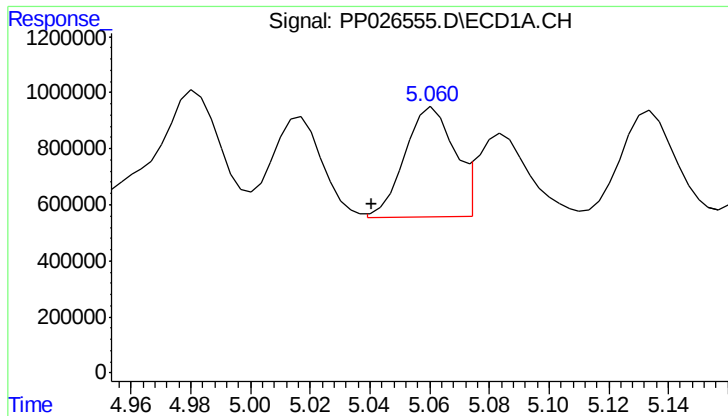

#13 Aroclor-1232-3


R.T.: 5.061 min
Delta R.T.: 0.021 min
Response: 4496018
Conc: 4372.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

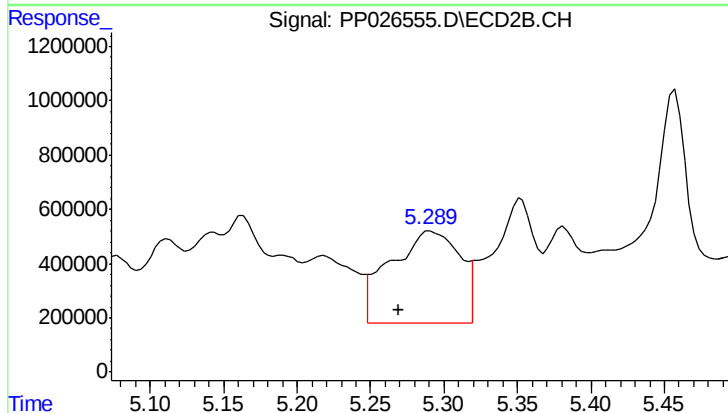


#13 Aroclor-1232-3

R.T.: 5.291 min
Delta R.T.: 0.022 min
Response: 11112479
Conc: 5379.96 ng/ml

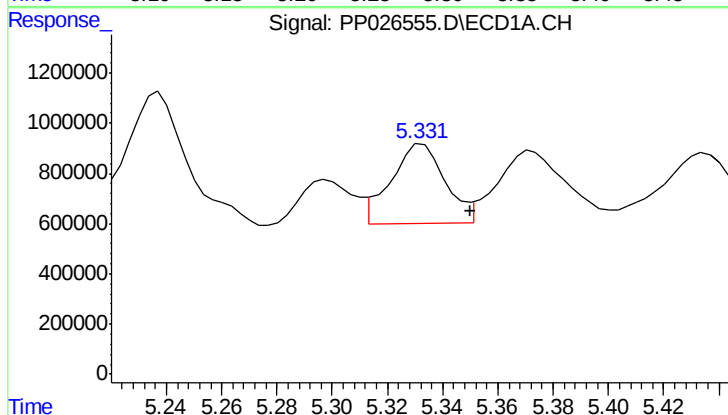


#14 Aroclor-1232-4

R.T.: 5.333 min
Delta R.T.: -0.017 min
Response: 4289407
Conc: 6724.25 ng/ml

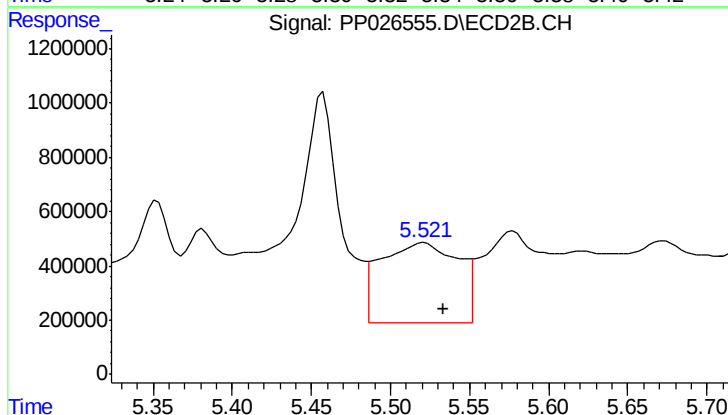

#14 Aroclor-1232-4


R.T.: 5.522 min
Delta R.T.: -0.012 min
Response: 10065563
Conc: 4781.80 ng/ml

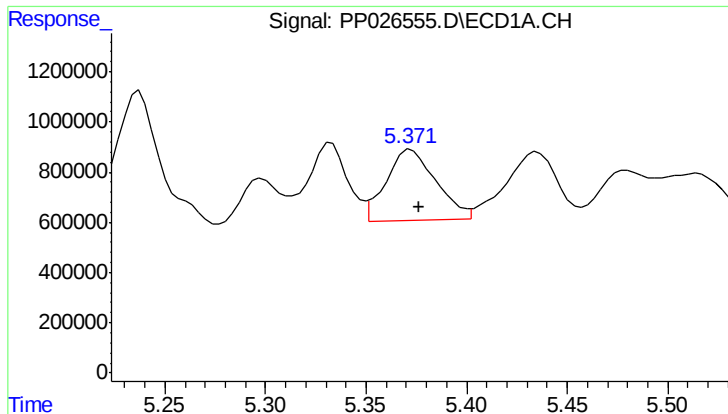

#15 Aroclor-1232-5


R.T.: 5.372 min
Delta R.T.: -0.004 min
Response: 4866637
Conc: 5673.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

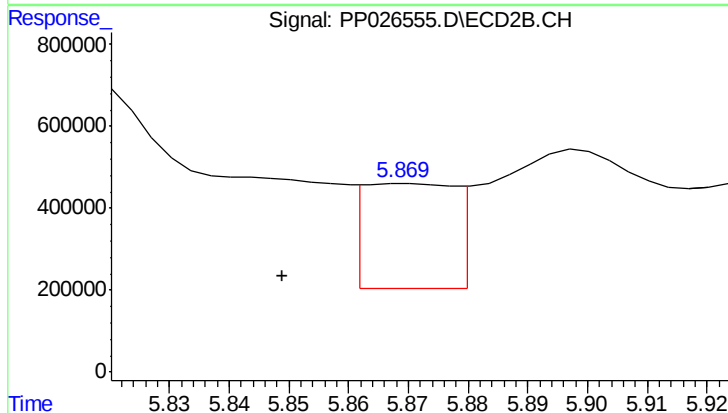


#15 Aroclor-1232-5

R.T.: 5.870 min
Delta R.T.: 0.021 min
Response: 2742710
Conc: 1130.08 ng/ml

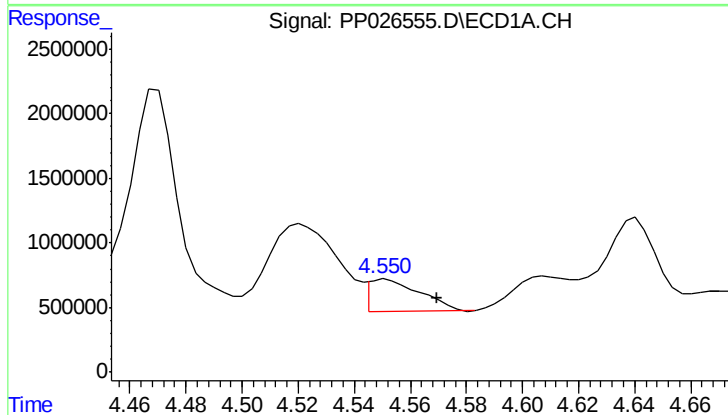


#16 Aroclor-1242-1

R.T.: 4.552 min
Delta R.T.: -0.018 min
Response: 3214873
Conc: 1566.28 ng/ml

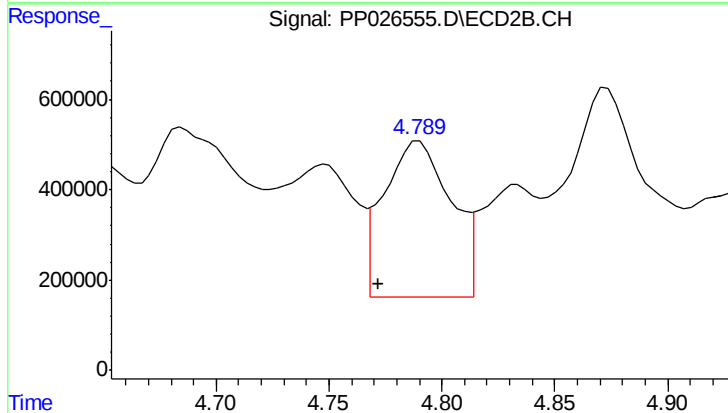

#16 Aroclor-1242-1


R.T.: 4.790 min
Delta R.T.: 0.018 min
Response: 7114479
Conc: 1165.78 ng/ml

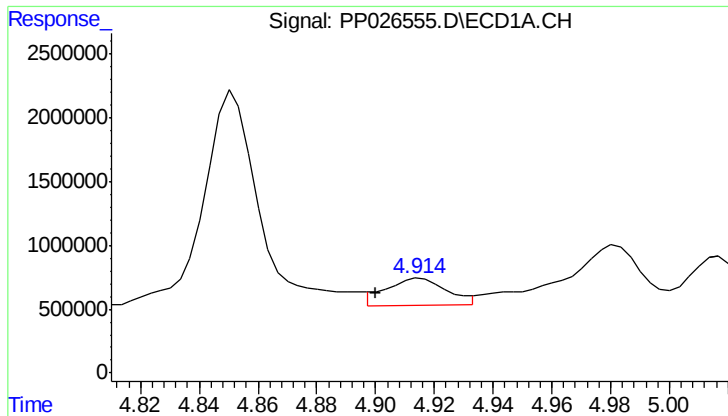

#17 Aroclor-1242-2


R.T.: 4.916 min
Delta R.T.: 0.015 min
Response: 3070562
Conc: 667.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

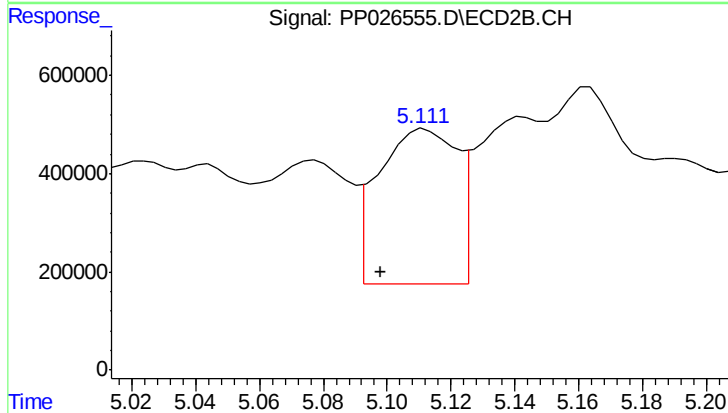


#17 Aroclor-1242-2

R.T.: 5.112 min
Delta R.T.: 0.014 min
Response: 5388396
Conc: 711.60 ng/ml

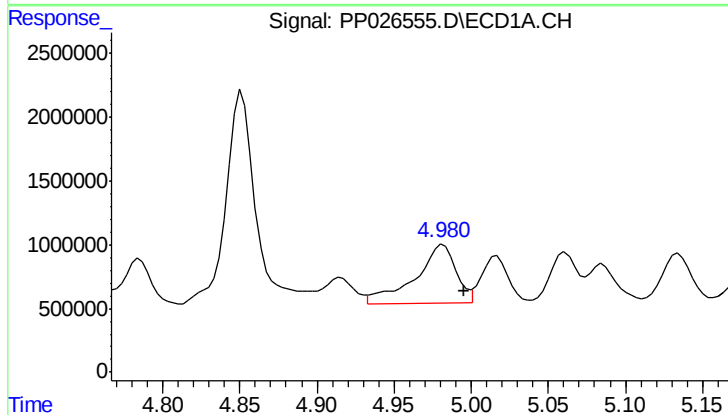


#18 Aroclor-1242-3

R.T.: 4.982 min
Delta R.T.: -0.014 min
Response: 8544978
Conc: 3983.59 ng/ml

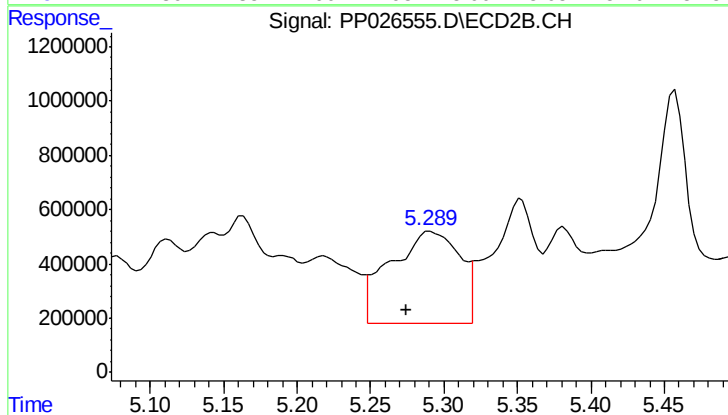

#18 Aroclor-1242-3


R.T.: 5.291 min
Delta R.T.: 0.016 min
Response: 11112479
Conc: 3690.96 ng/ml

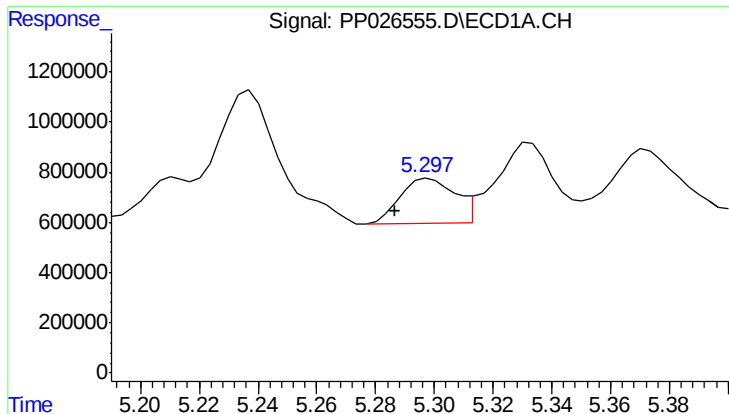

#19 Aroclor-1242-4


R.T.: 5.298 min
Delta R.T.: 0.011 min
Response: 2317342
Conc: 1135.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

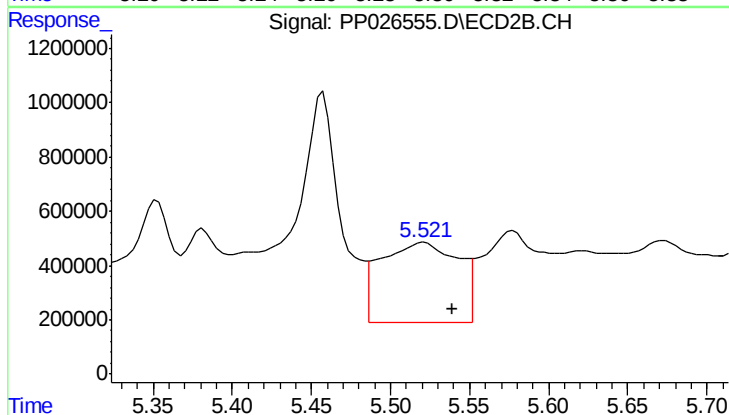


#19 Aroclor-1242-4

R.T.: 5.522 min
Delta R.T.: -0.018 min
Response: 10065563
Conc: 3022.17 ng/ml

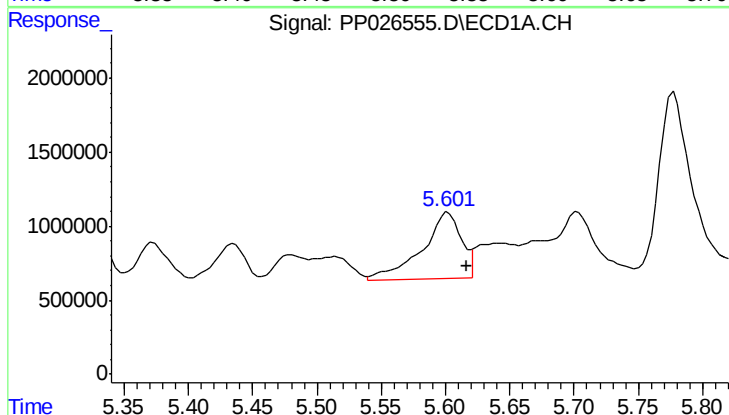


#20 Aroclor-1242-5

R.T.: 5.602 min
Delta R.T.: -0.015 min
Response: 9393475
Conc: 5286.03 ng/ml

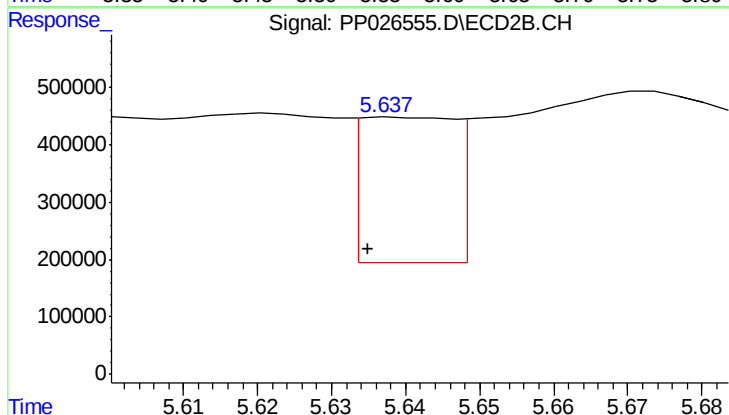

#20 Aroclor-1242-5


R.T.: 5.638 min
Delta R.T.: 0.003 min
Response: 2209329
Conc: 458.71 ng/ml

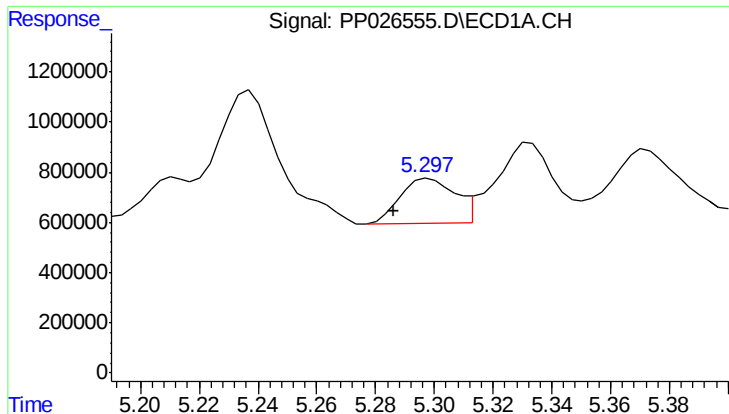

#21 Aroclor-1248-1


R.T.: 5.298 min
Delta R.T.: 0.012 min
Response: 2317342
Conc: 679.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

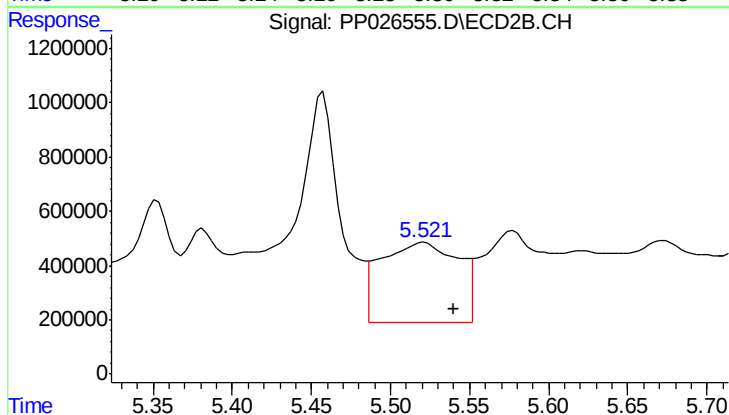


#21 Aroclor-1248-1

R.T.: 5.522 min
Delta R.T.: -0.018 min
Response: 10065563
Conc: 1636.50 ng/ml

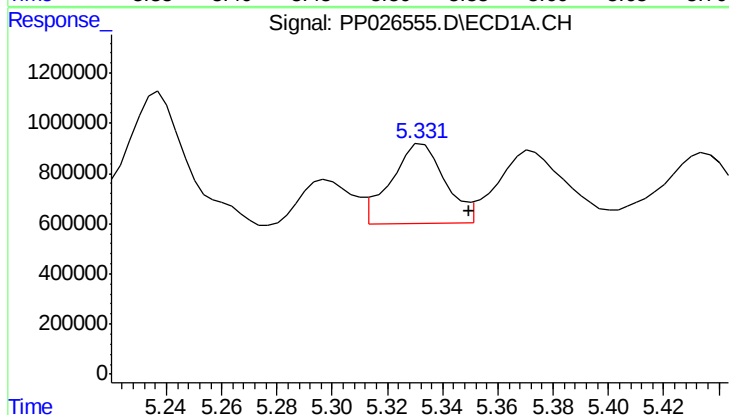


#22 Aroclor-1248-2

R.T.: 5.333 min
Delta R.T.: -0.017 min
Response: 4289407
Conc: 2227.69 ng/ml

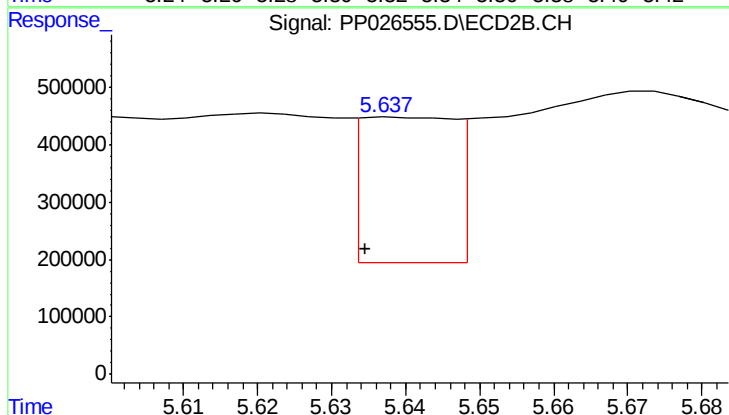

#22 Aroclor-1248-2


R.T.: 5.638 min
Delta R.T.: 0.003 min
Response: 2209329
Conc: 303.55 ng/ml

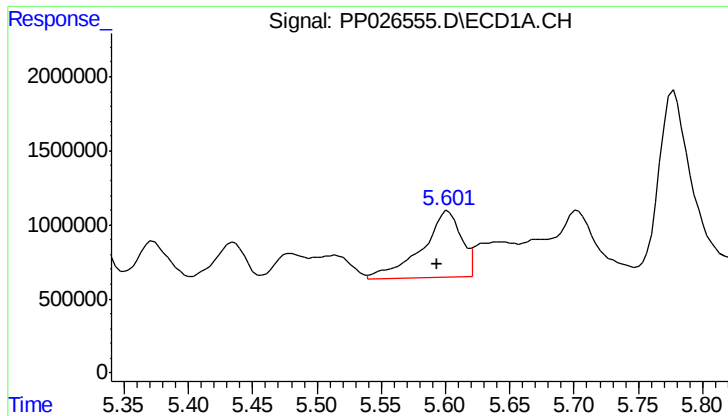

#23 Aroclor-1248-3


R.T.: 5.602 min
Delta R.T.: 0.009 min
Response: 9393475
Conc: 3103.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

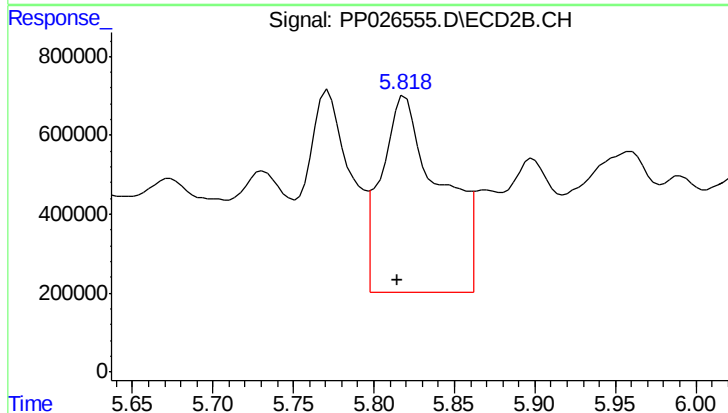


#23 Aroclor-1248-3

R.T.: 5.819 min
Delta R.T.: 0.005 min
Response: 12747370
Conc: 1812.74 ng/ml

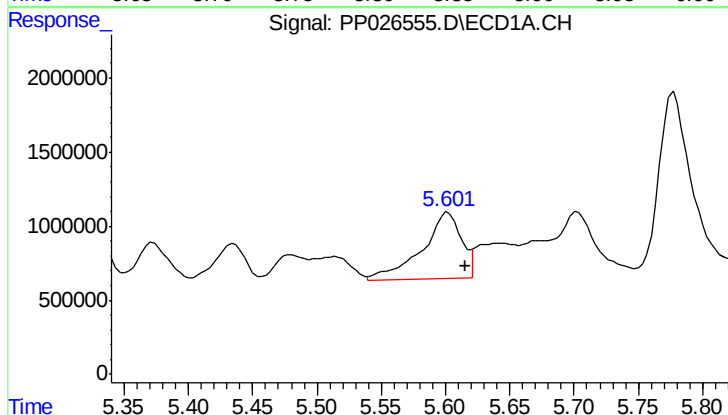


#24 Aroclor-1248-4

R.T.: 5.602 min
Delta R.T.: -0.014 min
Response: 9393475
Conc: 3045.22 ng/ml

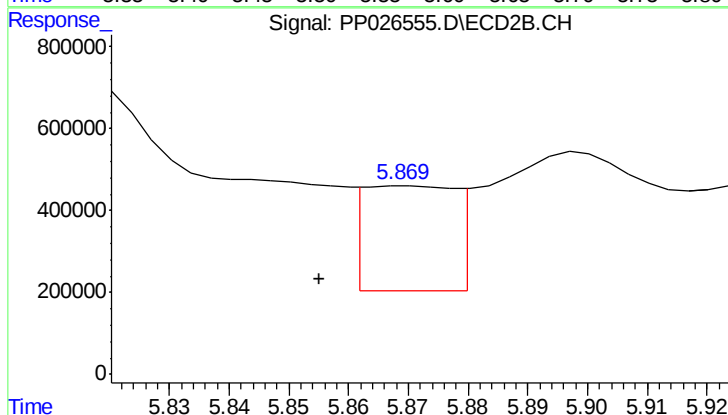

#24 Aroclor-1248-4


R.T.: 5.870 min
Delta R.T.: 0.015 min
Response: 2742710
Conc: 346.30 ng/ml

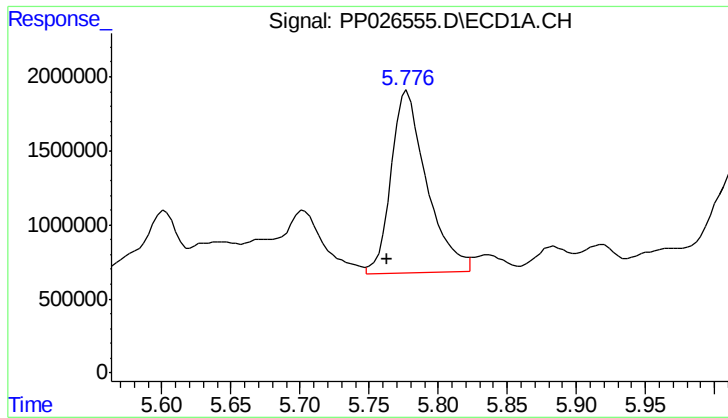

#25 Aroclor-1248-5


R.T.: 5.778 min
Delta R.T.: 0.015 min
Response: 21977760
Conc: 7454.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

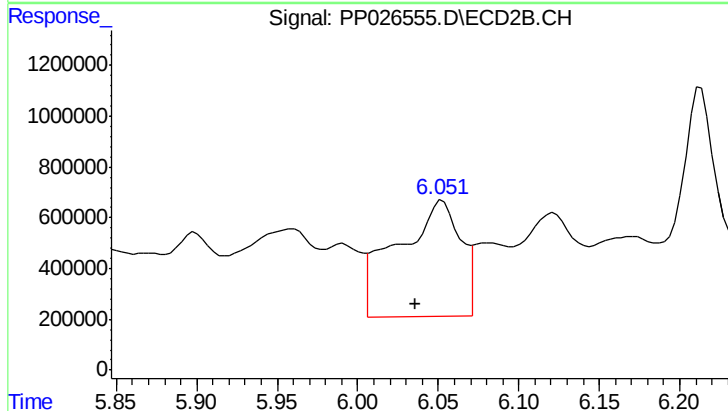


#25 Aroclor-1248-5

R.T.: 6.053 min
Delta R.T.: 0.017 min
Response: 12567540
Conc: 1700.50 ng/ml

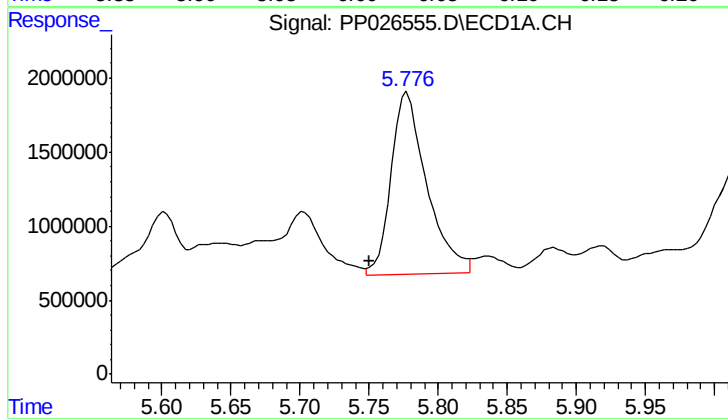


#26 Aroclor-1254-1

R.T.: 5.778 min
Delta R.T.: 0.028 min
Response: 21977760
Conc: 4765.29 ng/ml

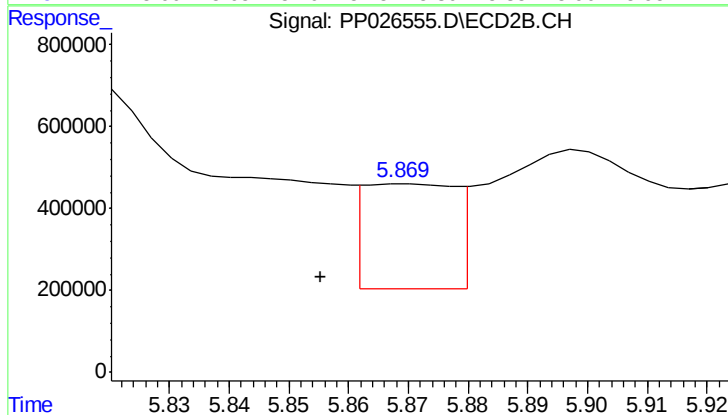

#26 Aroclor-1254-1


R.T.: 5.870 min
Delta R.T.: 0.015 min
Response: 2742710
Conc: 376.47 ng/ml

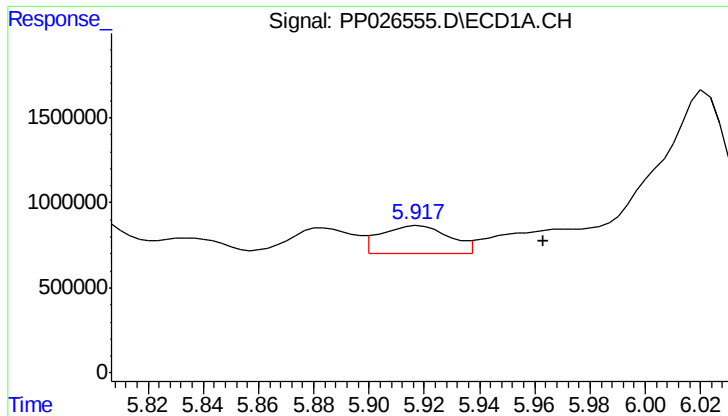

#27 Aroclor-1254-2


R.T.: 5.918 min
Delta R.T.: -0.045 min
Response: 2832836
Conc: 848.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

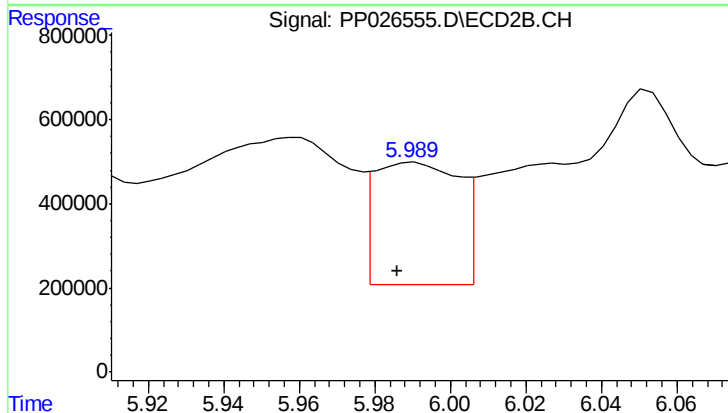


#27 Aroclor-1254-2

R.T.: 5.991 min
Delta R.T.: 0.005 min
Response: 4518120
Conc: 582.88 ng/ml

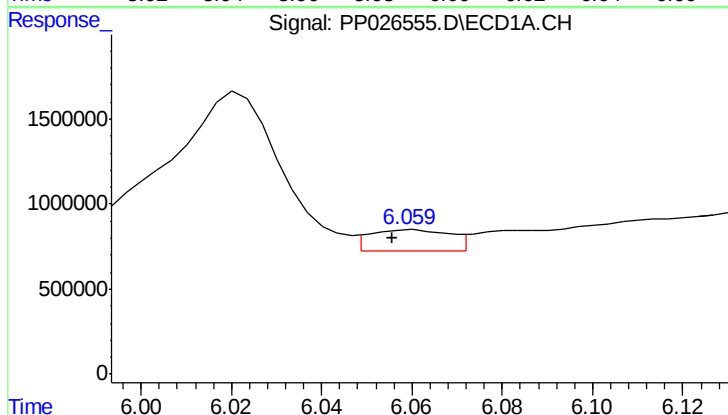


#28 Aroclor-1254-3

R.T.: 6.060 min
Delta R.T.: 0.005 min
Response: 1520569
Conc: 250.60 ng/ml

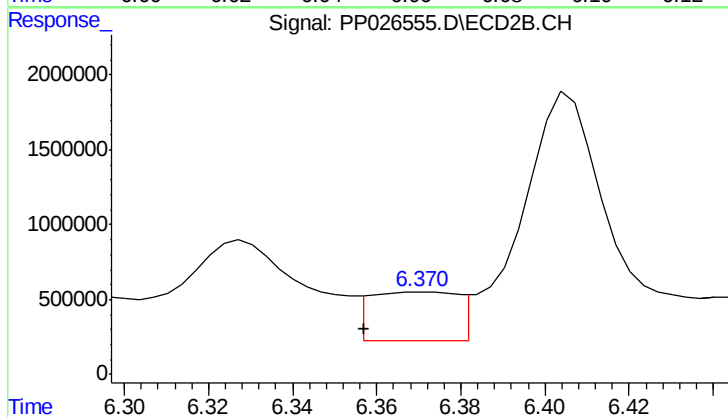

#28 Aroclor-1254-3


R.T.: 6.372 min
Delta R.T.: 0.015 min
Response: 4742474
Conc: 365.53 ng/ml

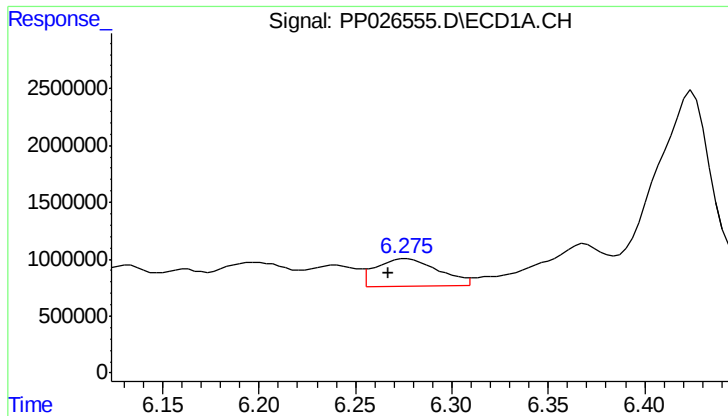

#29 Aroclor-1254-4


R.T.: 6.276 min
Delta R.T.: 0.009 min
Response: 5419213
Conc: 923.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

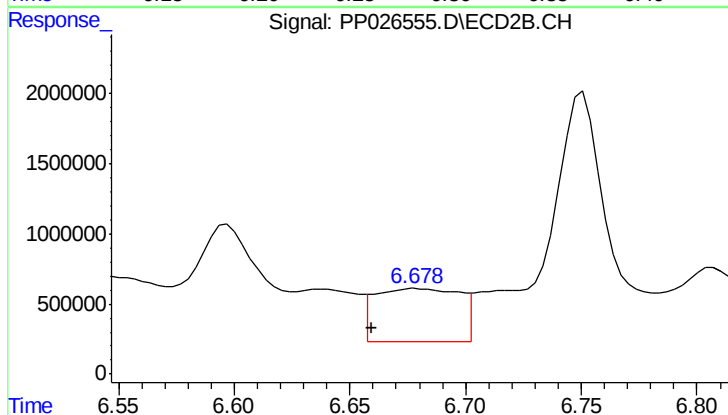


#29 Aroclor-1254-4

R.T.: 6.679 min
Delta R.T.: 0.020 min
Response: 9609239
Conc: 1865.82 ng/ml

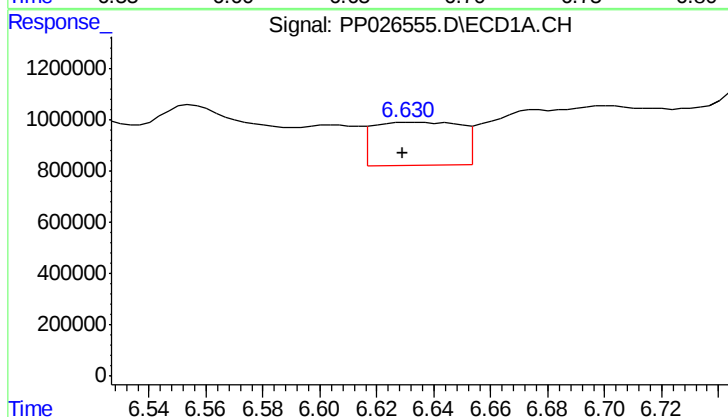


#30 Aroclor-1254-5

R.T.: 6.632 min
Delta R.T.: 0.003 min
Response: 3520232
Conc: 463.23 ng/ml

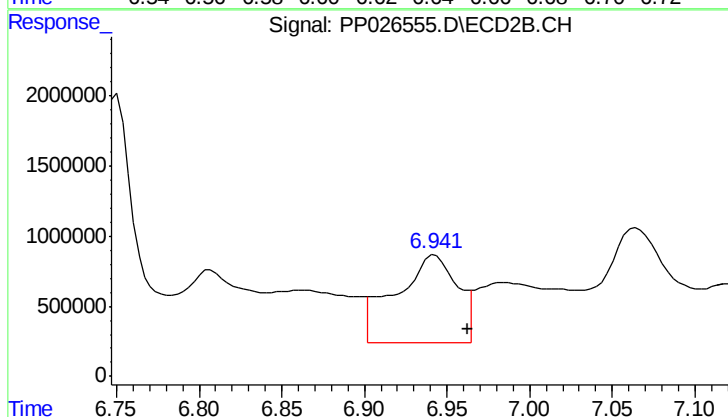

#30 Aroclor-1254-5


R.T.: 6.943 min
Delta R.T.: -0.020 min
Response: 16133090
Conc: 1494.57 ng/ml

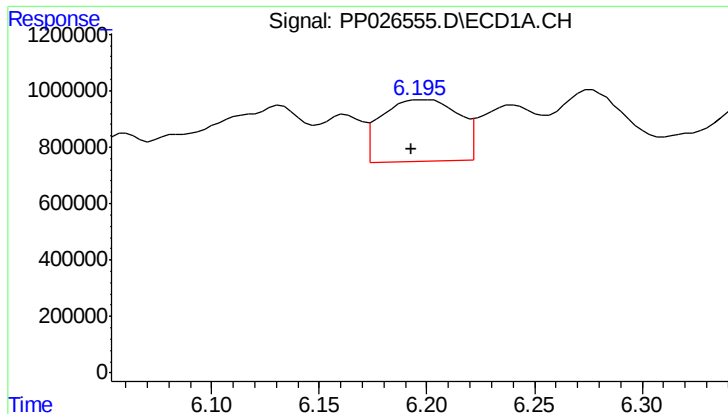

#31 Aroclor-1260-1


R.T.: 6.198 min
Delta R.T.: 0.005 min
Response: 5445056
Conc: 1527.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

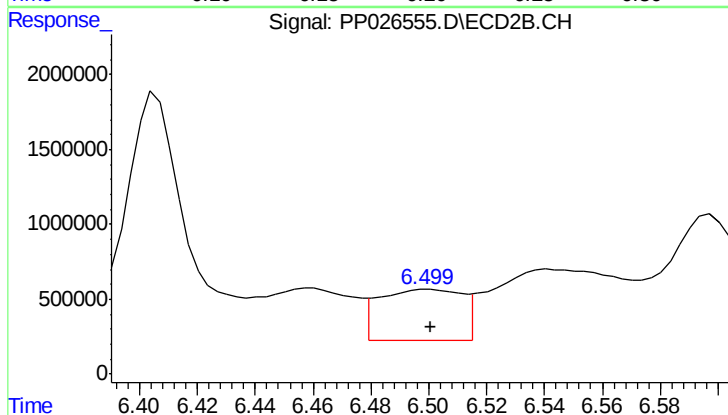


#31 Aroclor-1260-1

R.T.: 6.500 min
Delta R.T.: 0.000 min
Response: 6763098
Conc: 822.59 ng/ml

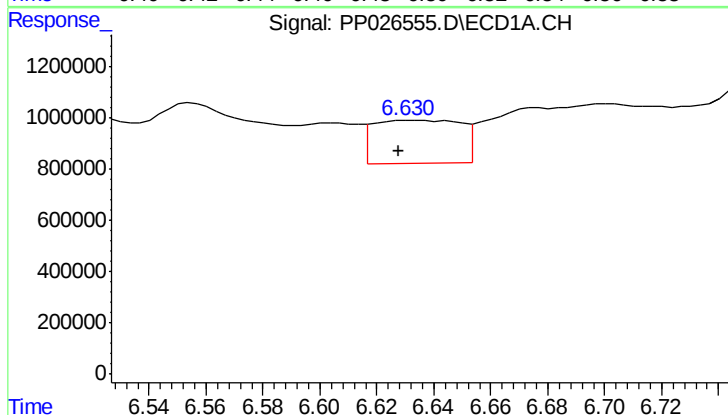


#32 Aroclor-1260-2

R.T.: 6.632 min
Delta R.T.: 0.004 min
Response: 3520232
Conc: 384.15 ng/ml

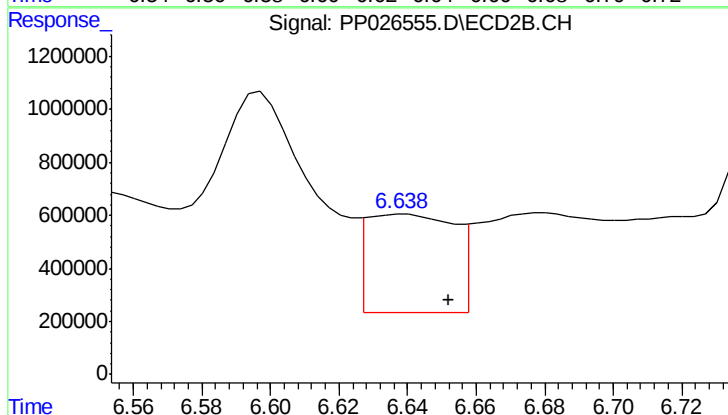

#32 Aroclor-1260-2


R.T.: 6.639 min
Delta R.T.: -0.013 min
Response: 6571858
Conc: 715.72 ng/ml

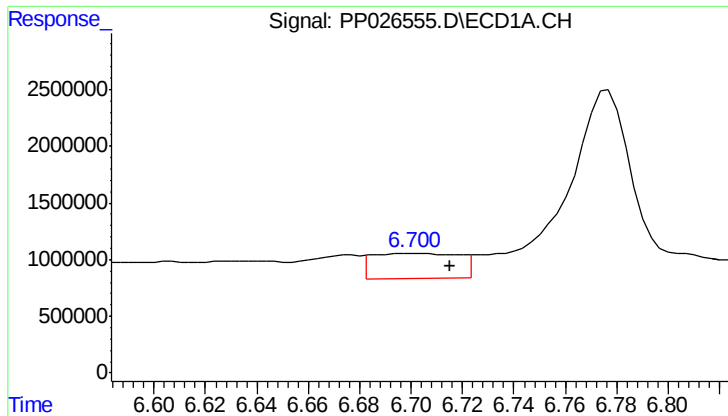

#33 Aroclor-1260-3


R.T.: 6.702 min
Delta R.T.: -0.013 min
Response: 5152720
Conc: 781.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

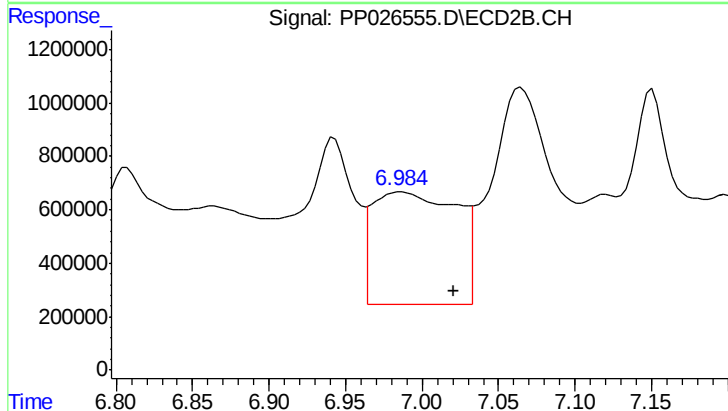


#33 Aroclor-1260-3

R.T.: 6.986 min
Delta R.T.: -0.035 min
Response: 15993275
Conc: 2440.60 ng/ml

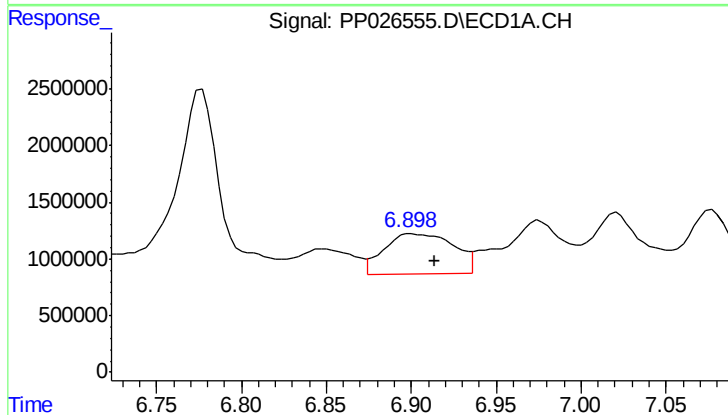


#34 Aroclor-1260-4

R.T.: 6.900 min
Delta R.T.: -0.014 min
Response: 10012483
Conc: 1932.39 ng/ml

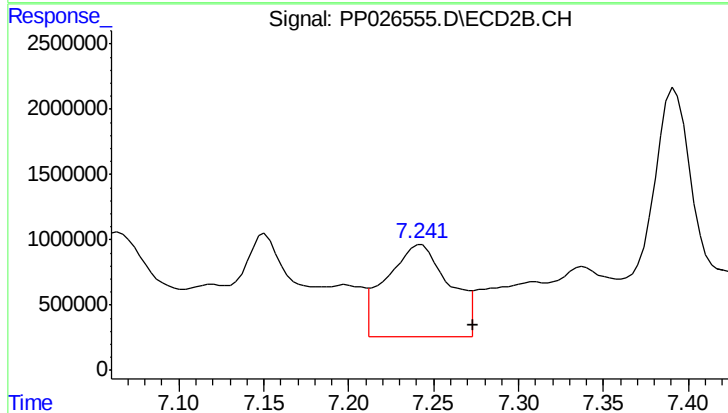

#34 Aroclor-1260-4


R.T.: 7.243 min
Delta R.T.: -0.031 min
Response: 18457610
Conc: 2515.23 ng/ml

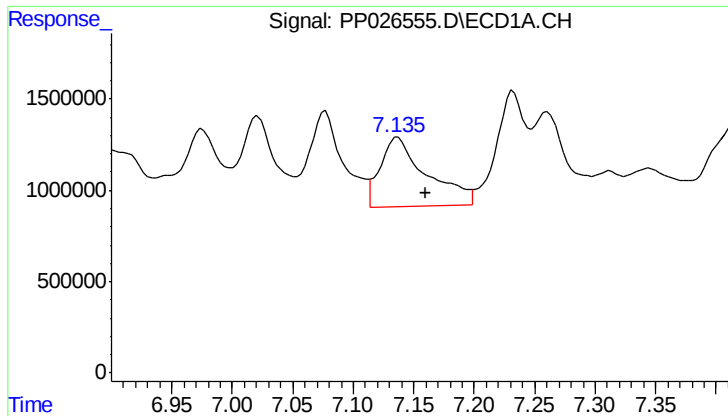

#35 Aroclor-1260-5


R.T.: 7.137 min
Delta R.T.: -0.023 min
Response: 10212224
Conc: 553.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

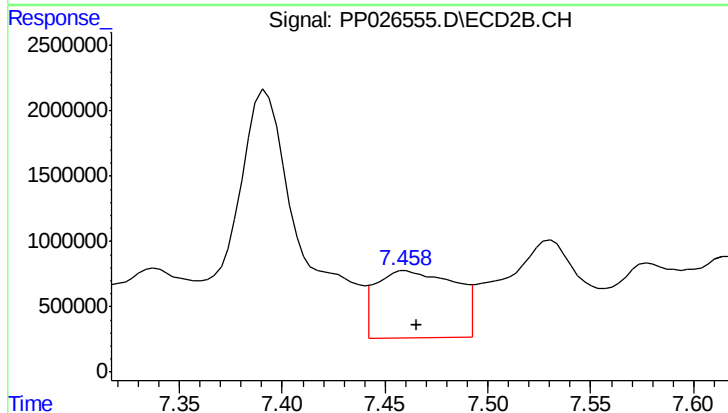


#35 Aroclor-1260-5

R.T.: 7.460 min
Delta R.T.: -0.006 min
Response: 13772249
Conc: 870.92 ng/ml

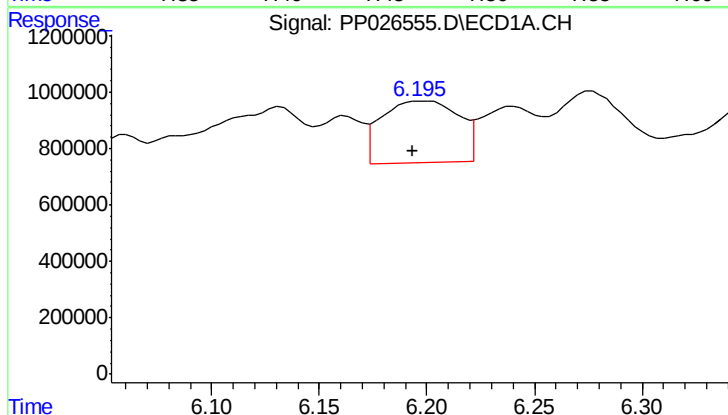


#36 Aroclor-1262-1

R.T.: 6.198 min
Delta R.T.: 0.004 min
Response: 5445056
Conc: 1634.27 ng/ml

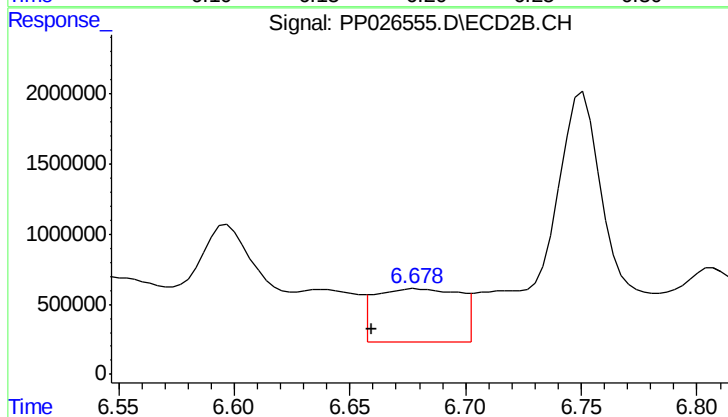

#36 Aroclor-1262-1


R.T.: 6.679 min
Delta R.T.: 0.020 min
Response: 9609239
Conc: 1178.95 ng/ml

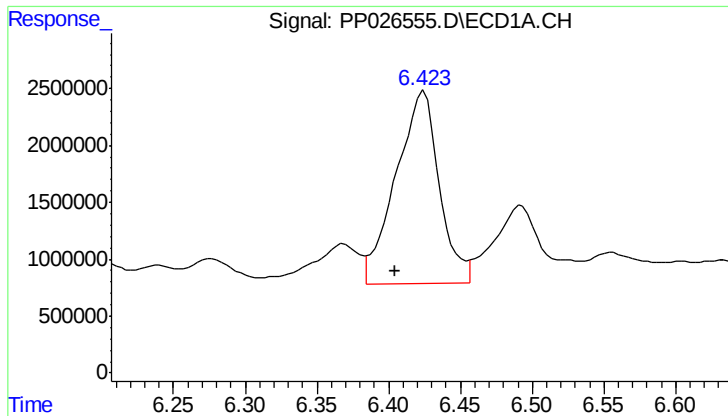

#37 Aroclor-1262-2


R.T.: 6.425 min
Delta R.T.: 0.020 min
Response: 35484903
Conc: 5289.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

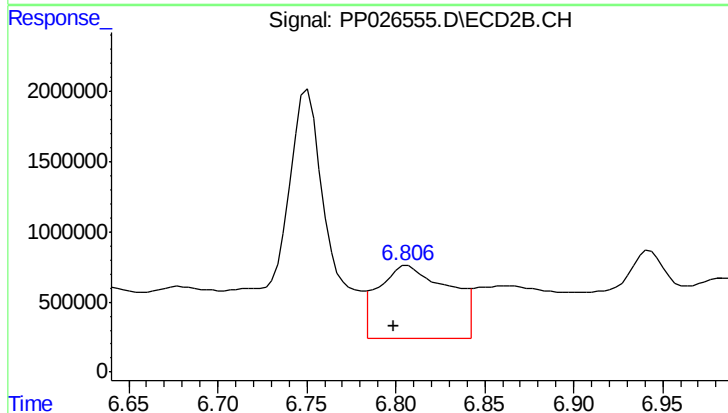


#37 Aroclor-1262-2

R.T.: 6.807 min
Delta R.T.: 0.009 min
Response: 14537709
Conc: 3088.04 ng/ml

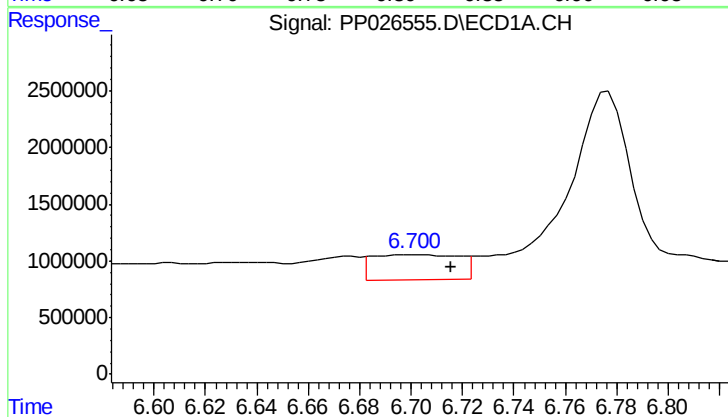


#38 Aroclor-1262-3

R.T.: 6.702 min
Delta R.T.: -0.014 min
Response: 5152720
Conc: 445.34 ng/ml

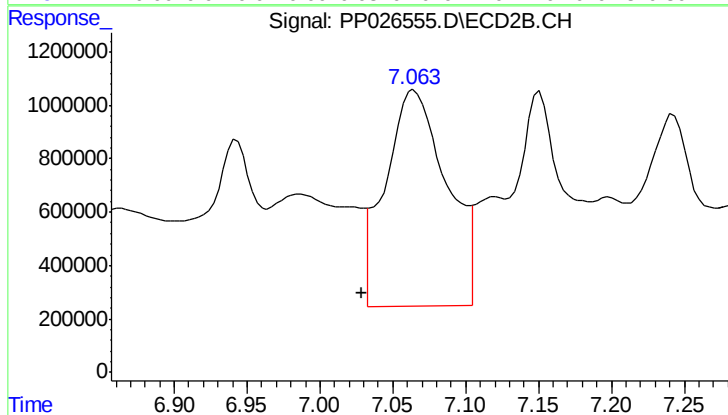

#38 Aroclor-1262-3


R.T.: 7.064 min
Delta R.T.: 0.036 min
Response: 23580420
Conc: 2138.92 ng/ml

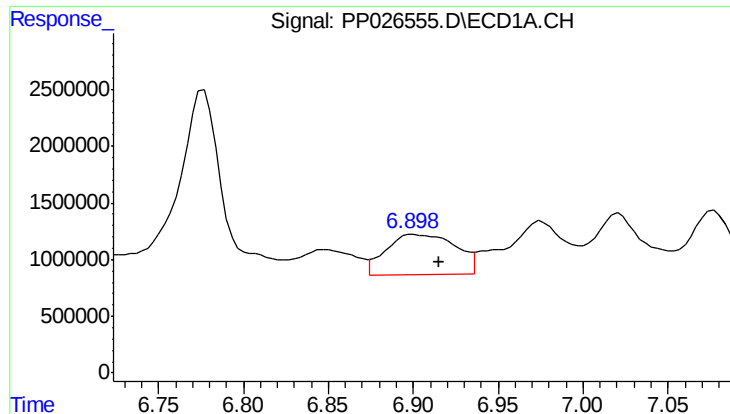

#39 Aroclor-1262-4


R.T.: 6.900 min
Delta R.T.: -0.015 min
Response: 10012483
Conc: 1238.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

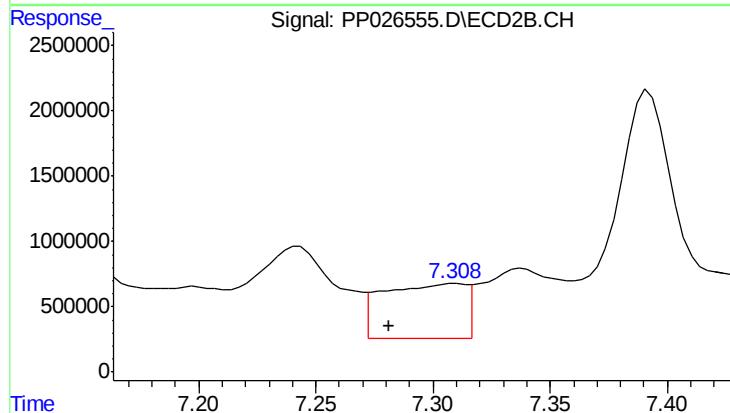


#39 Aroclor-1262-4

R.T.: 7.310 min
Delta R.T.: 0.029 min
Response: 10343585
Conc: 1035.01 ng/ml

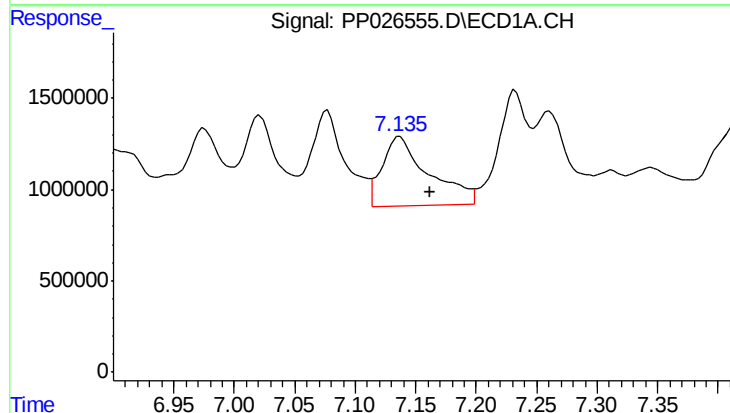


#40 Aroclor-1262-5

R.T.: 7.137 min
Delta R.T.: -0.025 min
Response: 10212224
Conc: 386.15 ng/ml

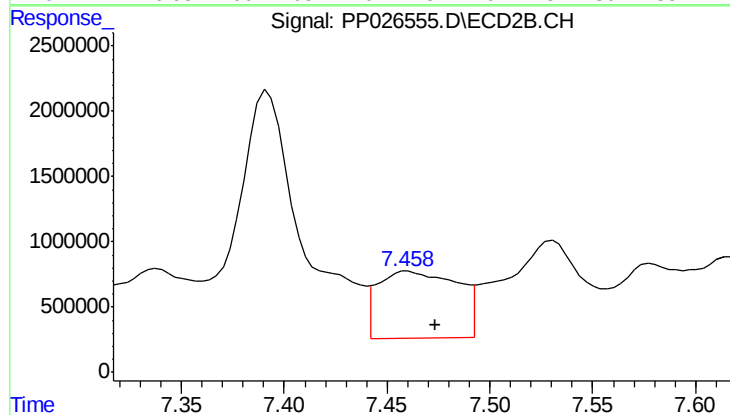

#40 Aroclor-1262-5


R.T.: 7.460 min
Delta R.T.: -0.014 min
Response: 13772249
Conc: 653.67 ng/ml

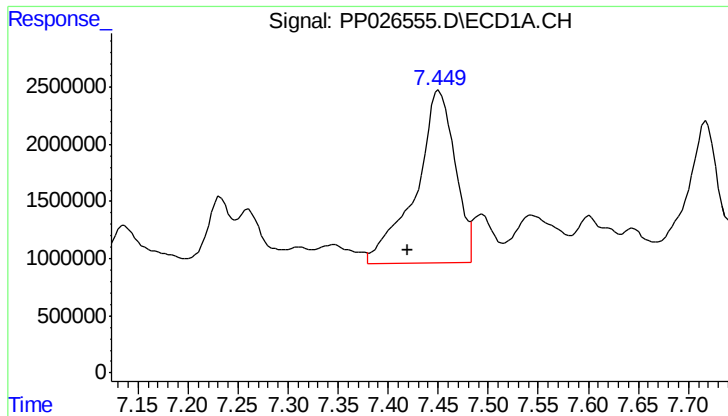

#41 Aroclor-1268-1


R.T.: 7.451 min
Delta R.T.: 0.031 min
Response: 41479073
Conc: 1528.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

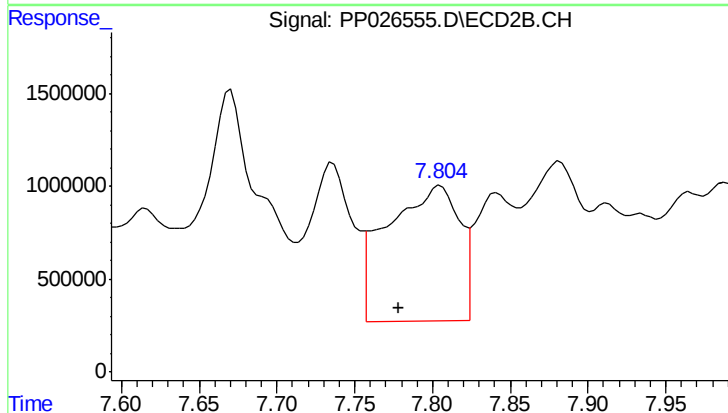


#41 Aroclor-1268-1

R.T.: 7.805 min
Delta R.T.: 0.027 min
Response: 23503305
Conc: 1141.48 ng/ml

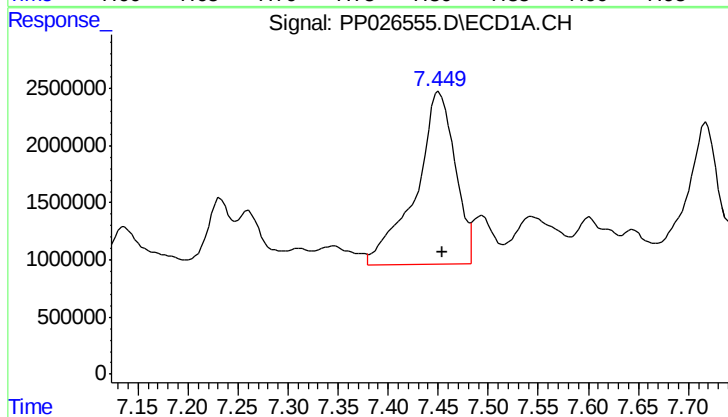


#42 Aroclor-1268-2

R.T.: 7.451 min
Delta R.T.: -0.004 min
Response: 41479073
Conc: 2007.84 ng/ml

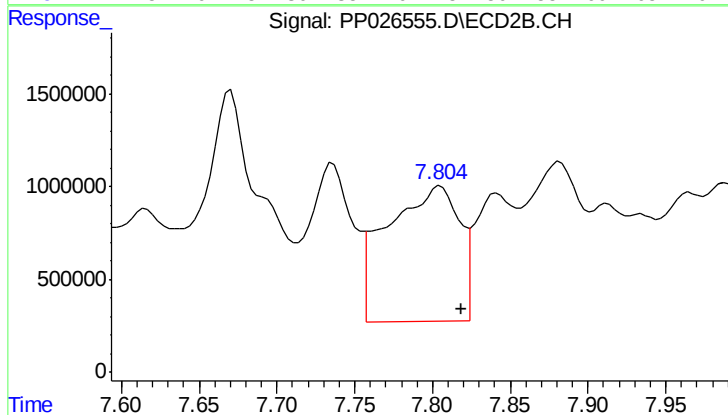

#42 Aroclor-1268-2


R.T.: 7.805 min
Delta R.T.: -0.014 min
Response: 23503305
Conc: 1251.28 ng/ml

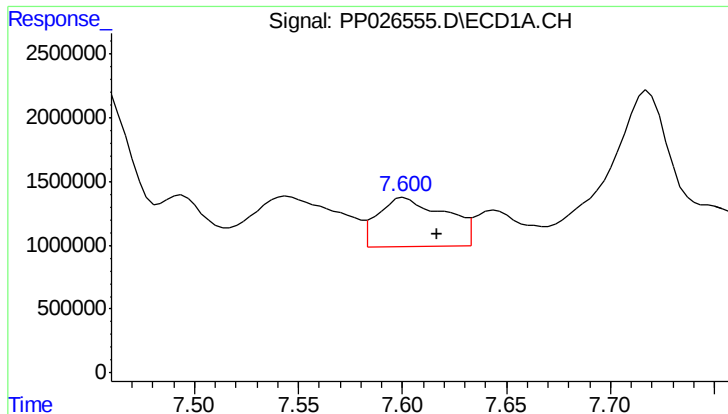

#43 Aroclor-1268-3


R.T.: 7.601 min
Delta R.T.: -0.016 min
Response: 8776121
Conc: 476.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

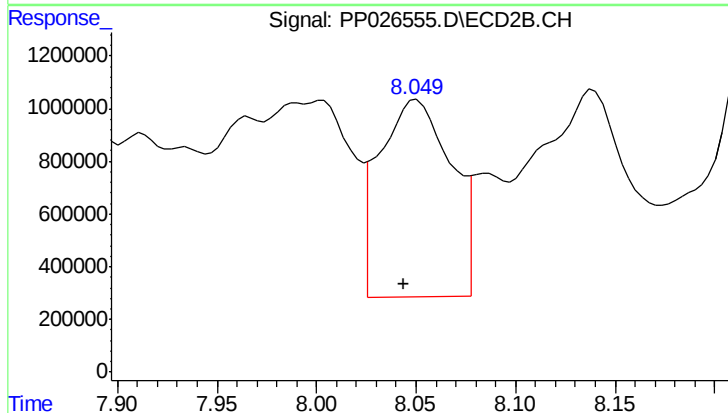


#43 Aroclor-1268-3

R.T.: 8.050 min
Delta R.T.: 0.006 min
Response: 18770227
Conc: 1216.03 ng/ml

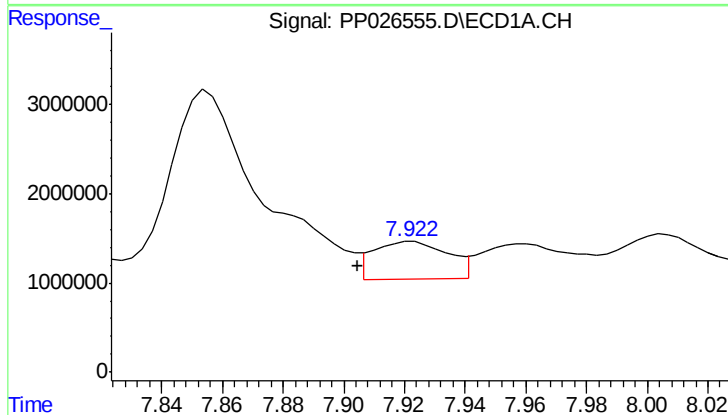


#44 Aroclor-1268-4

R.T.: 7.923 min
Delta R.T.: 0.018 min
Response: 7114038
Conc: 864.21 ng/ml

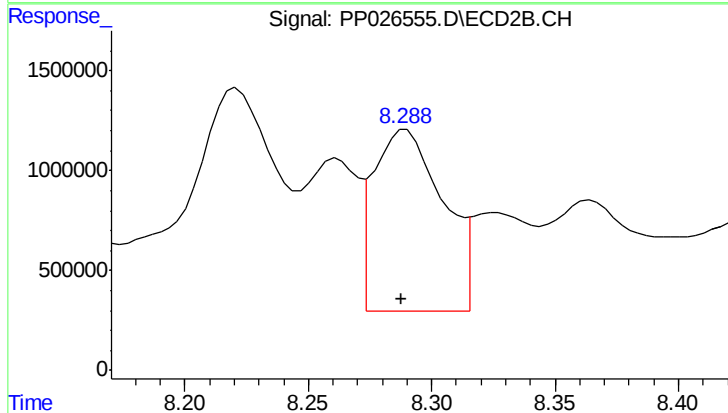

#44 Aroclor-1268-4


R.T.: 8.290 min
Delta R.T.: 0.002 min
Response: 17929678
Conc: 2418.21 ng/ml

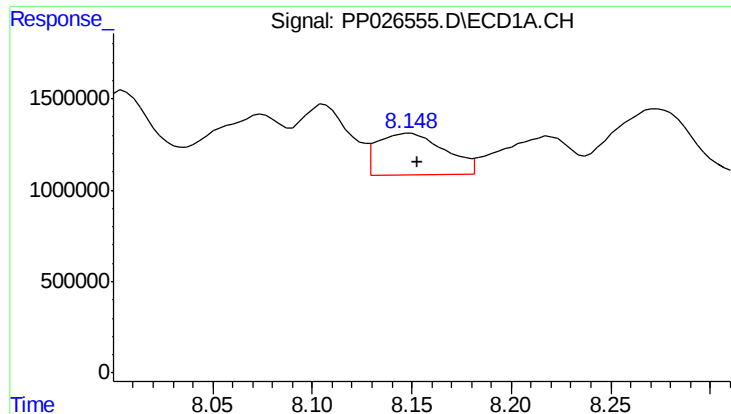

#45 Aroclor-1268-5

R.T.: 8.149 min
Delta R.T.: -0.003 min
Response: 5393637
Conc: 89.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPTW-04MSD

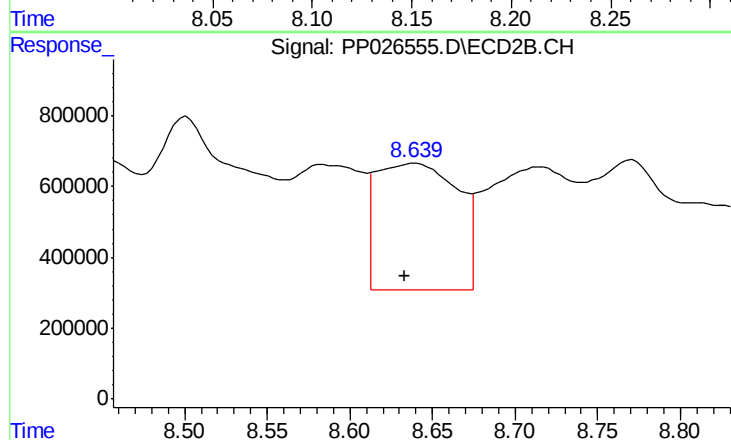

#45 Aroclor-1268-5

R.T.: 8.640 min
Delta R.T.: 0.007 min
Response: 12313116
Conc: 219.22 ng/ml