

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062218\
Data File : P0046068.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2018 10:01
Operator : SM/UA
Sample : J3603-13RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
26KV-TP-10RE

Manual Integrations
APPROVED

ugo
6/25/2018 2:58:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 10:19:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.382	3.610	9005134	4846812	18.832	19.280
2)	SA Decachlor...	10.055	8.584	4363142	1809348	10.409	11.553m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062218\
Data File : P0046068.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2018 10:01
Operator : SM/UA
Sample : J3603-13RE
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
26KV-TP-10RE


Manual Integrations
APPROVED

ugo
6/25/2018 2:58:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 10:19:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

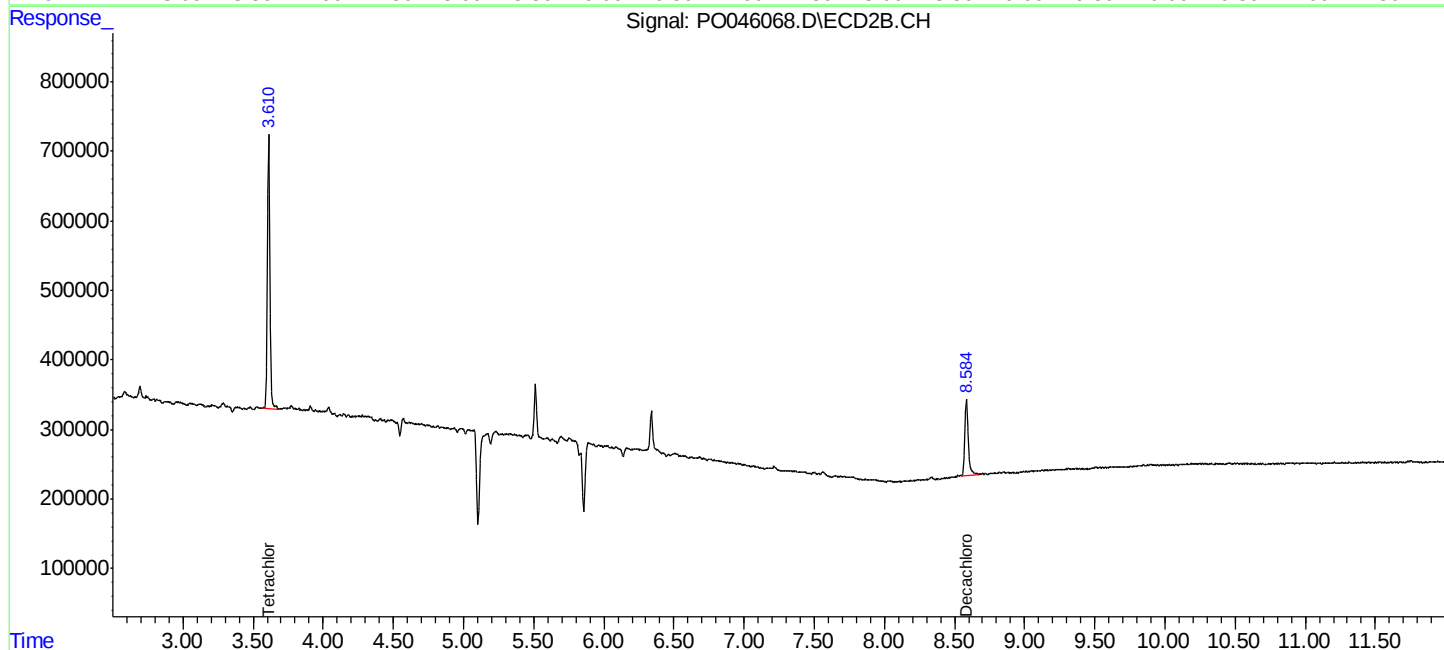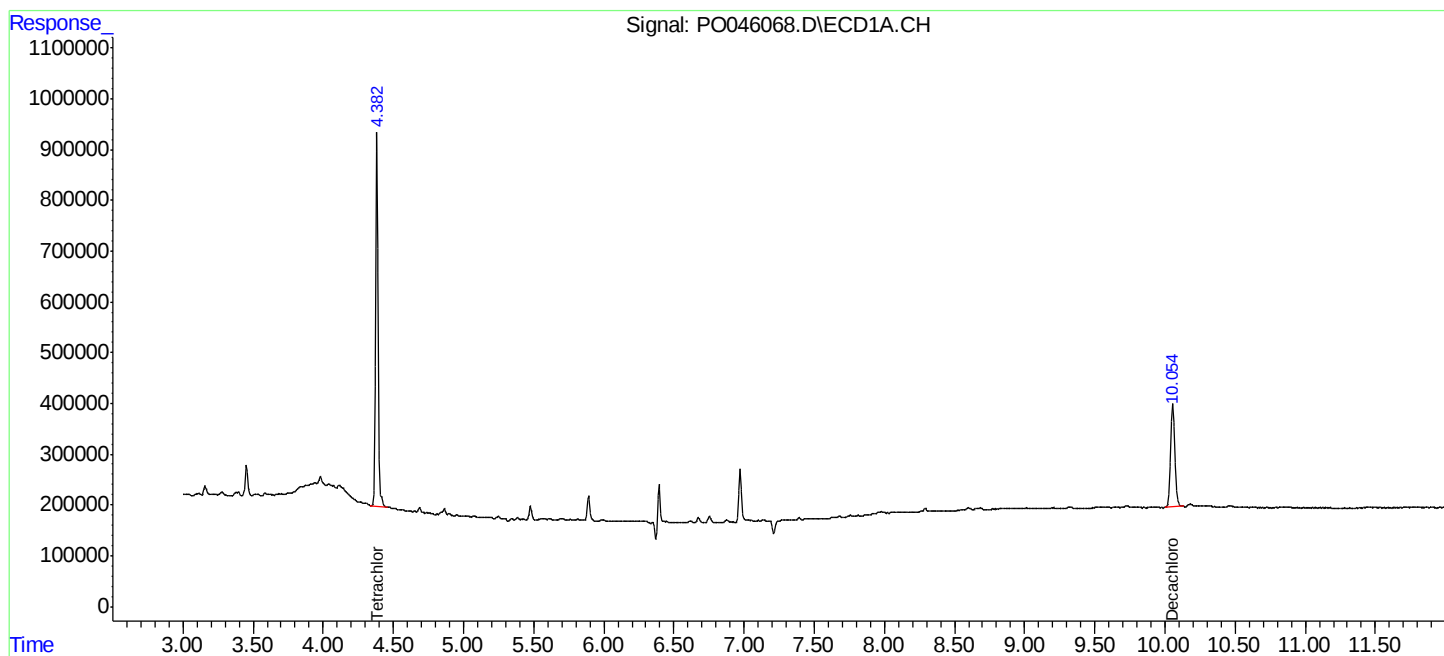

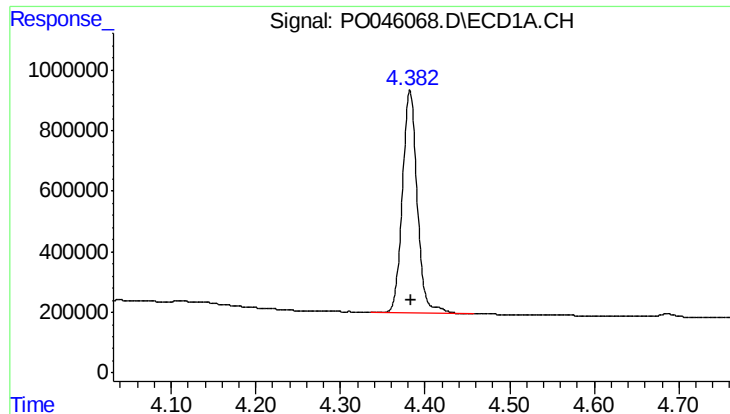


#1 Tetrachloro-m-xylene

R.T.: 4.382 min
Delta R.T.: -0.001 min
Response: 9005134
Conc: 18.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
26KV-TP-10RE


Manual Integrations
APPROVED

ugo
6/25/2018 2:58:54 PM

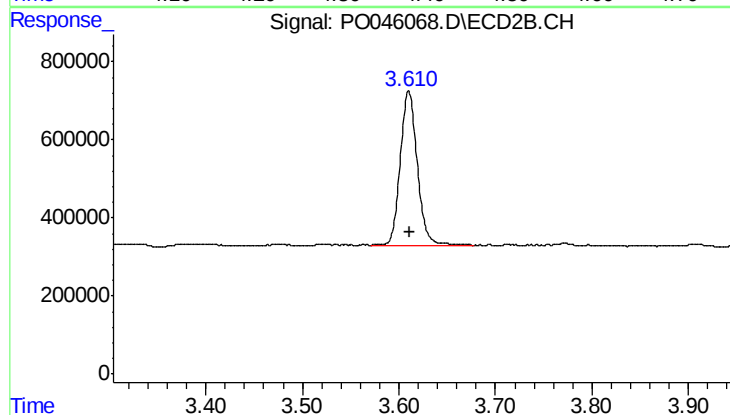


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: -0.002 min
Response: 4846812
Conc: 19.28 ng/ml

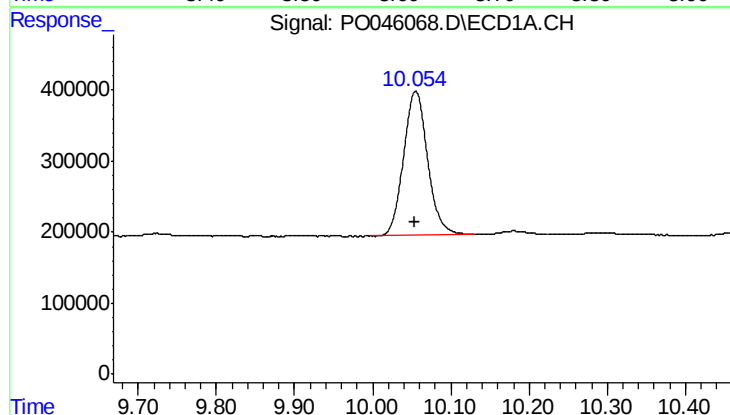

#2 Decachlorobiphenyl

R.T.: 10.055 min
Delta R.T.: 0.001 min
Response: 4363142
Conc: 10.41 ng/ml

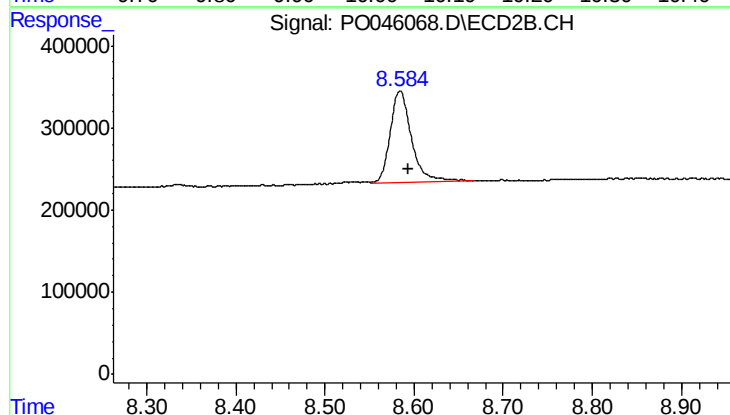

#2 Decachlorobiphenyl

R.T.: 8.584 min
Delta R.T.: -0.009 min
Response: 1809348
Conc: 11.55 ng/ml m