

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062218\
 Data File : P0046073.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2018 11:20
 Operator : SM/UA
 Sample : J3603-01RE
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 26KV-TP-1RE

Manual Integrations
 APPROVED

ugo
 6/25/2018 2:59:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 11:36:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 20 03:39:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.382	3.610	10779710	5187521	22.543	20.635
2) SA Decachlor...	10.054	8.584	4619960	1761387	11.022	11.247m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062218\
Data File : P0046073.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2018 11:20
Operator : SM/UA
Sample : J3603-01RE
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
26KV-TP-1RE


Manual Integrations
APPROVED

ugo
6/25/2018 2:59:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 11:36:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

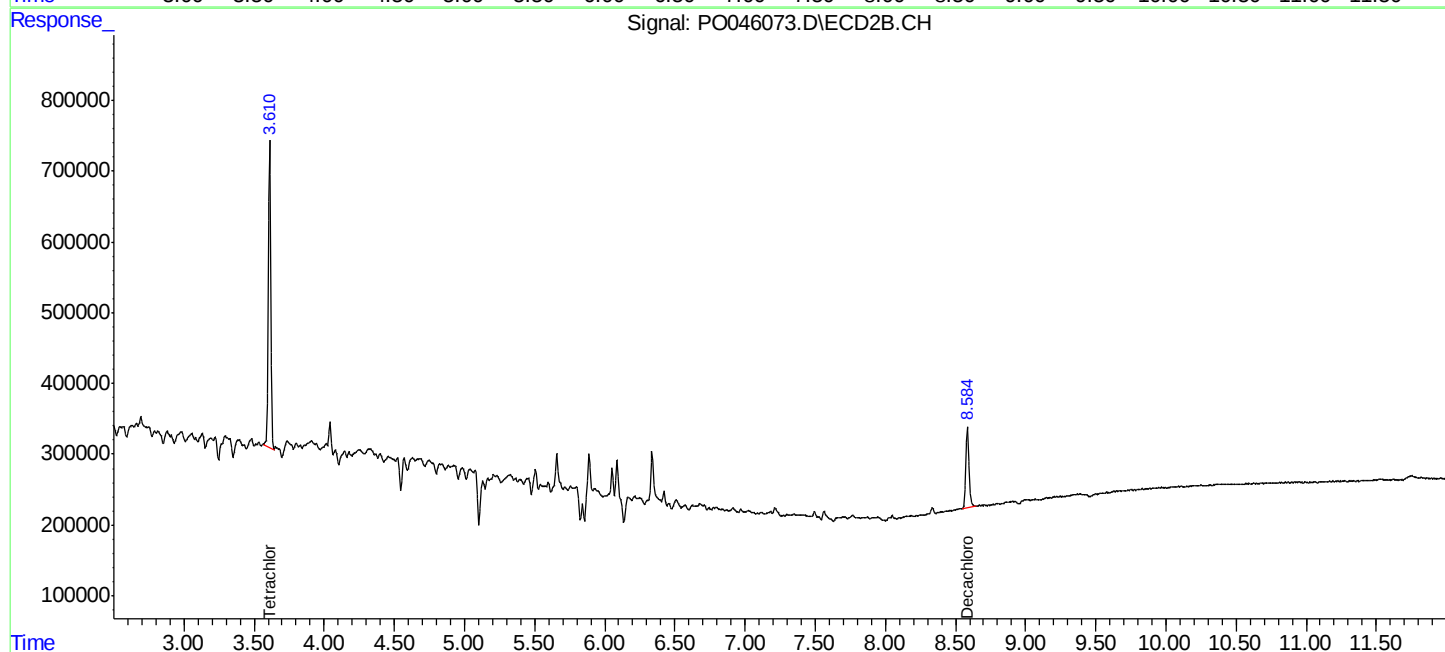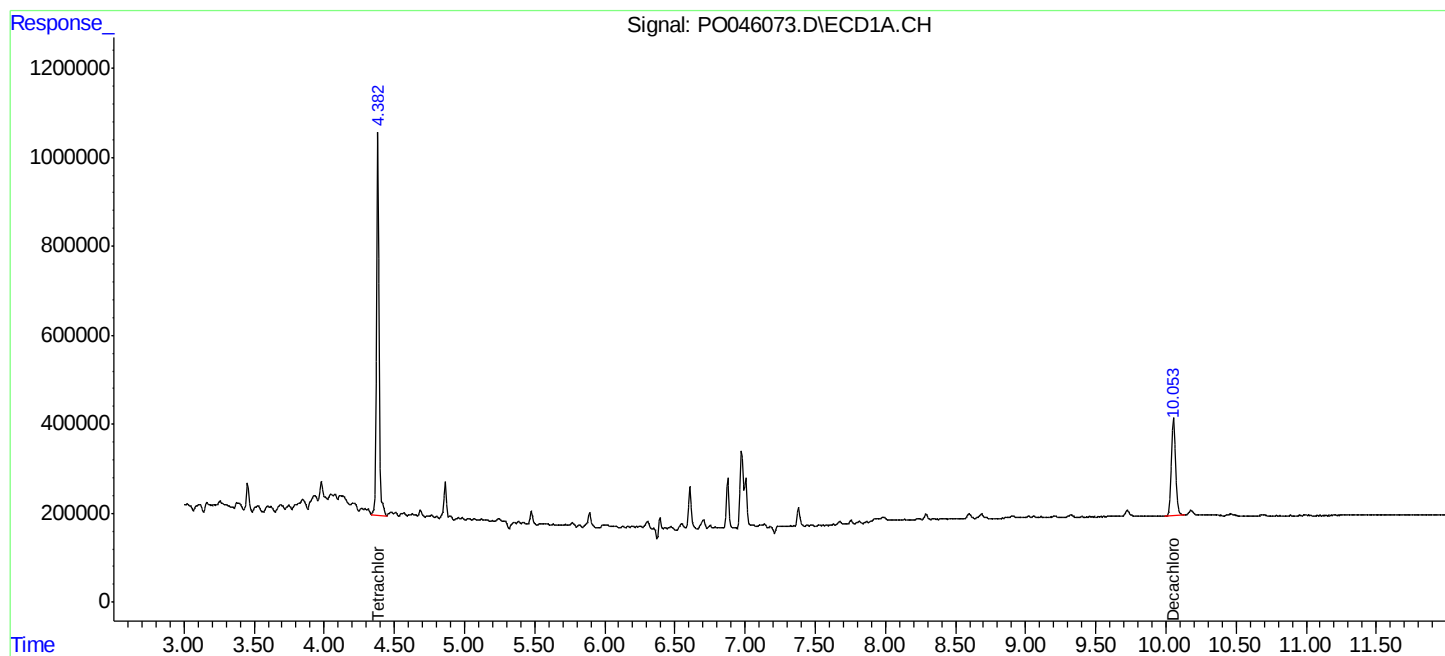

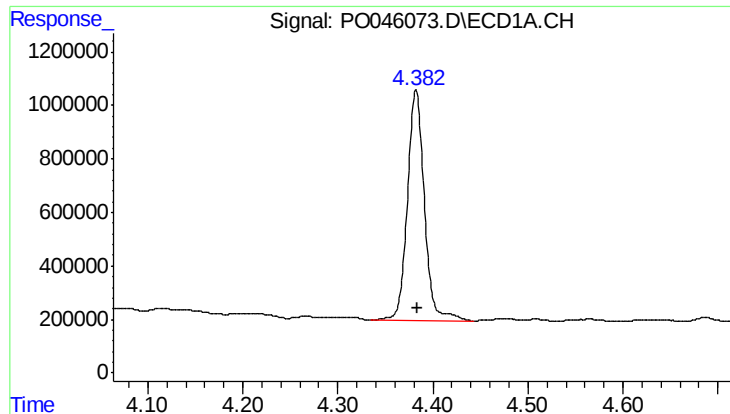


#1 Tetrachloro-m-xylene

R.T.: 4.382 min
Delta R.T.: -0.001 min
Response: 10779710
Conc: 22.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
26KV-TP-1RE


Manual Integrations
APPROVED

ugo
6/25/2018 2:59:03 PM

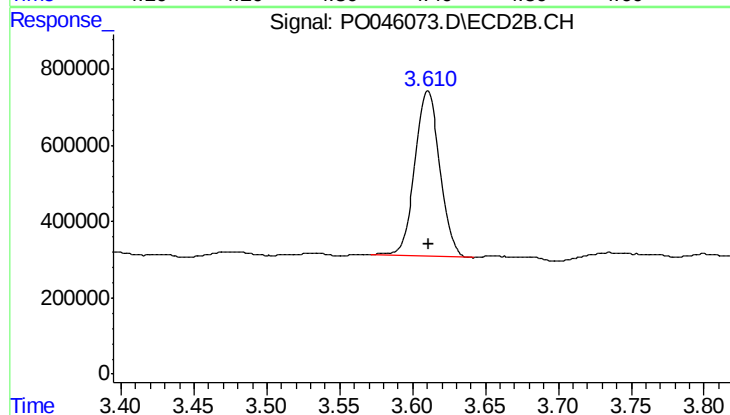


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: -0.001 min
Response: 5187521
Conc: 20.63 ng/ml

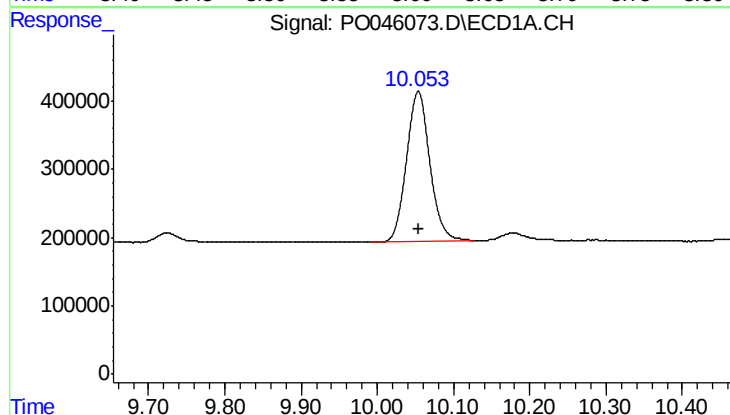

#2 Decachlorobiphenyl

R.T.: 10.054 min
Delta R.T.: 0.000 min
Response: 4619960
Conc: 11.02 ng/ml

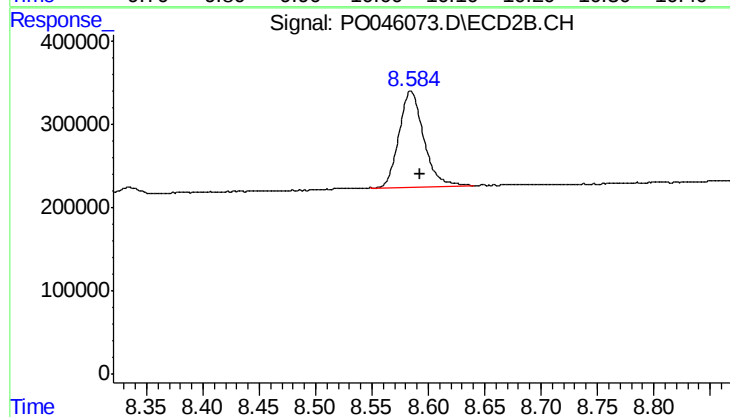

#2 Decachlorobiphenyl

R.T.: 8.584 min
Delta R.T.: -0.009 min
Response: 1761387
Conc: 11.25 ng/ml m