

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0062218\
 Data File : P0046113.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2018 00:08
 Operator : SM/UA
 Sample : J3573-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-48-COMP

Manual Integrations
 APPROVED

ugo
 6/25/2018 3:08:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 04:12:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 20 03:39:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.383	3.611	13166345	6352411	27.534	25.269
2) SA Decachlor...	10.056	8.584	5807828	2350248	13.856m	15.007m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062218\
Data File : P0046113.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2018 00:08
Operator : SM/UA
Sample : J3573-03
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-48-COMP


Manual Integrations
APPROVED

ugo
6/25/2018 3:08:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 04:12:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

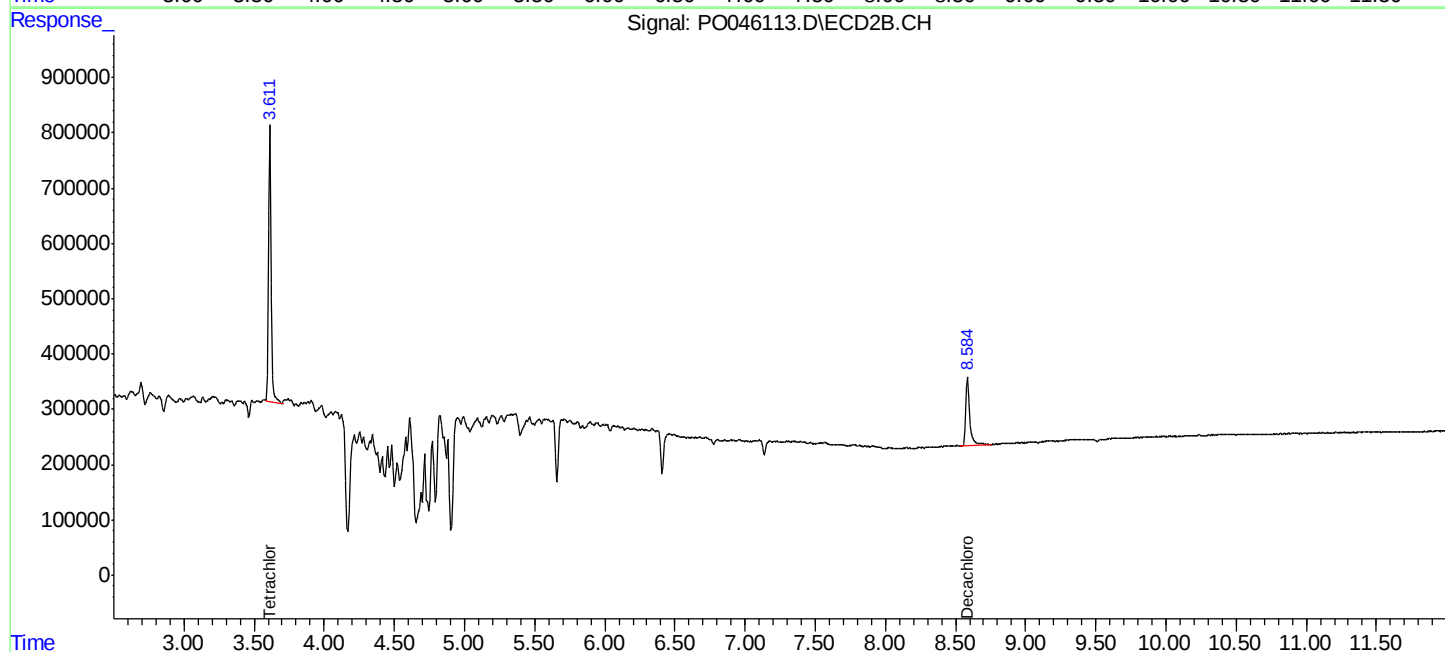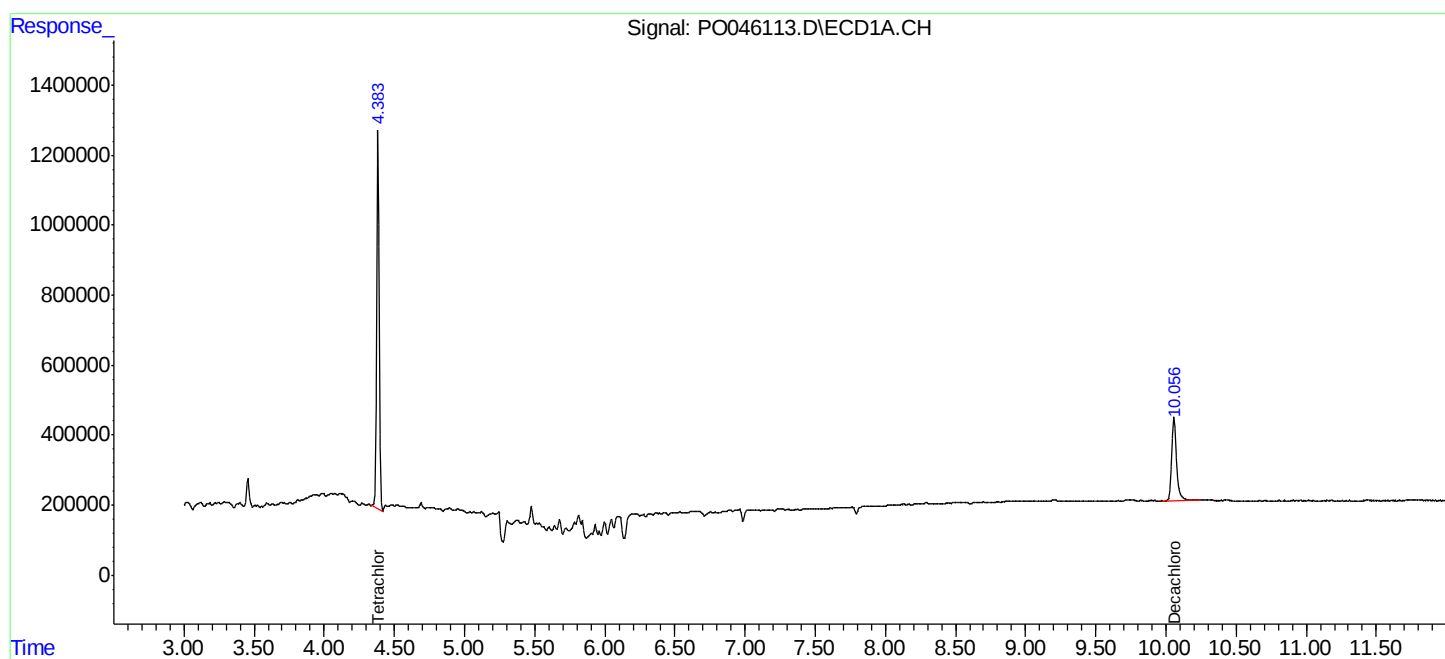

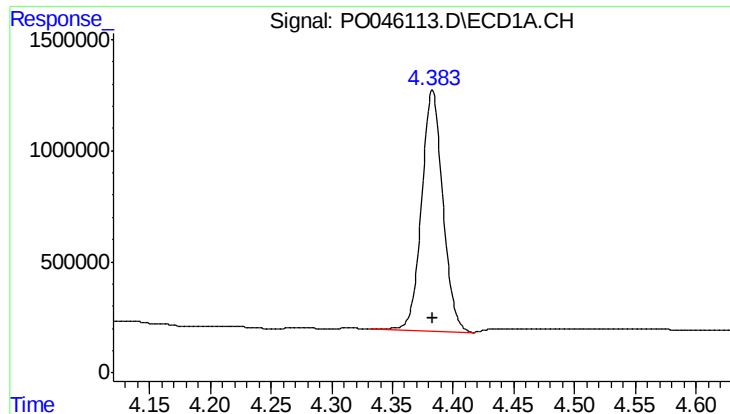


#1 Tetrachloro-m-xylene

R.T.: 4.383 min
Delta R.T.: 0.000 min
Response: 13166345
Conc: 27.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-48-COMP


Manual Integrations
APPROVED

ugo
6/25/2018 3:08:49 PM

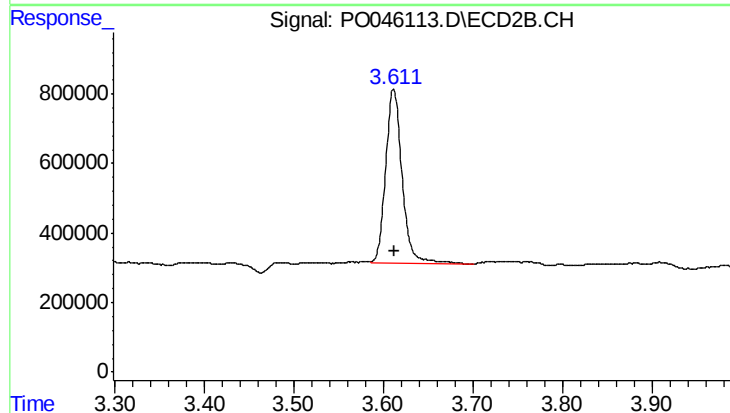


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: 0.000 min
Response: 6352411
Conc: 25.27 ng/ml

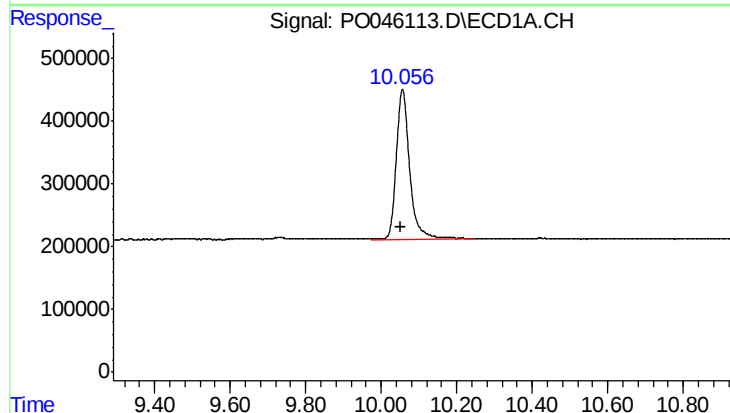

#2 Decachlorobiphenyl

R.T.: 10.056 min
Delta R.T.: 0.002 min
Response: 5807828
Conc: 13.86 ng/ml m

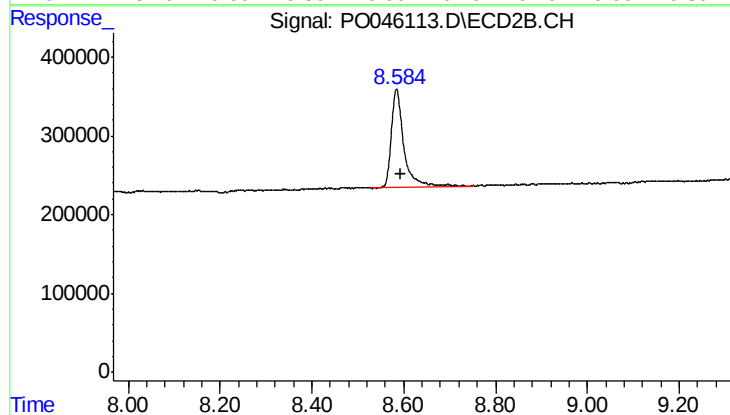

#2 Decachlorobiphenyl

R.T.: 8.584 min
Delta R.T.: -0.009 min
Response: 2350248
Conc: 15.01 ng/ml m