

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0062218\
 Data File : P0046072.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2018 11:04
 Operator : SM/UA
 Sample : J3603-21RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 26KV-TP-6RE

Manual Integrations
 APPROVED

ugo
 6/25/2018 2:59:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 14:03:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 20 03:39:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.381	3.609	7624270	3543797	15.944	14.096
2) SA Decachlor...	10.054	8.584	2600858	1135901	6.205	7.253m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062218\
Data File : P0046072.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2018 11:04
Operator : SM/UA
Sample : J3603-21RE
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
26KV-TP-6RE


Manual Integrations
APPROVED

ugo
6/25/2018 2:59:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 14:03:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

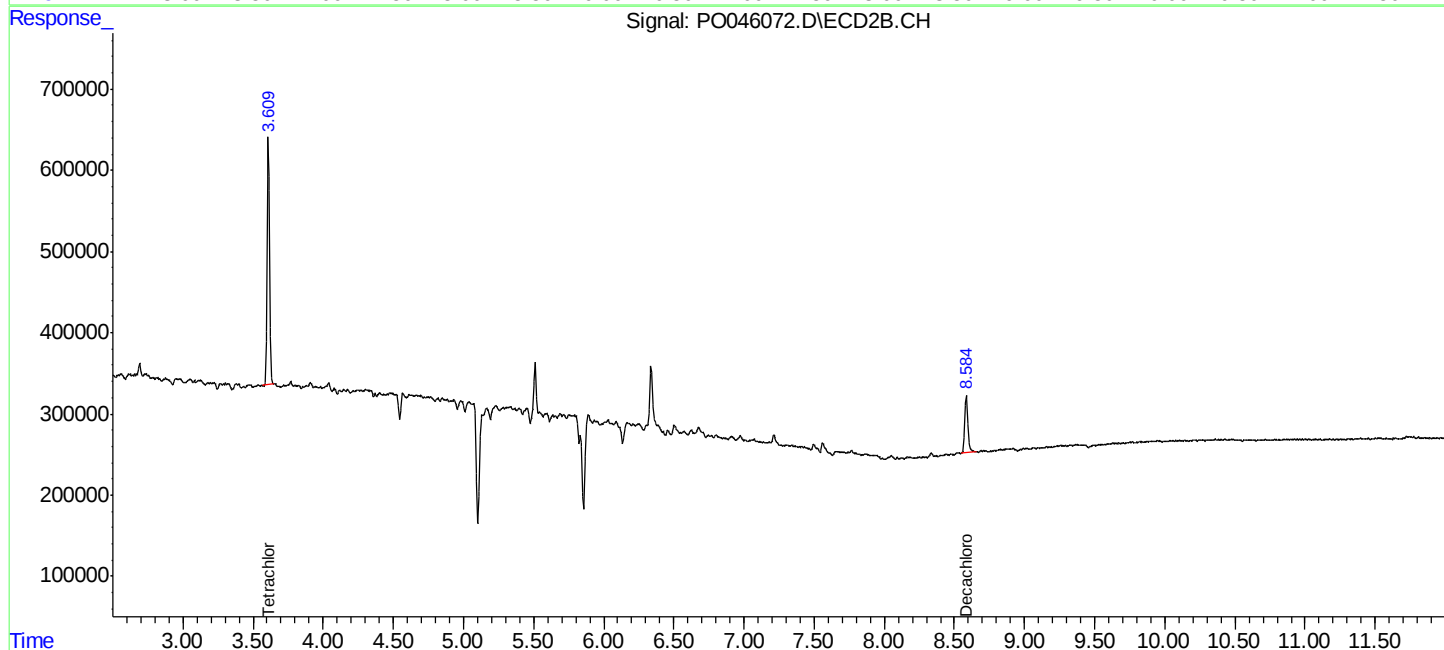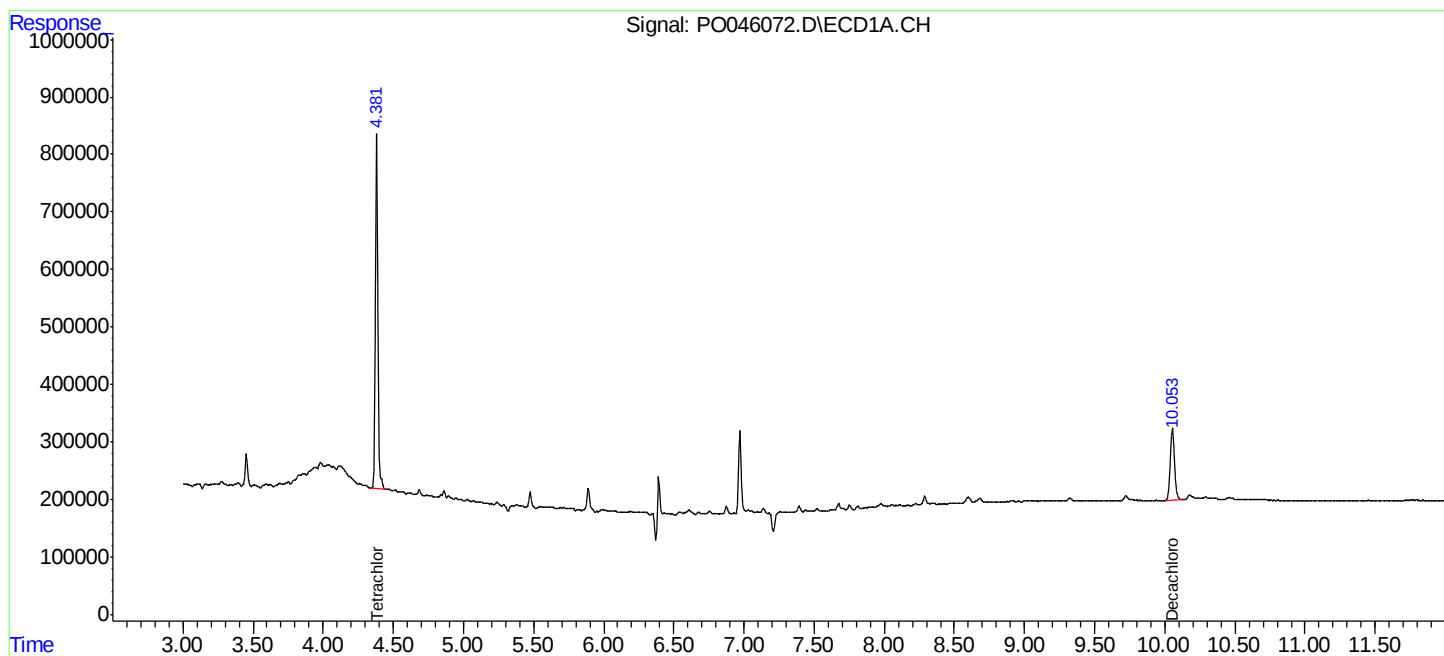

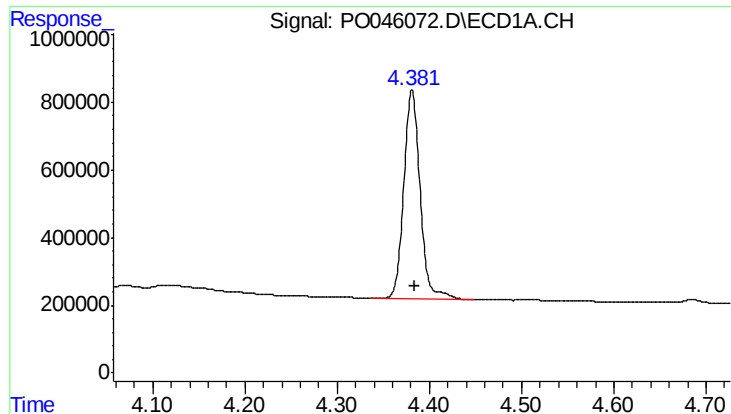


#1 Tetrachloro-m-xylene

R.T.: 4.381 min
Delta R.T.: -0.003 min
Response: 7624270
Conc: 15.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
26KV-TP-6RE


Manual Integrations
APPROVED

ugo
6/25/2018 2:59:00 PM

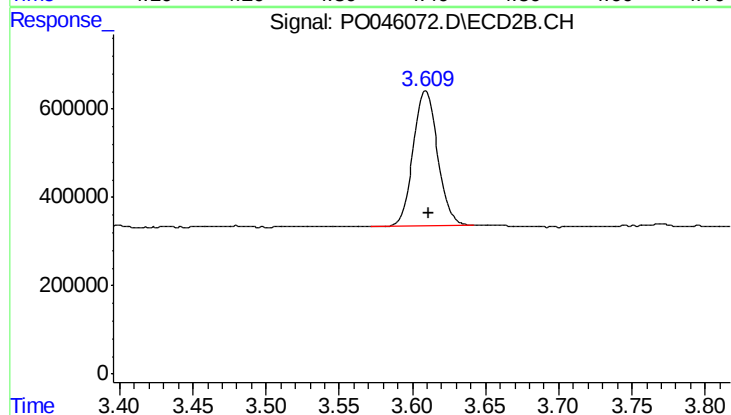


#1 Tetrachloro-m-xylene

R.T.: 3.609 min
Delta R.T.: -0.003 min
Response: 3543797
Conc: 14.10 ng/ml

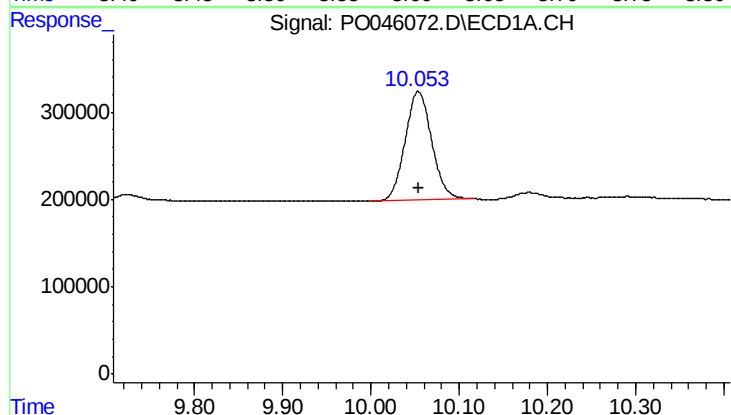

#2 Decachlorobiphenyl

R.T.: 10.054 min
Delta R.T.: 0.000 min
Response: 2600858
Conc: 6.20 ng/ml

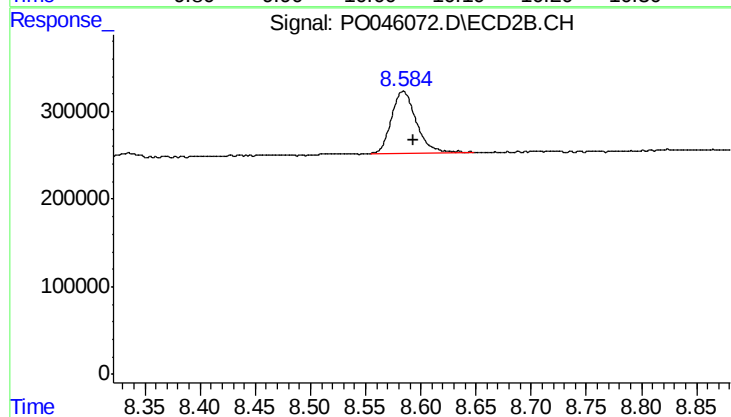

#2 Decachlorobiphenyl

R.T.: 8.584 min
Delta R.T.: -0.009 min
Response: 1135901
Conc: 7.25 ng/ml m