

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0062218\
Data File : P0046105.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2018 22:01
Operator : SM/UA
Sample : J3501-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-10-S1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 03:51:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.384	3.613	22331828	11448075	46.701	45.538
2) SA Decachlor...	10.057	8.586	11604376	4957434	27.685	31.654

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062218\
Data File : P0046105.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2018 22:01
Operator : SM/UA
Sample : J3501-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-10-S1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 03:51:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061918.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 20 03:39:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

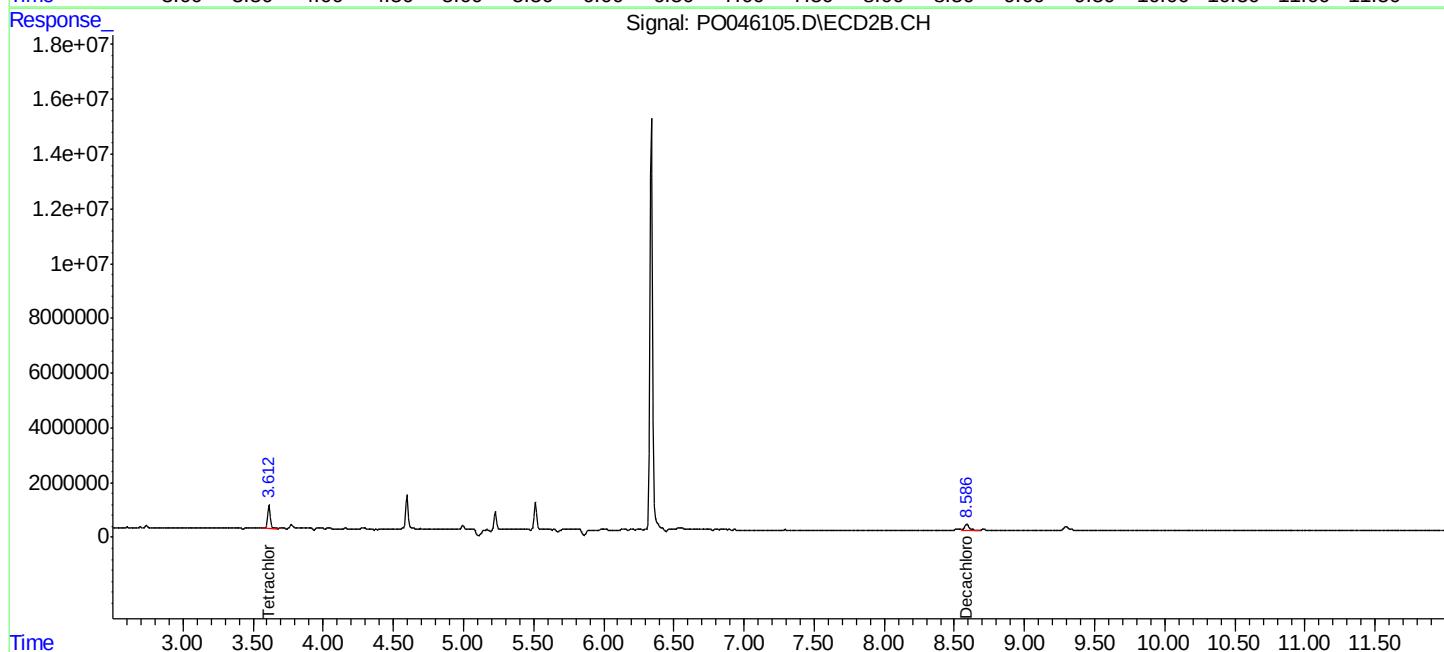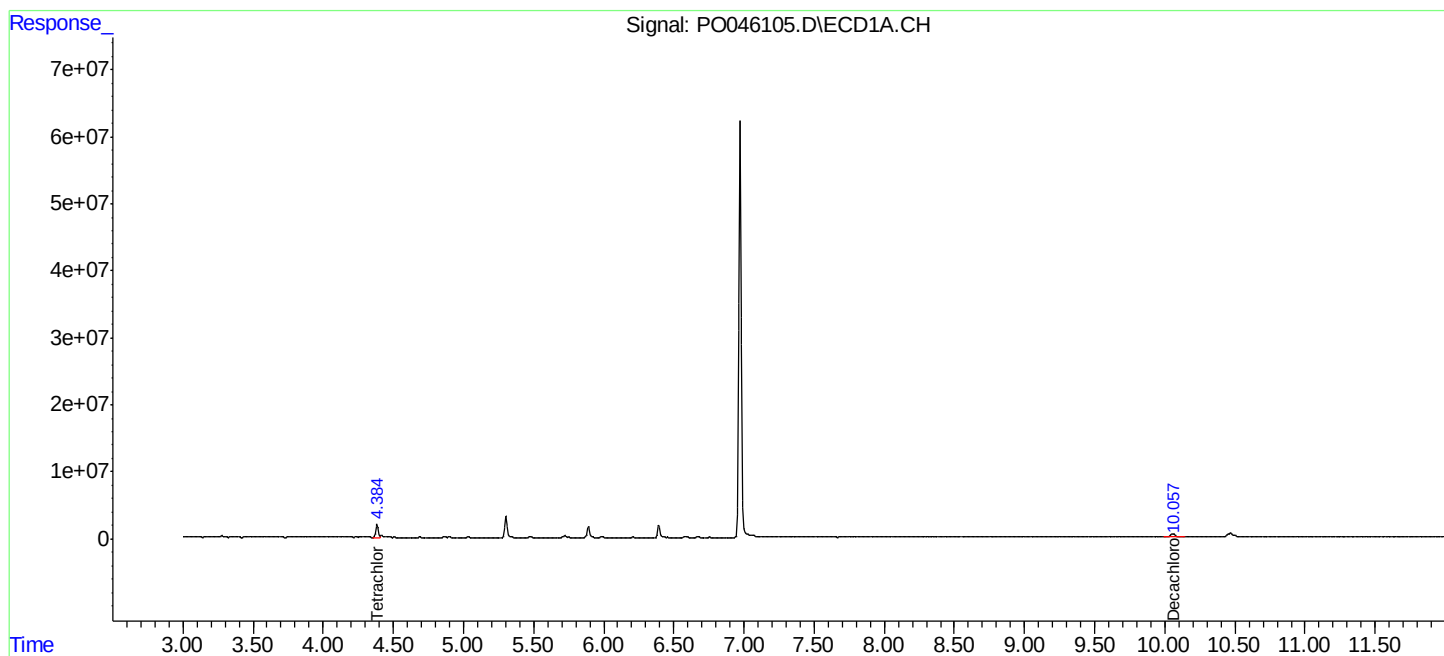


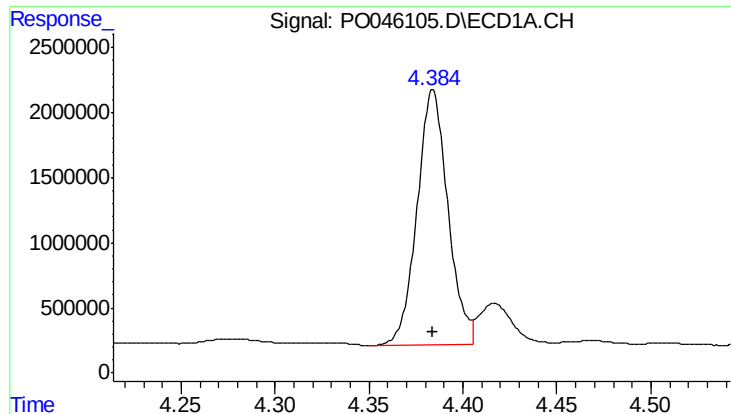

#1 Tetrachloro-m-xylene


R.T.: 4.384 min
Delta R.T.: 0.000 min
Response: 22331828
Conc: 46.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-10-S1

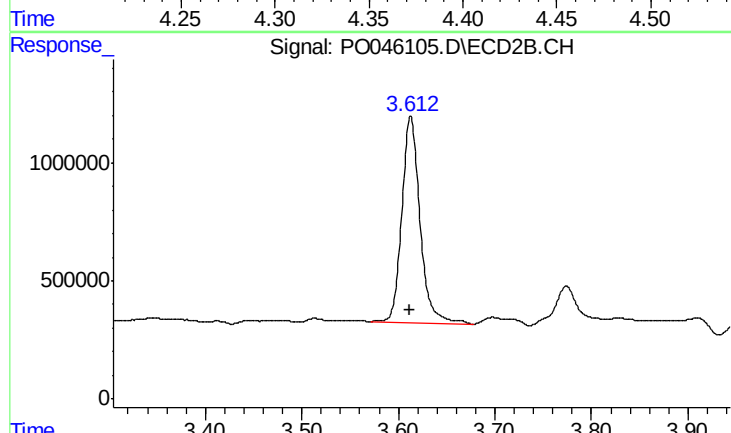


#1 Tetrachloro-m-xylene

R.T.: 3.613 min
Delta R.T.: 0.001 min
Response: 11448075
Conc: 45.54 ng/ml

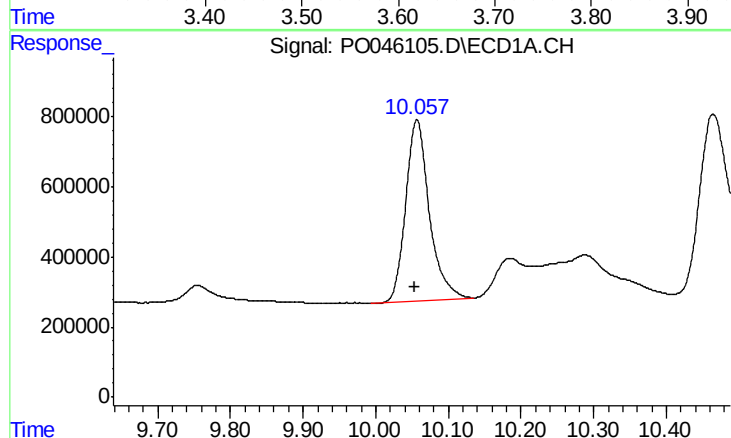

#2 Decachlorobiphenyl

R.T.: 10.057 min
Delta R.T.: 0.003 min
Response: 11604376
Conc: 27.68 ng/ml

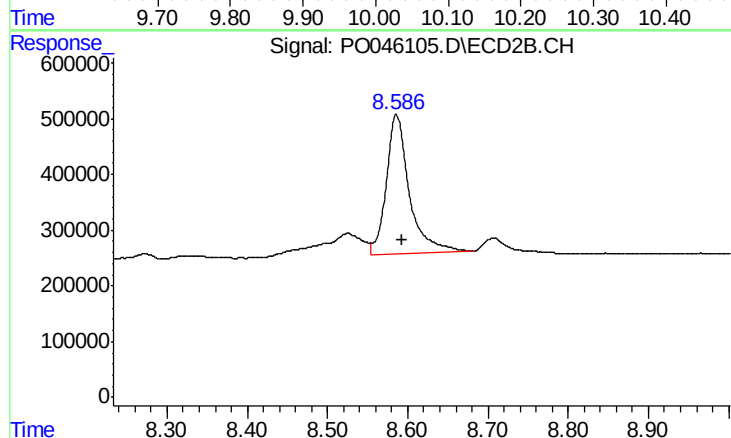

#2 Decachlorobiphenyl

R.T.: 8.586 min
Delta R.T.: -0.007 min
Response: 4957434
Conc: 31.65 ng/ml