

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062220\
 Data File : P0069089.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2020 15:03
 Operator : DD\AJ
 Sample : L3079-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 JFK-SB-01-0.0-72.0-D

Manual Integrations
 APPROVED

Sohil
 6/23/2020 8:07:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 19:42:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 19 05:15:02 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.405	3.565	766035	941908	25.894	24.472
2) SA Decachlor...	10.074	8.773	974472	1131990	20.517m	20.795

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062220\
Data File : P0069089.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2020 15:03
Operator : DD\AJ
Sample : L3079-10
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
JFK-SB-01-0.0-72.0-D


Manual Integrations
APPROVED

Sohil
6/23/2020 8:07:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 19:42:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 19 05:15:02 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

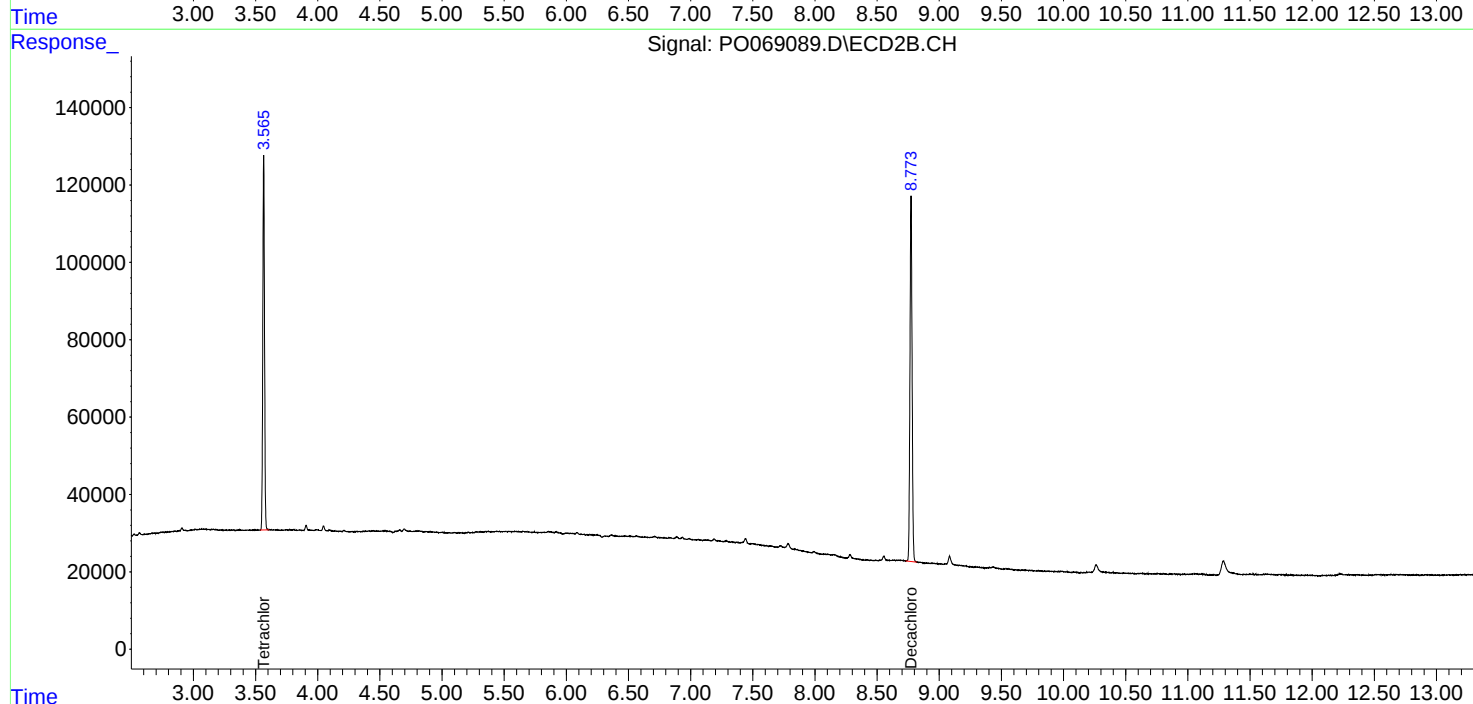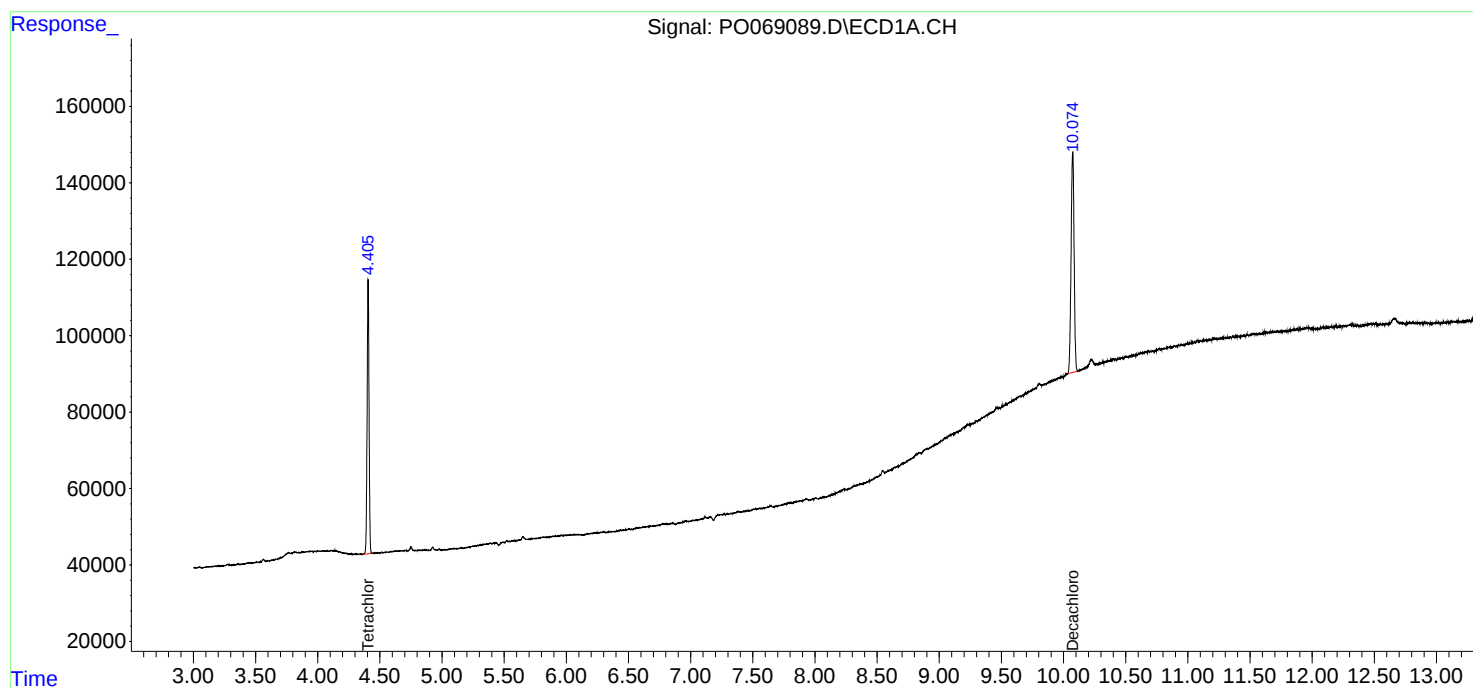

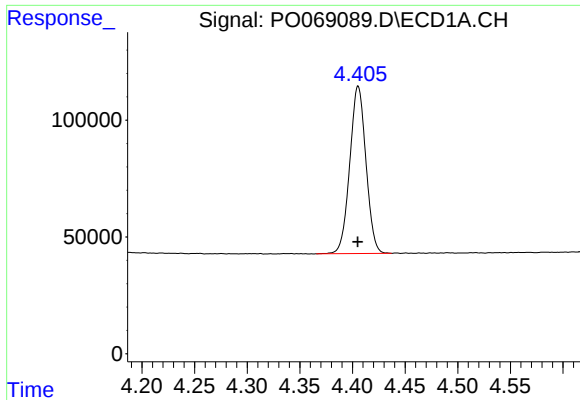


#1 Tetrachloro-m-xylene

R.T.: 4.405 min
Delta R.T.: 0.000 min
Response: 766035
Conc: 25.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
JFK-SB-01-0.0-72.0-D


Manual Integrations
APPROVED

Sohil
6/23/2020 8:07:19 AM

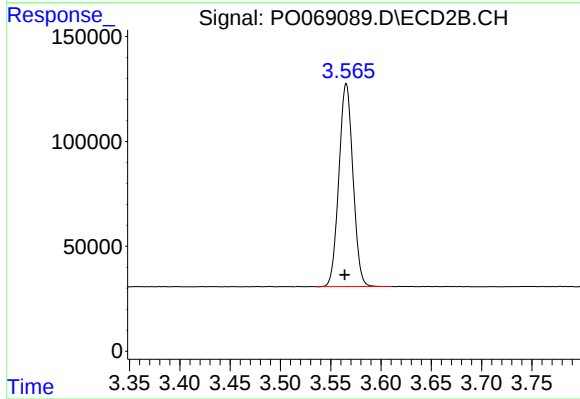


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.001 min
Response: 941908
Conc: 24.47 ng/ml

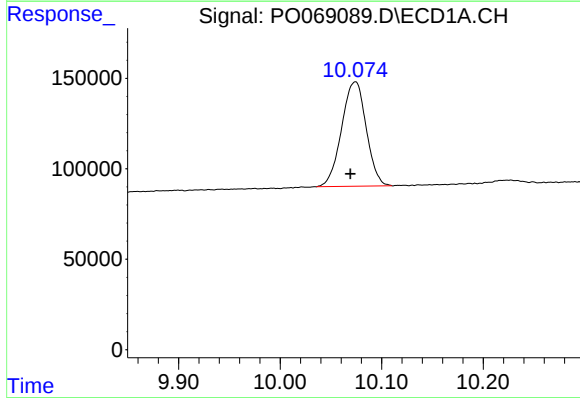

#2 Decachlorobiphenyl

R.T.: 10.074 min
Delta R.T.: 0.005 min
Response: 974472
Conc: 20.52 ng/ml m

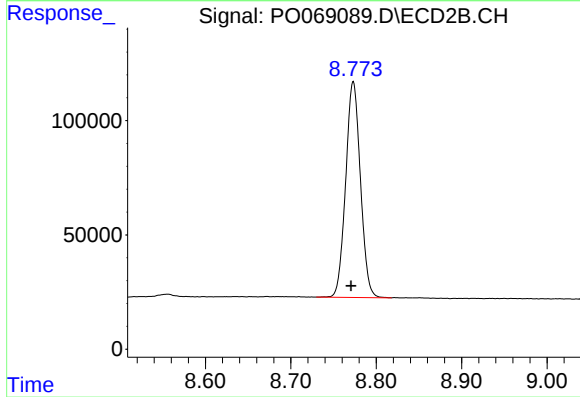

#2 Decachlorobiphenyl

R.T.: 8.773 min
Delta R.T.: 0.003 min
Response: 1131990
Conc: 20.80 ng/ml