

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062220\
 Data File : P0069109.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2020 20:50
 Operator : DD\AJ
 Sample : L3082-17
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-18

Manual Integrations
 APPROVED

Sohil
 6/23/2020 2:20:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 05:31:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 19 05:15:02 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.404	3.565	706930	846352	23.896m	21.989
2) SA Decachlor...	10.070	8.773	922124	1000573	19.415	18.381

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062220\
Data File : P0069109.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2020 20:50
Operator : DD\AJ
Sample : L3082-17
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB-18


Manual Integrations
APPROVED

Sohil
6/23/2020 2:20:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 05:31:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 19 05:15:02 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

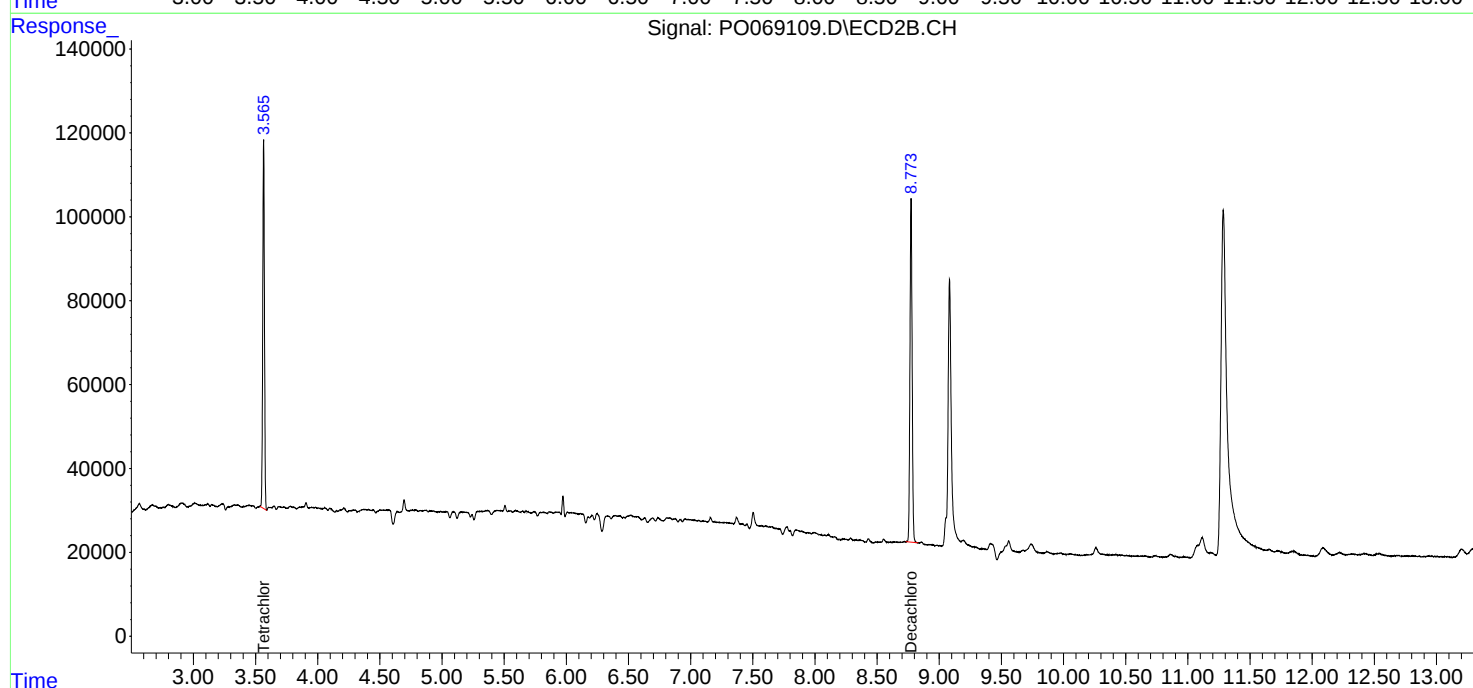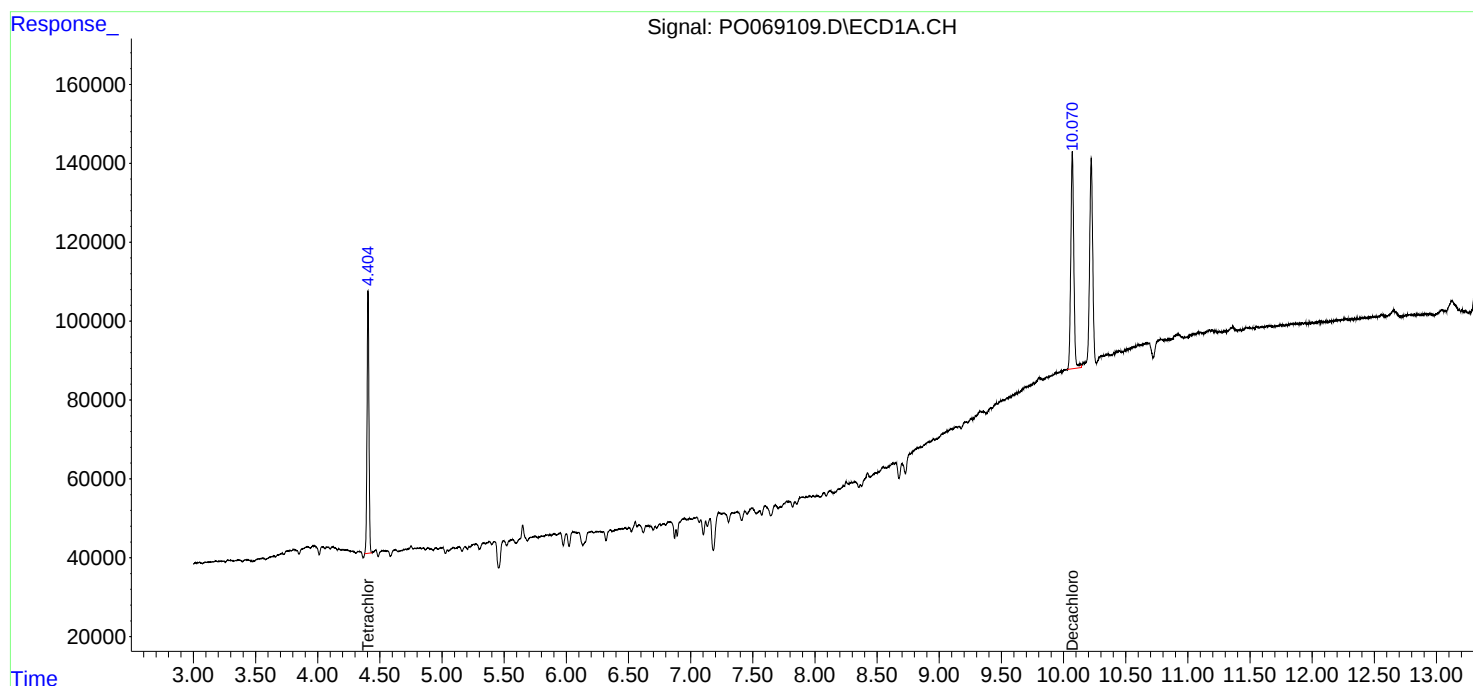

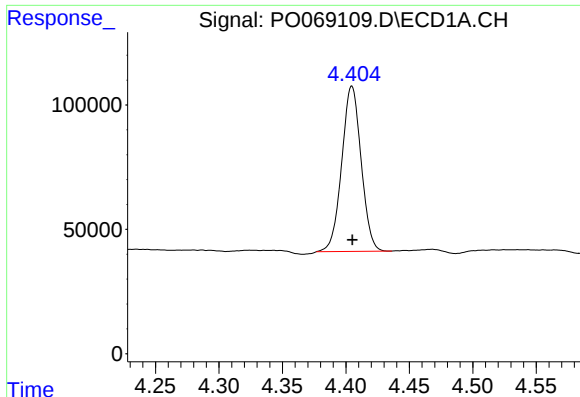


#1 Tetrachloro-m-xylene

R.T.: 4.404 min
Delta R.T.: 0.000 min
Response: 706930
Conc: 23.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-18


Manual Integrations
APPROVED

Sohil
6/23/2020 2:20:41 PM

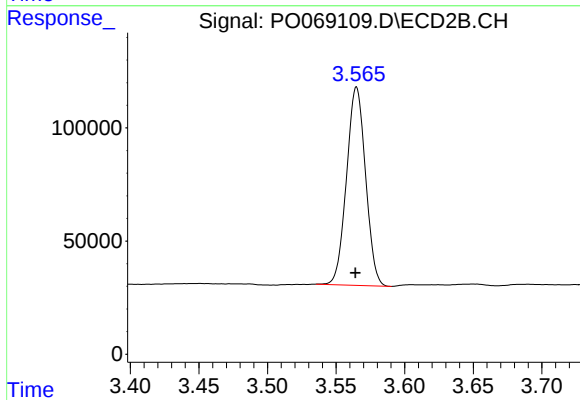


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 846352
Conc: 21.99 ng/ml

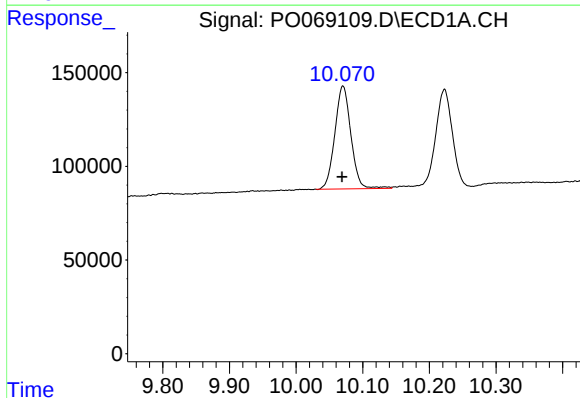

#2 Decachlorobiphenyl

R.T.: 10.070 min
Delta R.T.: 0.001 min
Response: 922124
Conc: 19.41 ng/ml

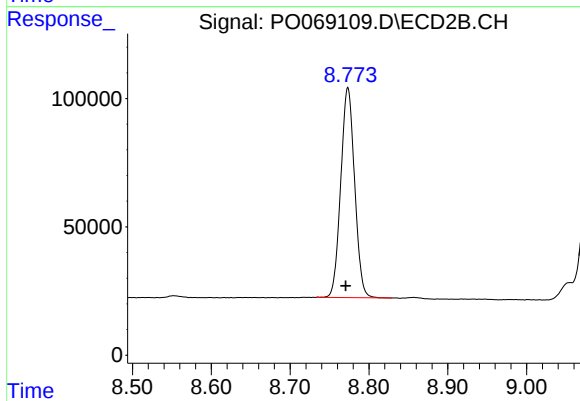

#2 Decachlorobiphenyl

R.T.: 8.773 min
Delta R.T.: 0.003 min
Response: 1000573
Conc: 18.38 ng/ml