

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062320\
 Data File : P0069139.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2020 19:40
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 01:25:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 19 05:15:02 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.405	3.565	739847	889248	25.009	23.104
2)	SA Decachlor...	10.072	8.774	1032477	1179821	21.738	21.674
Target Compounds							
20)	L4 AR-1242-5	6.620	0.000	18415	0	20.637	N.D. #
24)	L5 AR-1248-4	6.620	0.000	18415	0	12.244	N.D. #
25)	L5 AR-1248-5	6.620	0.000	18415	0	12.717	N.D. #
26)	L6 AR-1254-1	6.620	0.000	18415	0	12.155	N.D. #
40)	L8 AR-1262-5	9.461	0.000	9150	0	5.099	N.D. #
43)	L9 AR-1268-3	9.058	0.000	15829	0	3.382	N.D. #
44)	L9 AR-1268-4	9.461	0.000	9150	0	4.366	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062320\
Data File : P0069139.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2020 19:40
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 01:25:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 19 05:15:02 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

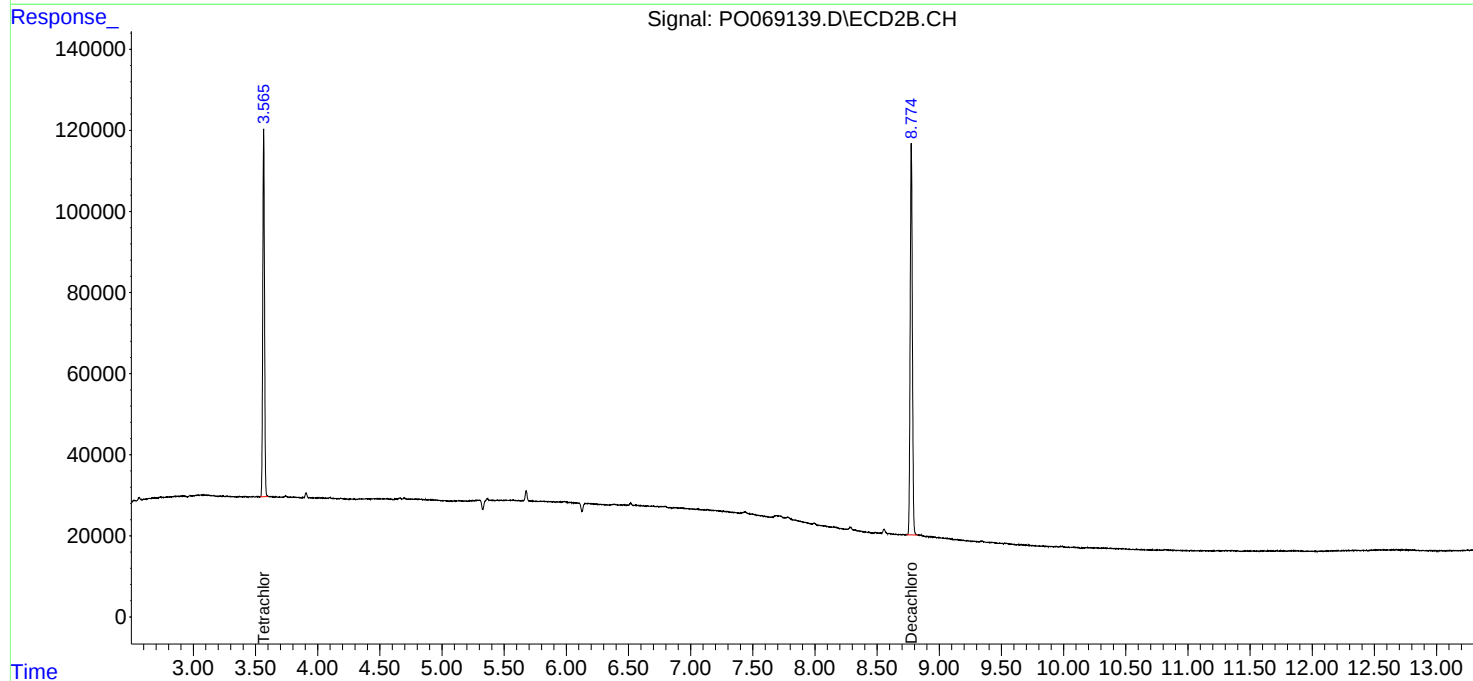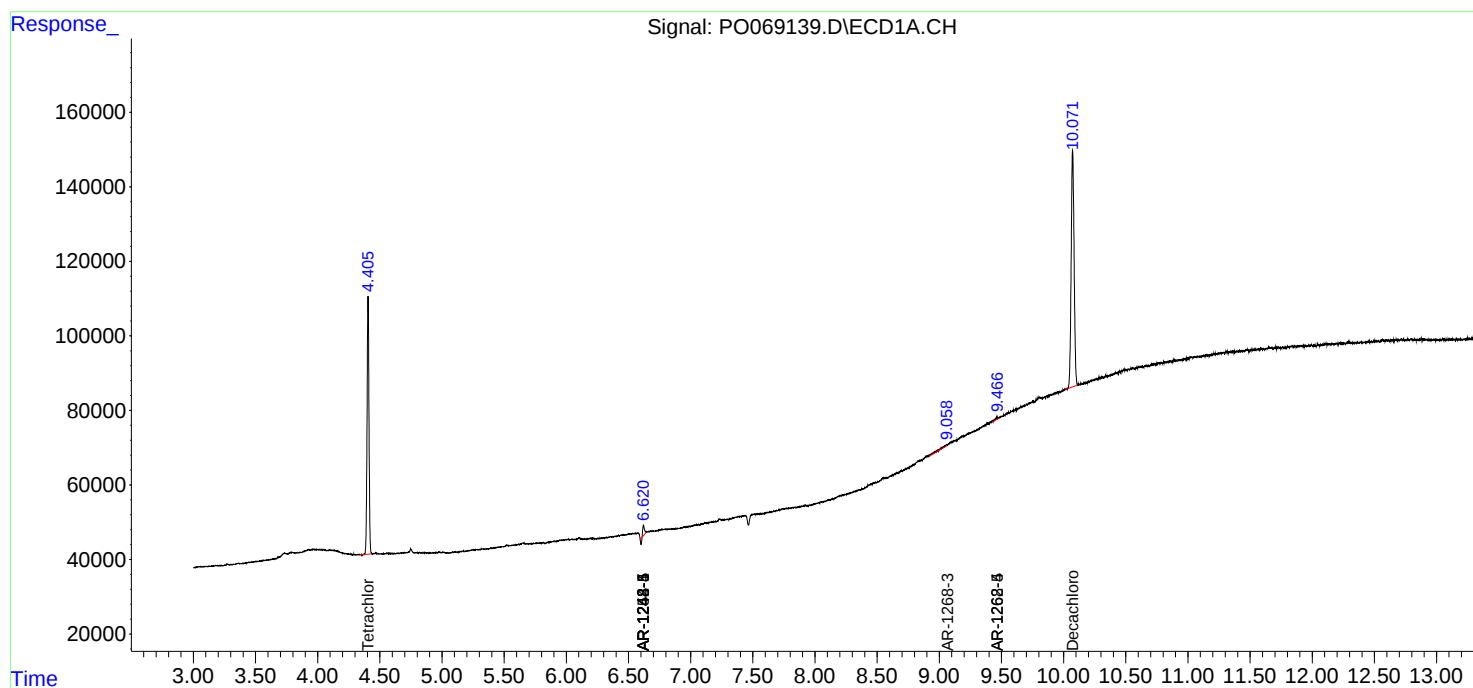


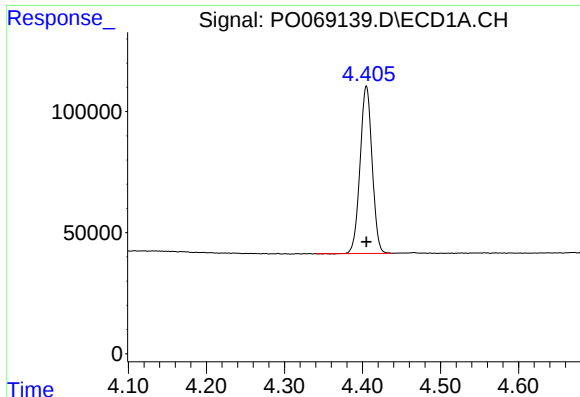

#1 Tetrachloro-m-xylene


R.T.: 4.405 min
Delta R.T.: 0.000 min
Response: 739847
Conc: 25.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

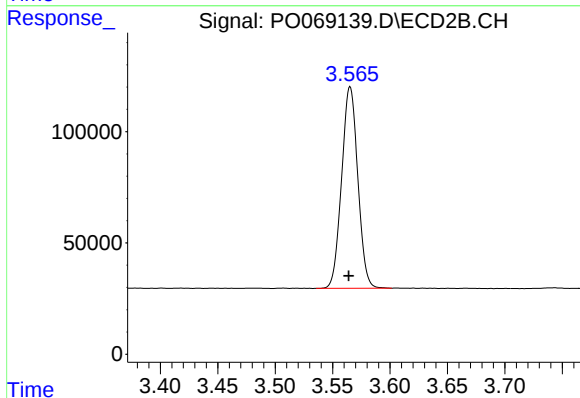


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.001 min
Response: 889248
Conc: 23.10 ng/ml

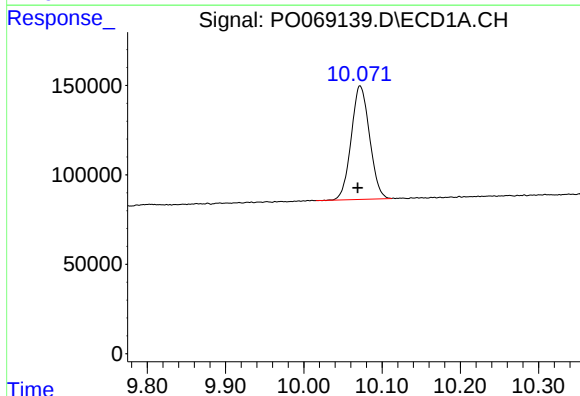


#2 Decachlorobiphenyl

R.T.: 10.072 min
Delta R.T.: 0.003 min
Response: 1032477
Conc: 21.74 ng/ml

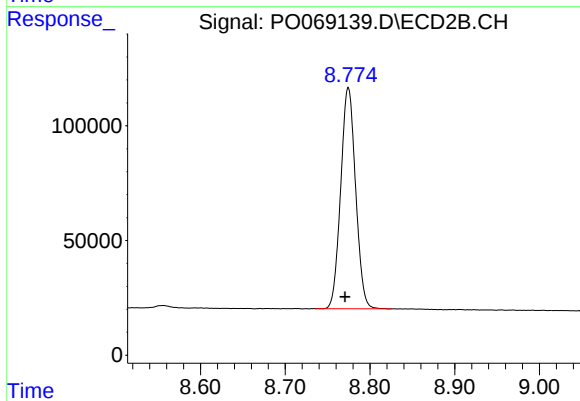

#2 Decachlorobiphenyl


R.T.: 8.774 min
Delta R.T.: 0.004 min
Response: 1179821
Conc: 21.67 ng/ml

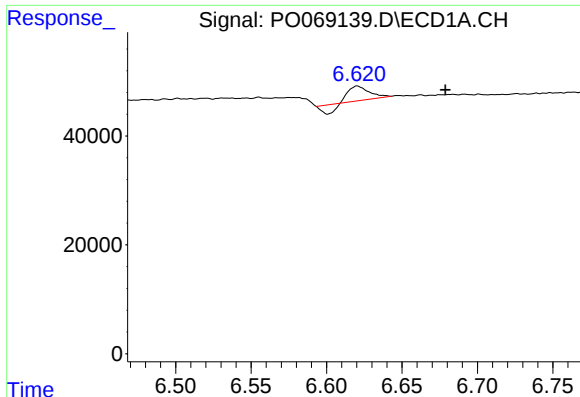

#20 AR-1242-5


R.T.: 6.620 min
Delta R.T.: -0.058 min
Response: 18415
Conc: 20.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

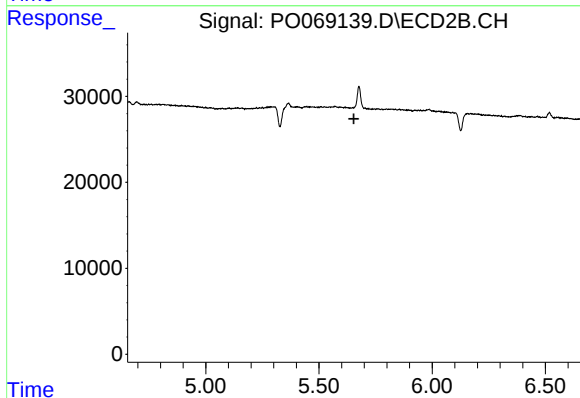


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.655 min
Response: 0
Conc: N.D.

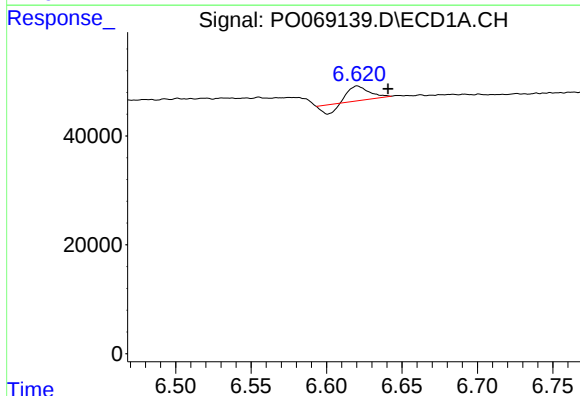


#24 AR-1248-4

R.T.: 6.620 min
Delta R.T.: -0.020 min
Response: 18415
Conc: 12.24 ng/ml

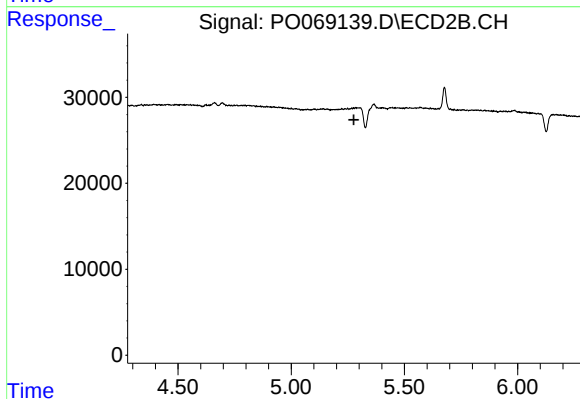

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

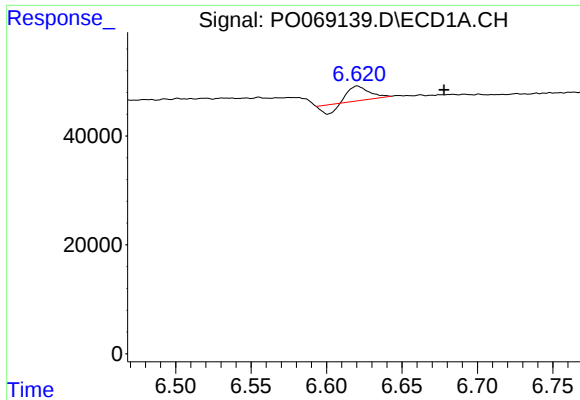

#25 AR-1248-5


R.T.: 6.620 min
Delta R.T.: -0.057 min
Response: 18415
Conc: 12.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

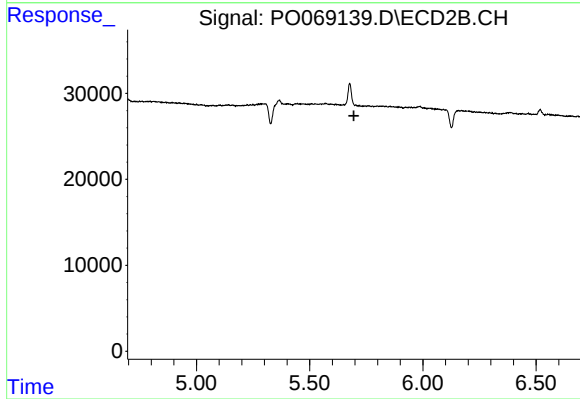


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.695 min
Response: 0
Conc: N.D.

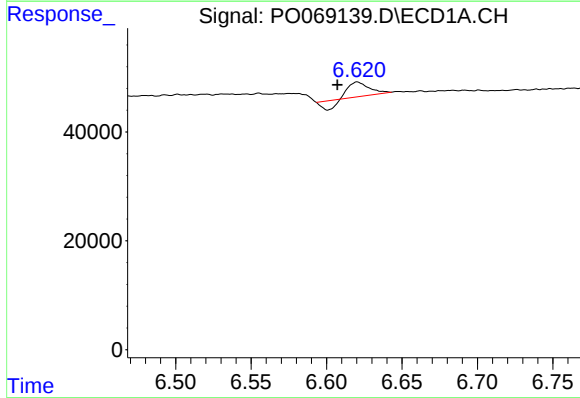


#26 AR-1254-1

R.T.: 6.620 min
Delta R.T.: 0.013 min
Response: 18415
Conc: 12.16 ng/ml

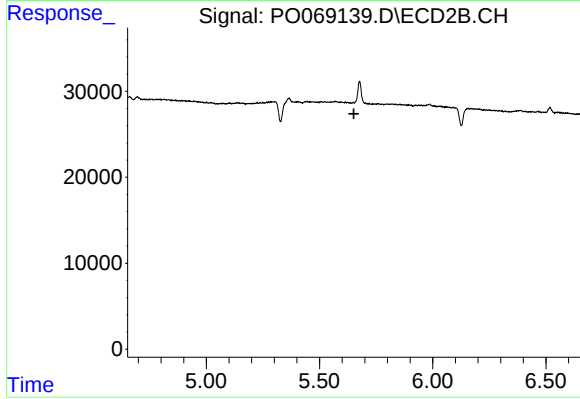

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.652 min
Response: 0
Conc: N.D.

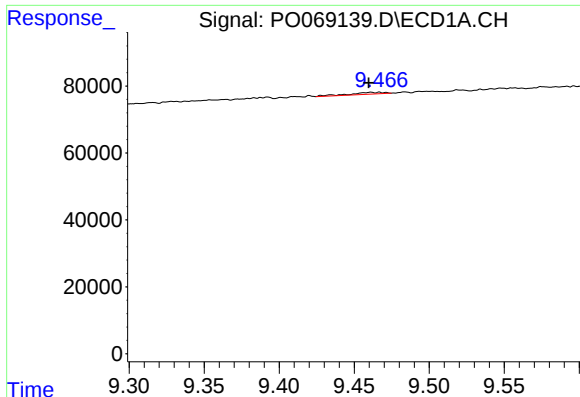

#40 AR-1262-5


R.T.: 9.461 min
Delta R.T.: 0.002 min
Response: 9150
Conc: 5.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

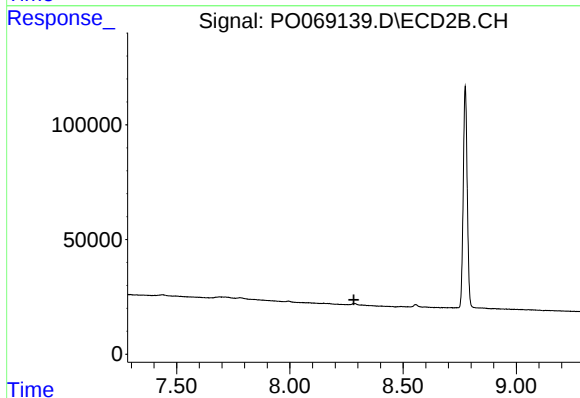


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.283 min
Response: 0
Conc: N.D.

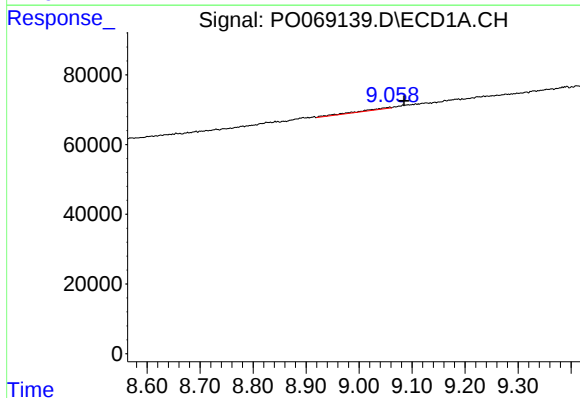


#43 AR-1268-3

R.T.: 9.058 min
Delta R.T.: -0.027 min
Response: 15829
Conc: 3.38 ng/ml

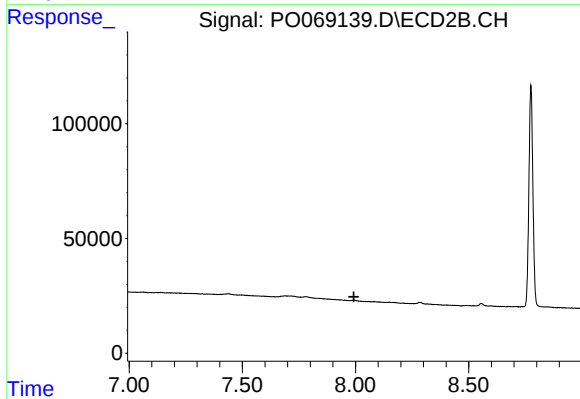

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 7.992 min
Response: 0
Conc: N.D.

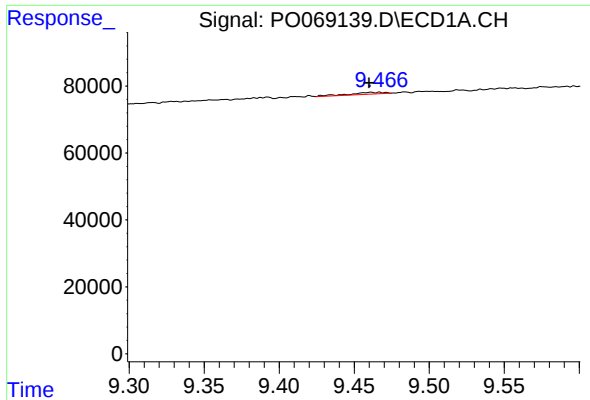

#44 AR-1268-4

R.T.: 9.461 min
Delta R.T.: 0.001 min
Response: 9150
Conc: 4.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

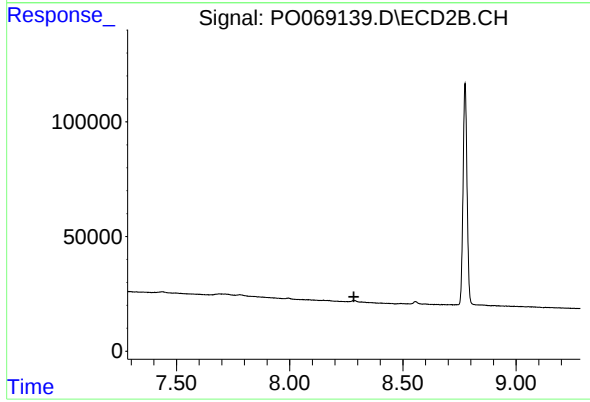

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.283 min
Response: 0
Conc: N.D.