

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062320\
 Data File : P0069133.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2020 17:57
 Operator : DD\AJ
 Sample : L3084-13 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 401039-D112-4-0-6

Manual Integrations
 APPROVED

Sohil
 6/25/2020 8:52:22 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 18:44:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 19 05:15:02 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.405	3.566	88830	103577	3.003	2.691
2) SA Decachlor...	10.073	8.774	236974	311010	4.989m	5.713

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062320\
Data File : P0069133.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2020 17:57
Operator : DD\AJ
Sample : L3084-13 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
401039-D112-4-0-6


Manual Integrations
APPROVED

Sohil
6/25/2020 8:52:22 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 18:44:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 19 05:15:02 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

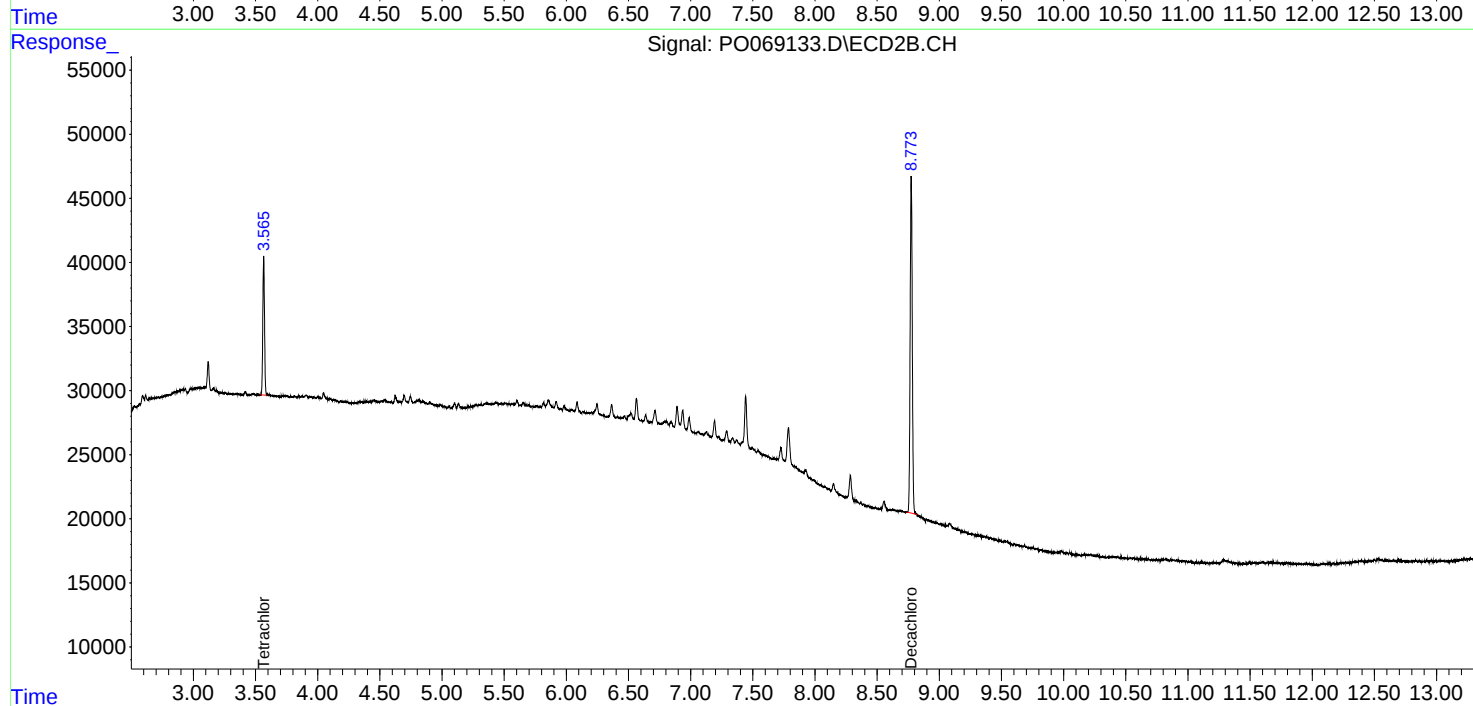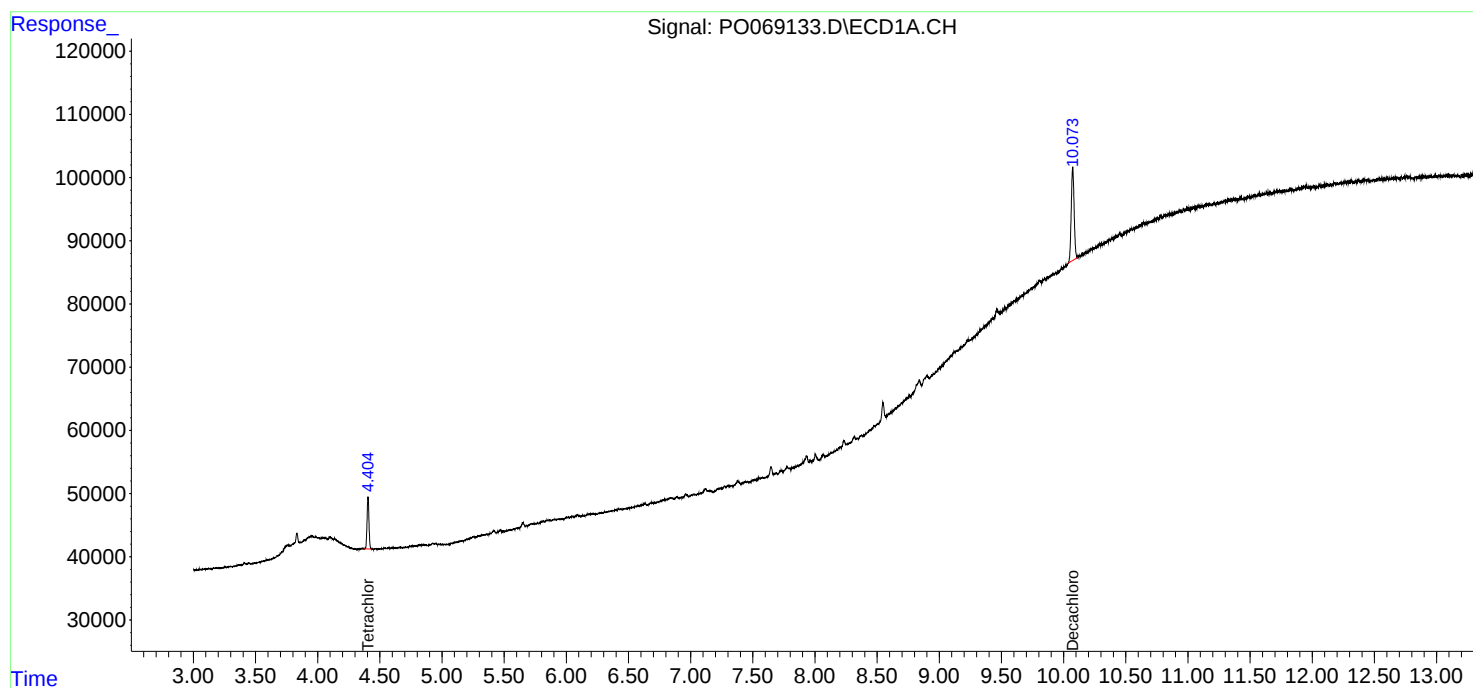

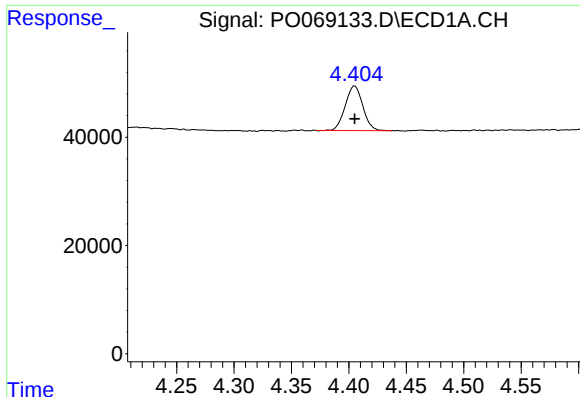


#1 Tetrachloro-m-xylene

R.T.: 4.405 min
Delta R.T.: 0.000 min
Response: 88830
Conc: 3.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
401039-D112-4-0-6


Manual Integrations
APPROVED

Sohil
6/25/2020 8:52:22 AM

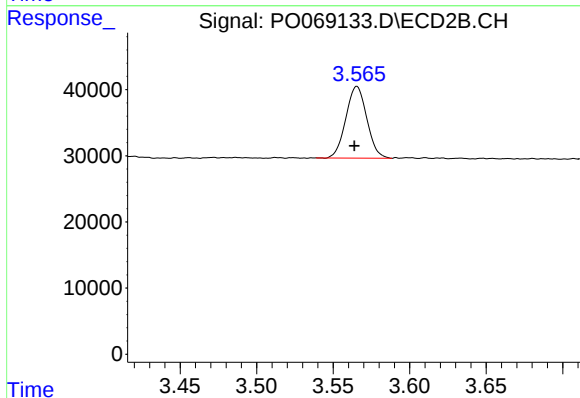


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.002 min
Response: 103577
Conc: 2.69 ng/ml

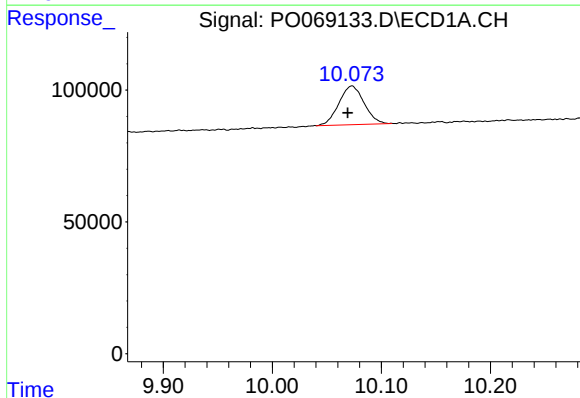

#2 Decachlorobiphenyl

R.T.: 10.073 min
Delta R.T.: 0.004 min
Response: 236974
Conc: 4.99 ng/ml m

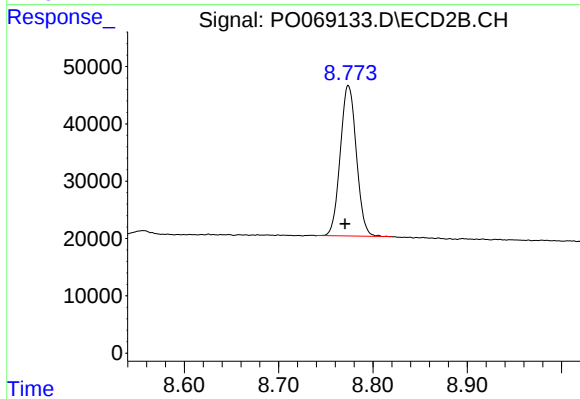

#2 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: 0.003 min
Response: 311010
Conc: 5.71 ng/ml