

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062419\
 Data File : P0057397.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jun 2019 13:49
 Operator : SM/SJ
 Sample : K3303-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BAT-B03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 14:05:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.240	3.555	822299	769139	20.933	21.874
2) SA Decachlor...	9.795	8.479	934315	632088	16.615	16.898

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062419\
Data File : P0057397.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jun 2019 13:49
Operator : SM/SJ
Sample : K3303-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BAT-B03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 14:05:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

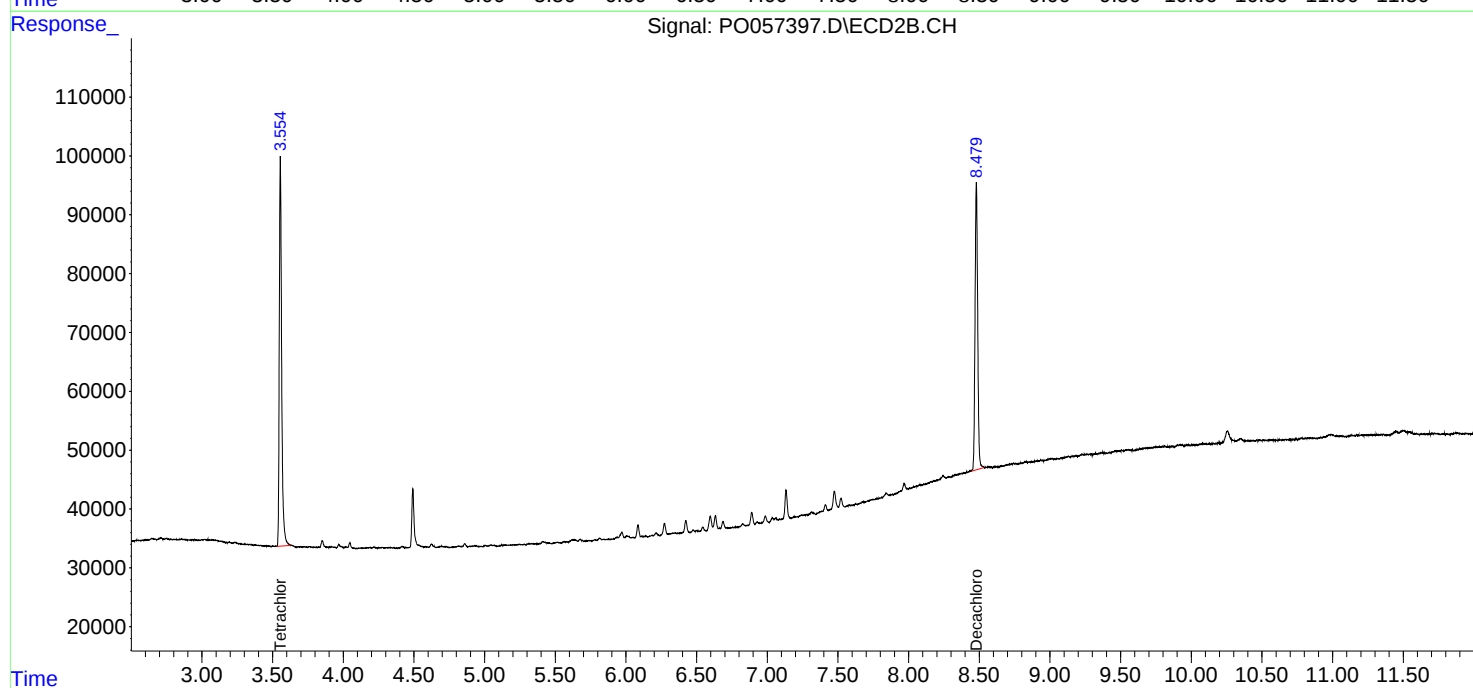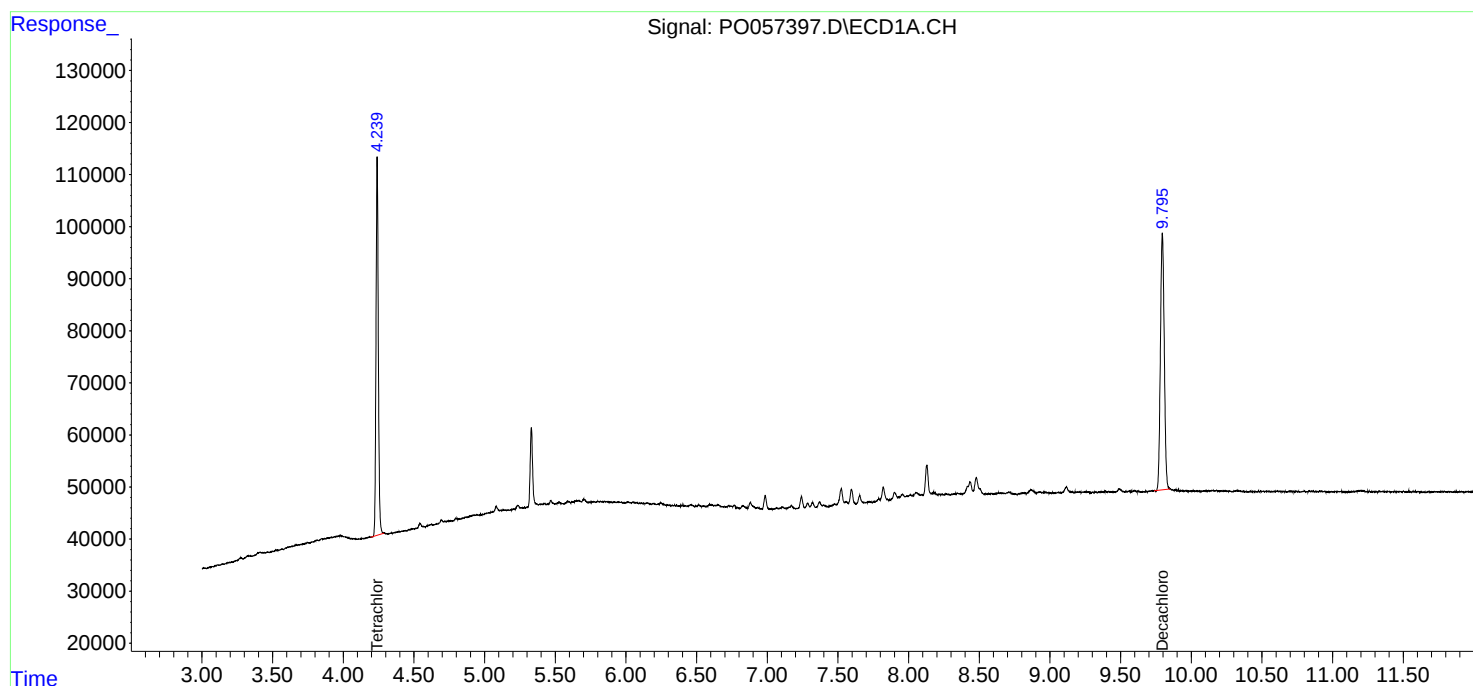


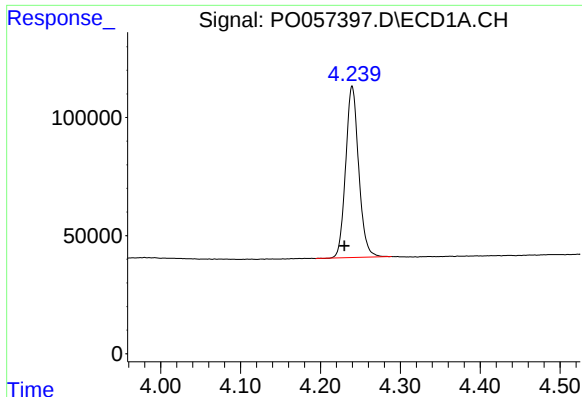

#1 Tetrachloro-m-xylene


R.T.: 4.240 min
Delta R.T.: 0.010 min
Response: 822299
Conc: 20.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
BAT-B03

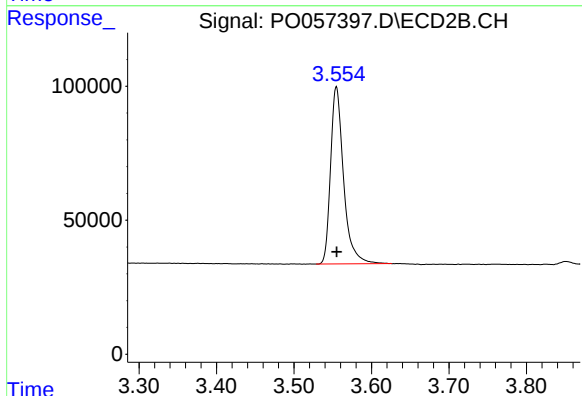


#1 Tetrachloro-m-xylene

R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 769139
Conc: 21.87 ng/ml

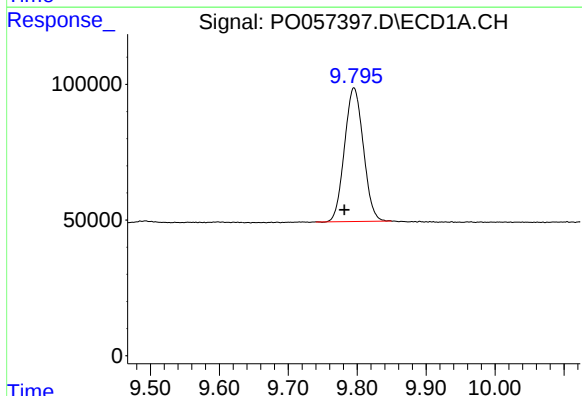

#2 Decachlorobiphenyl

R.T.: 9.795 min
Delta R.T.: 0.014 min
Response: 934315
Conc: 16.62 ng/ml

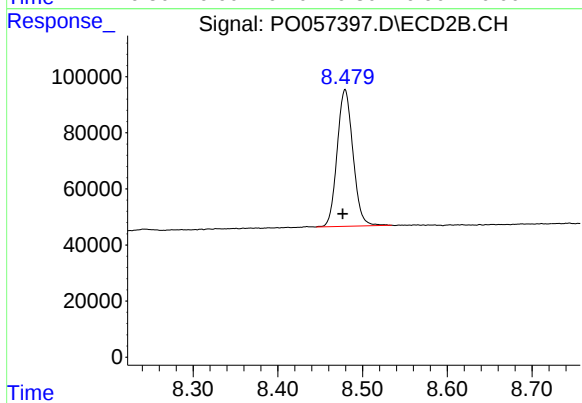

#2 Decachlorobiphenyl

R.T.: 8.479 min
Delta R.T.: 0.003 min
Response: 632088
Conc: 16.90 ng/ml