

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062420\
 Data File : P0069147.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jun 2020 9:08
 Operator : DD\AJ
 Sample : L3084-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 401039-D112-2-0-6

Manual Integrations
 APPROVED

Ankita
 6/26/2020 9:20:22 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 10:40:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 19 05:15:02 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.404	3.565	559621	666398	18.917	17.314
2) SA Decachlor...	10.071	8.773	273200	356786	5.752m	6.554
Target Compounds						
31) L7 AR-1260-1	7.377	6.363	499434	592545	261.699m	253.229
32) L7 AR-1260-2	7.644	6.564	710952	815226	303.758m	286.393
33) L7 AR-1260-3	8.004	6.712	494773	564574	278.500	209.912
34) L7 AR-1260-4	8.231	7.192	490234	561279	235.074	234.270
35) L7 AR-1260-5	8.546	7.442	1171027	1451226	266.419	250.497

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062420\
Data File : P0069147.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jun 2020 9:08
Operator : DD\AJ
Sample : L3084-10
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
401039-D112-2-0-6


Manual Integrations
APPROVED

Ankita
6/26/2020 9:20:22 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 10:40:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 19 05:15:02 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

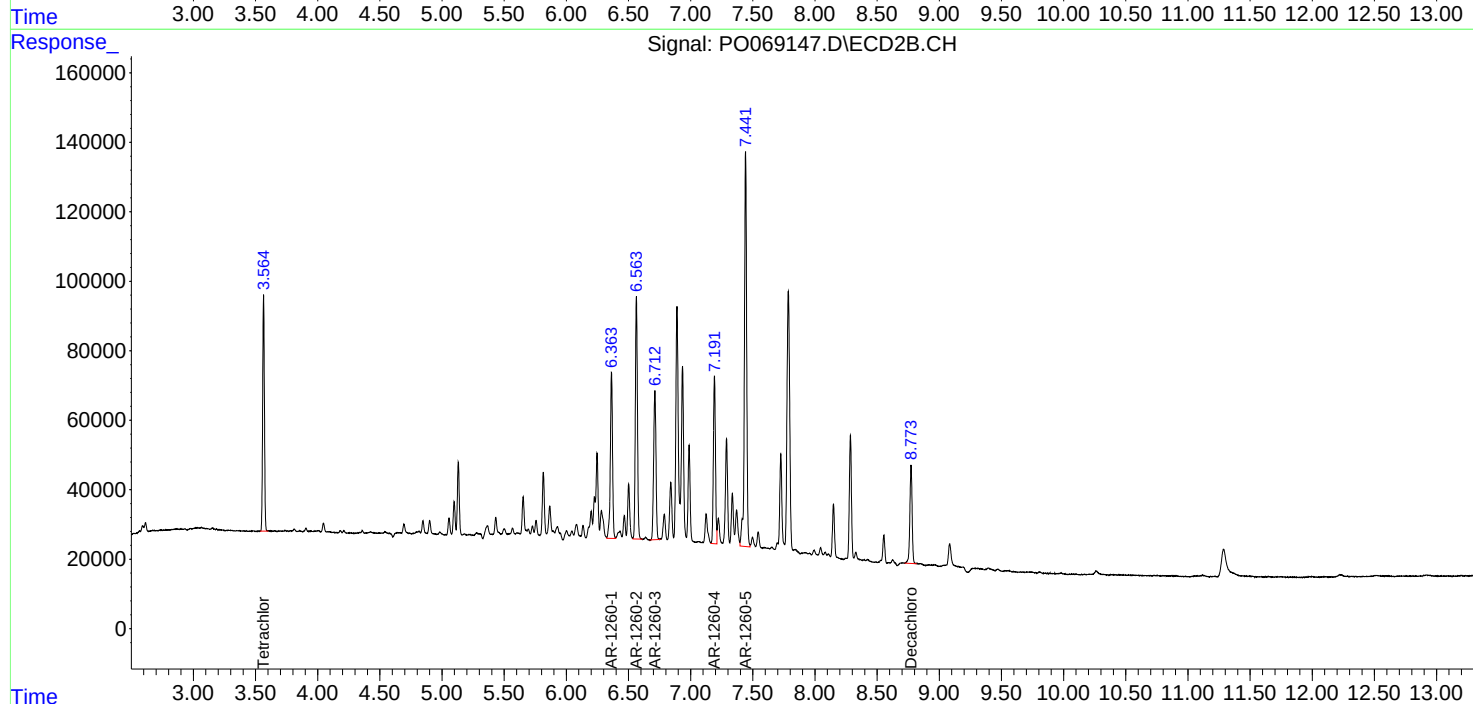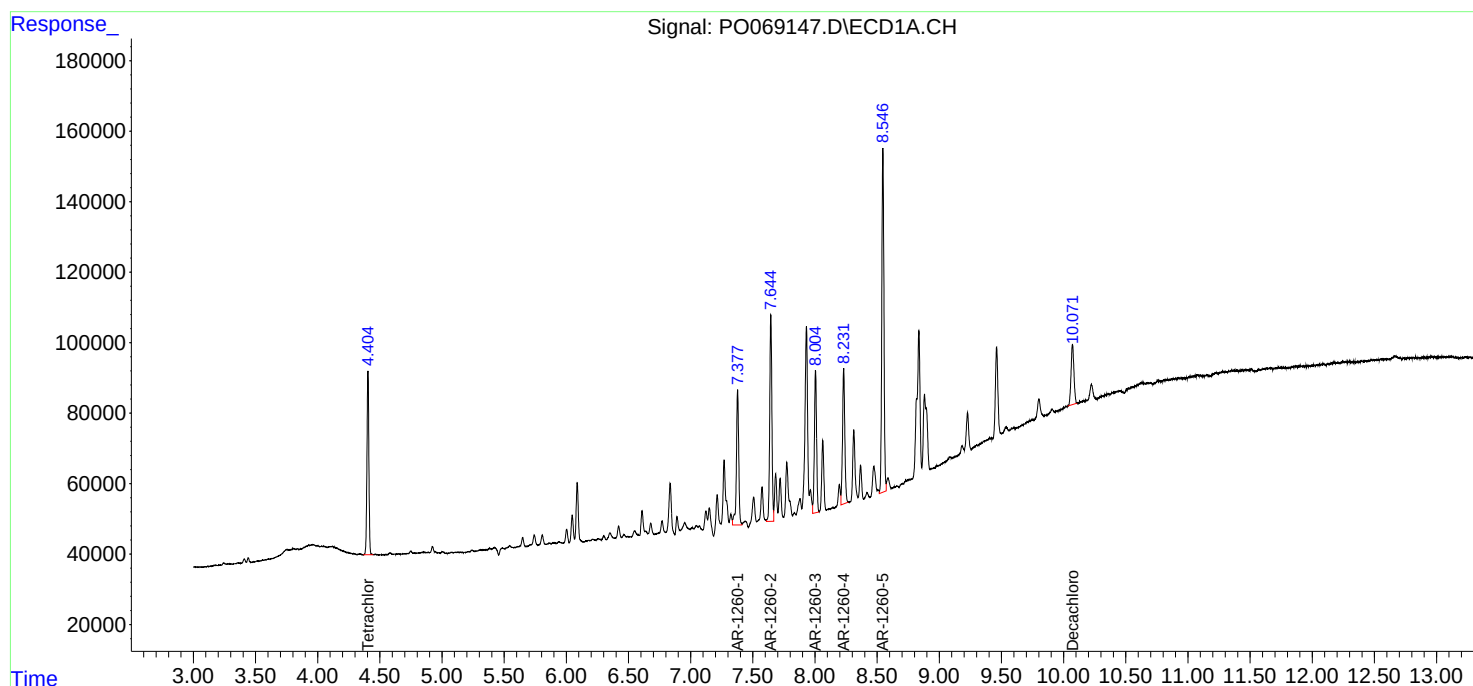

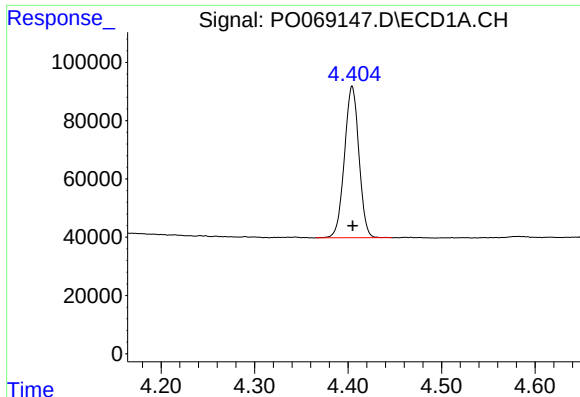


#1 Tetrachloro-m-xylene

R.T.: 4.404 min
Delta R.T.: 0.000 min
Response: 559621
Conc: 18.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
401039-D112-2-0-6


Manual Integrations
APPROVED

Ankita
6/26/2020 9:20:22 AM

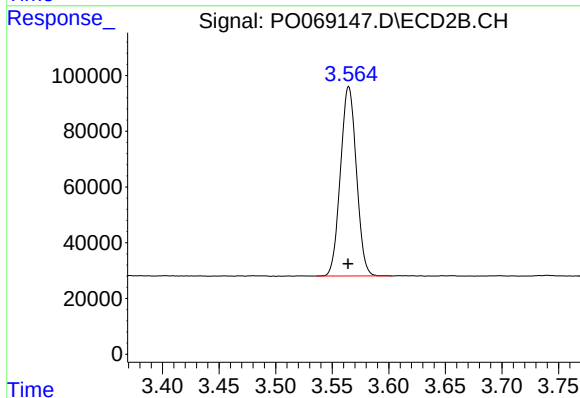


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 666398
Conc: 17.31 ng/ml

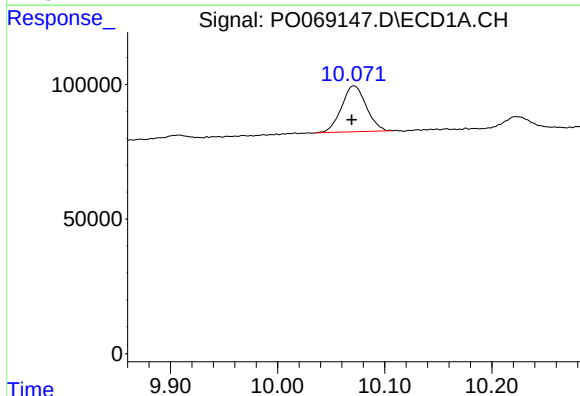


#2 Decachlorobiphenyl

R.T.: 10.071 min
Delta R.T.: 0.002 min
Response: 273200
Conc: 5.75 ng/ml m

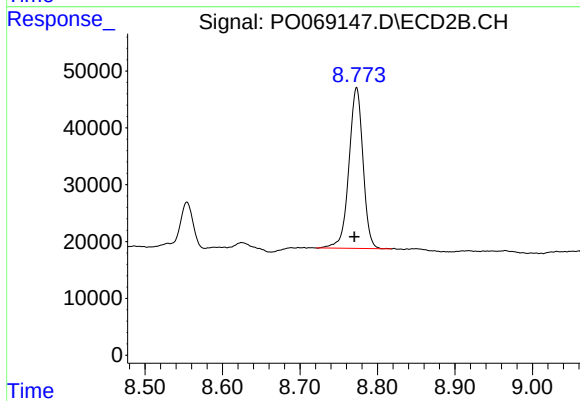

#2 Decachlorobiphenyl

R.T.: 8.773 min
Delta R.T.: 0.003 min
Response: 356786
Conc: 6.55 ng/ml

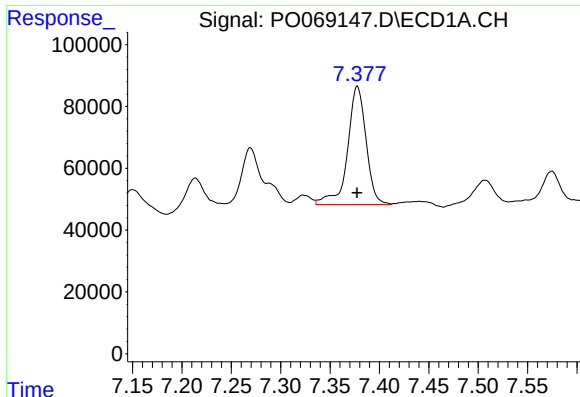


#31 AR-1260-1

R.T.: 7.377 min
Delta R.T.: 0.000 min
Response: 499434
Conc: 261.70 ng/ml m

Instrument :
ECD_O
ClientSampleId :
401039-D112-2-0-6


Manual Integrations
APPROVED

Ankita
6/26/2020 9:20:22 AM

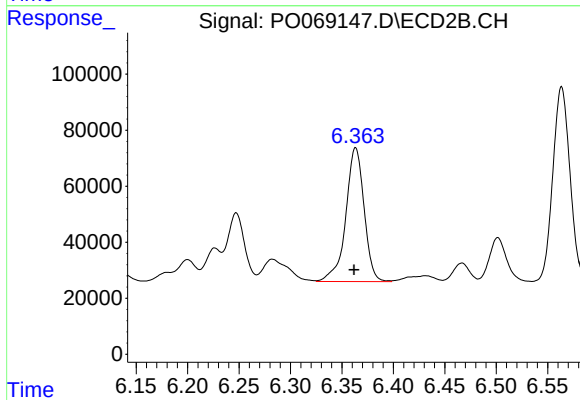


#31 AR-1260-1

R.T.: 6.363 min
Delta R.T.: 0.001 min
Response: 592545
Conc: 253.23 ng/ml

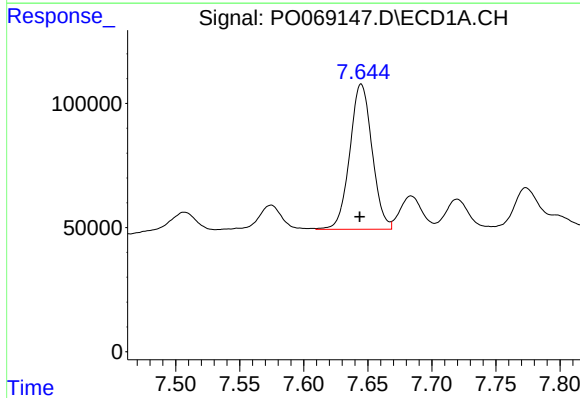


#32 AR-1260-2

R.T.: 7.644 min
Delta R.T.: 0.000 min
Response: 710952
Conc: 303.76 ng/ml m

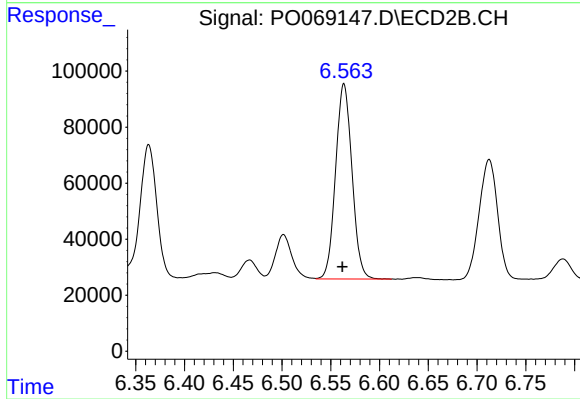

#32 AR-1260-2

R.T.: 6.564 min
Delta R.T.: 0.002 min
Response: 815226
Conc: 286.39 ng/ml

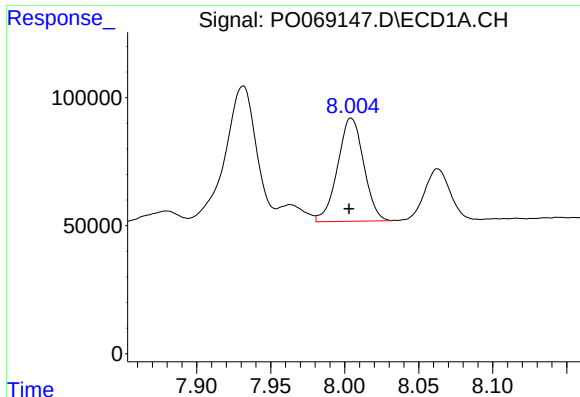


#33 AR-1260-3

R.T.: 8.004 min
Delta R.T.: 0.001 min
Response: 494773
Conc: 278.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
401039-D112-2-0-6


Manual Integrations
APPROVED

Ankita
6/26/2020 9:20:22 AM

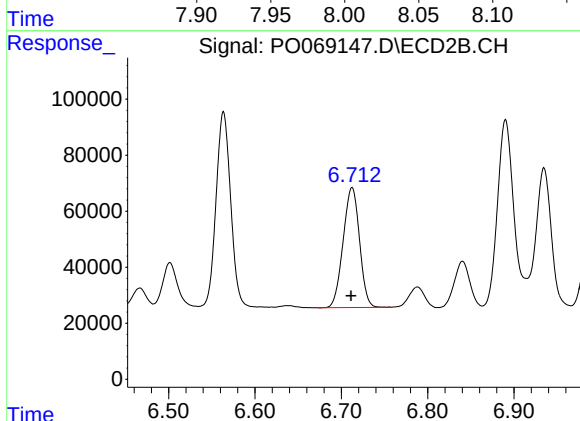


#33 AR-1260-3

R.T.: 6.712 min
Delta R.T.: 0.001 min
Response: 564574
Conc: 209.91 ng/ml

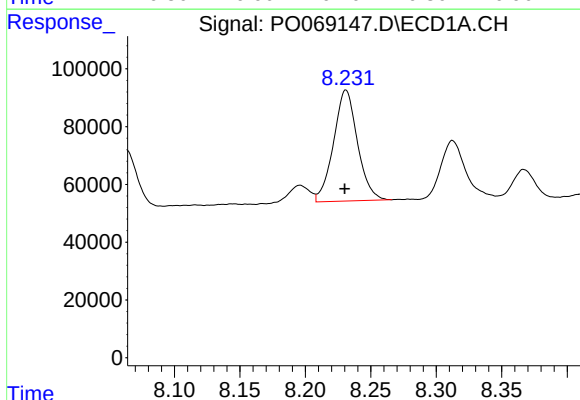


#34 AR-1260-4

R.T.: 8.231 min
Delta R.T.: 0.000 min
Response: 490234
Conc: 235.07 ng/ml

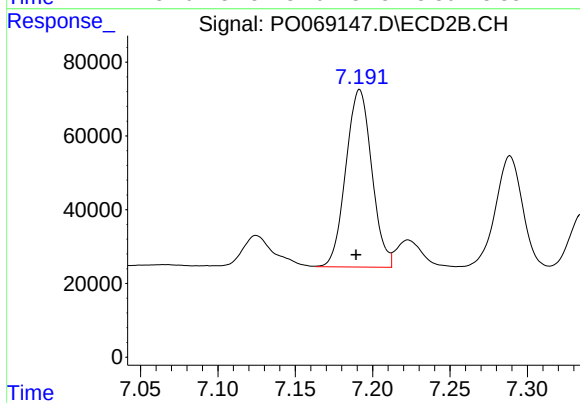

#34 AR-1260-4

R.T.: 7.192 min
Delta R.T.: 0.002 min
Response: 561279
Conc: 234.27 ng/ml

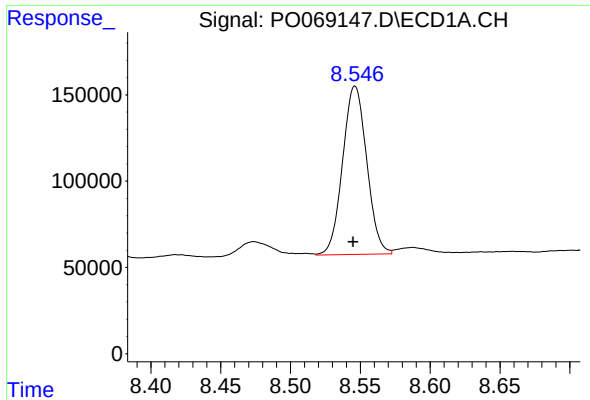


#35 AR-1260-5

R.T.: 8.546 min
Delta R.T.: 0.002 min
Response: 1171027
Conc: 266.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
401039-D112-2-0-6

Manual Integrations
APPROVED

Ankita
6/26/2020 9:20:22 AM

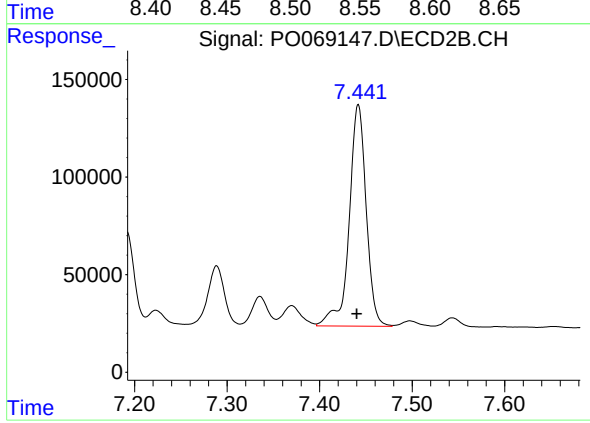

#35 AR-1260-5

R.T.: 7.442 min
Delta R.T.: 0.002 min
Response: 1451226
Conc: 250.50 ng/ml