

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062420\
 Data File : P0069160.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jun 2020 13:27
 Operator : DD\AJ
 Sample : L3094-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BRENNAN-FL-001

Manual Integrations
 APPROVED

Ankita
 6/26/2020 9:21:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 18:01:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 19 05:15:02 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.403	3.565	787395	954285	26.616m	24.793
2) SA Decachlor...	10.071	8.773	1043832	1123003	21.977	20.630

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062420\
Data File : P0069160.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jun 2020 13:27
Operator : DD\AJ
Sample : L3094-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BRENNAN-FL-001


Manual Integrations
APPROVED

Ankita
6/26/2020 9:21:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 18:01:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 19 05:15:02 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

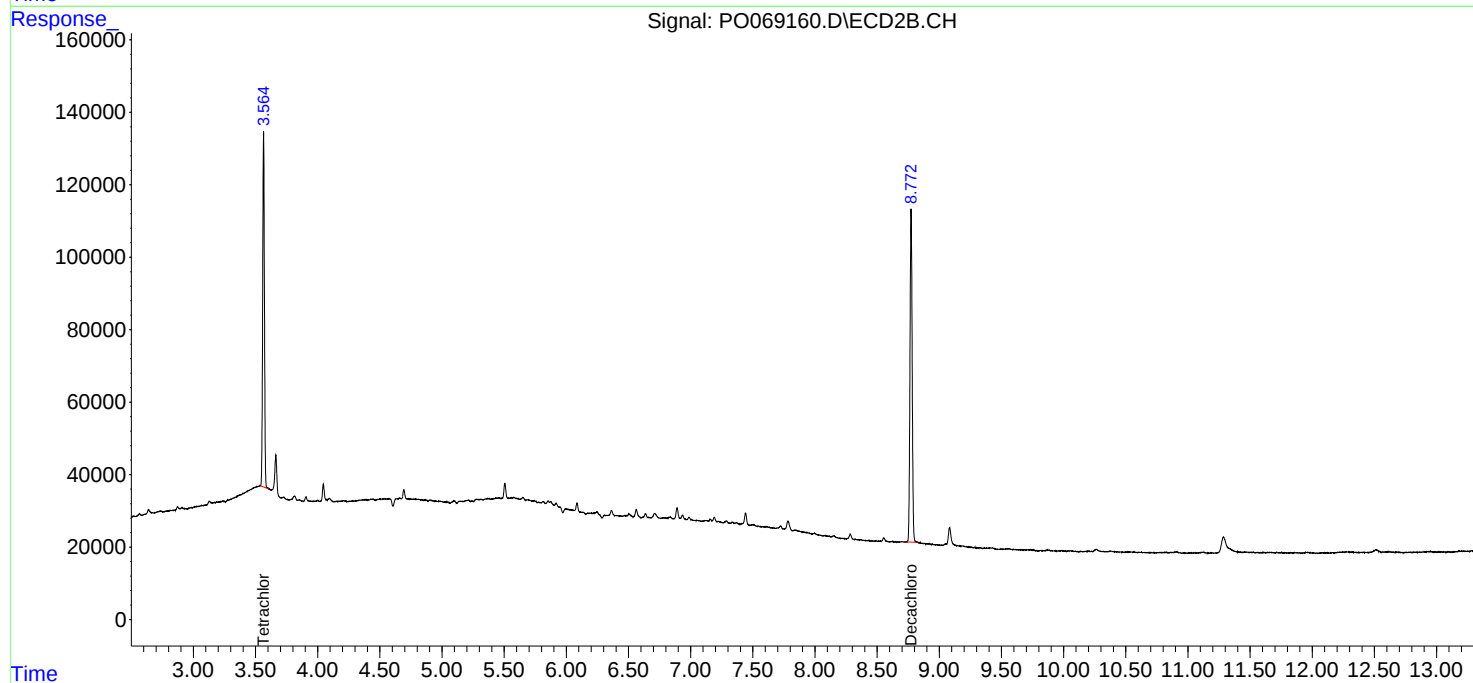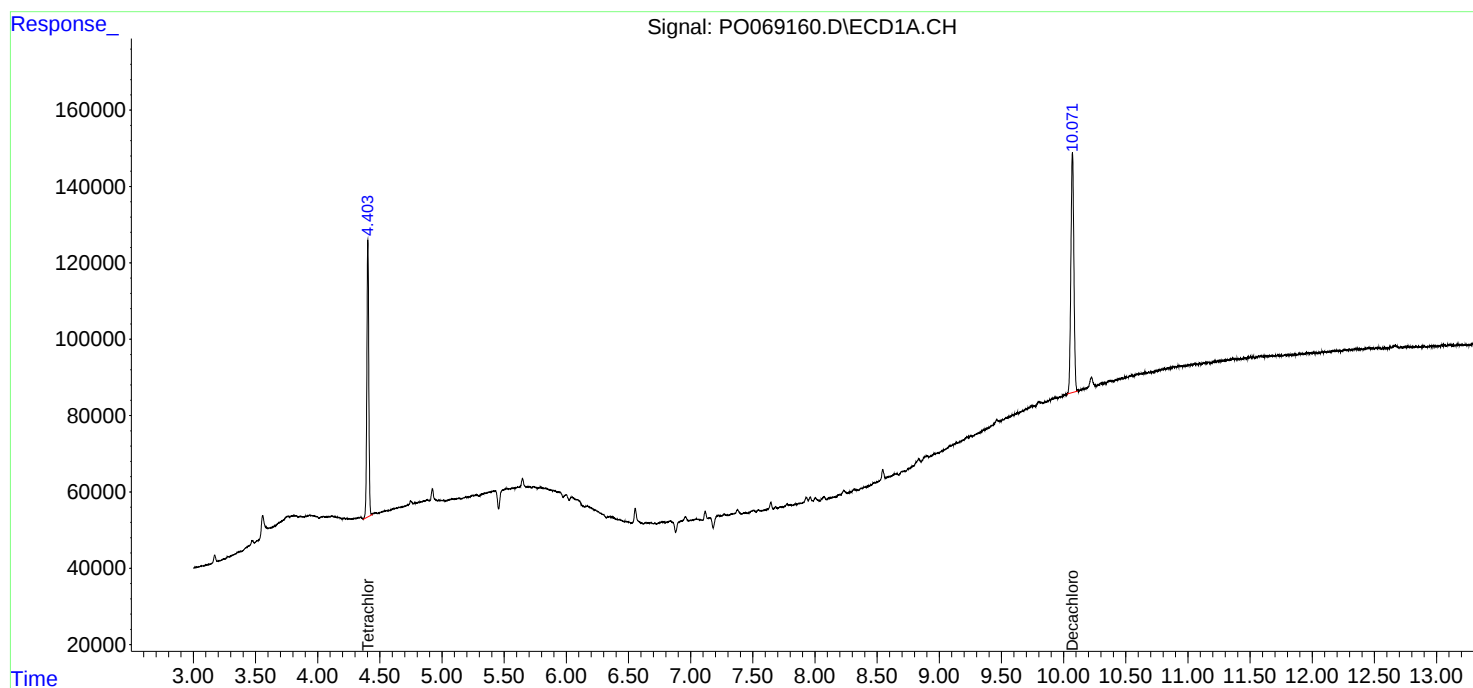

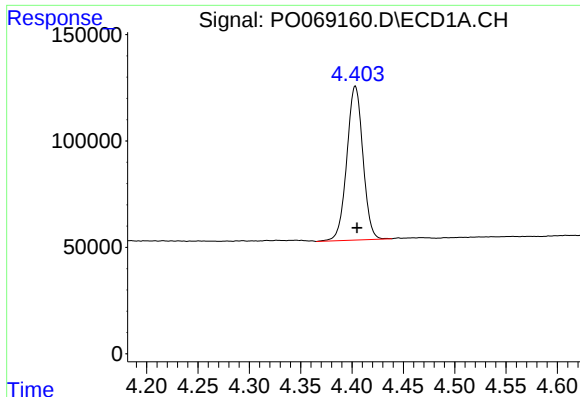


#1 Tetrachloro-m-xylene

R.T.: 4.403 min
Delta R.T.: -0.002 min
Response: 787395
Conc: 26.62 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BRENNAN-FL-001


Manual Integrations
APPROVED

Ankita
6/26/2020 9:21:13 AM

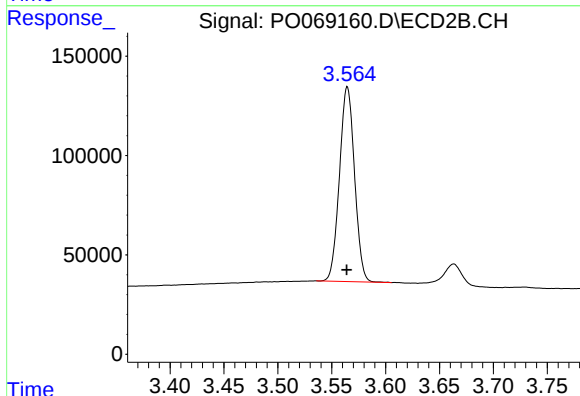


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 954285
Conc: 24.79 ng/ml

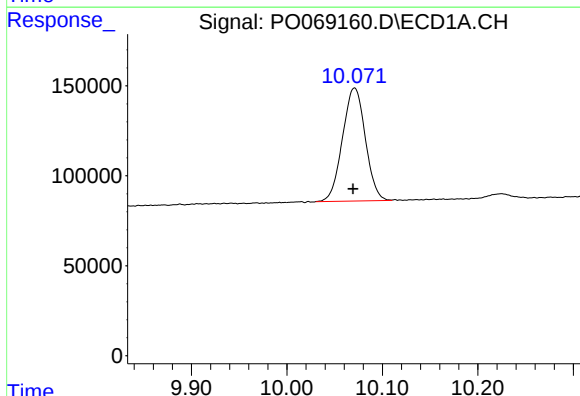

#2 Decachlorobiphenyl

R.T.: 10.071 min
Delta R.T.: 0.002 min
Response: 1043832
Conc: 21.98 ng/ml

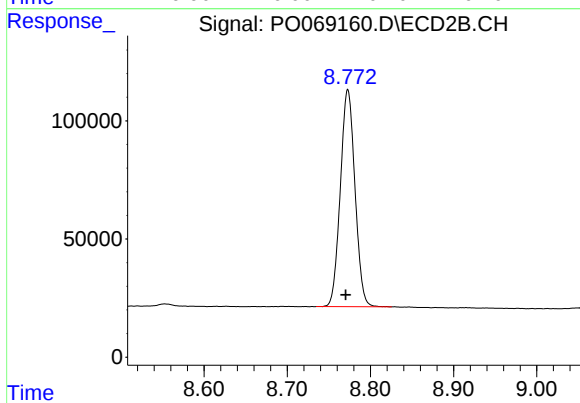

#2 Decachlorobiphenyl

R.T.: 8.773 min
Delta R.T.: 0.002 min
Response: 1123003
Conc: 20.63 ng/ml