

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062420\
 Data File : P0069169.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jun 2020 16:01
 Operator : DD\AJ
 Sample : L3090-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 359-RO

Manual Integrations
 APPROVED

Ankita
 6/26/2020 9:21:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 18:05:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 19 05:15:02 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.403	3.565	898740	1041155	30.380	27.050
2) SA Decachlor...	10.070	8.773	1030009	1044944	21.686	19.196
Target Compounds						
21) L5 AR-1248-1	5.710	4.797	20254	21696	25.980m	25.084m
22) L5 AR-1248-2	6.001	5.056	69648	95213	68.112	78.926
23) L5 AR-1248-3	6.213	5.098	96879	95528	78.310	84.430
24) L5 AR-1248-4	6.639	5.277	89488	127763	59.501	88.354 #
25) L5 AR-1248-5	6.676	5.695	172921	142194	119.412	98.288

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062420\
Data File : P0069169.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jun 2020 16:01
Operator : DD\AJ
Sample : L3090-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
359-RO


Manual Integrations
APPROVED

Ankita
6/26/2020 9:21:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 18:05:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 19 05:15:02 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

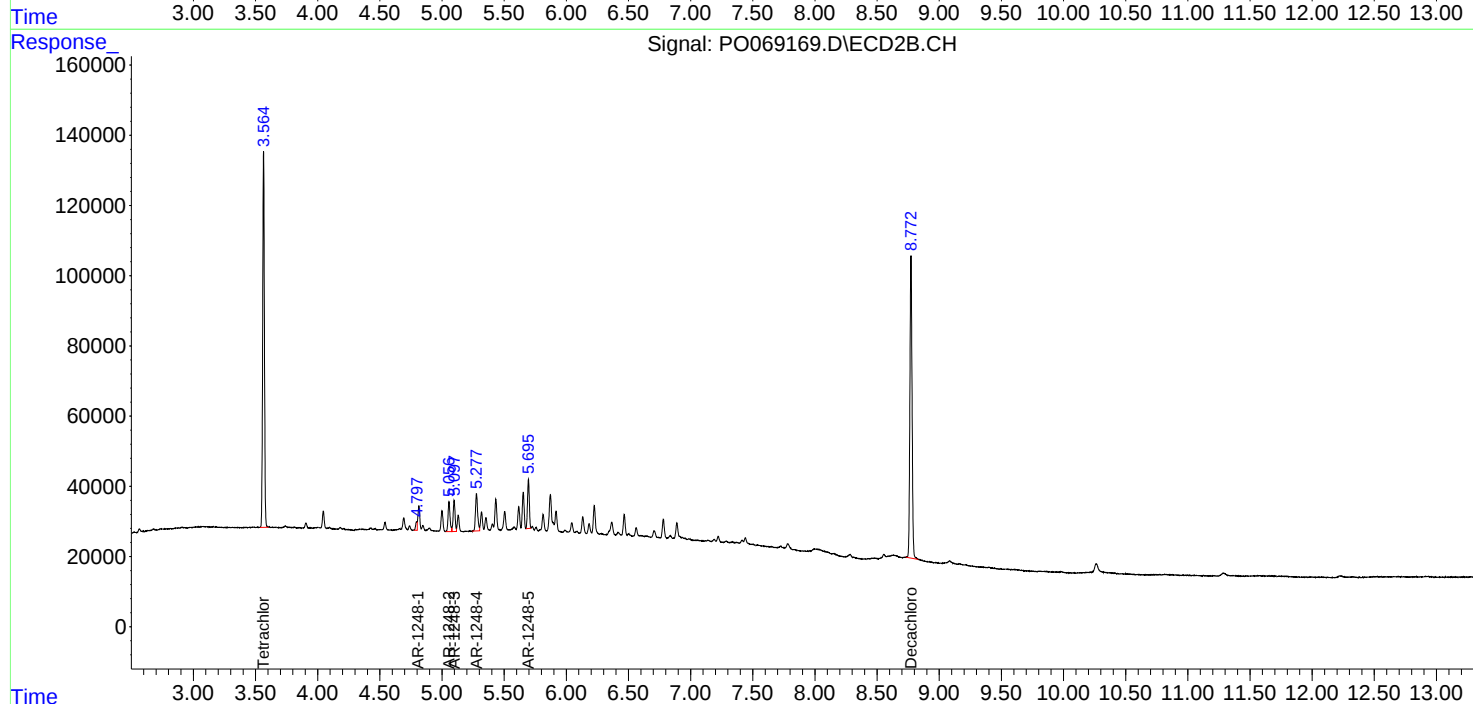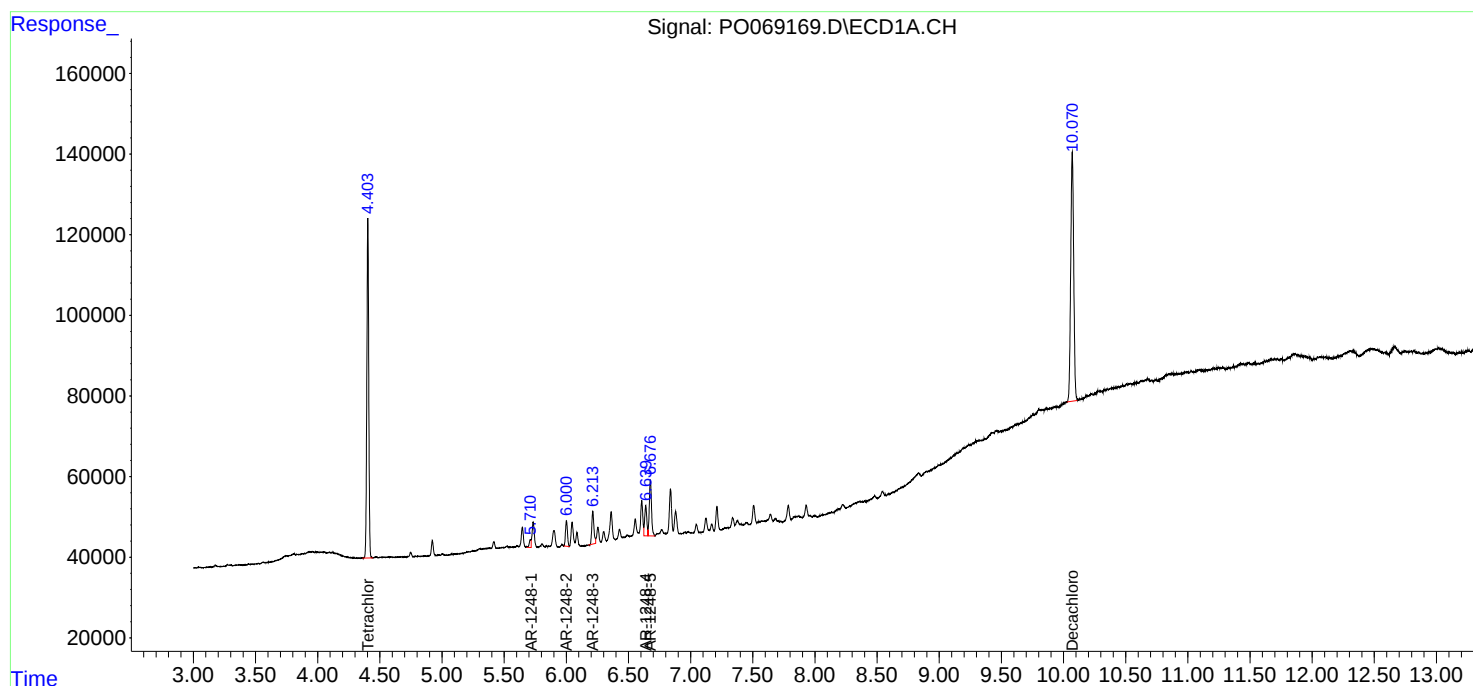

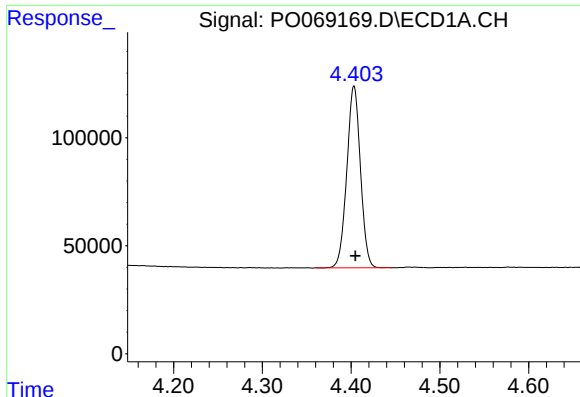


#1 Tetrachloro-m-xylene

R.T.: 4.403 min
Delta R.T.: -0.002 min
Response: 898740
Conc: 30.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
359-RO


Manual Integrations
APPROVED

Ankita
6/26/2020 9:21:20 AM

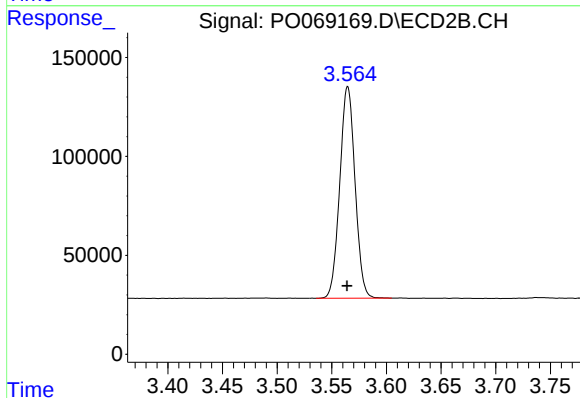


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 1041155
Conc: 27.05 ng/ml

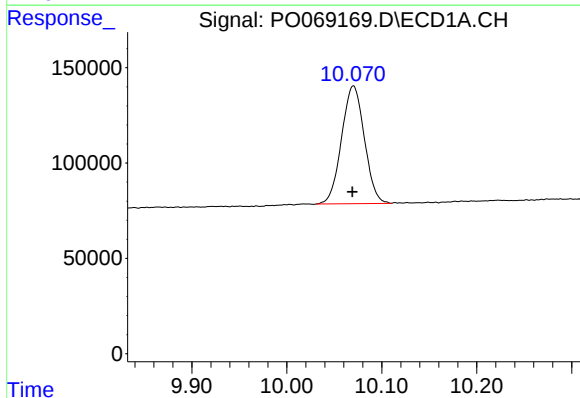


#2 Decachlorobiphenyl

R.T.: 10.070 min
Delta R.T.: 0.000 min
Response: 1030009
Conc: 21.69 ng/ml

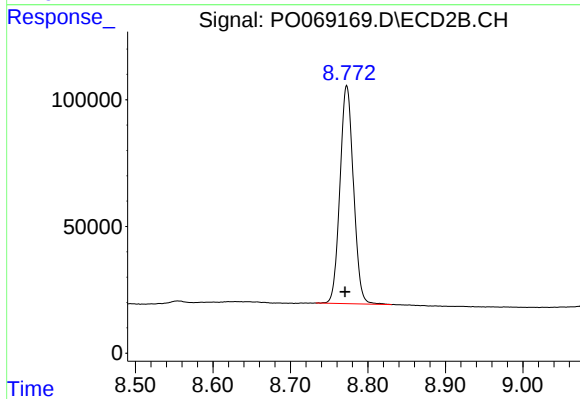

#2 Decachlorobiphenyl

R.T.: 8.773 min
Delta R.T.: 0.002 min
Response: 1044944
Conc: 19.20 ng/ml

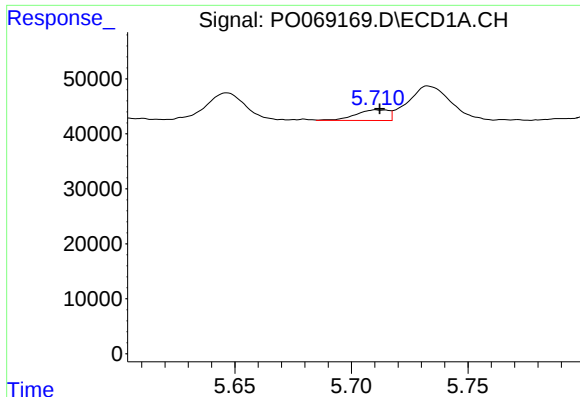


#21 AR-1248-1

R.T.: 5.710 min
Delta R.T.: -0.002 min
Response: 20254
Conc: 25.98 ng/ml m

Instrument :
ECD_O
ClientSampleId :
359-RO


Manual Integrations
APPROVED

Ankita
6/26/2020 9:21:20 AM

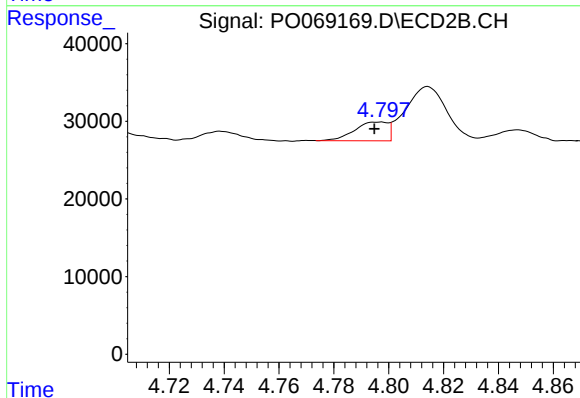


#21 AR-1248-1

R.T.: 4.797 min
Delta R.T.: 0.002 min
Response: 21696
Conc: 25.08 ng/ml m

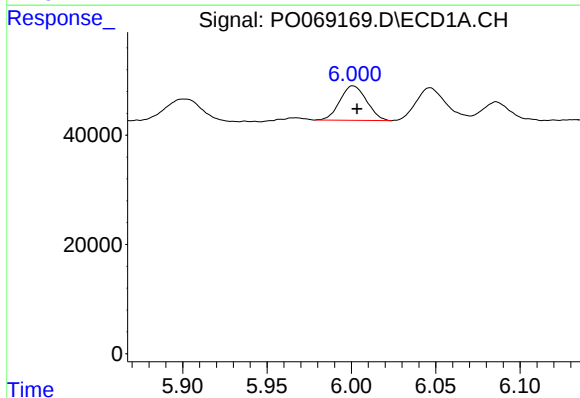


#22 AR-1248-2

R.T.: 6.001 min
Delta R.T.: -0.002 min
Response: 69648
Conc: 68.11 ng/ml

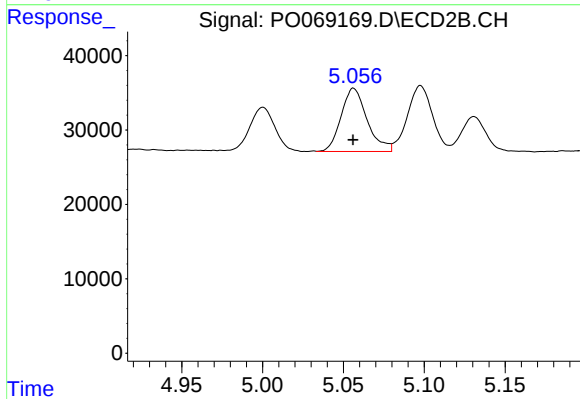

#22 AR-1248-2

R.T.: 5.056 min
Delta R.T.: 0.000 min
Response: 95213
Conc: 78.93 ng/ml

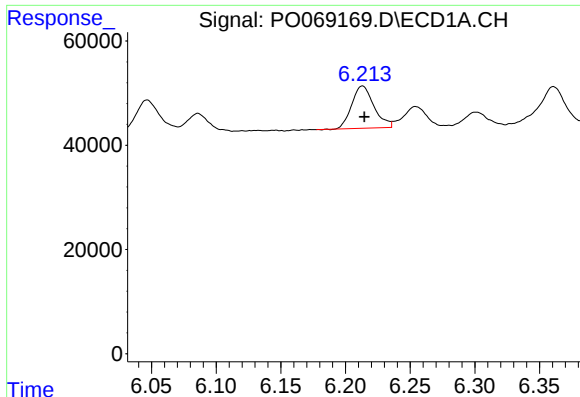


#23 AR-1248-3

R.T.: 6.213 min
Delta R.T.: -0.001 min
Response: 96879
Conc: 78.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
359-RO


Manual Integrations
APPROVED

Ankita
6/26/2020 9:21:20 AM

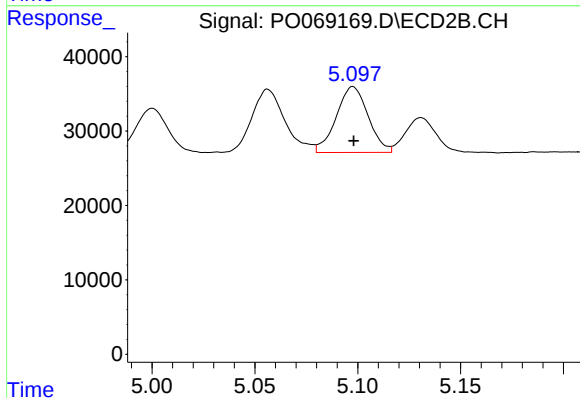


#23 AR-1248-3

R.T.: 5.098 min
Delta R.T.: 0.000 min
Response: 95528
Conc: 84.43 ng/ml

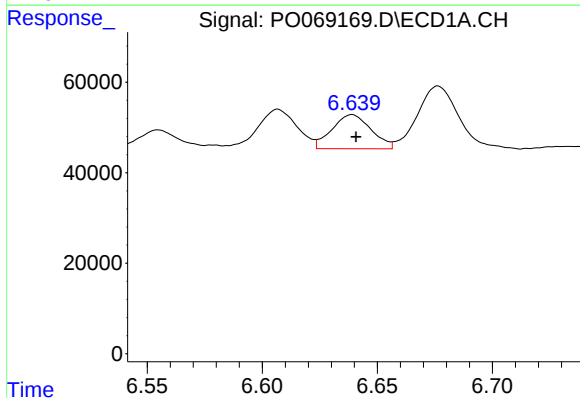


#24 AR-1248-4

R.T.: 6.639 min
Delta R.T.: -0.002 min
Response: 89488
Conc: 59.50 ng/ml

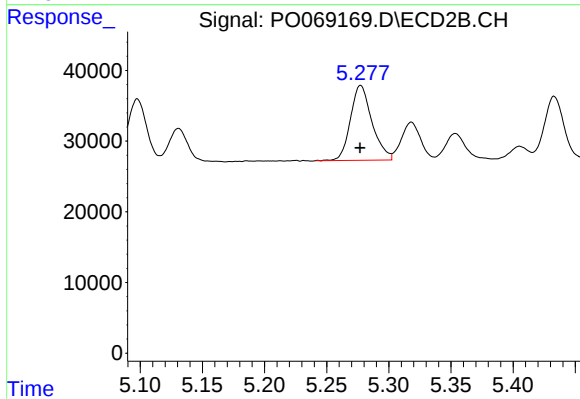

#24 AR-1248-4

R.T.: 5.277 min
Delta R.T.: 0.000 min
Response: 127763
Conc: 88.35 ng/ml

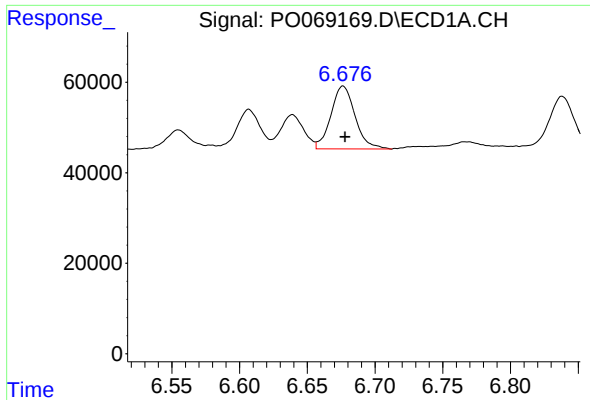


#25 AR-1248-5

R.T.: 6.676 min
Delta R.T.: -0.001 min
Response: 172921
Conc: 119.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
359-RO

Manual Integrations
APPROVED

Ankita
6/26/2020 9:21:20 AM

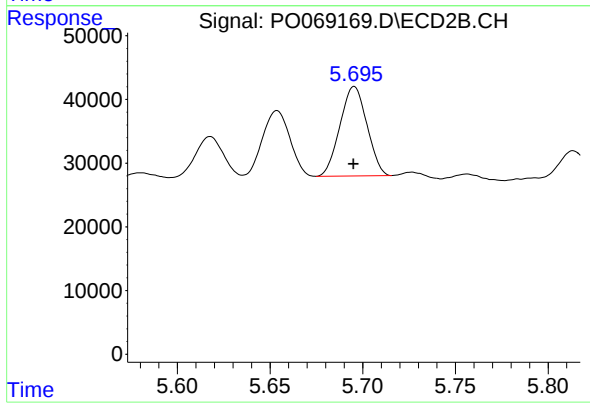

#25 AR-1248-5

R.T.: 5.695 min
Delta R.T.: 0.000 min
Response: 142194
Conc: 98.29 ng/ml