

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062420\
 Data File : P0069172.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jun 2020 16:53
 Operator : DD\AJ
 Sample : L3096-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-GF-03-011-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 18:06:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 19 05:15:02 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.405	3.566	905592	1048598	30.612	27.244
2) SA Decachlor...	10.072	8.774	1235741	1229932	26.018	22.594

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062420\
Data File : P0069172.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jun 2020 16:53
Operator : DD\AJ
Sample : L3096-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-GF-03-011-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 18:06:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 19 05:15:02 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

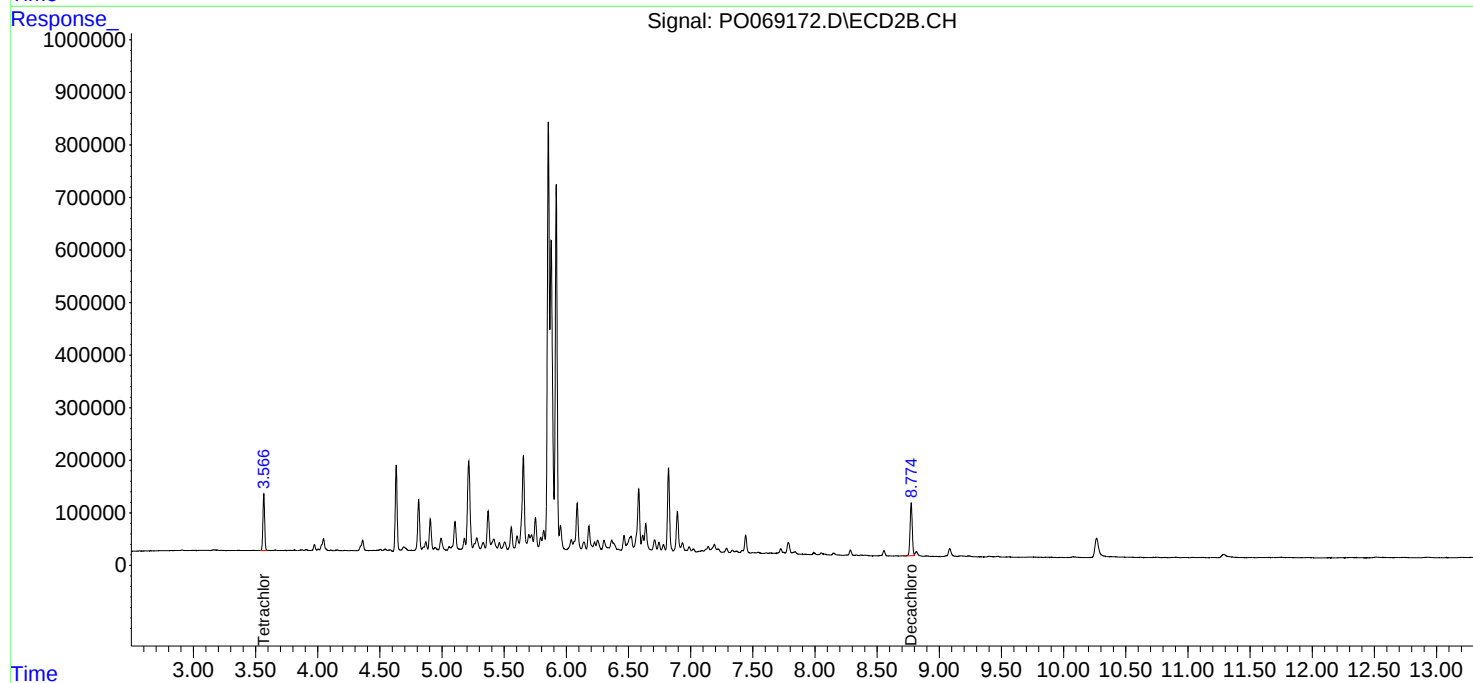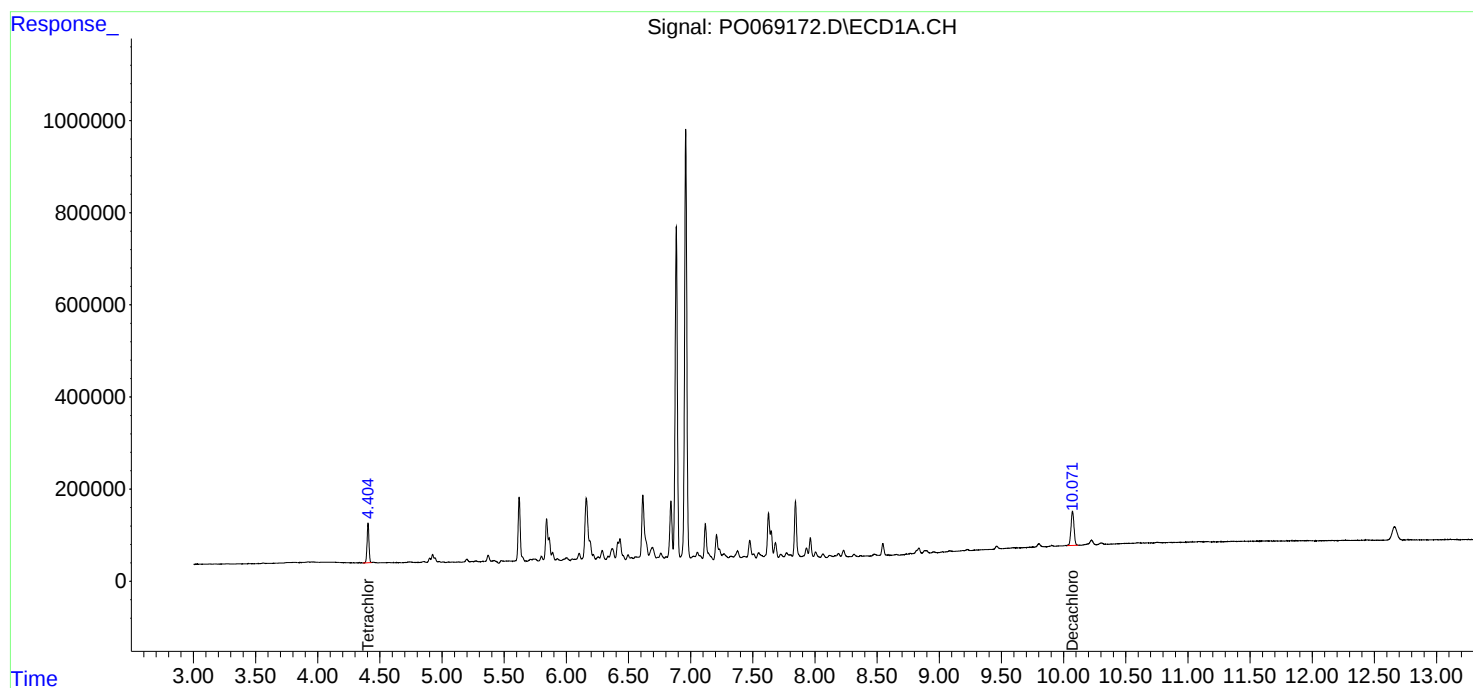


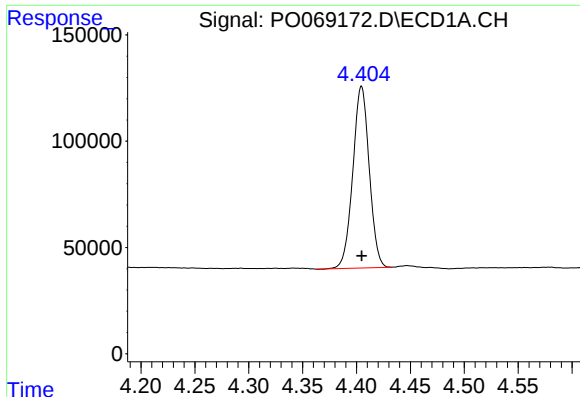

#1 Tetrachloro-m-xylene


R.T.: 4.405 min
Delta R.T.: 0.000 min
Response: 905592
Conc: 30.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-03-011-A

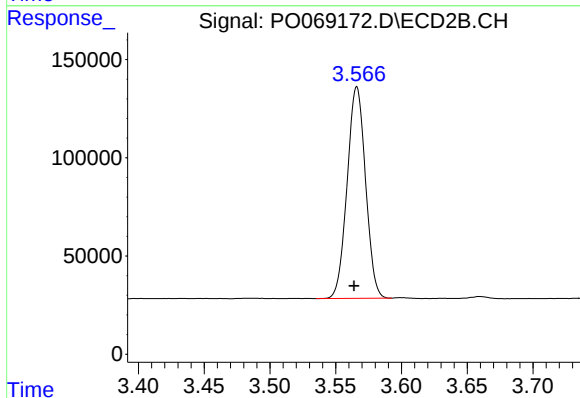


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.002 min
Response: 1048598
Conc: 27.24 ng/ml

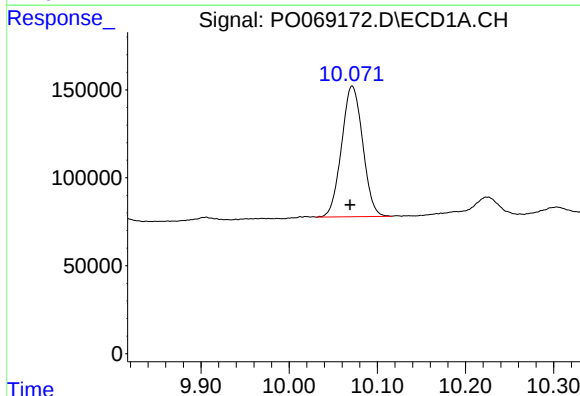

#2 Decachlorobiphenyl

R.T.: 10.072 min
Delta R.T.: 0.002 min
Response: 1235741
Conc: 26.02 ng/ml

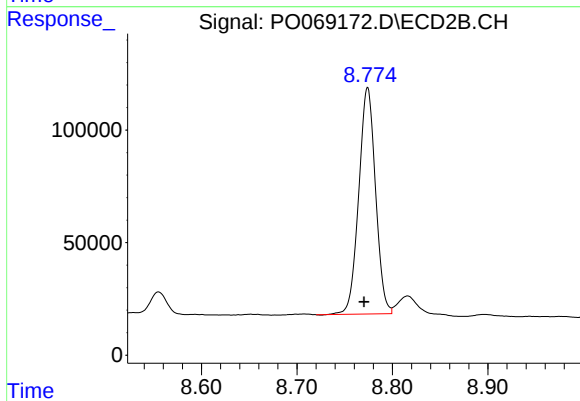

#2 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: 0.004 min
Response: 1229932
Conc: 22.59 ng/ml