

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0062518\
 Data File : P0046241.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jun 2018 00:35
 Operator : SM/UA
 Sample : J3642-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TEST-PIT-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 01:07:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 25 12:44:17 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.379	3.606	9023823	4049324	15.675	16.495
2) SA Decachlor...	10.044	8.574	5143673	2144429	11.359	13.040
Target Compounds						
7) L1 AR-1016-5	0.000	5.493	0	185701	N.D.	29.270 #
12) L3 AR-1232-2	5.474	0.000	250452	0	28.861	N.D. #
23) L5 AR-1248-3	0.000	5.493	0	185701	N.D.	15.196 #
24) L5 AR-1248-4	0.000	5.493	0	185701	N.D.	20.629 #
26) L6 AR-1254-1	0.000	5.493	0	185701	N.D.	14.683 #
30) L6 AR-1254-5	0.000	6.514	0	710976	N.D.	90.503 #
32) L7 AR-1260-2	7.342	0.000	1199577	0	36.165	N.D. #
37) L8 AR-1262-2	7.342	6.514	1199577	710976	45.813	62.955 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062518\
Data File : P0046241.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2018 00:35
Operator : SM/UA
Sample : J3642-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:07:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 25 12:44:17 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

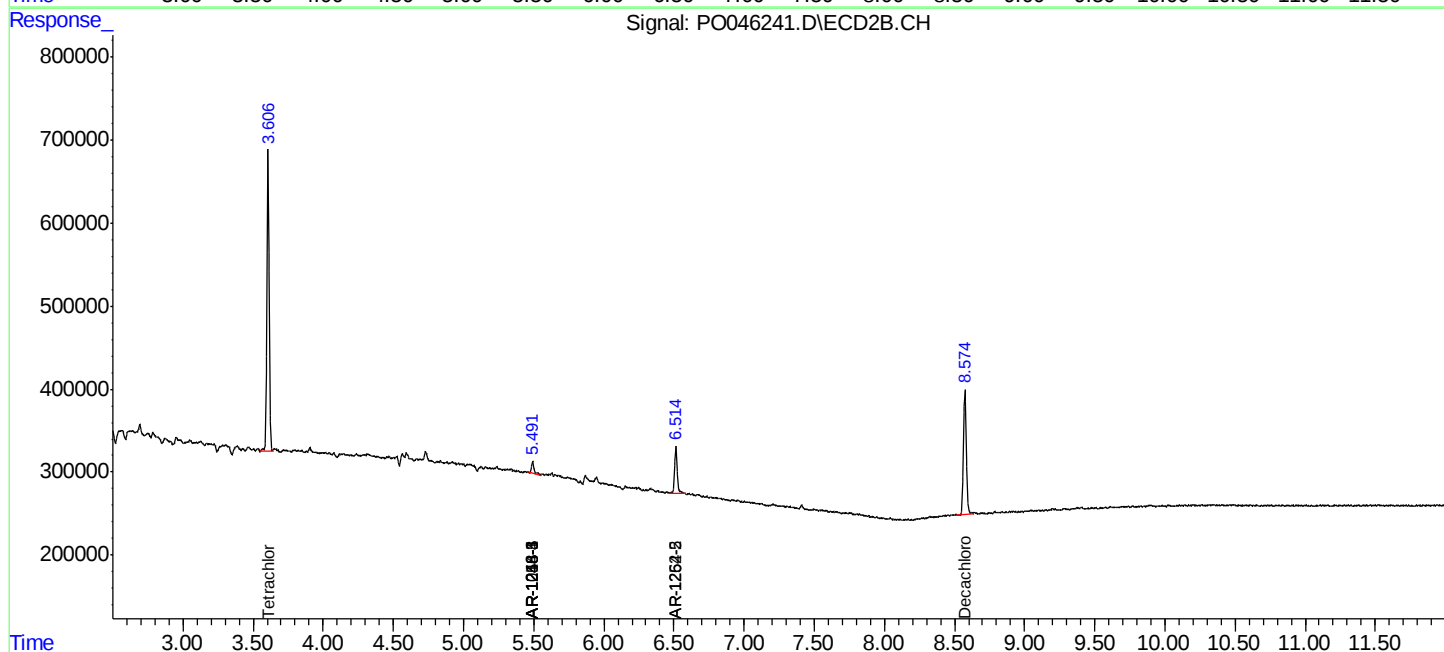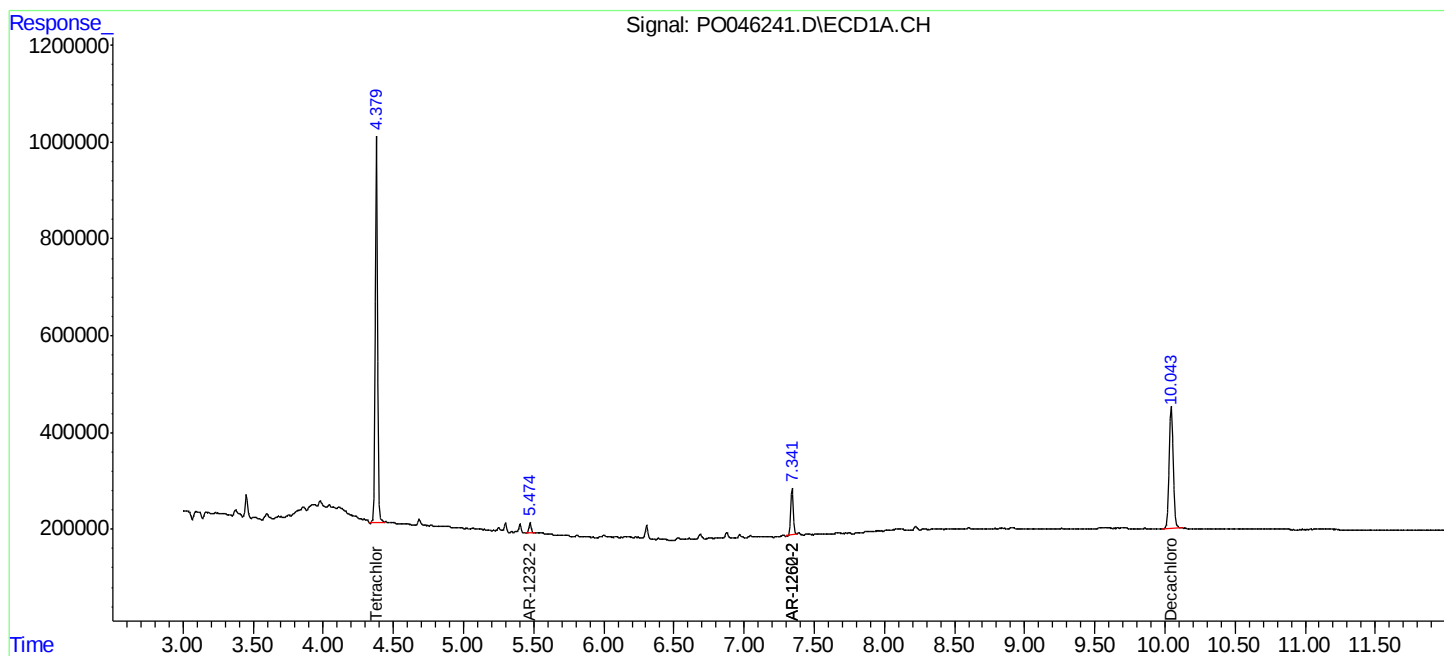


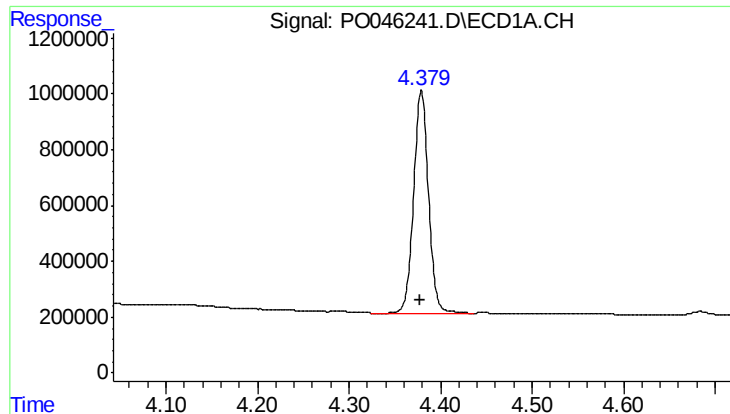

#1 Tetrachloro-m-xylene


R.T.: 4.379 min
Delta R.T.: 0.000 min
Response: 9023823
Conc: 15.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-1

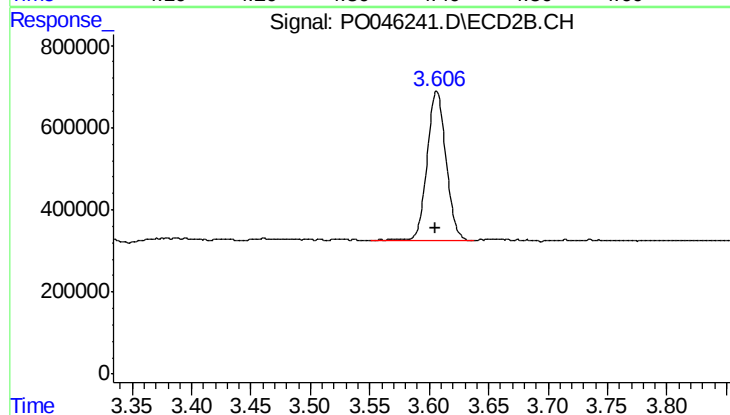


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 4049324
Conc: 16.49 ng/ml

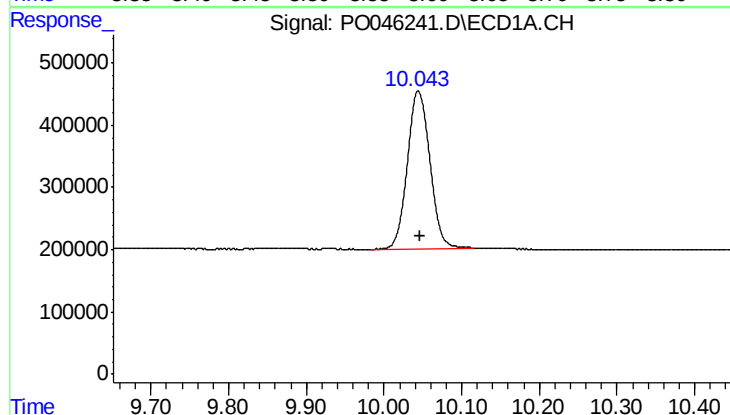


#2 Decachlorobiphenyl

R.T.: 10.044 min
Delta R.T.: -0.002 min
Response: 5143673
Conc: 11.36 ng/ml

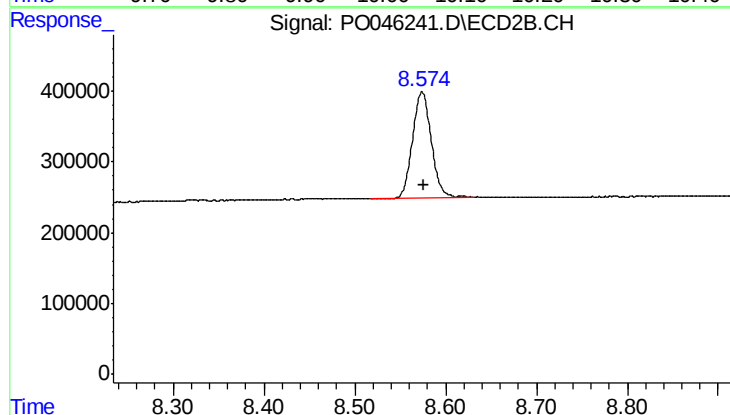

#2 Decachlorobiphenyl


R.T.: 8.574 min
Delta R.T.: -0.002 min
Response: 2144429
Conc: 13.04 ng/ml

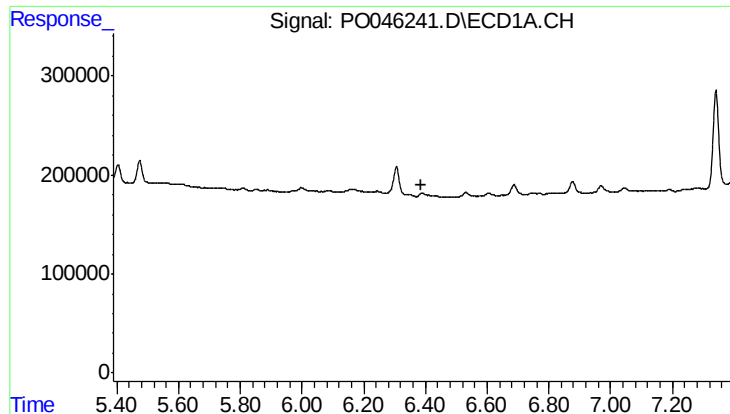

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-1

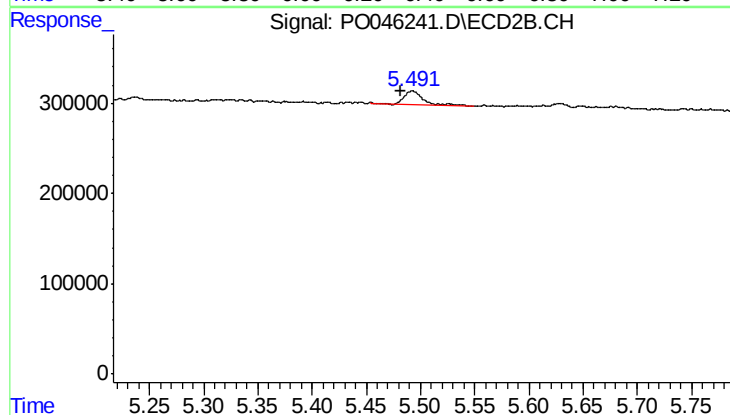


#7 AR-1016-5

R.T.: 5.493 min
Delta R.T.: 0.010 min
Response: 185701
Conc: 29.27 ng/ml

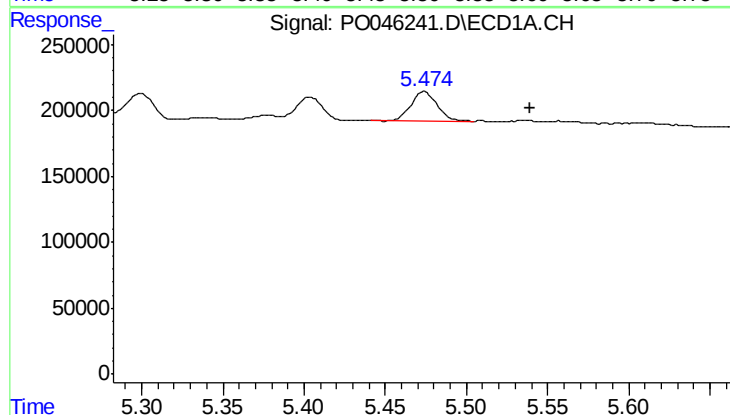


#12 AR-1232-2

R.T.: 5.474 min
Delta R.T.: -0.065 min
Response: 250452
Conc: 28.86 ng/ml

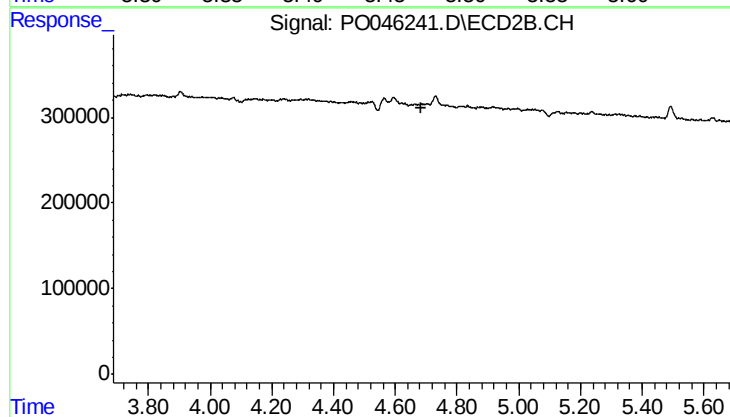

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 4.686 min
Response: 0
Conc: N.D.

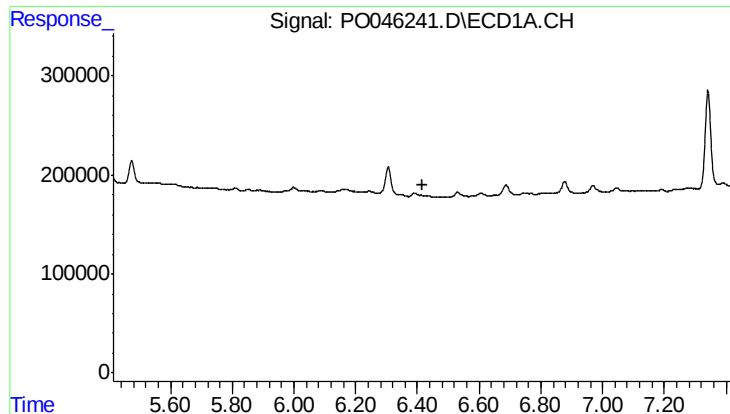

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.415 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-1

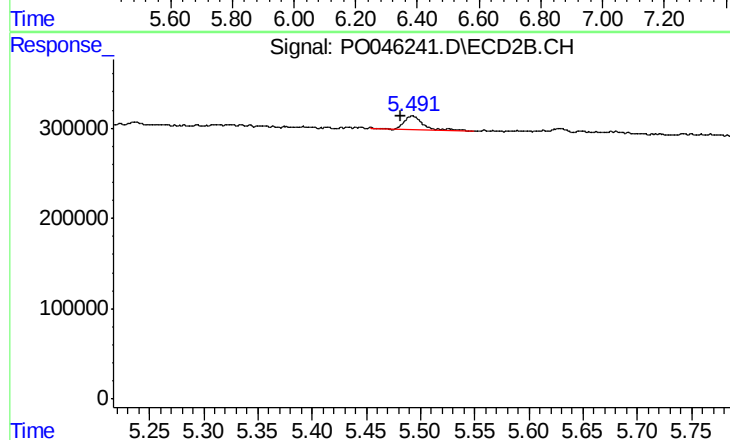


#23 AR-1248-3

R.T.: 5.493 min
Delta R.T.: 0.011 min
Response: 185701
Conc: 15.20 ng/ml

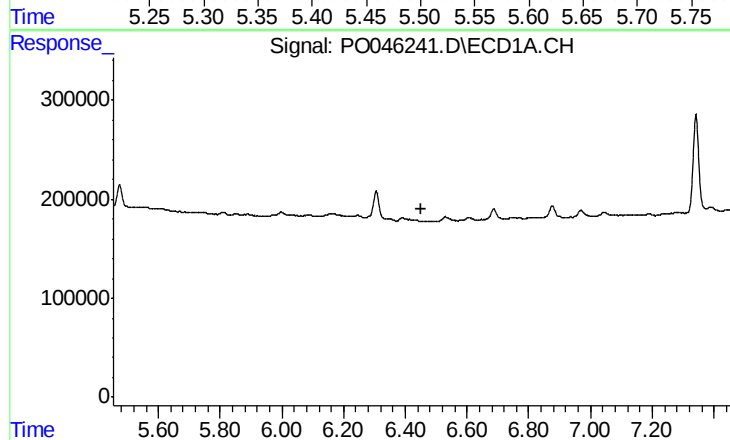


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.454 min
Response: 0
Conc: N.D.

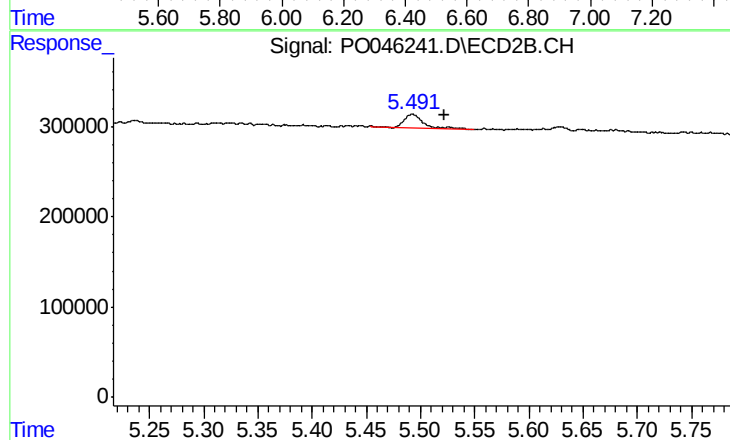

#24 AR-1248-4


R.T.: 5.493 min
Delta R.T.: -0.030 min
Response: 185701
Conc: 20.63 ng/ml

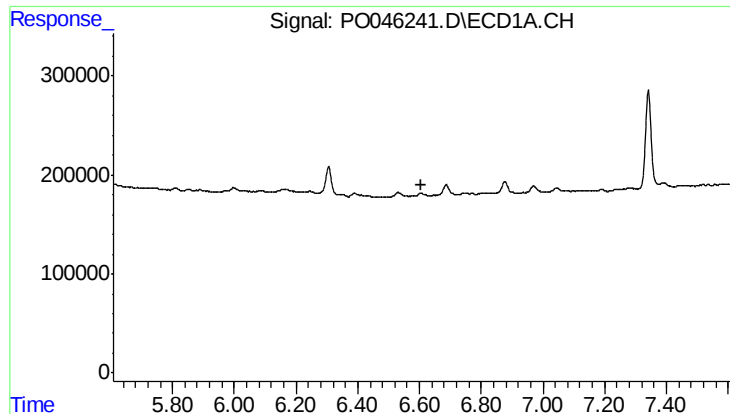

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-1

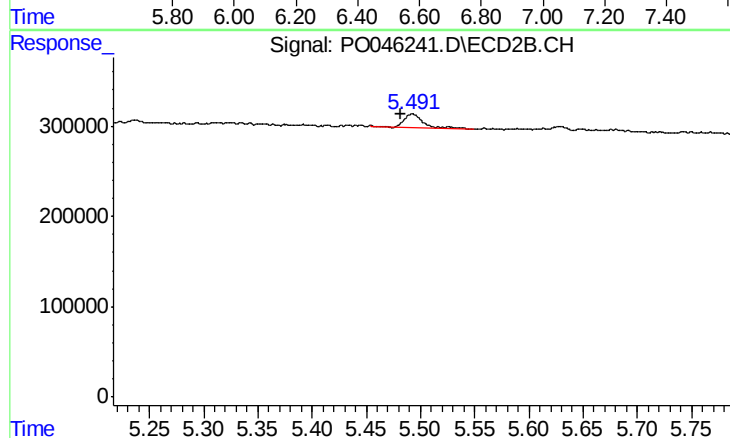


#26 AR-1254-1

R.T.: 5.493 min
Delta R.T.: 0.011 min
Response: 185701
Conc: 14.68 ng/ml

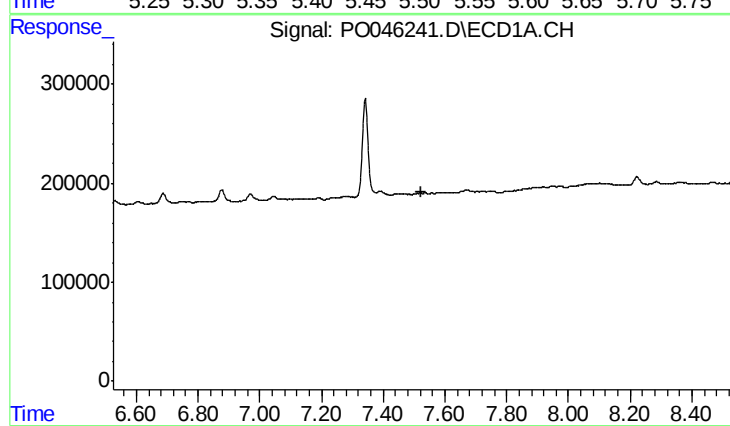


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.525 min
Response: 0
Conc: N.D.

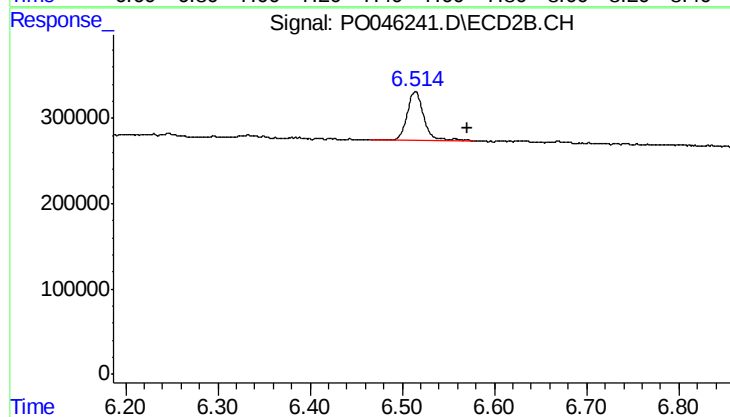

#30 AR-1254-5


R.T.: 6.514 min
Delta R.T.: -0.057 min
Response: 710976
Conc: 90.50 ng/ml

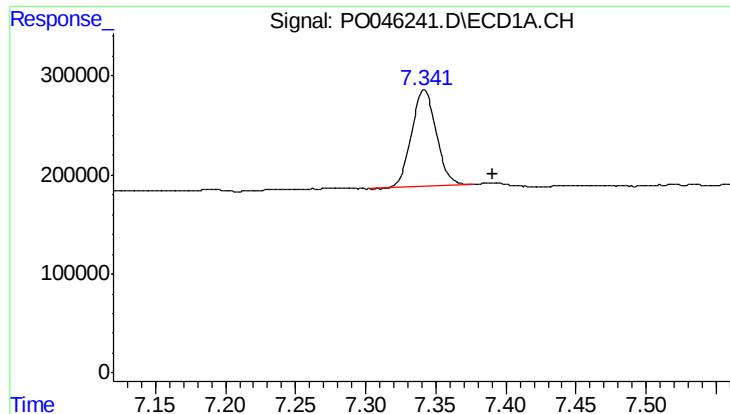

#32 AR-1260-2


R.T.: 7.342 min
Delta R.T.: -0.049 min
Response: 1199577
Conc: 36.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-1

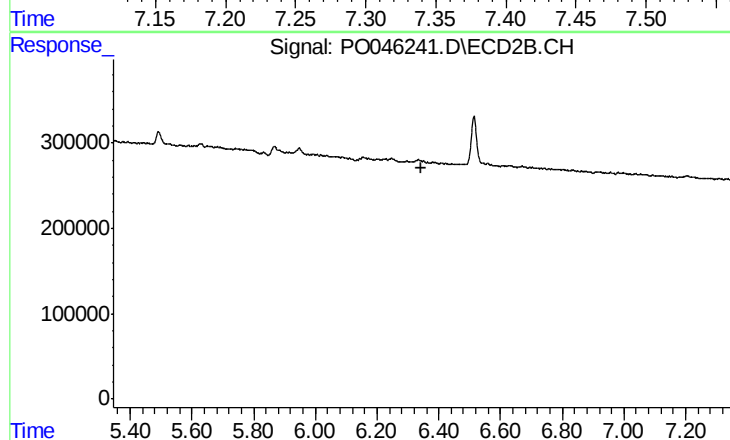


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 6.345 min
Response: 0
Conc: N.D.

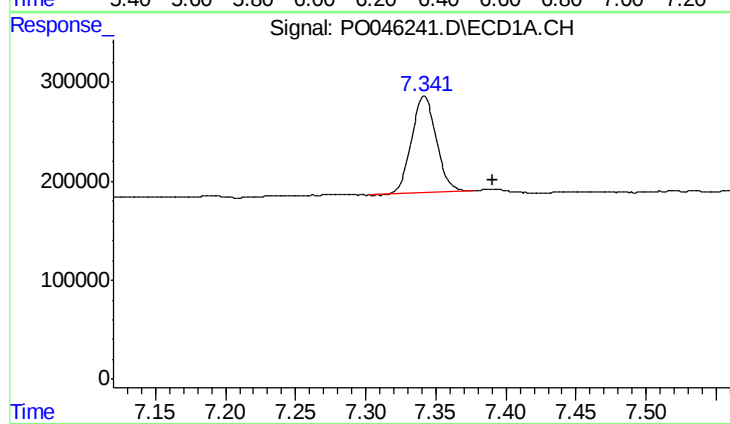

#37 AR-1262-2

R.T.: 7.342 min
Delta R.T.: -0.049 min
Response: 1199577
Conc: 45.81 ng/ml

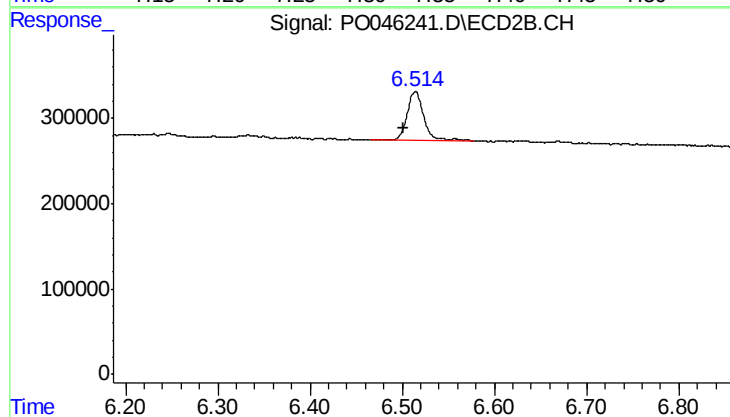

#37 AR-1262-2

R.T.: 6.514 min
Delta R.T.: 0.013 min
Response: 710976
Conc: 62.95 ng/ml