

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062518\
Data File : P0046202.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2018 13:47
Operator : SM/UA
Sample : J3627-03 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
26KV-CC-2

Manual Integrations
APPROVED

ugo
6/26/2018 10:09:16 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 16:27:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 25 12:49:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.378	3.604	1232880	644453	2.109m	2.596
2)	SA Decachlor...	10.047	8.575	939243	409359	2.037	2.447

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062518\
Data File : P0046202.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2018 13:47
Operator : SM/UA
Sample : J3627-03 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
26KV-CC-2


Manual Integrations
APPROVED

ugo
6/26/2018 10:09:16 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 16:27:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 25 12:49:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

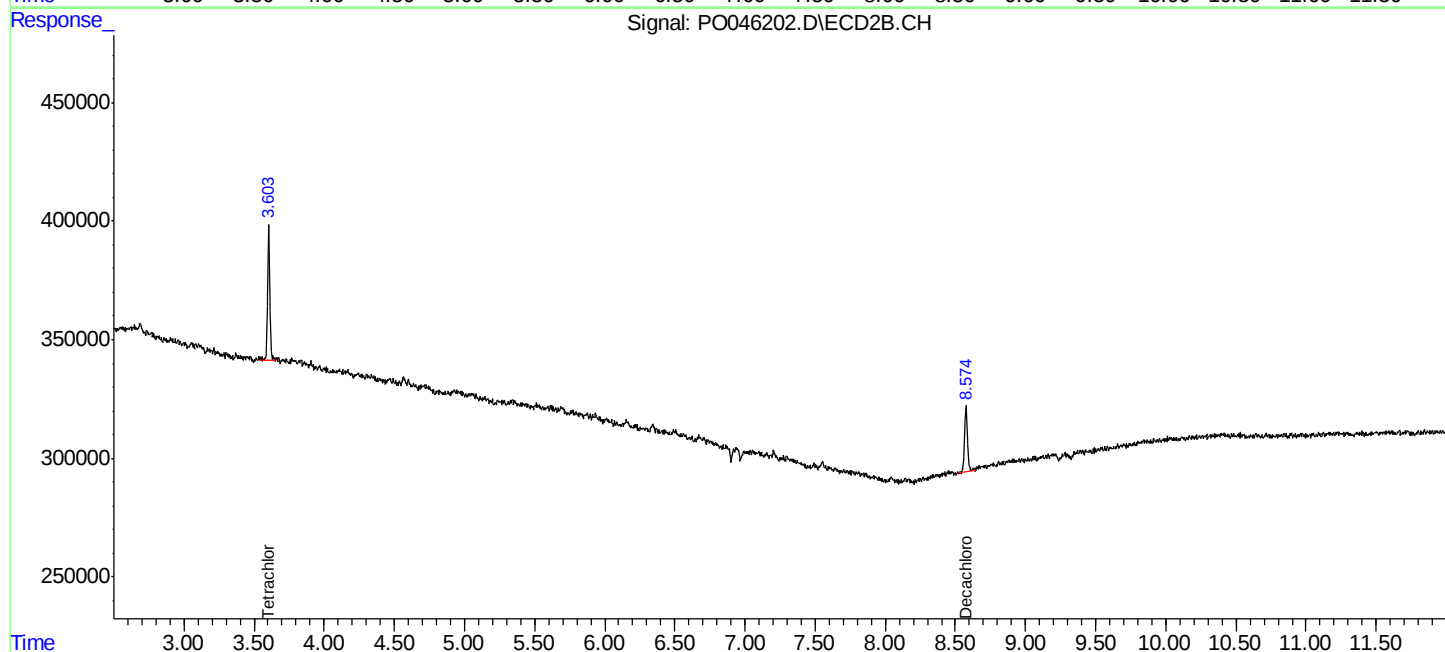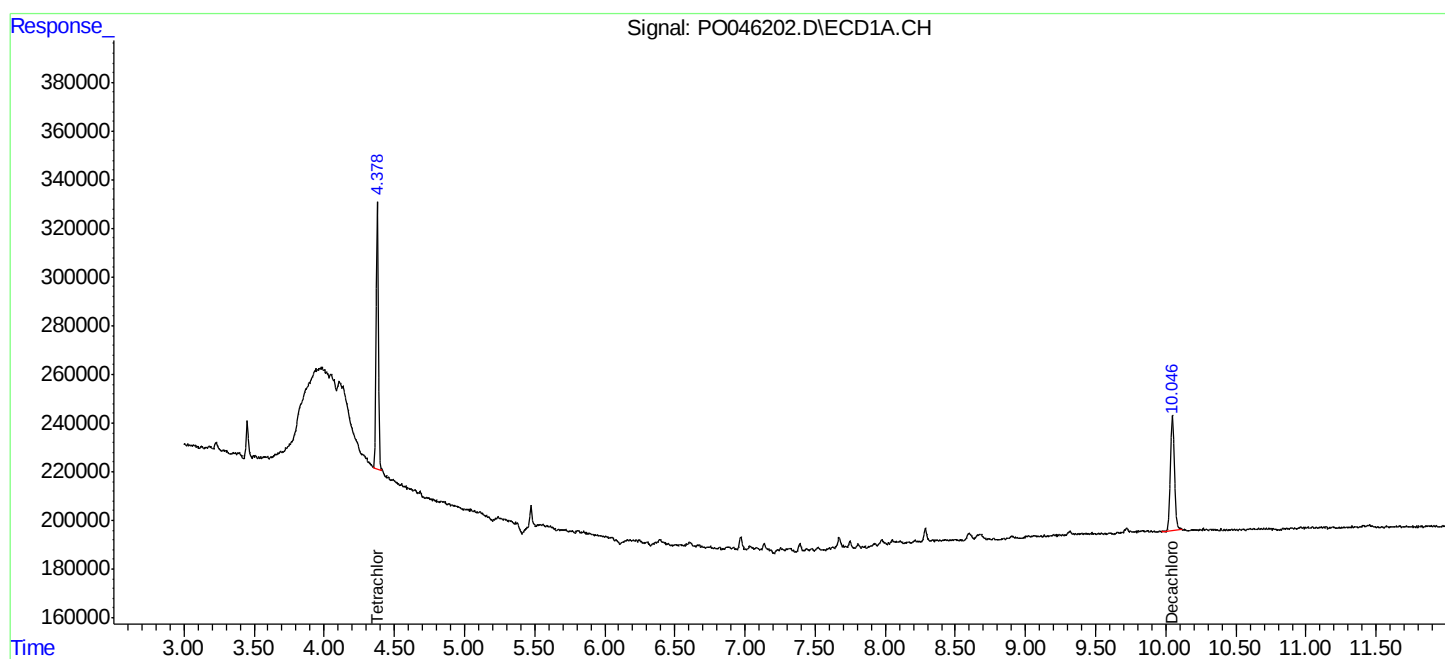

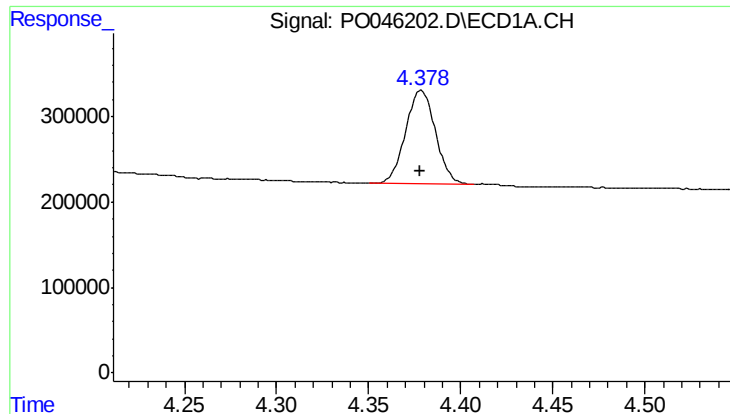


#1 Tetrachloro-m-xylene

R.T.: 4.378 min
Delta R.T.: 0.000 min
Response: 1232880
Conc: 2.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
26KV-CC-2


Manual Integrations
APPROVED

ugo
6/26/2018 10:09:16 AM

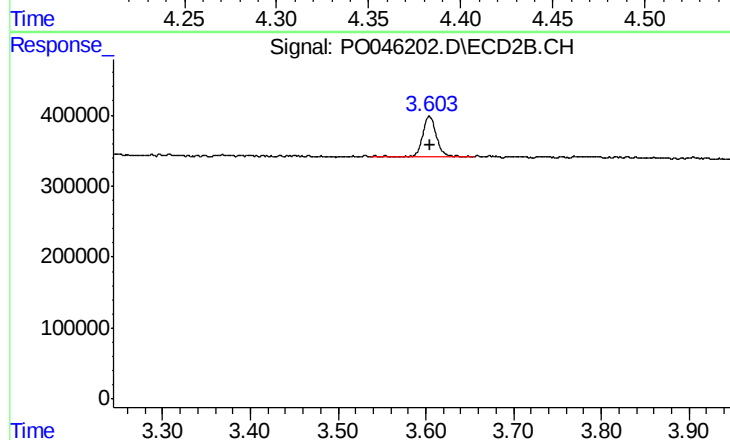


#1 Tetrachloro-m-xylene

R.T.: 3.604 min
Delta R.T.: 0.000 min
Response: 644453
Conc: 2.60 ng/ml

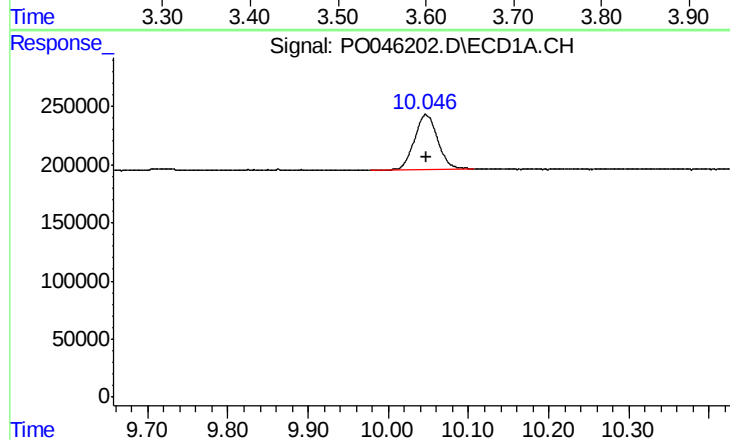

#2 Decachlorobiphenyl

R.T.: 10.047 min
Delta R.T.: 0.000 min
Response: 939243
Conc: 2.04 ng/ml

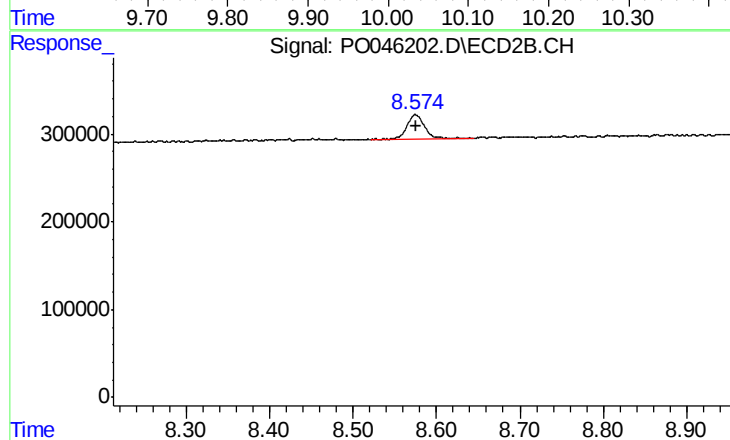

#2 Decachlorobiphenyl

R.T.: 8.575 min
Delta R.T.: 0.000 min
Response: 409359
Conc: 2.45 ng/ml